

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 15:45
 Operator : AJ\SJ
 Sample : J4280-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 00:59:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.905	92498860	39348008	13.232	14.677
28)	SA Decachlor...	7.958	8.892	69770571	31046741	9.934	13.379 #
Target Compounds							
2)	A alpha-BHC	3.686f	4.323f	14810387	7859299	1.253	1.866 #
9)	A Endosulfan I	5.323	0.000	2535734	0	0.290	N.D. #
10)	B gamma-Chl...	5.202	0.000	11814698	0	1.196	N.D. #
11)	B alpha-Chl...	5.202f	0.000	11814698	0	1.230	N.D. #
12)	B 4,4'-DDE	5.407	0.000	9173982	0	0.958	N.D. #
17)	MA 4,4'-DDT	6.148	0.000	16630687	0	2.194	N.D. #
23)	Chlordane-1	4.155	0.000	5527180	0	17.459	N.D. #
25)	Chlordane-3	5.202	0.000	11814698	0	10.817	N.D. #
26)	Chlordane-4	5.202	0.000	11814698	0	11.822	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 15:45
Operator : AJ\SJ
Sample : J4280-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 00:59:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

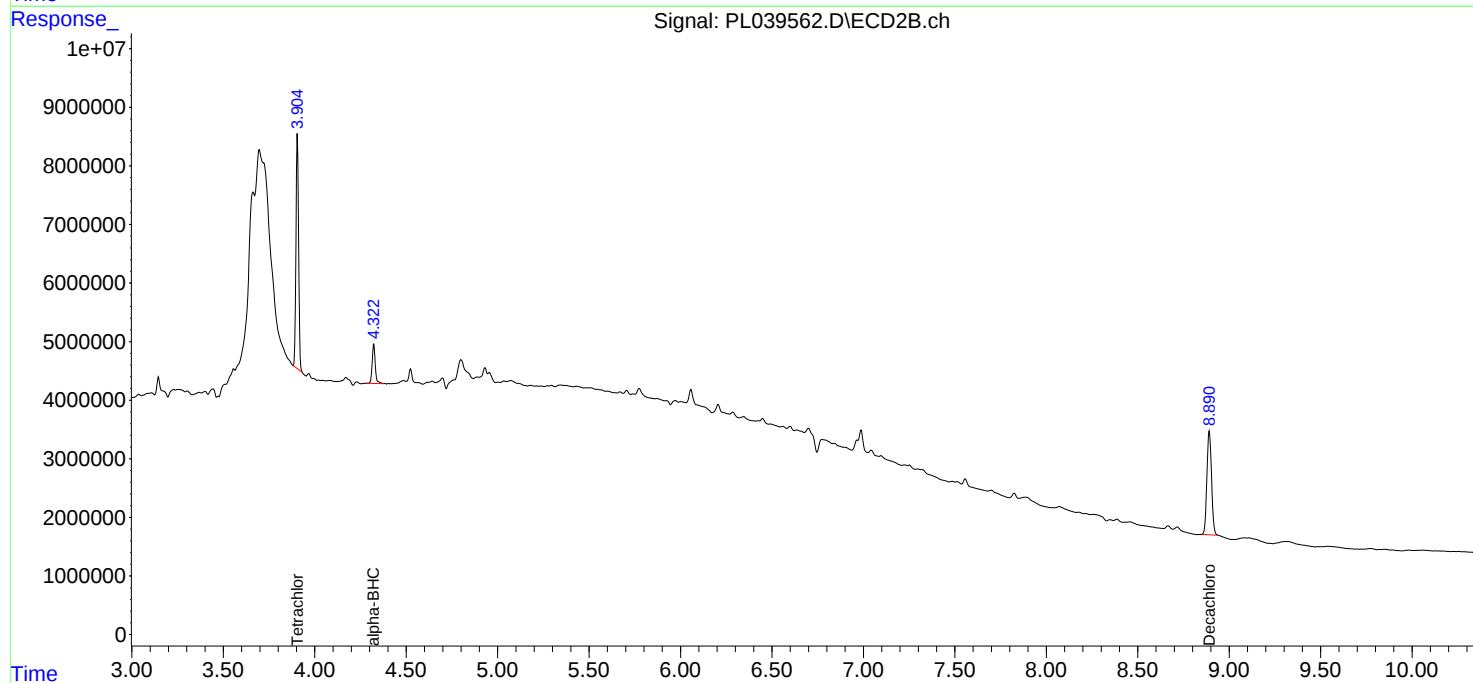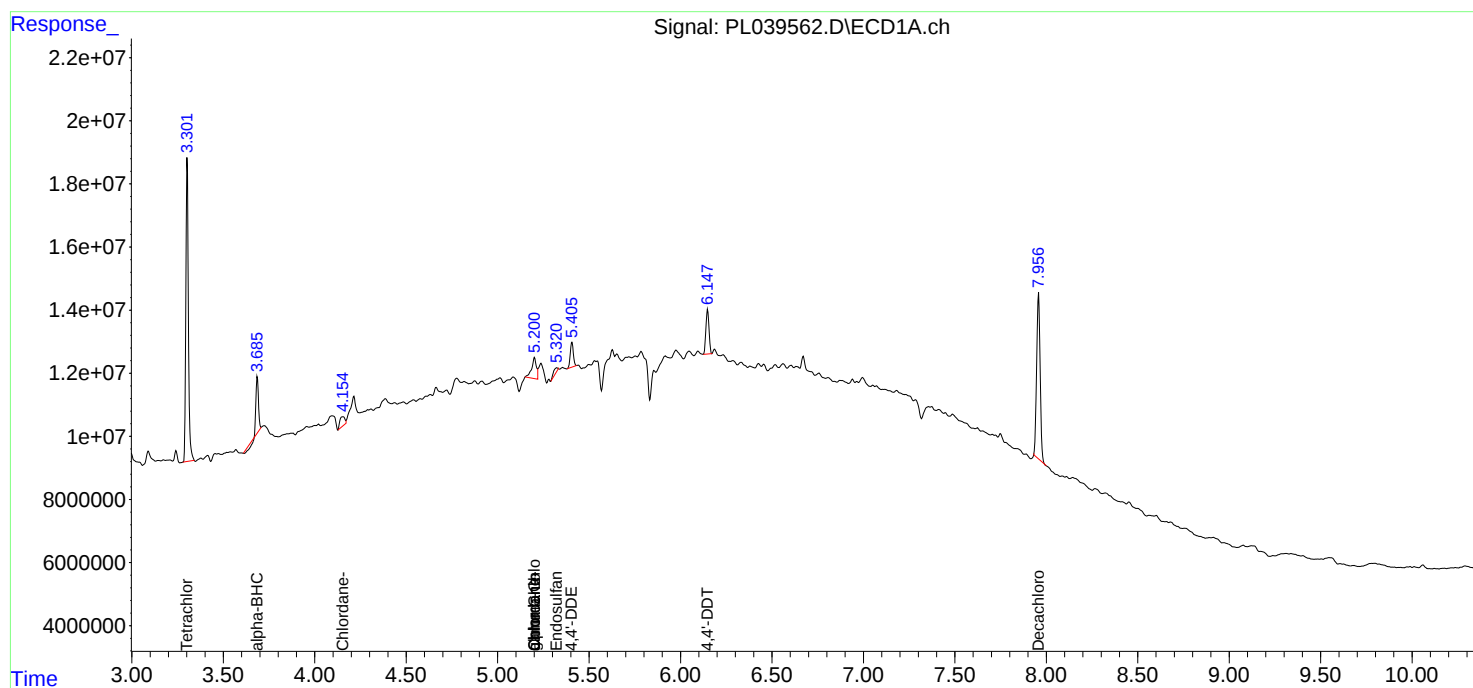


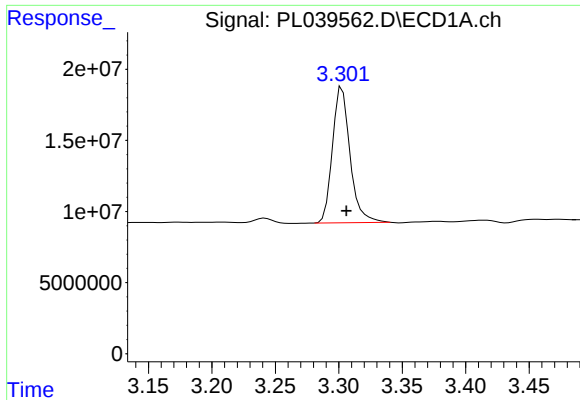

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 92498860
Conc: 13.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

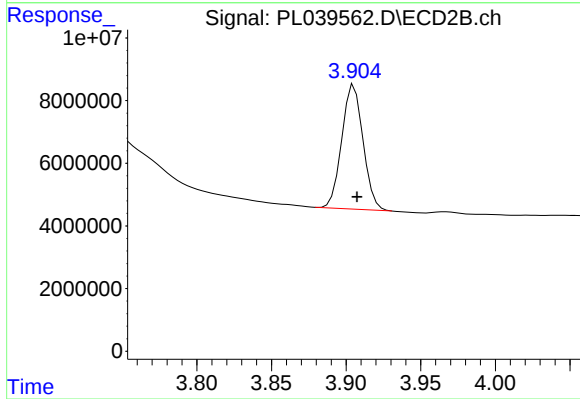


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 39348008
Conc: 14.68 ng/ml

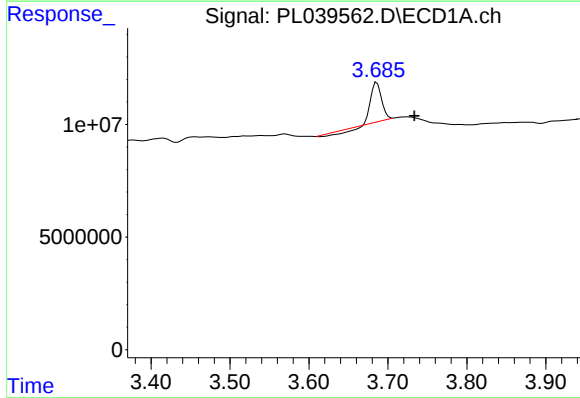


#2 alpha-BHC

R.T.: 3.686 min
Delta R.T.: -0.048 min
Response: 14810387
Conc: 1.25 ng/ml

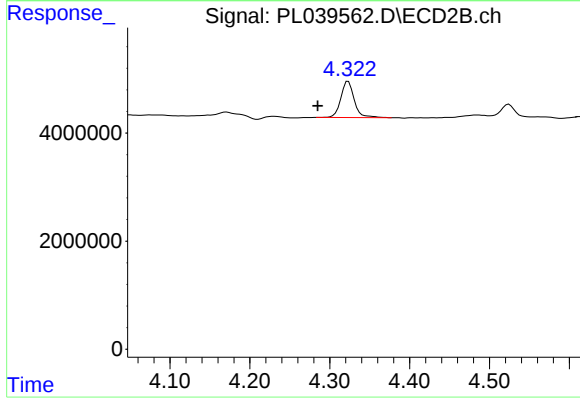

#2 alpha-BHC


R.T.: 4.323 min
Delta R.T.: 0.038 min
Response: 7859299
Conc: 1.87 ng/ml

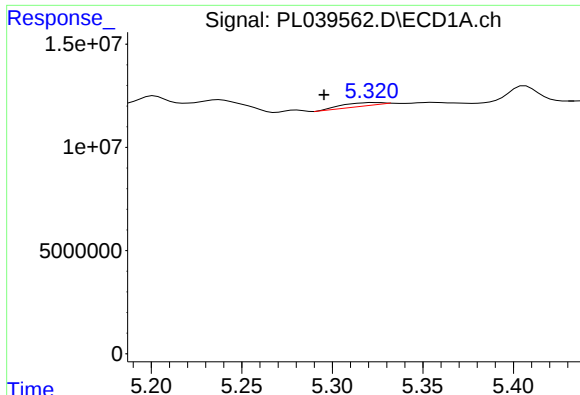

#9 Endosulfan I


R.T.: 5.323 min
Delta R.T.: 0.028 min
Response: 2535734
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

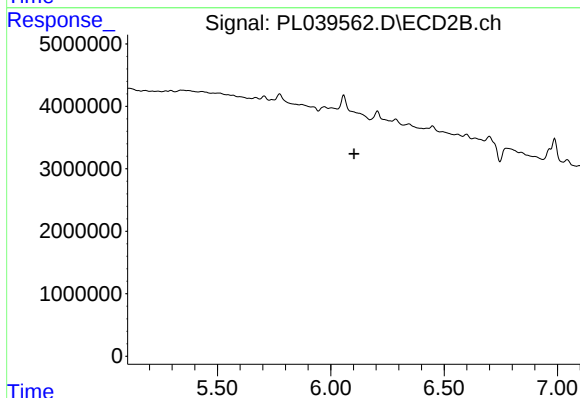


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

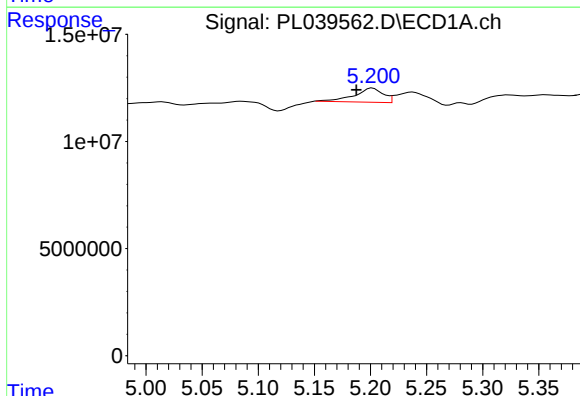


#10 gamma-Chlordane

R.T.: 5.202 min
Delta R.T.: 0.014 min
Response: 11814698
Conc: 1.20 ng/ml

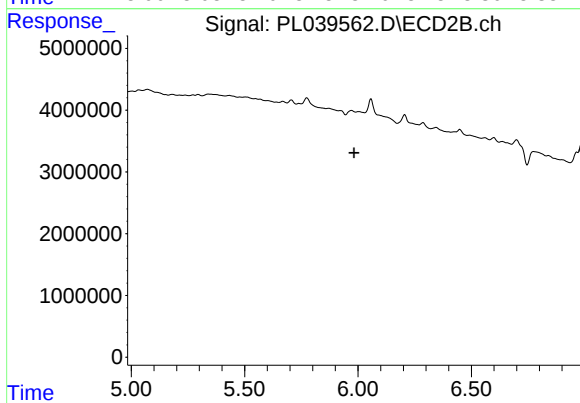

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

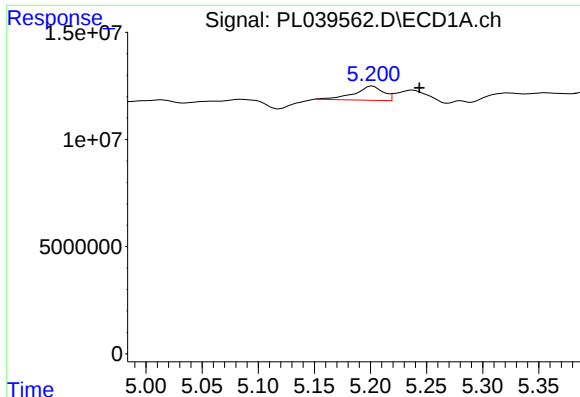

#11 alpha-Chlordane


R.T.: 5.202 min
Delta R.T.: -0.042 min
Response: 11814698
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

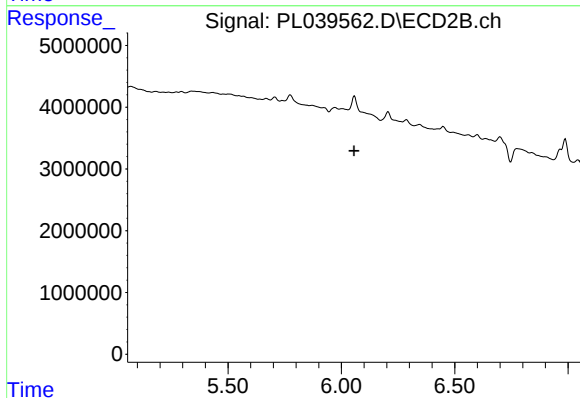


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

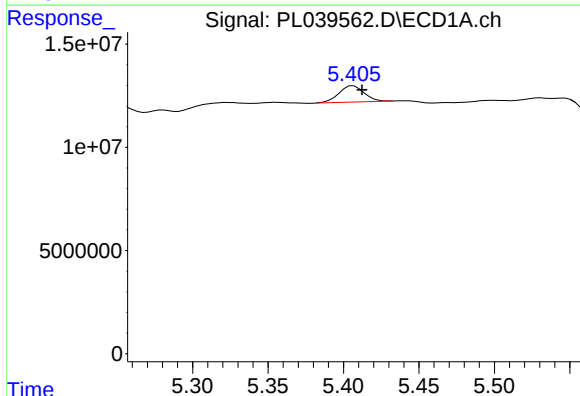


#12 4,4'-DDE

R.T.: 5.407 min
Delta R.T.: -0.006 min
Response: 9173982
Conc: 0.96 ng/ml

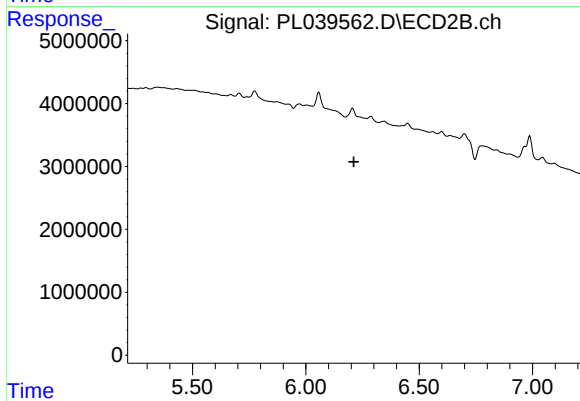

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

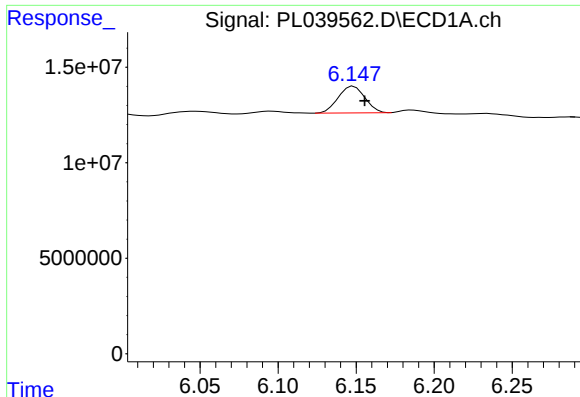

#17 4,4'-DDT


R.T.: 6.148 min
Delta R.T.: -0.007 min
Response: 16630687
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

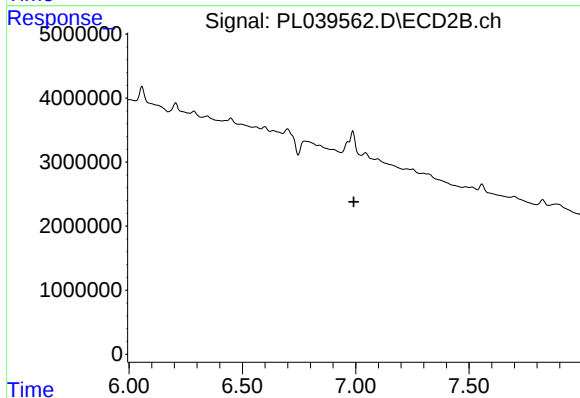


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

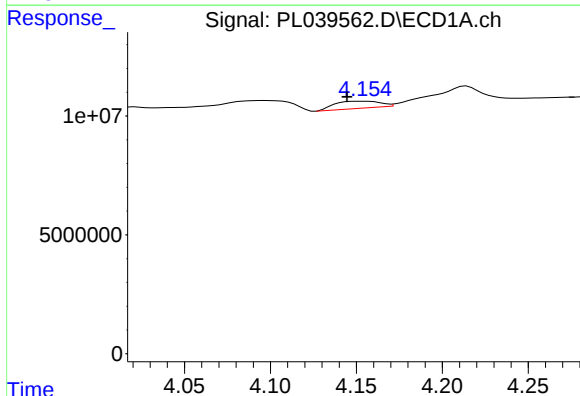


#23 Chlordane-1

R.T.: 4.155 min
Delta R.T.: 0.011 min
Response: 5527180
Conc: 17.46 ng/ml

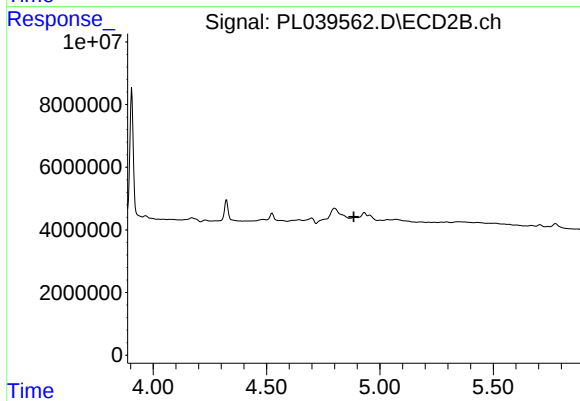

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

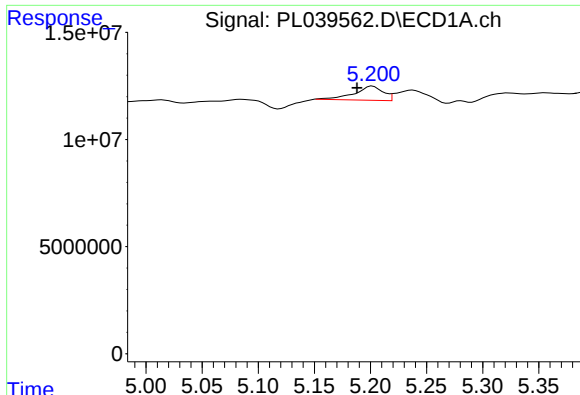

#25 Chlordane-3


R.T.: 5.202 min
Delta R.T.: 0.014 min
Response: 11814698
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

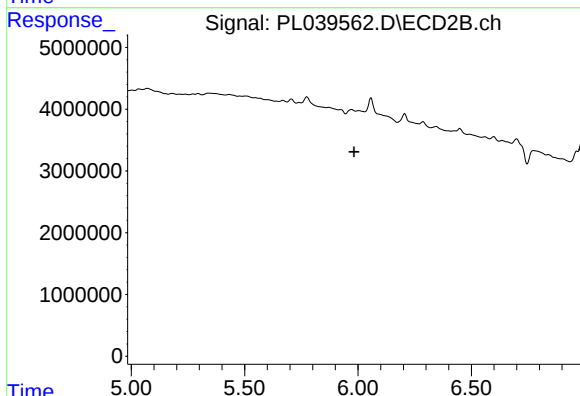


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

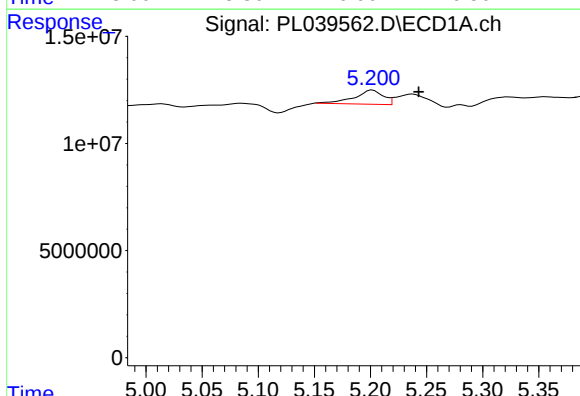


#26 Chlordane-4

R.T.: 5.202 min
Delta R.T.: -0.041 min
Response: 11814698
Conc: 11.82 ng/ml

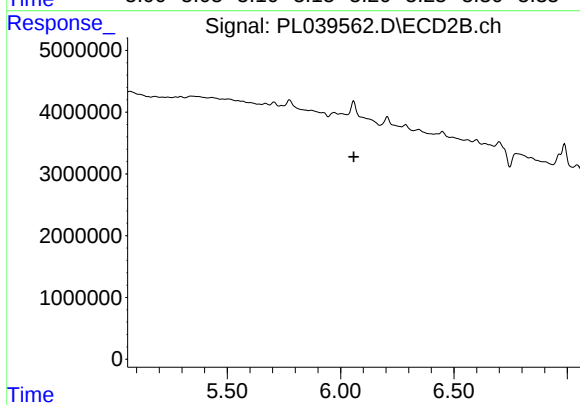

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

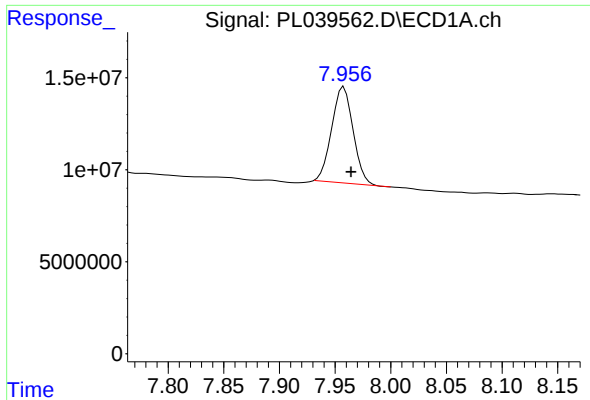

#28 Decachlorobiphenyl


R.T.: 7.958 min

Delta R.T.: -0.007 min

Response: 69770571

Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

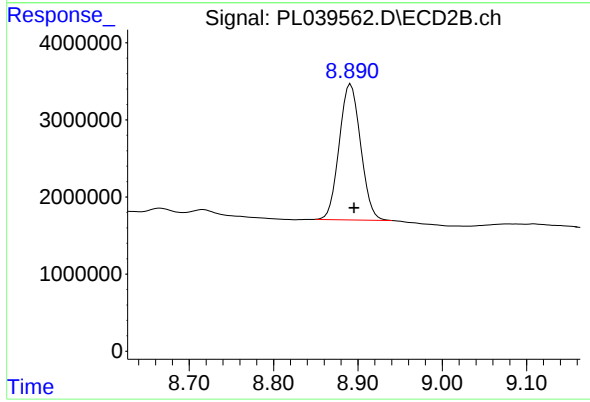

#28 Decachlorobiphenyl

R.T.: 8.892 min

Delta R.T.: -0.004 min

Response: 31046741

Conc: 13.38 ng/ml