

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 15:59
 Operator : AJ\SJ
 Sample : J4280-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 00:59:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.905	100.1E6	43252128	14.321	16.133
28)	SA Decachlor...	7.957	8.892	75274044	30987361	10.718	13.353
Target Compounds							
2)	A alpha-BHC	3.686f	4.323f	32322650	12261680	2.735	2.912
10)	B gamma-Chl...	5.201	0.000	6533829	0	0.662	N.D. #
11)	B alpha-Chl...	5.201f	0.000	6533829	0	0.680	N.D. #
12)	B 4,4'-DDE	5.406	0.000	12408361	0	1.296	N.D. #
17)	MA 4,4'-DDT	6.148	0.000	21004911	0	2.771	N.D. #
20)	A Methoxychlor	6.671	0.000	9928647	0	2.426	N.D. #
23)	Chlordane-1	4.214	0.000	11522099	0	36.395	N.D. #
25)	Chlordane-3	5.201	0.000	6533829	0	5.982	N.D. #
26)	Chlordane-4	5.201	0.000	6533829	0	6.538	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 15:59
Operator : AJ\SJ
Sample : J4280-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 00:59:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

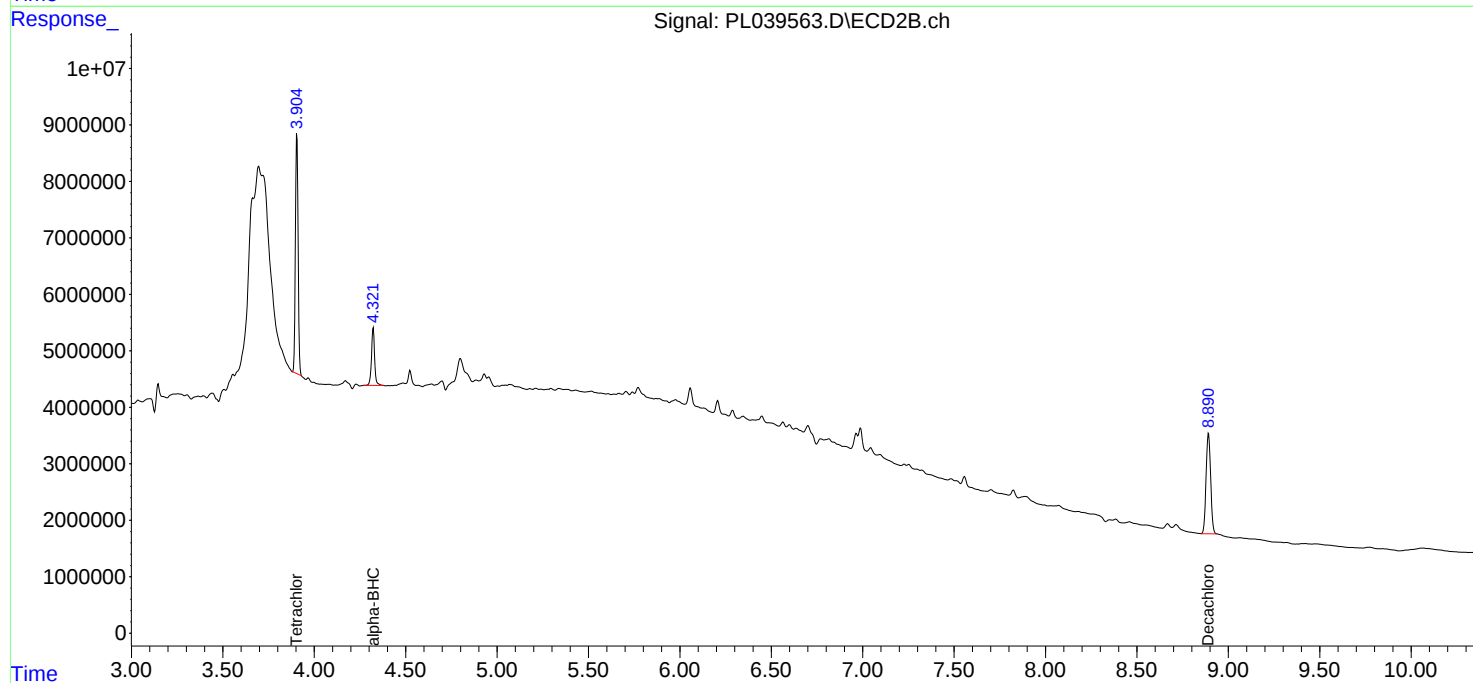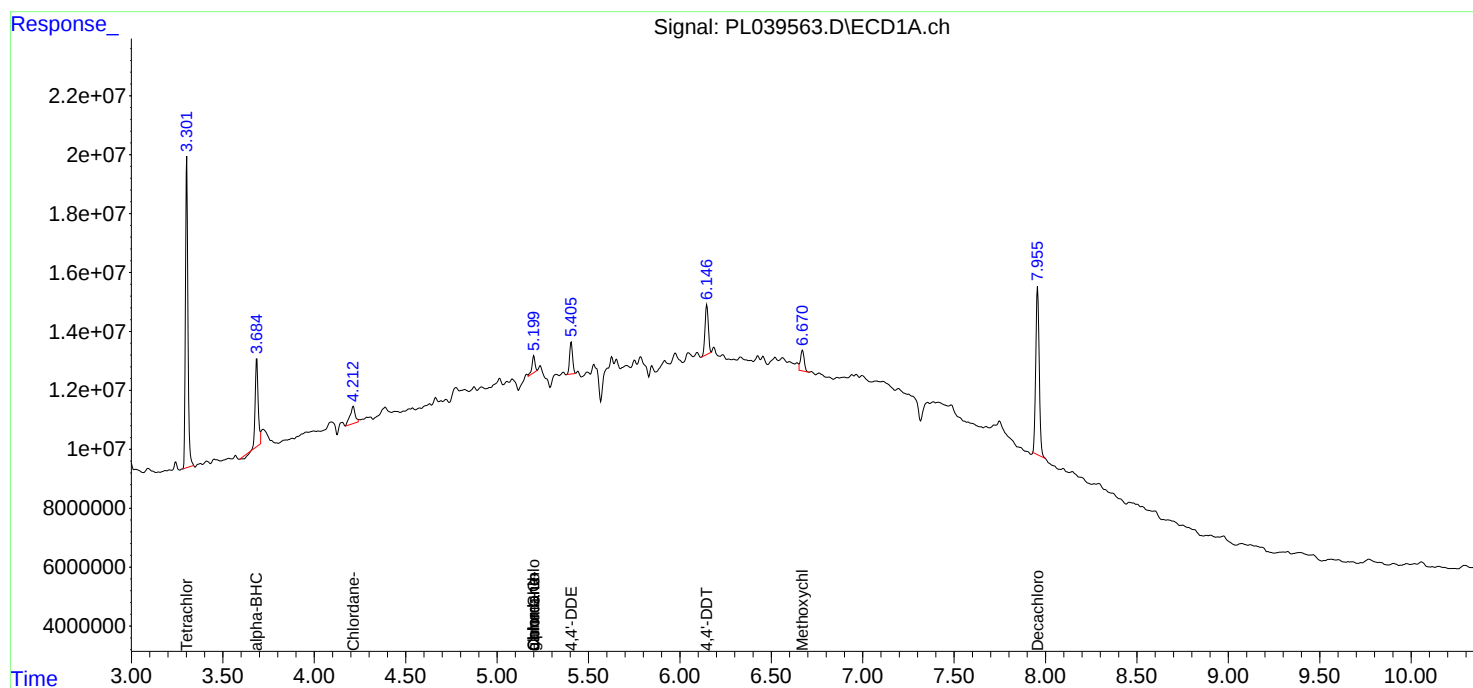


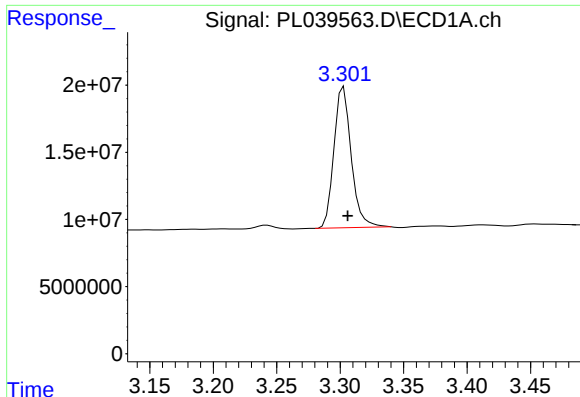

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 100112601
Conc: 14.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

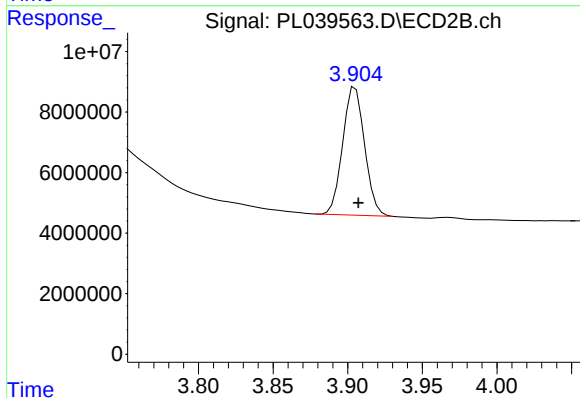


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 43252128
Conc: 16.13 ng/ml

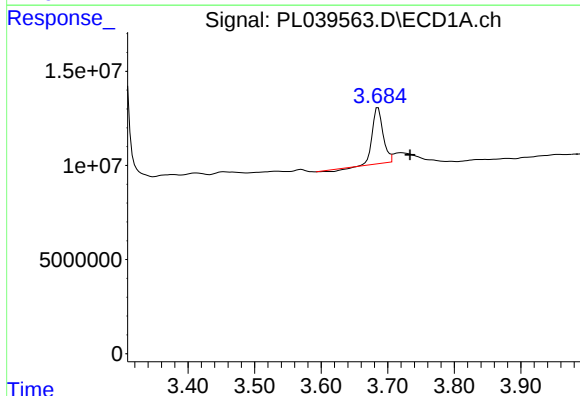


#2 alpha-BHC

R.T.: 3.686 min
Delta R.T.: -0.048 min
Response: 32322650
Conc: 2.73 ng/ml

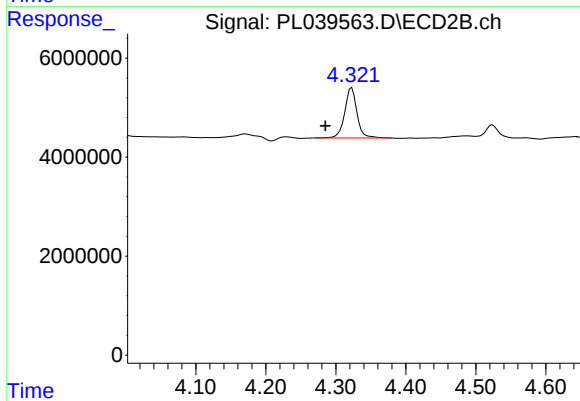

#2 alpha-BHC


R.T.: 4.323 min
Delta R.T.: 0.038 min
Response: 12261680
Conc: 2.91 ng/ml

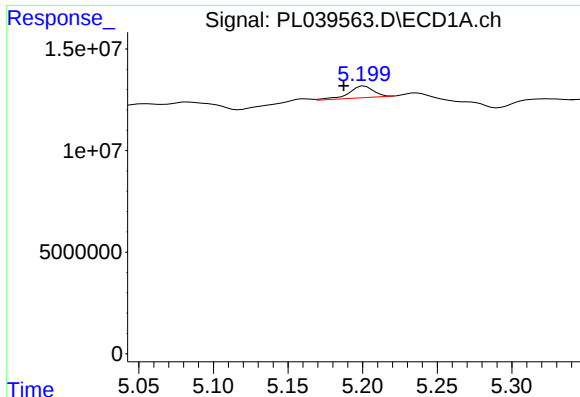

#10 gamma-Chlordane


R.T.: 5.201 min
Delta R.T.: 0.014 min
Response: 6533829
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

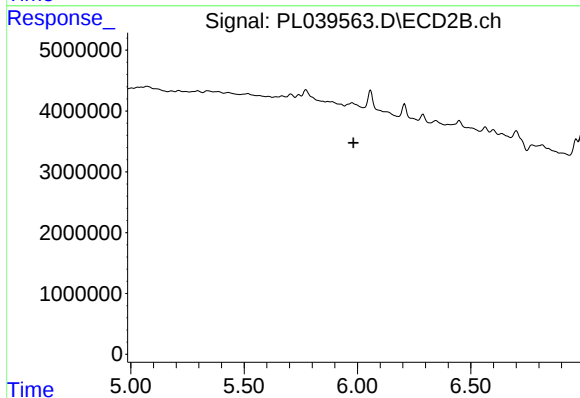


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

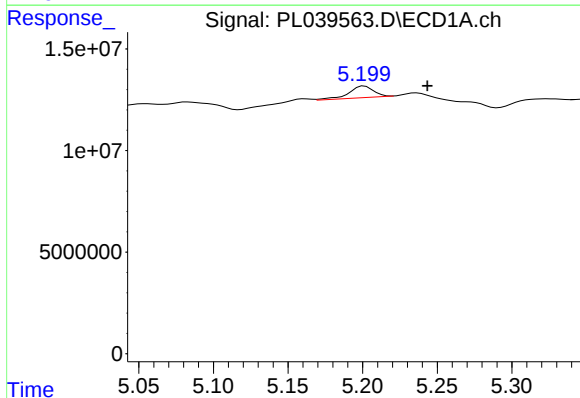


#11 alpha-Chlordane

R.T.: 5.201 min
Delta R.T.: -0.042 min
Response: 6533829
Conc: 0.68 ng/ml

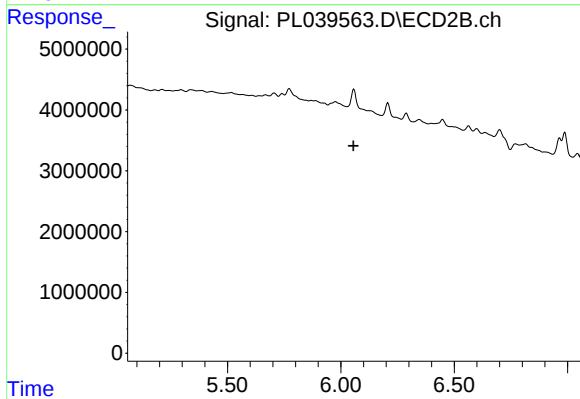

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

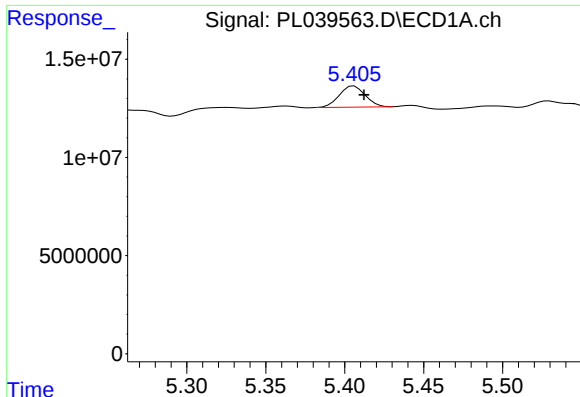

#12 4,4'-DDE


R.T.: 5.406 min
Delta R.T.: -0.006 min
Response: 12408361
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

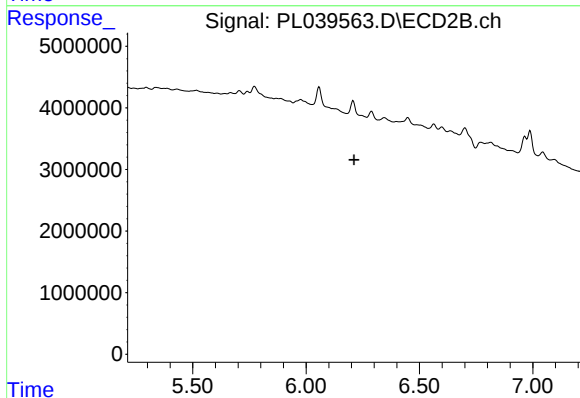


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

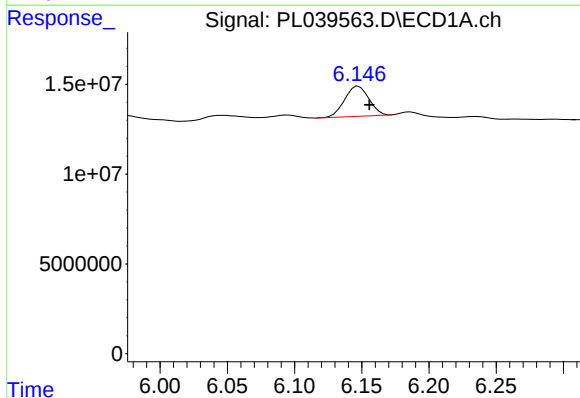


#17 4,4'-DDT

R.T.: 6.148 min
Delta R.T.: -0.008 min
Response: 21004911
Conc: 2.77 ng/ml

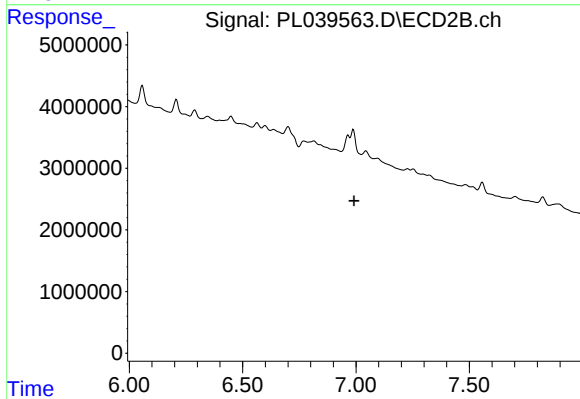

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

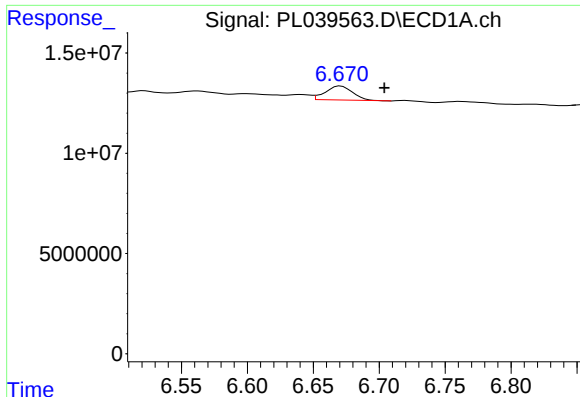

#20 Methoxychlor


R.T.: 6.671 min
Delta R.T.: -0.033 min
Response: 9928647
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

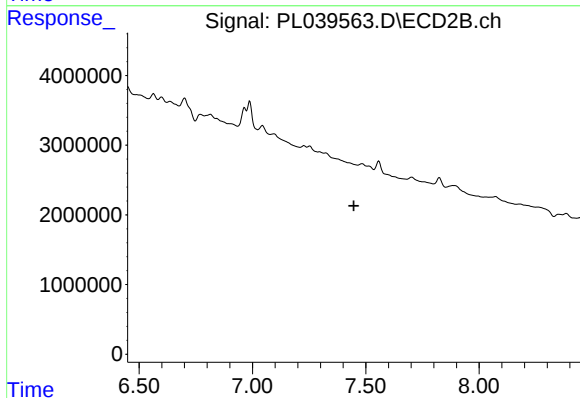


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

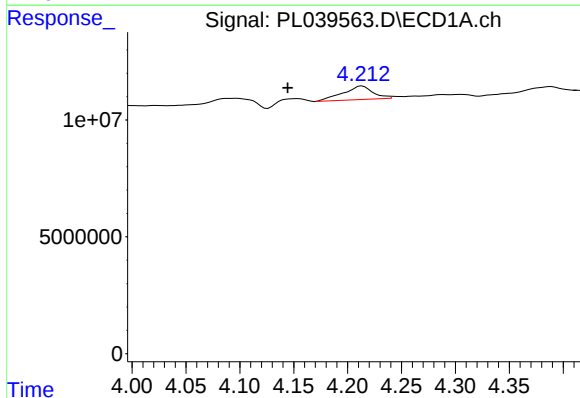


#23 Chlordane-1

R.T.: 4.214 min
Delta R.T.: 0.069 min
Response: 11522099
Conc: 36.39 ng/ml

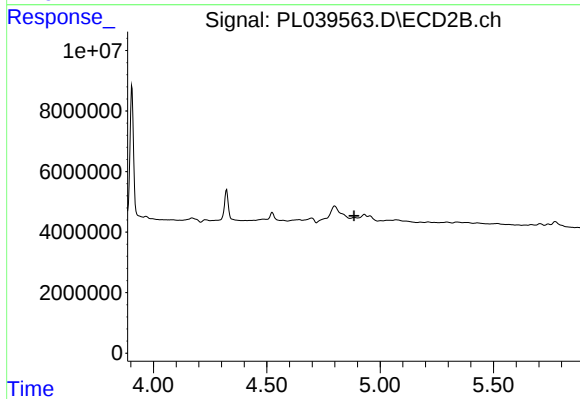

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

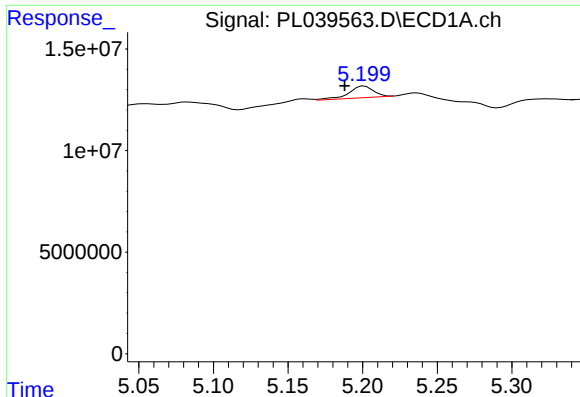

#25 Chlordane-3


R.T.: 5.201 min
Delta R.T.: 0.013 min
Response: 6533829
Conc: 5.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

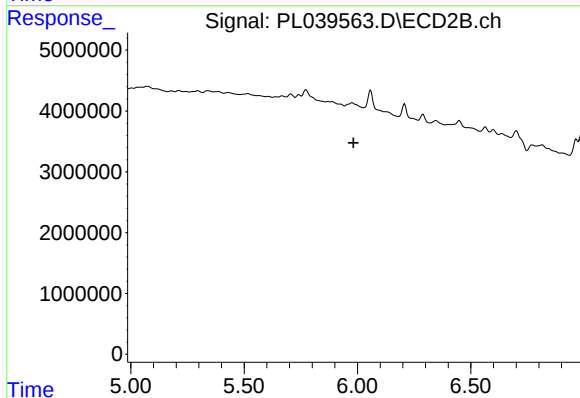


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

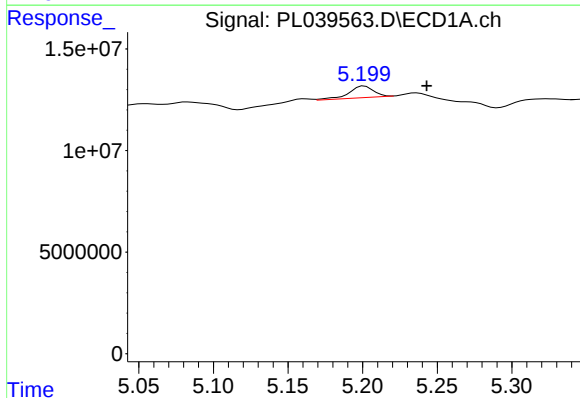


#26 Chlordane-4

R.T.: 5.201 min
Delta R.T.: -0.042 min
Response: 6533829
Conc: 6.54 ng/ml

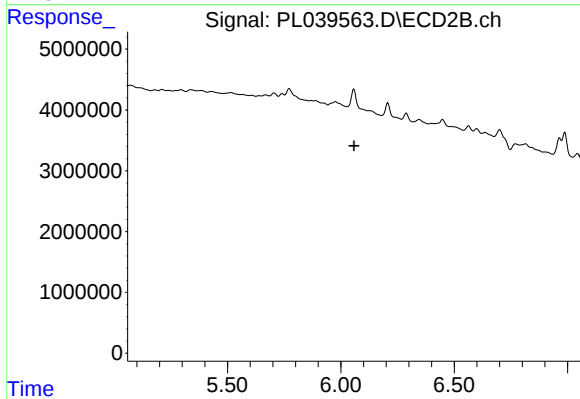

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

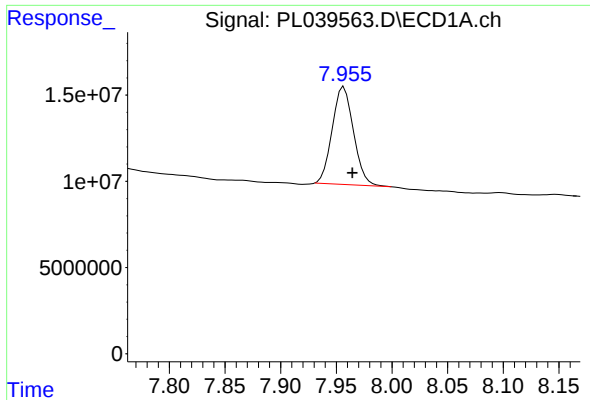

#28 Decachlorobiphenyl


R.T.: 7.957 min

Delta R.T.: -0.008 min

Response: 75274044

Conc: 10.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

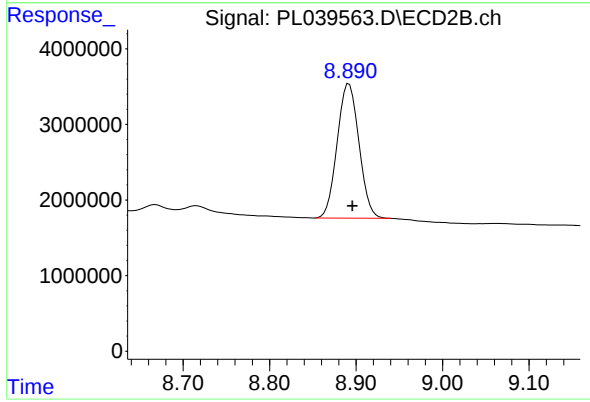

#28 Decachlorobiphenyl

R.T.: 8.892 min

Delta R.T.: -0.004 min

Response: 30987361

Conc: 13.35 ng/ml