

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 17:55
 Operator : AJ\SJ
 Sample : PB112435BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:03:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	138.7E6	56899665	19.848	21.224
28)	SA Decachlor...	7.957	8.893	117.4E6	45759065	16.710	19.719
Target Compounds							
6)	B beta-BHC	4.215f	0.000	13070311	0	2.814	N.D. #
8)	B Heptachlo...	4.915f	0.000	6414310	0	0.672	N.D. #
9)	A Endosulfan I	5.252f	0.000	7529550	0	0.860	N.D. #
10)	B gamma-Chl...	5.252f	0.000	7529550	0	0.762	N.D. #
11)	B alpha-Chl...	5.252	0.000	7529550	0	0.784	N.D. #
23)	Chlordane-1	4.174	0.000	4016884	0	12.688	N.D. #
25)	Chlordane-3	5.252	0.000	7529550	0	6.894	N.D. #
26)	Chlordane-4	5.252	0.000	7529550	0	7.534	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 17:55
Operator : AJ\SJ
Sample : PB112435BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:03:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

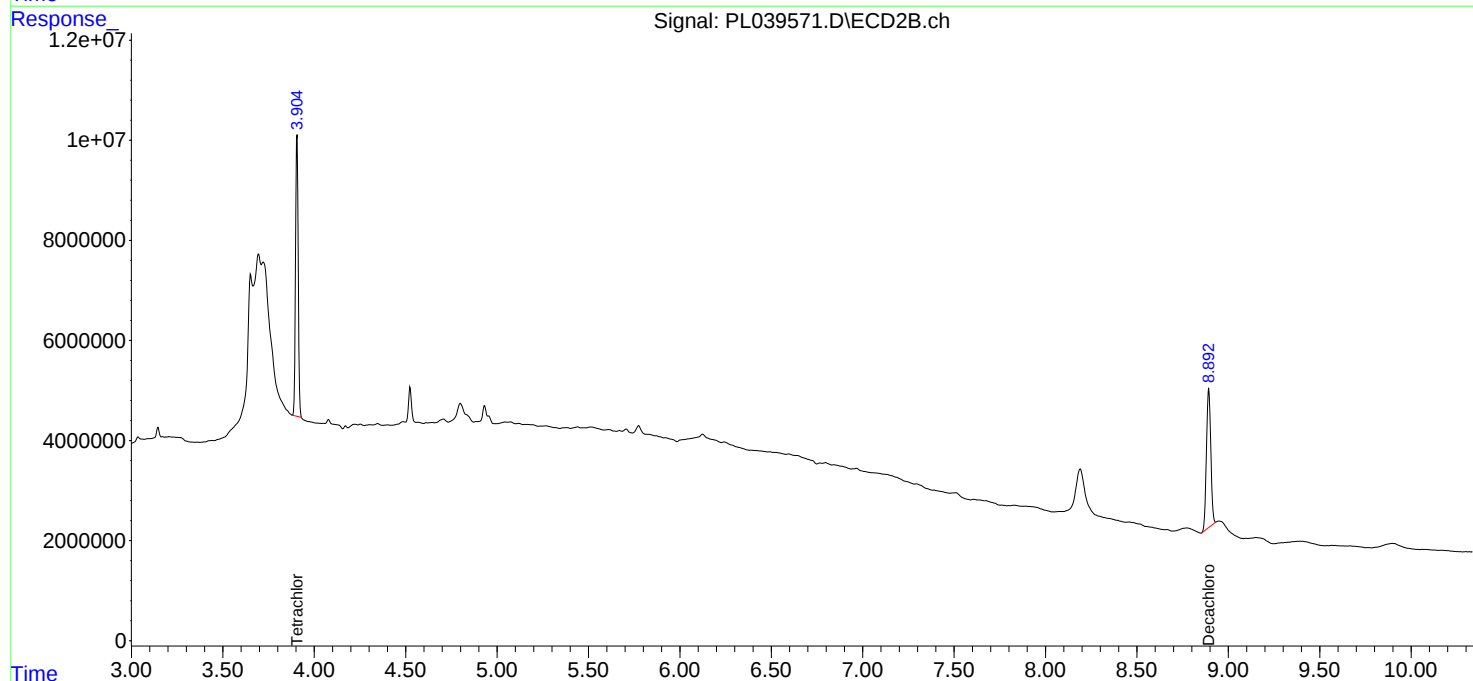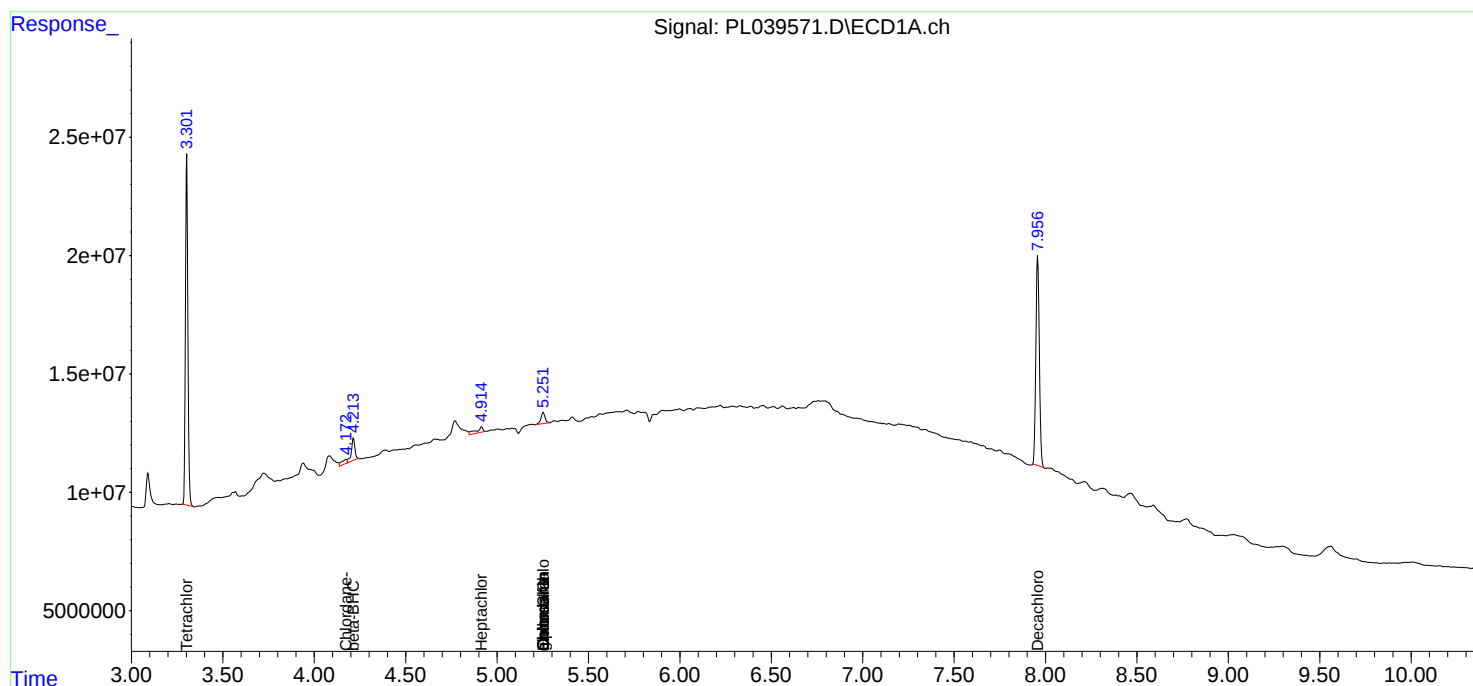


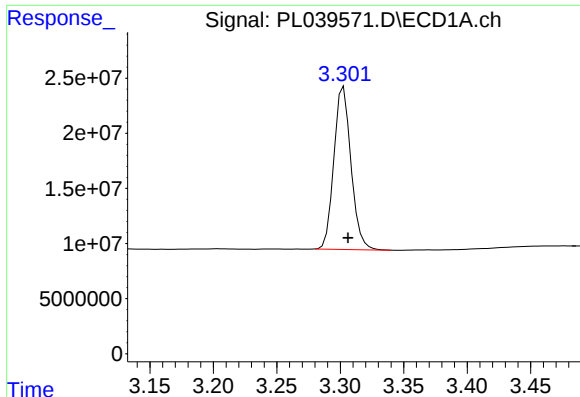

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 138746061
Conc: 19.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

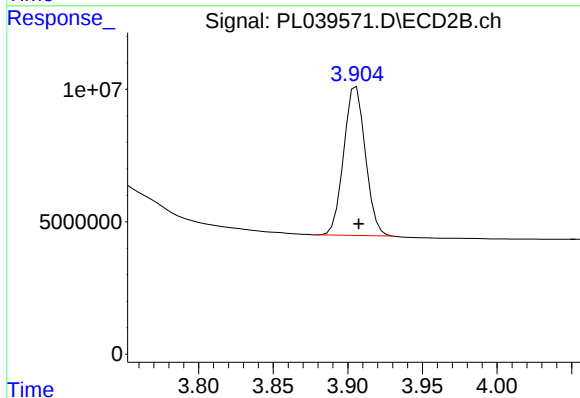


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 56899665
Conc: 21.22 ng/ml

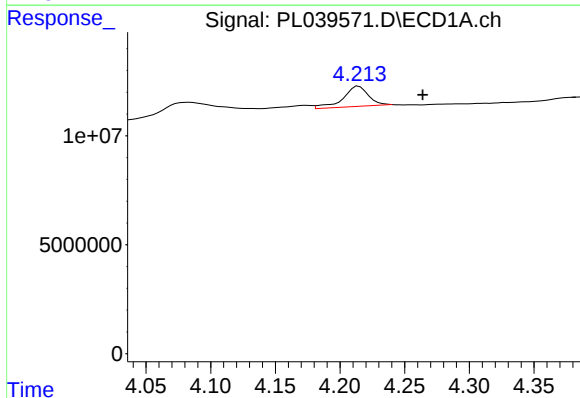


#6 beta-BHC

R.T.: 4.215 min
Delta R.T.: -0.050 min
Response: 13070311
Conc: 2.81 ng/ml

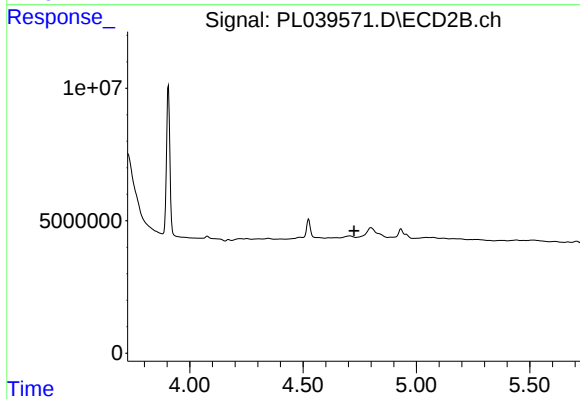

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

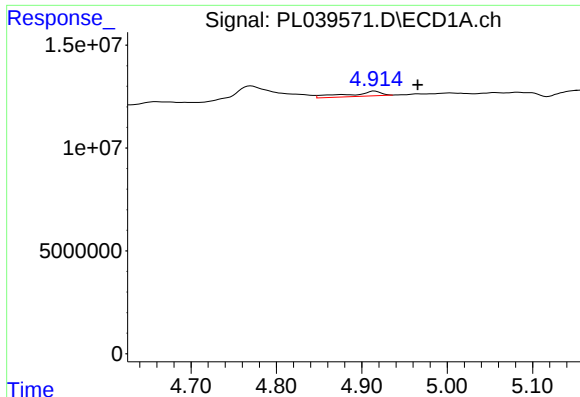

#8 Heptachlor epoxide


R.T.: 4.915 min
Delta R.T.: -0.051 min
Response: 6414310
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

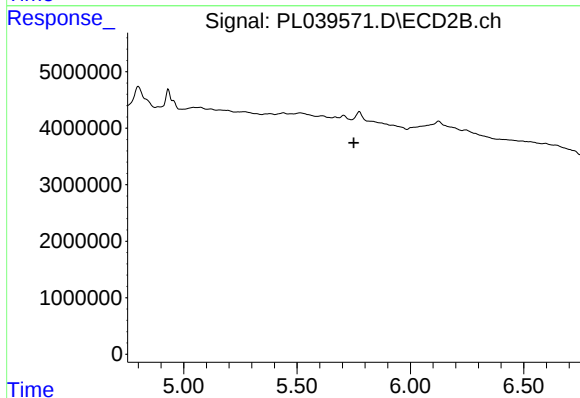


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

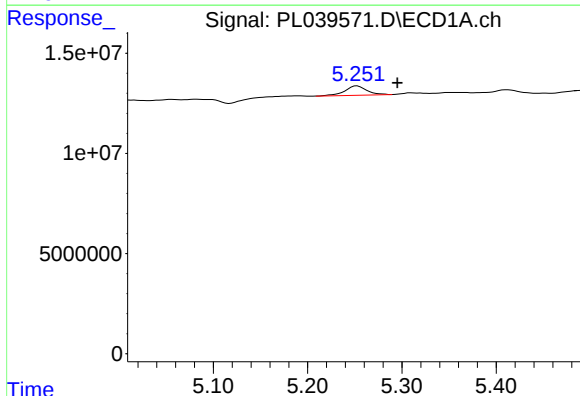


#9 Endosulfan I

R.T.: 5.252 min
Delta R.T.: -0.043 min
Response: 7529550
Conc: 0.86 ng/ml

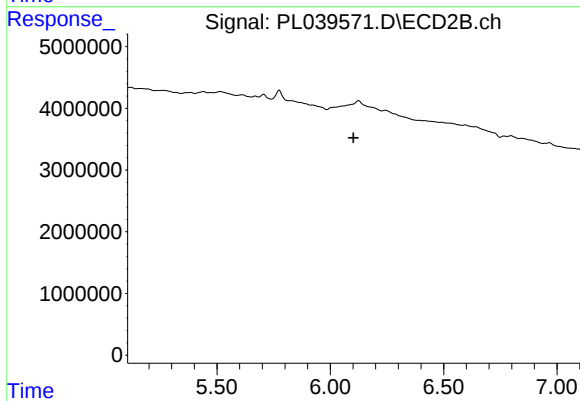

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

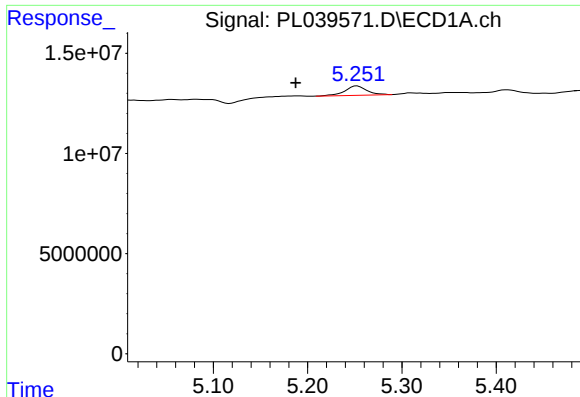

#10 gamma-Chlordane


R.T.: 5.252 min
Delta R.T.: 0.065 min
Response: 7529550
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

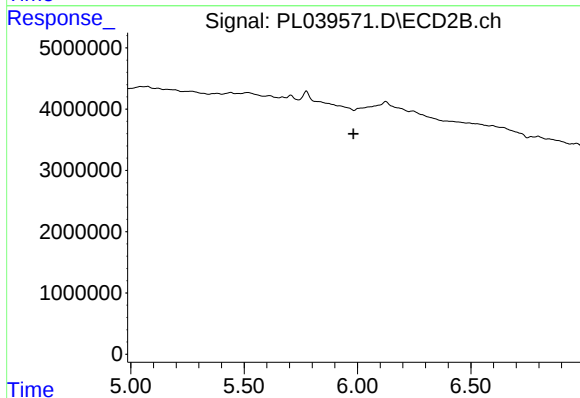


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

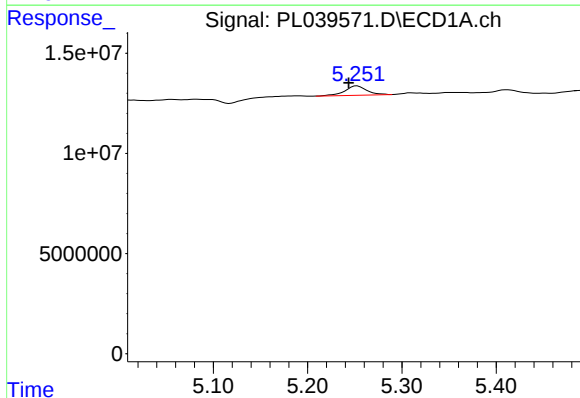


#11 alpha-Chlordane

R.T.: 5.252 min
Delta R.T.: 0.009 min
Response: 7529550
Conc: 0.78 ng/ml

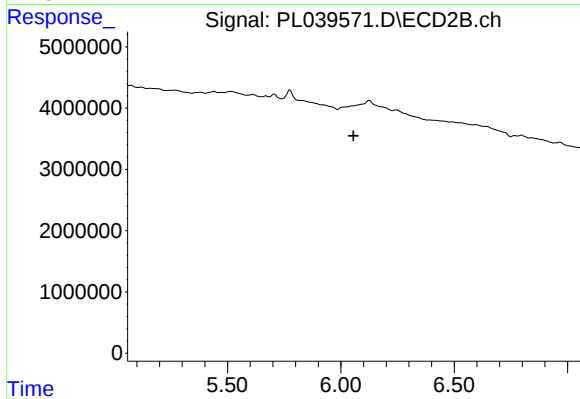

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

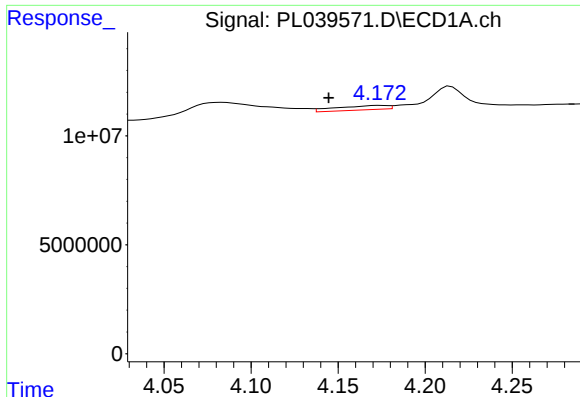

#23 Chlordane-1


R.T.: 4.174 min
Delta R.T.: 0.030 min
Response: 4016884
Conc: 12.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

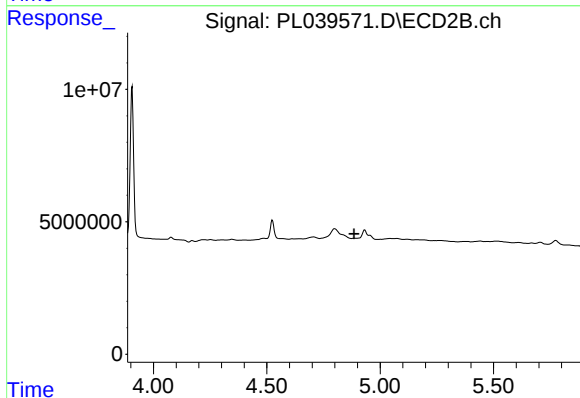


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

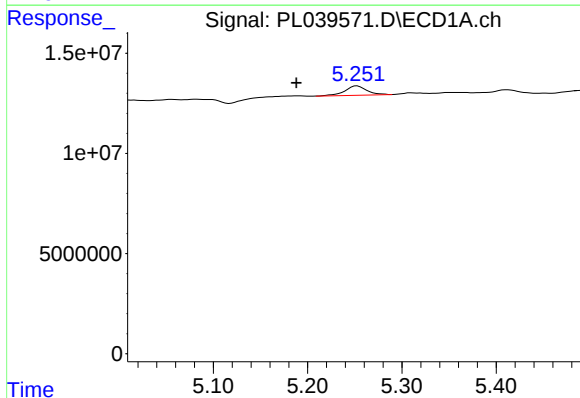


#25 Chlordane-3

R.T.: 5.252 min
Delta R.T.: 0.064 min
Response: 7529550
Conc: 6.89 ng/ml

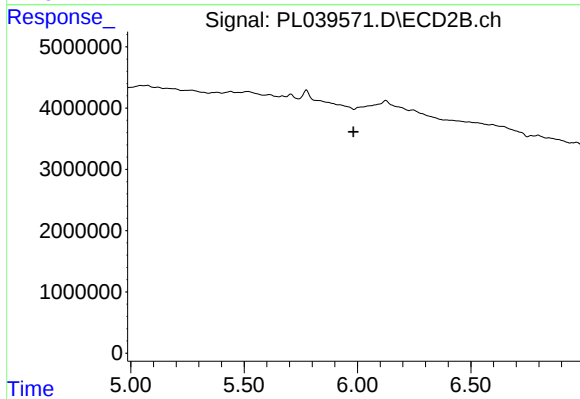

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

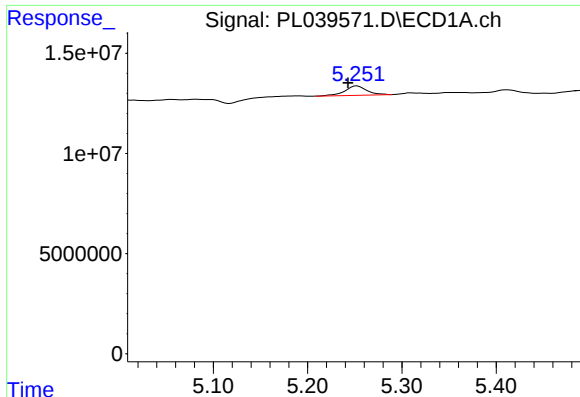

#26 Chlordane-4


R.T.: 5.252 min
Delta R.T.: 0.009 min
Response: 7529550
Conc: 7.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

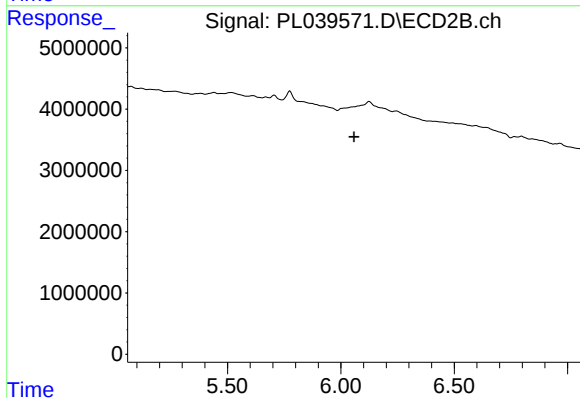


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

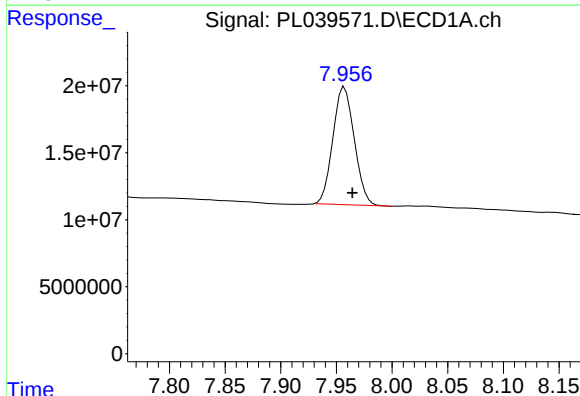

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 117358686
Conc: 16.71 ng/ml

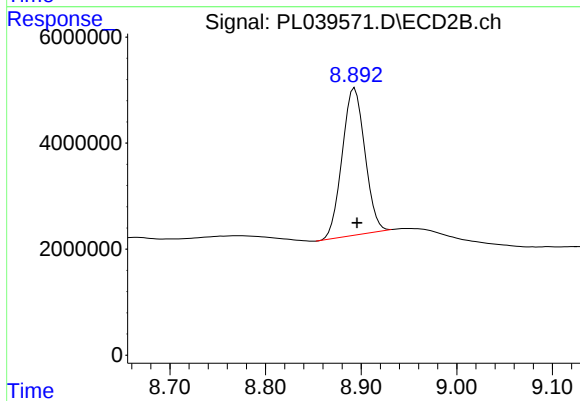

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 45759065
Conc: 19.72 ng/ml