

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 18:37
 Operator : AJ\SJ
 Sample : J4274-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:04:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	142.1E6	57997378	20.331	21.634
28)	SA Decachlor...	7.957	8.893	132.9E6	53344864	18.929	22.987
Target Compounds							
6)	B beta-BHC	4.215f	0.000	19114279	0	4.115	N.D. #
7)	B delta-BHC	0.000	4.931	0	11265236	N.D.	2.829 #
8)	B Heptachlo...	5.035f	5.775	20578554	3834332	2.155	1.140 #
9)	A Endosulfan I	5.324	0.000	8042804	0	0.919	N.D. #
15)	B Endosulfa...	6.053	0.000	5724857	0	0.658	N.D. #
19)	B Endosulfa...	6.454	0.000	6614381	0	0.813	N.D. #
23)	Chlordane-1	4.155	4.931	6691737	11265236	21.137	90.169 #
27)	Chlordane-5	6.053	0.000	5724857	0	17.651	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 18:37
Operator : AJ\SJ
Sample : J4274-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:04:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

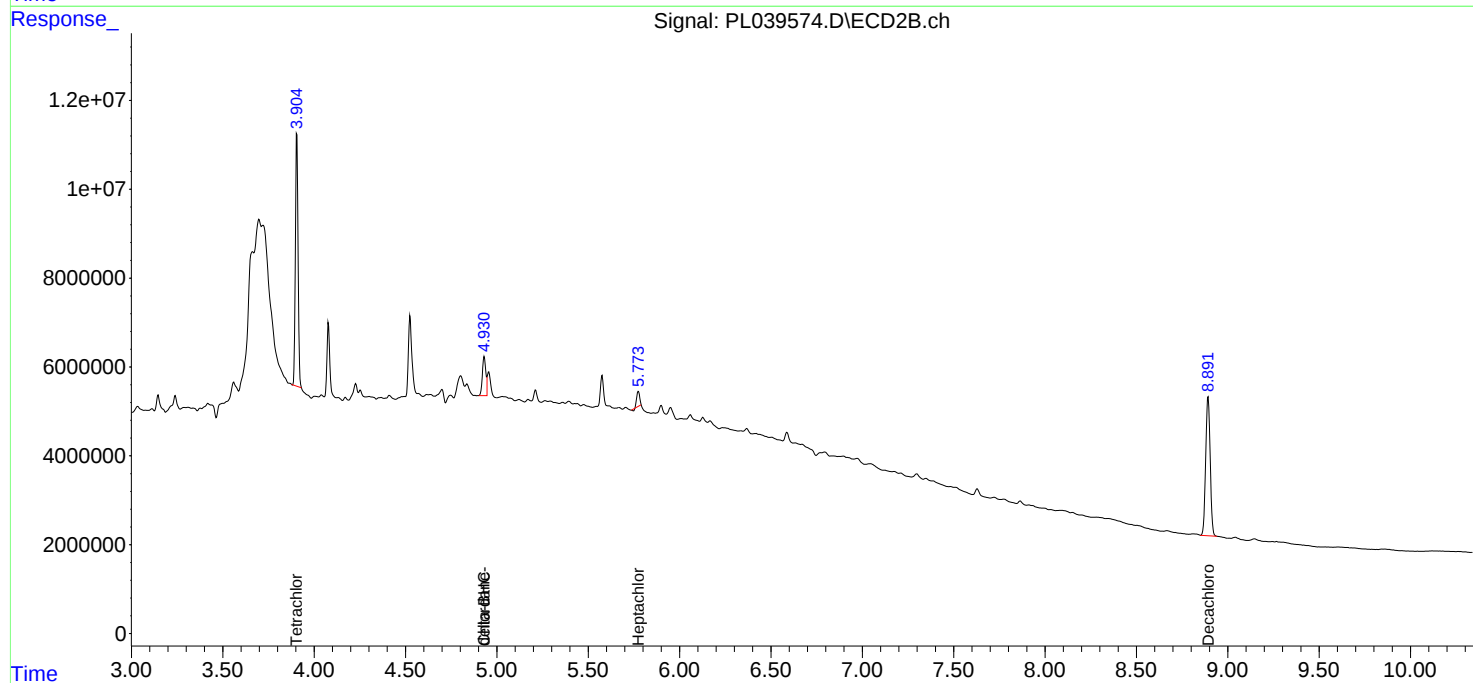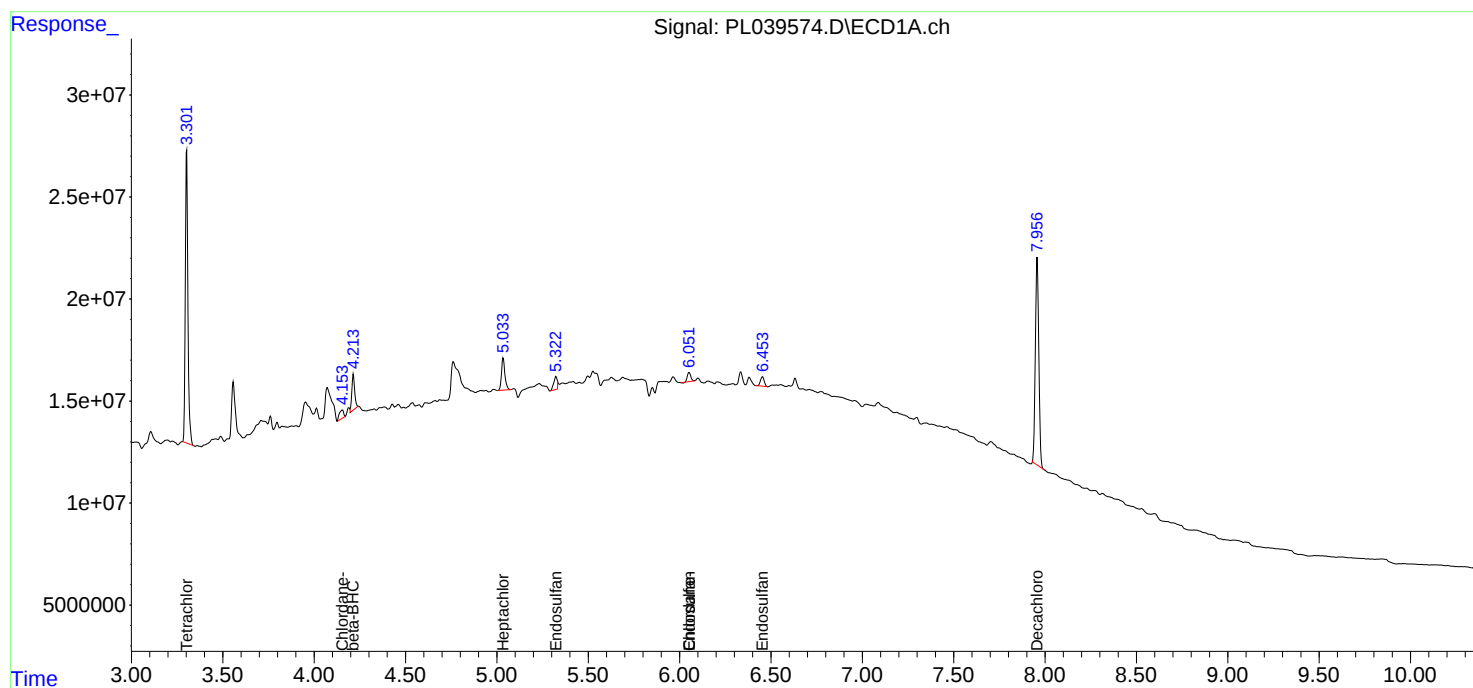


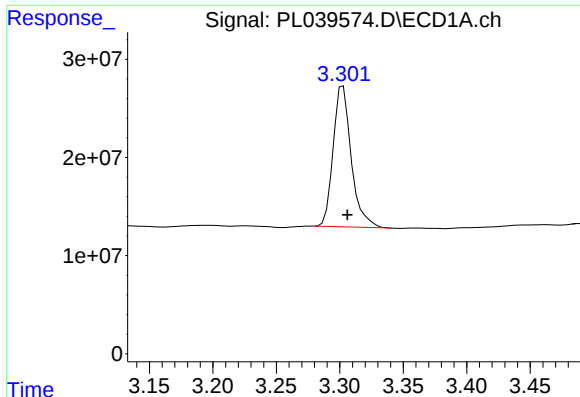

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 142125155
Conc: 20.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

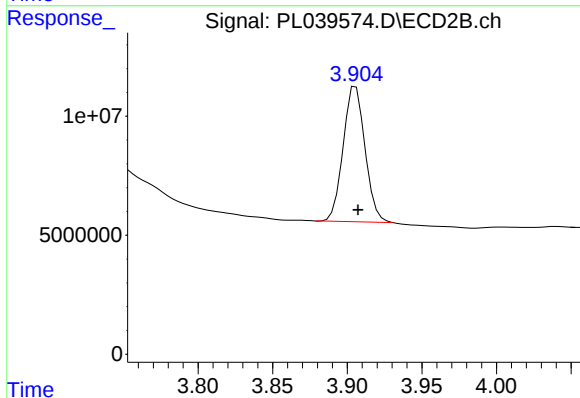


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 57997378
Conc: 21.63 ng/ml

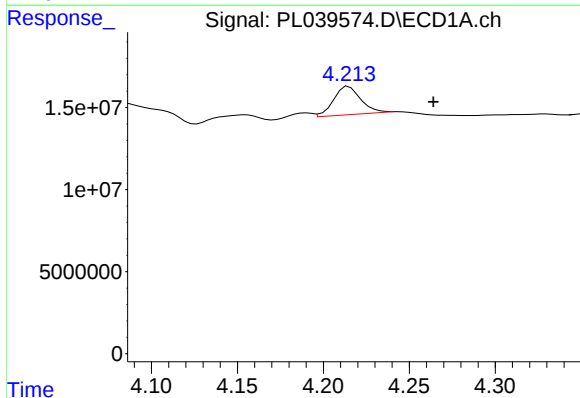


#6 beta-BHC

R.T.: 4.215 min
Delta R.T.: -0.049 min
Response: 19114279
Conc: 4.11 ng/ml

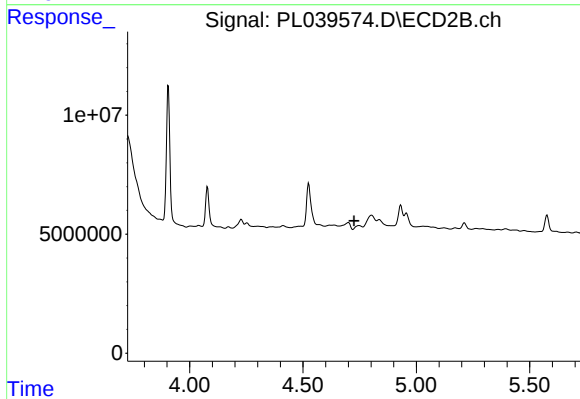

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

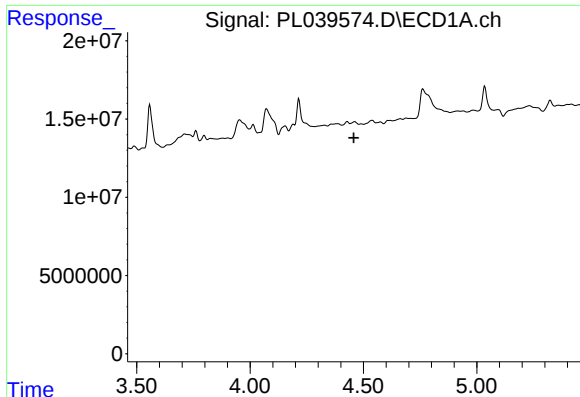

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

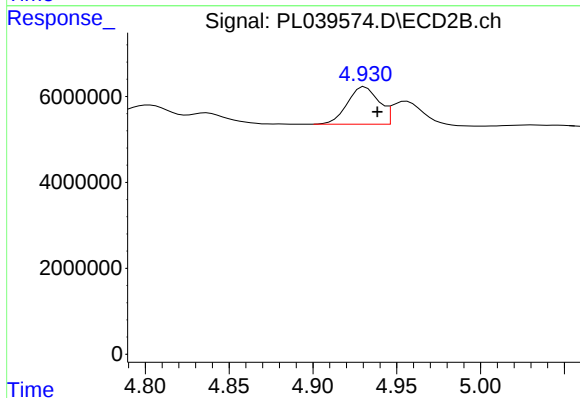


#7 delta-BHC

R.T.: 4.931 min
Delta R.T.: -0.007 min
Response: 11265236
Conc: 2.83 ng/ml

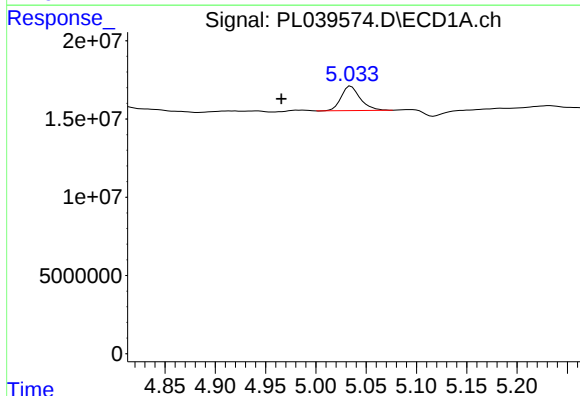


#8 Heptachlor epoxide

R.T.: 5.035 min
Delta R.T.: 0.069 min
Response: 20578554
Conc: 2.15 ng/ml

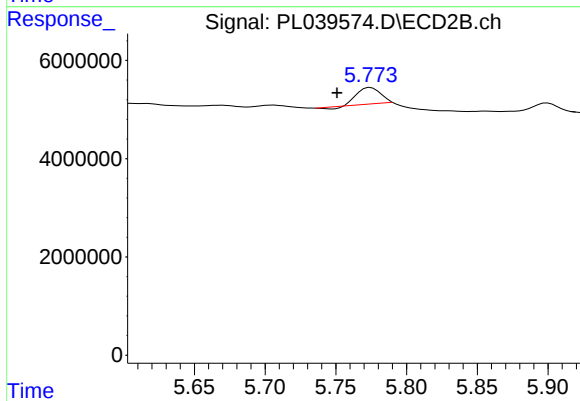

#8 Heptachlor epoxide


R.T.: 5.775 min
Delta R.T.: 0.024 min
Response: 3834332
Conc: 1.14 ng/ml

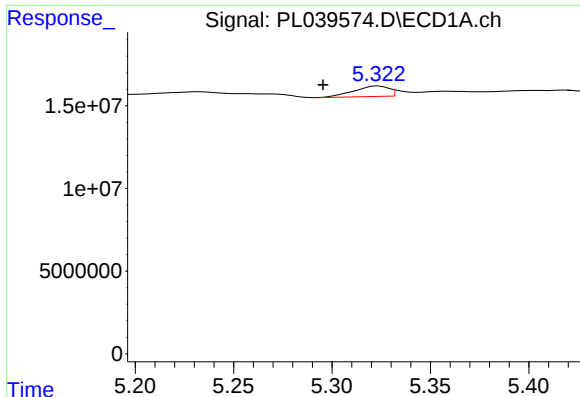

#9 Endosulfan I


R.T.: 5.324 min
Delta R.T.: 0.028 min
Response: 8042804
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

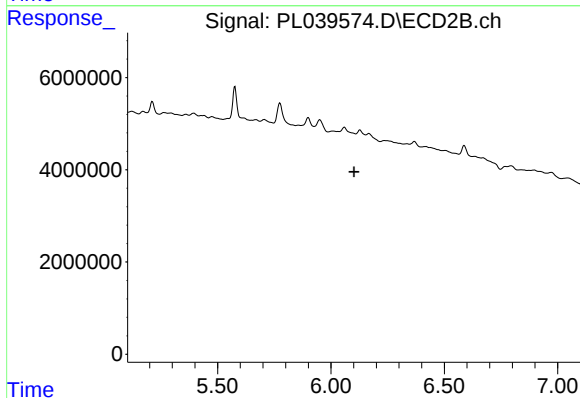


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

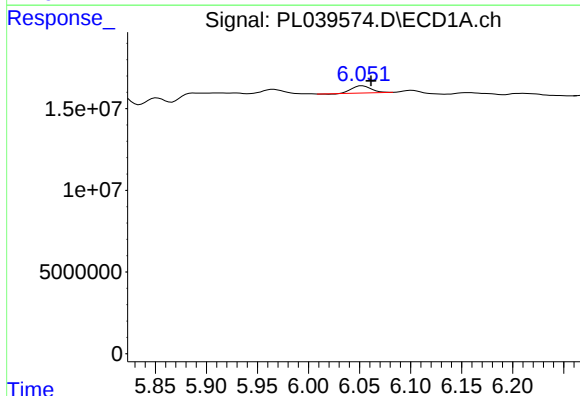


#15 Endosulfan II

R.T.: 6.053 min
Delta R.T.: -0.009 min
Response: 5724857
Conc: 0.66 ng/ml

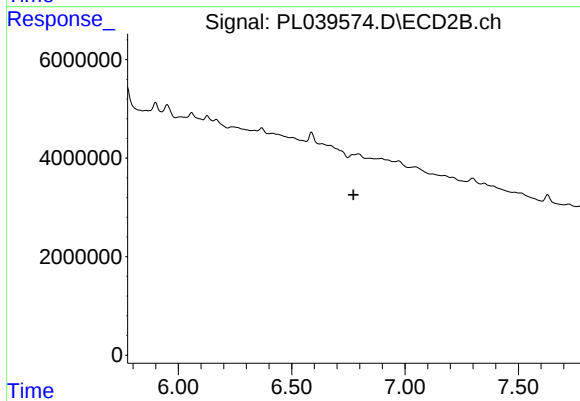

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

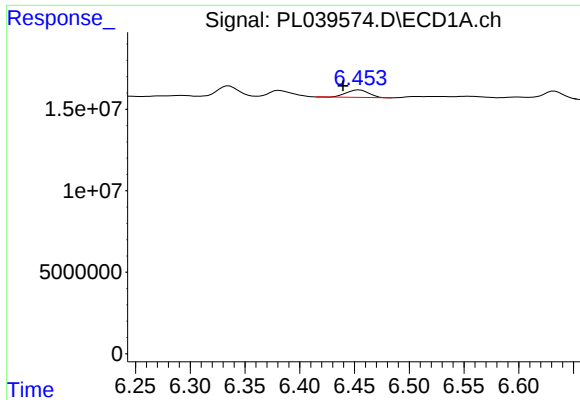

#19 Endosulfan Sulfate


R.T.: 6.454 min
Delta R.T.: 0.015 min
Response: 6614381
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

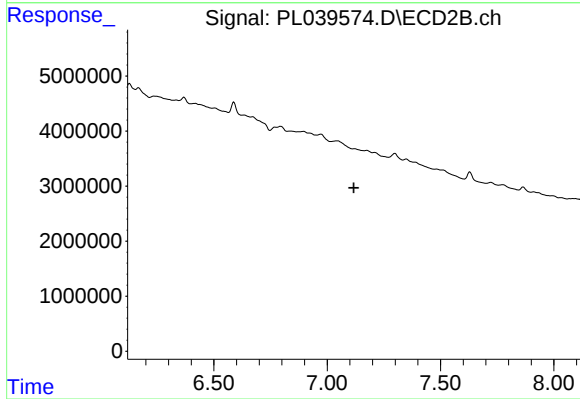


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

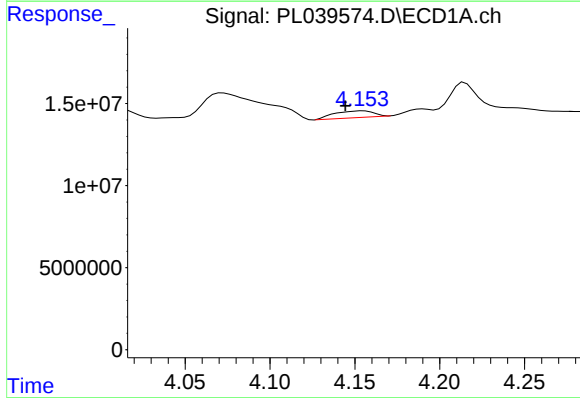


#23 Chlordane-1

R.T.: 4.155 min
Delta R.T.: 0.010 min
Response: 6691737
Conc: 21.14 ng/ml

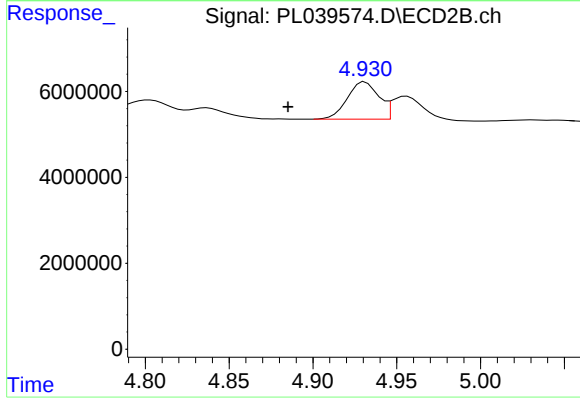

#23 Chlordane-1


R.T.: 4.931 min
Delta R.T.: 0.046 min
Response: 11265236
Conc: 90.17 ng/ml

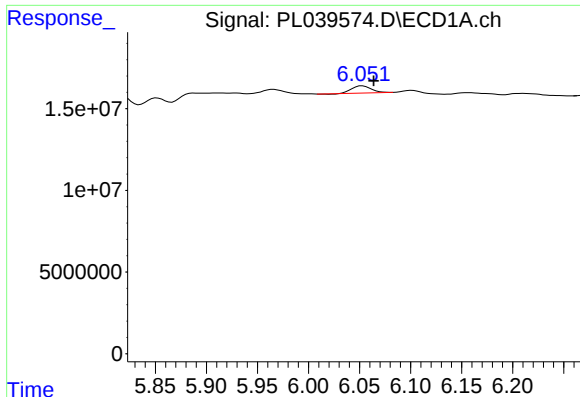

#27 Chlordane-5


R.T.: 6.053 min
Delta R.T.: -0.011 min
Response: 5724857
Conc: 17.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

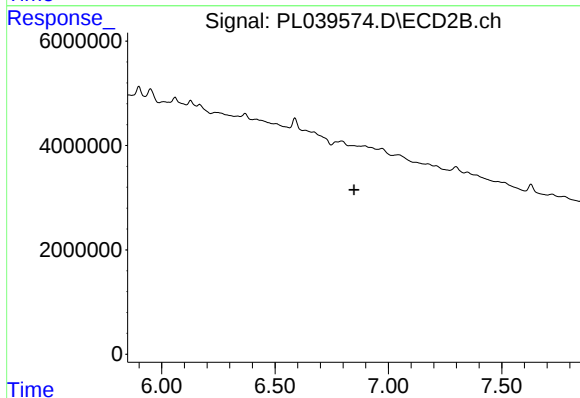


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

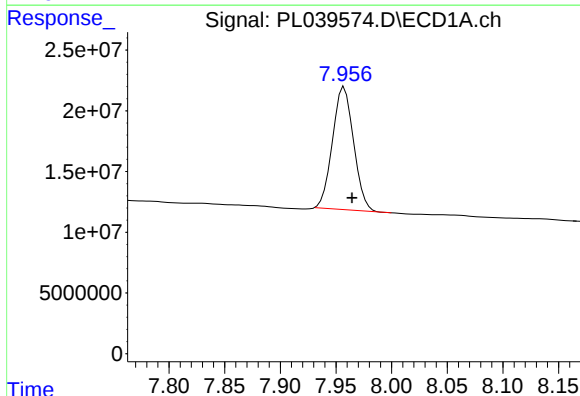

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 132944073
Conc: 18.93 ng/ml

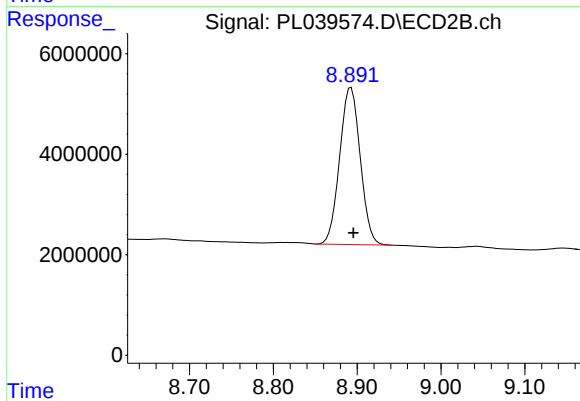

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.003 min
Response: 53344864
Conc: 22.99 ng/ml