

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 19:20
 Operator : AJ\SJ
 Sample : J4276-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:05:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	160.7E6	68877553	22.983	25.692
28)	SA Decachlor...	7.958	8.893	157.8E6	62102455	22.475	26.761
Target Compounds							
4)	MA Heptachlor	4.355f	0.000	2754940	0	0.262	N.D. #
6)	B beta-BHC	4.216f	0.000	16980953	0	3.655	N.D. #
7)	B delta-BHC	0.000	4.932	0	8119140	N.D.	2.039 #
8)	B Heptachlo...	0.000	5.775	0	4962938	N.D.	1.476 #
9)	A Endosulfan I	5.323	0.000	5387473	0	0.615	N.D. #
13)	MA Dieldrin	5.527	0.000	9713936	0	0.996	N.D. #
15)	B Endosulfa...	6.052	0.000	8896386	0	1.023	N.D. #
19)	B Endosulfa...	6.453	0.000	12185651	0	1.498	N.D. #
23)	Chlordane-1	4.155	4.932	3004317	8119140	9.490	64.987 #
27)	Chlordane-5	6.052	0.000	8896386	0	27.430	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 19:20
Operator : AJ\SJ
Sample : J4276-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:05:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

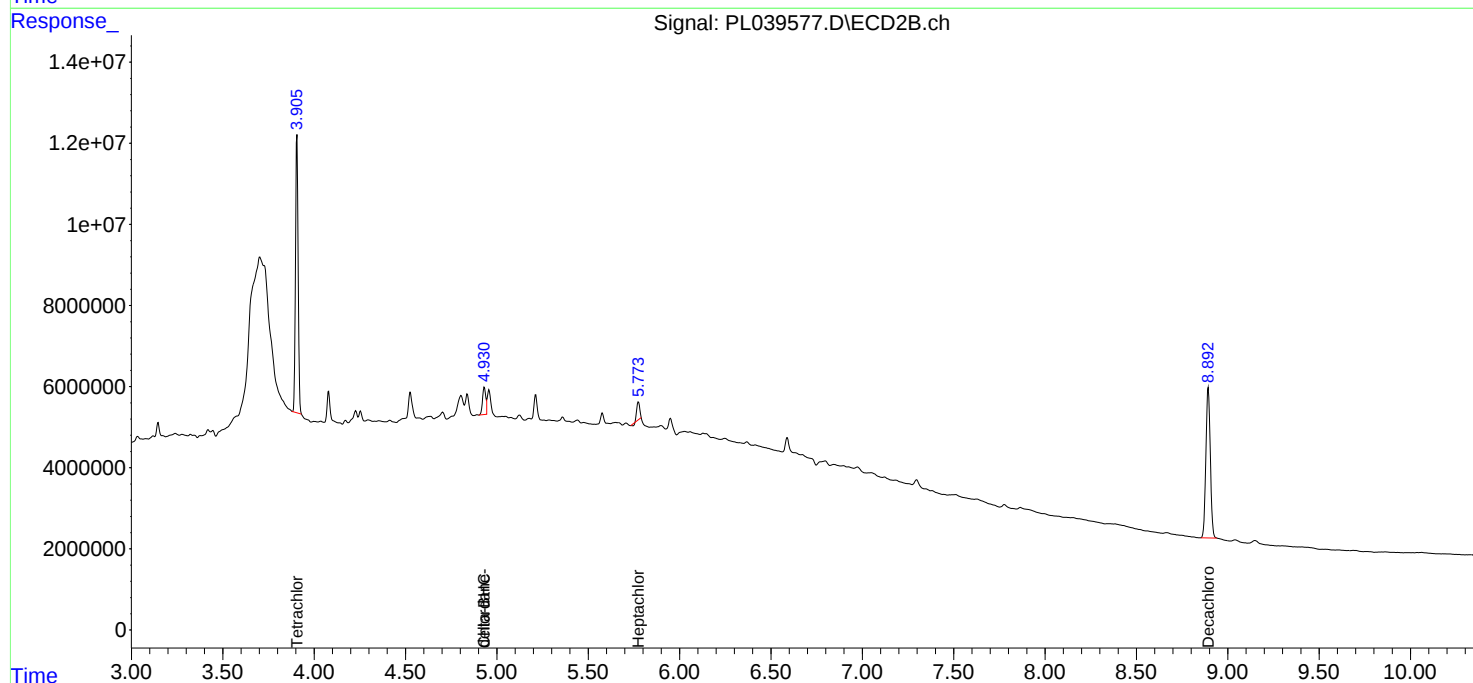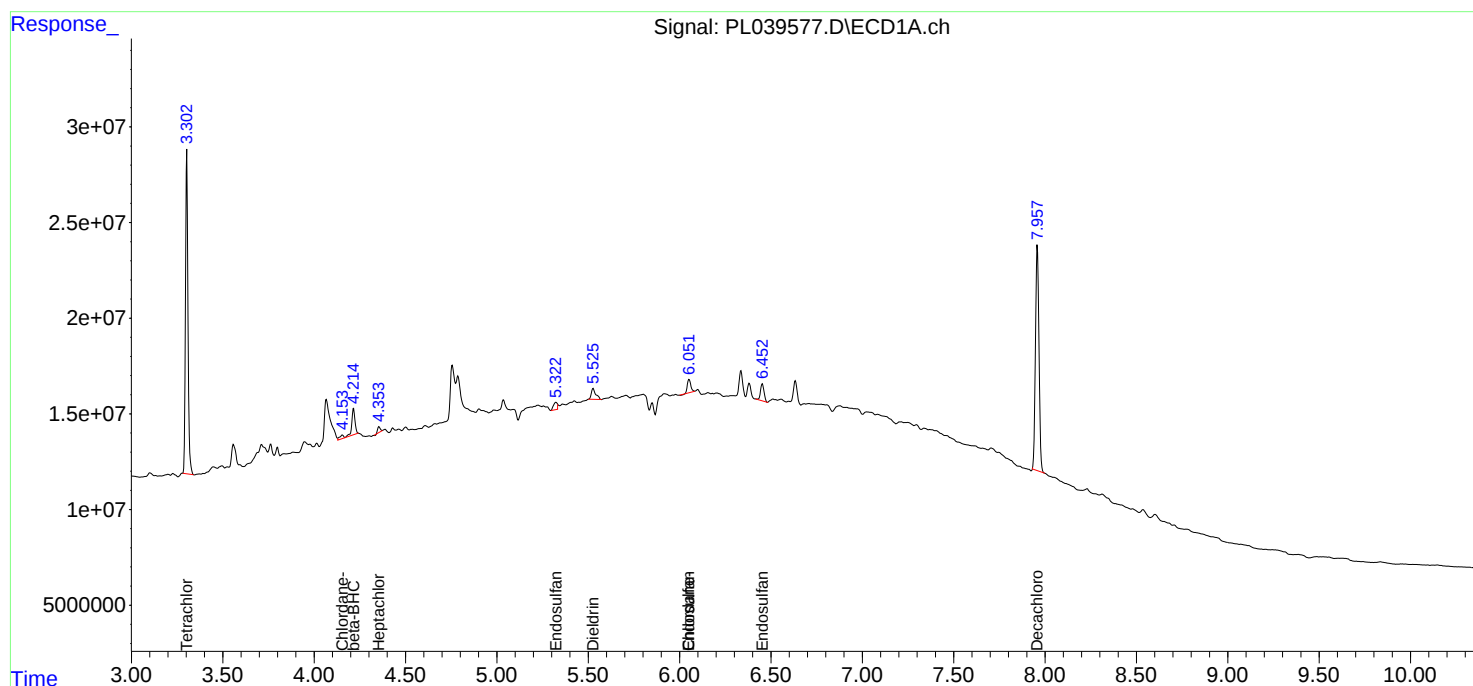


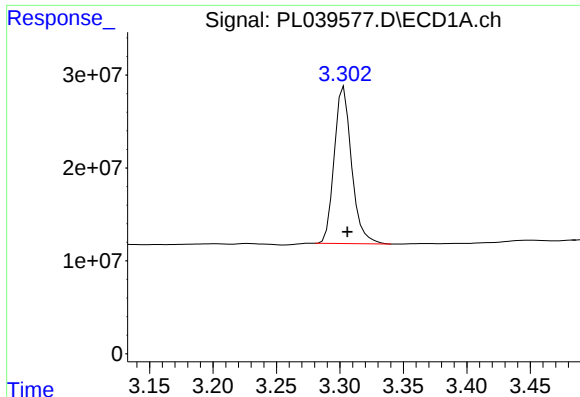

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 160660906
Conc: 22.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

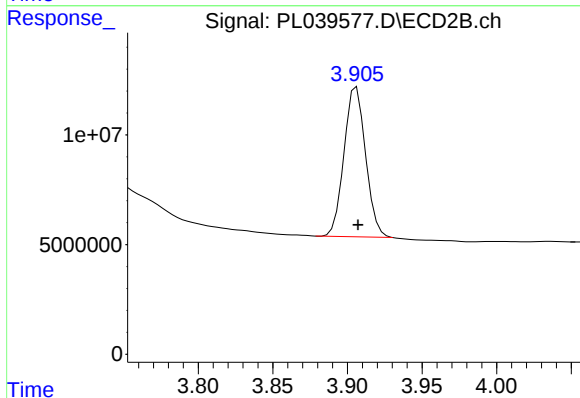


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 68877553
Conc: 25.69 ng/ml

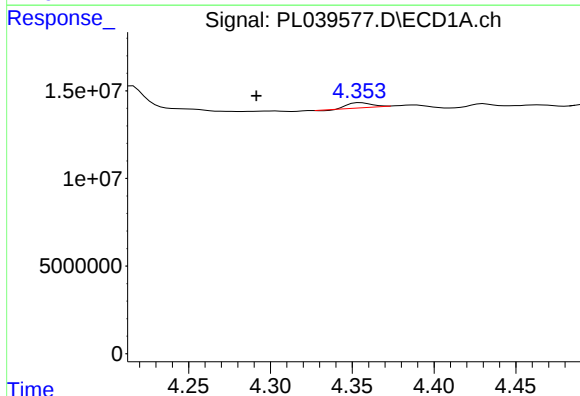


#4 Heptachlor

R.T.: 4.355 min
Delta R.T.: 0.064 min
Response: 2754940
Conc: 0.26 ng/ml

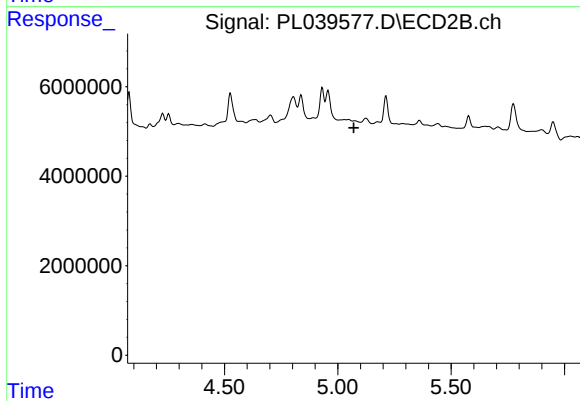

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

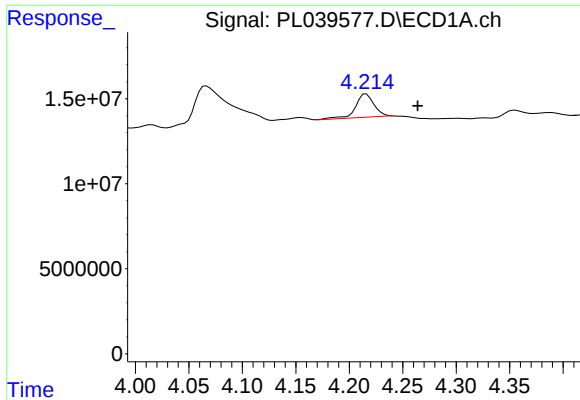

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 16980953
Conc: 3.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

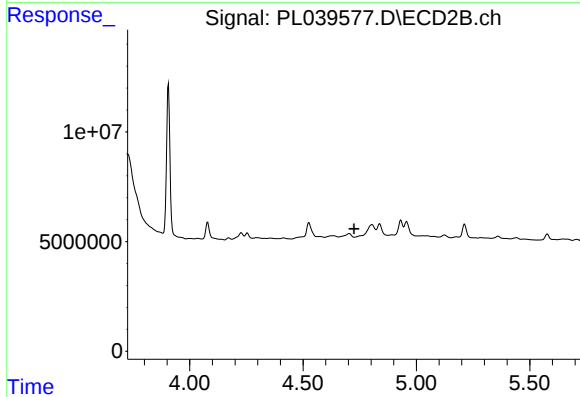


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

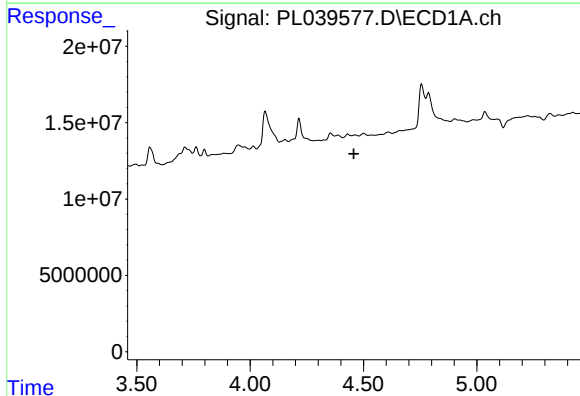


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

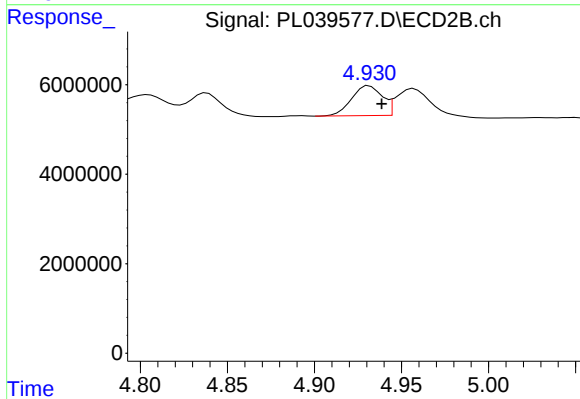

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 8119140
Conc: 2.04 ng/ml

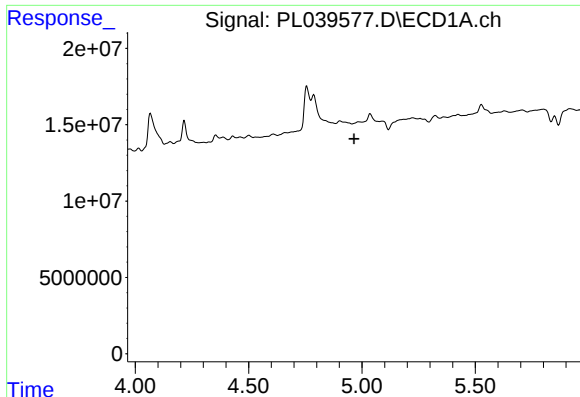

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

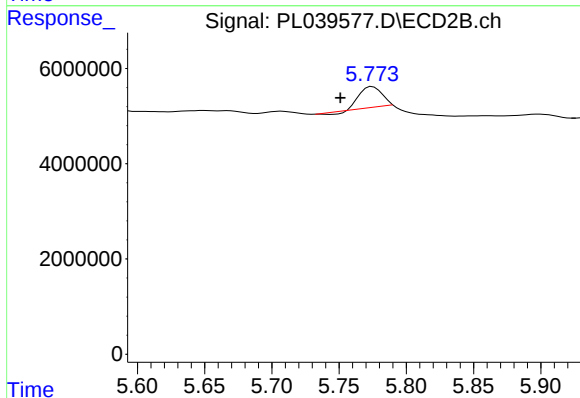


#8 Heptachlor epoxide

R.T.: 5.775 min
Delta R.T.: 0.024 min
Response: 4962938
Conc: 1.48 ng/ml

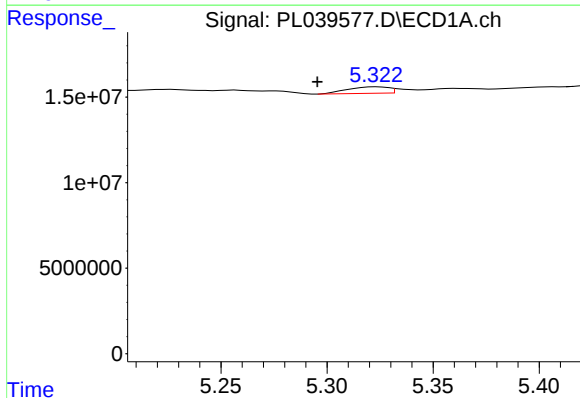


#9 Endosulfan I

R.T.: 5.323 min
Delta R.T.: 0.028 min
Response: 5387473
Conc: 0.62 ng/ml

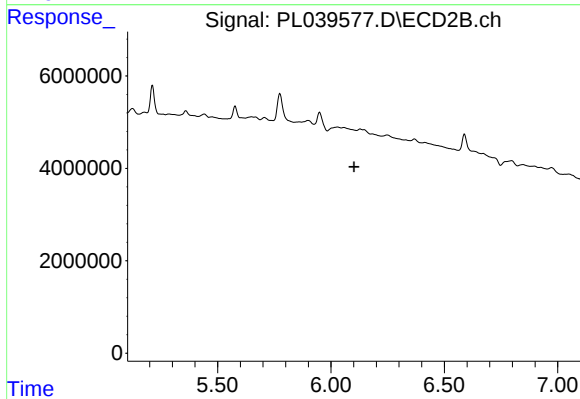

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.102 min
Response: 0
Conc: N.D.

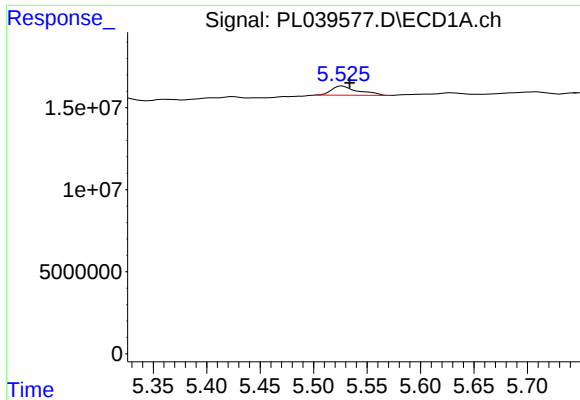

#13 Dieldrin


R.T.: 5.527 min
Delta R.T.: -0.007 min
Response: 9713936
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

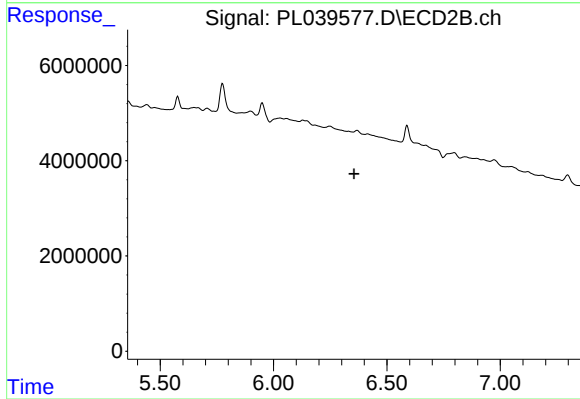


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

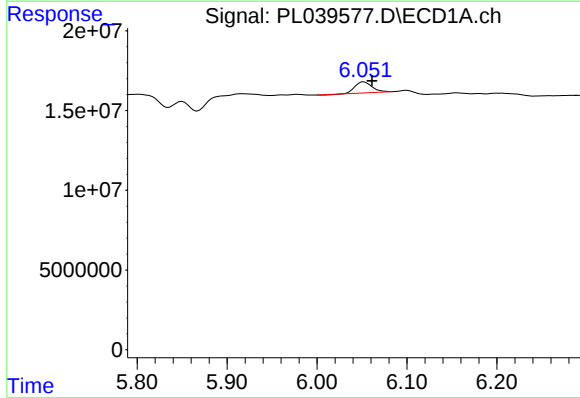


#15 Endosulfan II

R.T.: 6.052 min
Delta R.T.: -0.009 min
Response: 8896386
Conc: 1.02 ng/ml

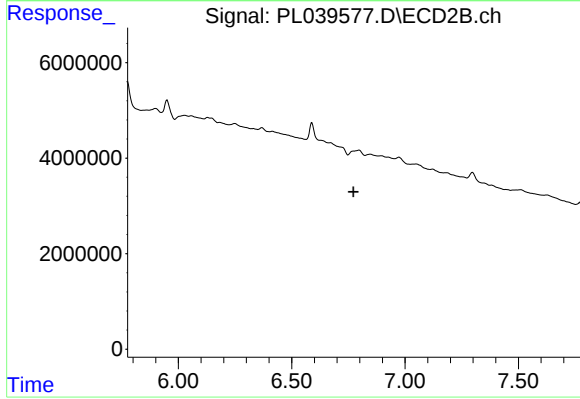

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

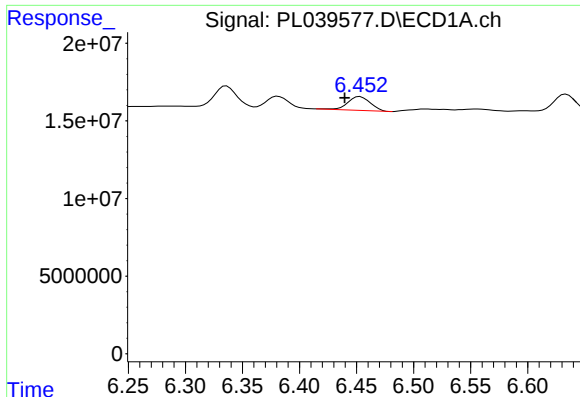

#19 Endosulfan Sulfate


R.T.: 6.453 min
Delta R.T.: 0.013 min
Response: 12185651
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

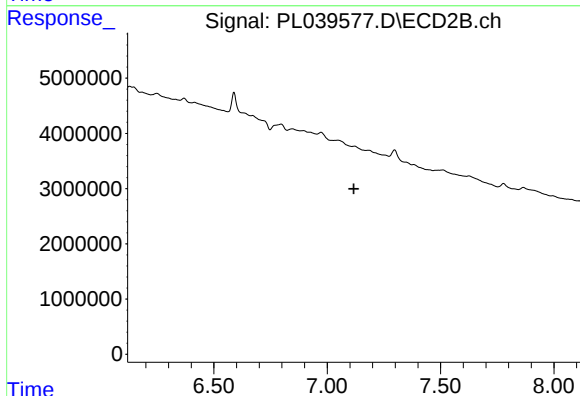


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

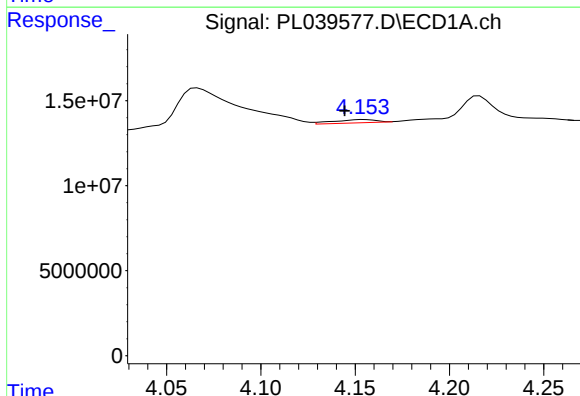


#23 Chlordane-1

R.T.: 4.155 min
Delta R.T.: 0.010 min
Response: 3004317
Conc: 9.49 ng/ml

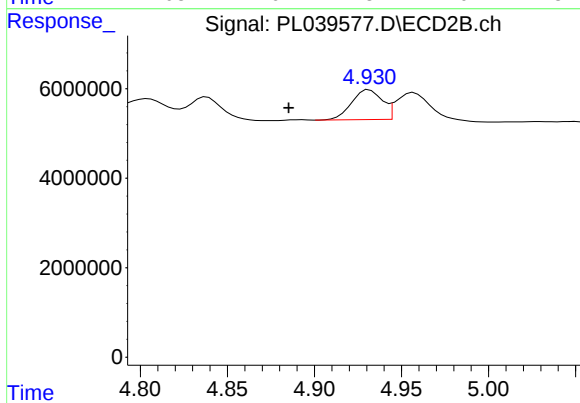

#23 Chlordane-1


R.T.: 4.932 min
Delta R.T.: 0.046 min
Response: 8119140
Conc: 64.99 ng/ml

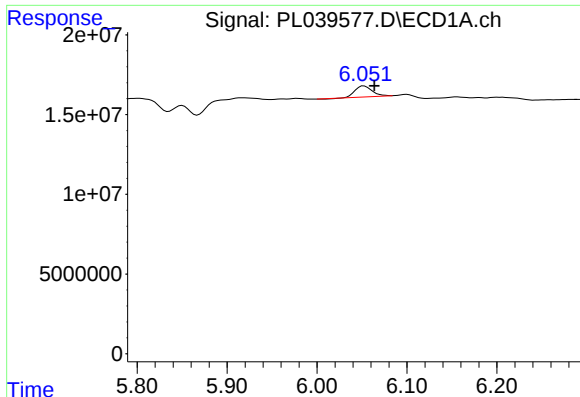

#27 Chlordane-5


R.T.: 6.052 min
Delta R.T.: -0.012 min
Response: 8896386
Conc: 27.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

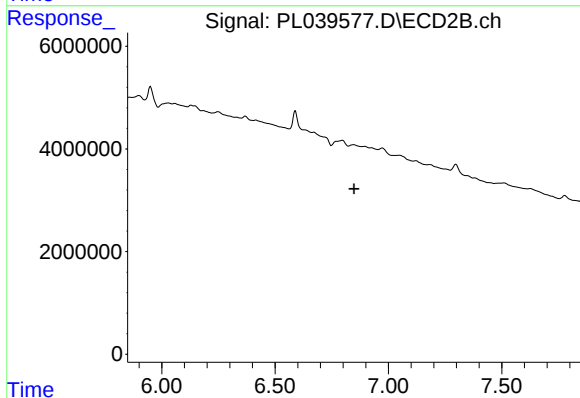


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

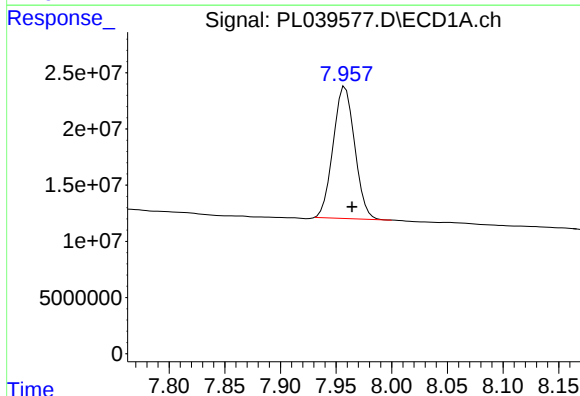

#28 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.006 min
Response: 157849197
Conc: 22.47 ng/ml

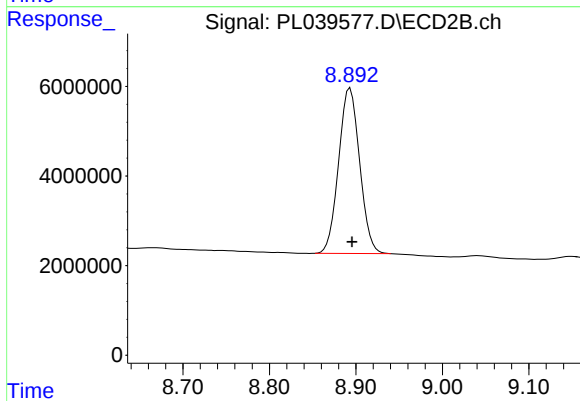

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 62102455
Conc: 26.76 ng/ml