

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 20:16
 Operator : AJ\SJ
 Sample : J4277-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:06:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	161.0E6	68909963	23.029	25.704
28)	SA Decachlor...	7.958	8.894	161.4E6	63643179	22.976	27.425
Target Compounds							
6)	B beta-BHC	4.216f	0.000	24915880	0	5.363	N.D. #
7)	B delta-BHC	0.000	4.932	0	12110066	N.D.	3.042 #
8)	B Heptachlo...	0.000	5.775	0	4759391	N.D.	1.415 #
9)	A Endosulfan I	5.325	0.000	4982666	0	0.569	N.D. #
13)	MA Dieldrin	5.527	0.000	10064577	0	1.032	N.D. #
15)	B Endosulfa...	6.054	0.000	9934707	0	1.143	N.D. #
19)	B Endosulfa...	6.454	0.000	11489562	0	1.412	N.D. #
20)	A Methoxychlor	6.634f	0.000	17007717	0	4.156	N.D. #
23)	Chlordane-1	4.155	4.932	2950790	12110066	9.321	96.931 #
27)	Chlordane-5	6.054	0.000	9934707	0	30.631	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 20:16
Operator : AJ\SJ
Sample : J4277-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:06:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

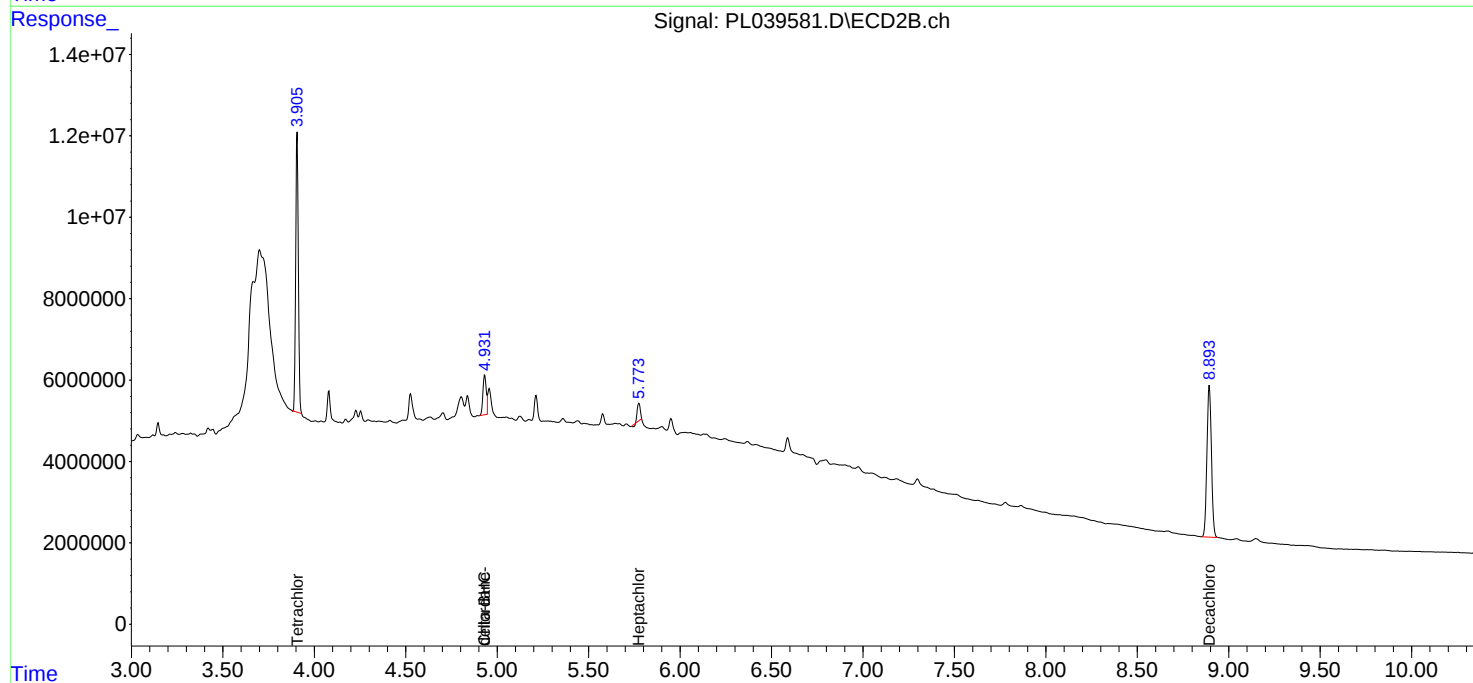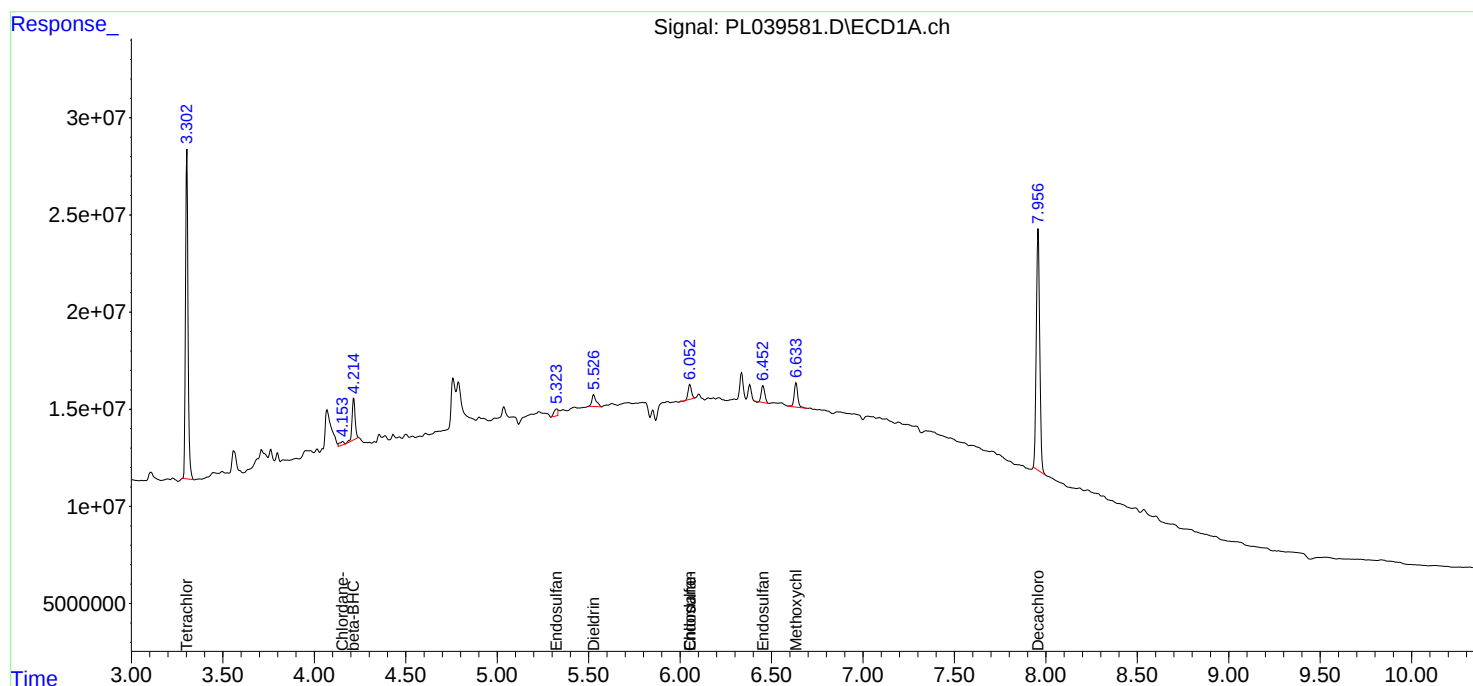


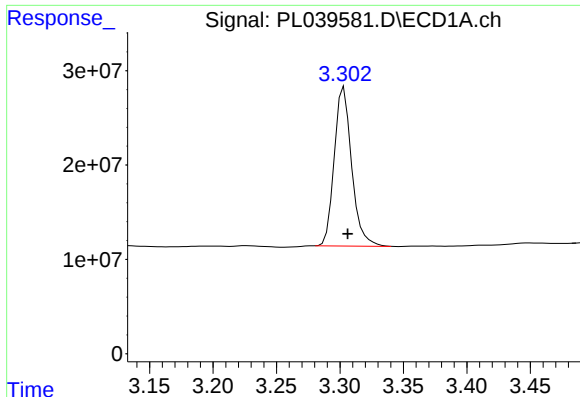

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 160979119
Conc: 23.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

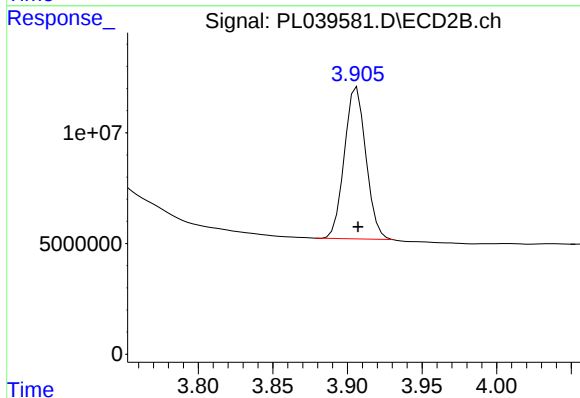


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 68909963
Conc: 25.70 ng/ml

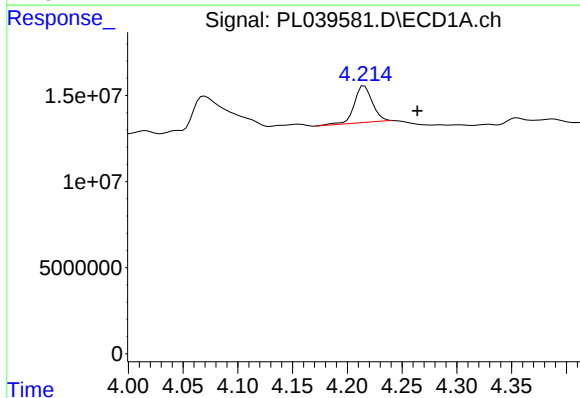


#6 beta-BHC

R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 24915880
Conc: 5.36 ng/ml

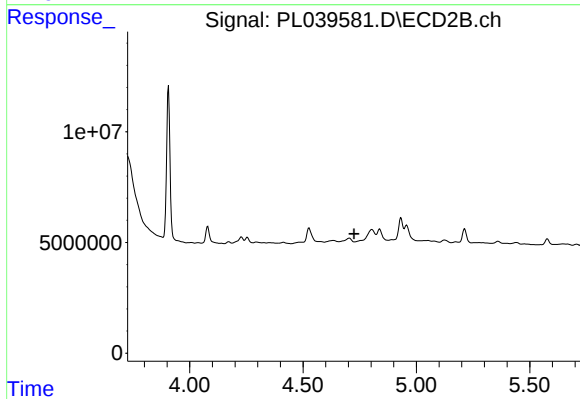

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

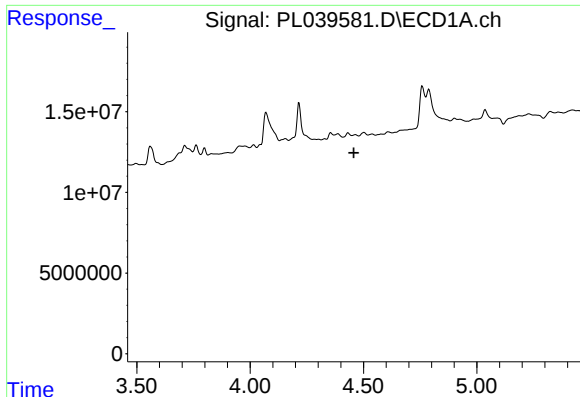

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

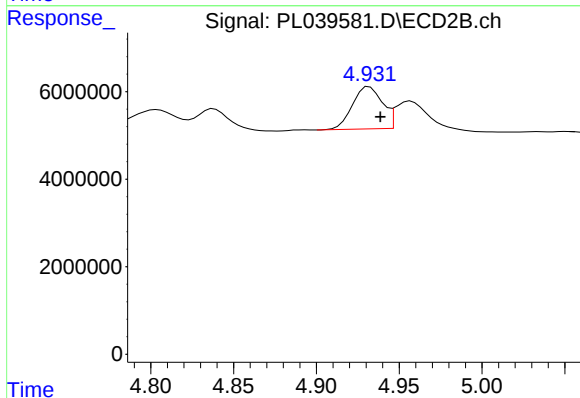


#7 delta-BHC

R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 12110066
Conc: 3.04 ng/ml

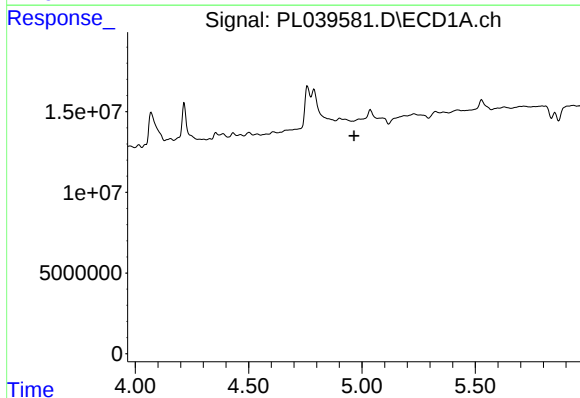


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

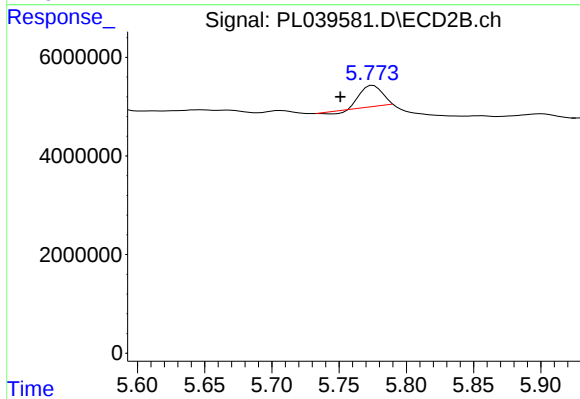

#8 Heptachlor epoxide


R.T.: 5.775 min
Delta R.T.: 0.024 min
Response: 4759391
Conc: 1.42 ng/ml

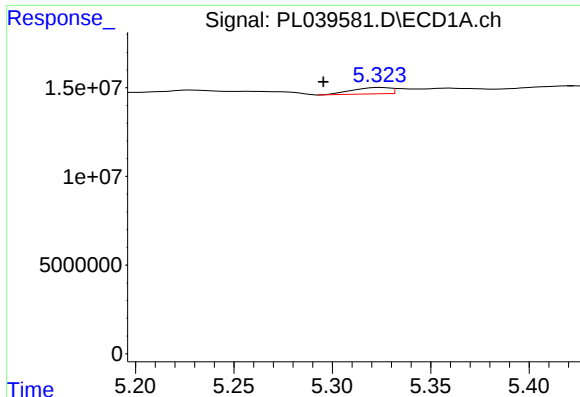

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.029 min
Response: 4982666
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

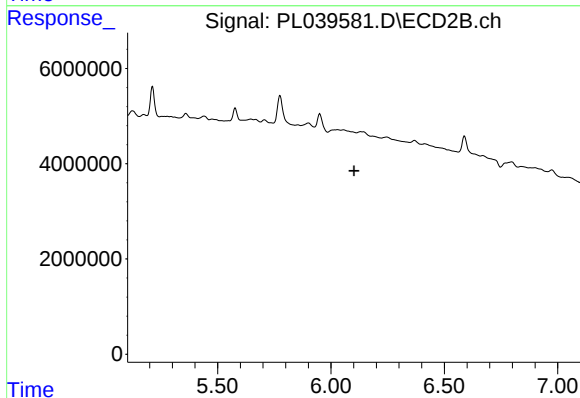


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

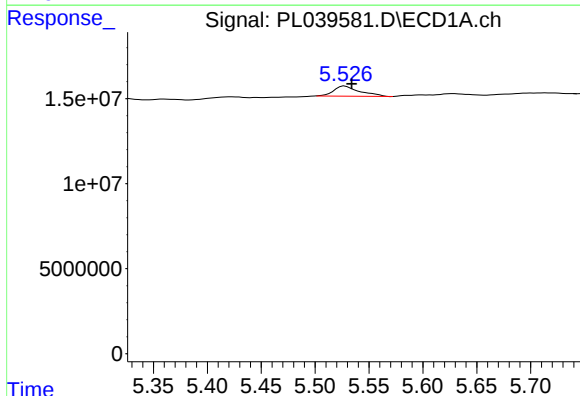


#13 Dieldrin

R.T.: 5.527 min
Delta R.T.: -0.007 min
Response: 10064577
Conc: 1.03 ng/ml

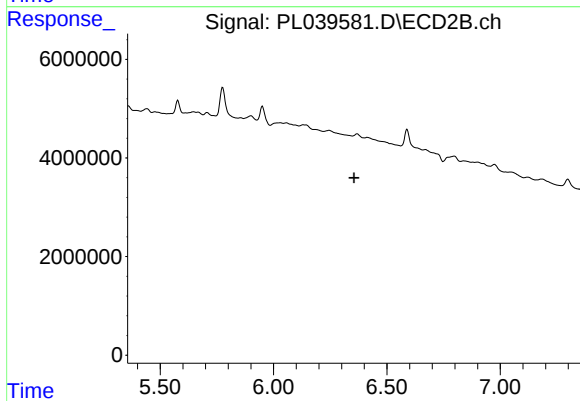

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

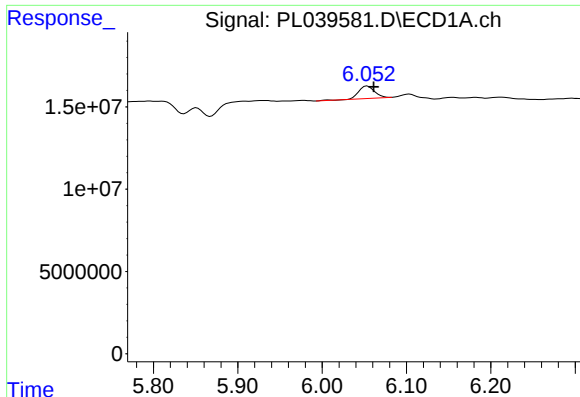

#15 Endosulfan II


R.T.: 6.054 min
Delta R.T.: -0.008 min
Response: 9934707
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

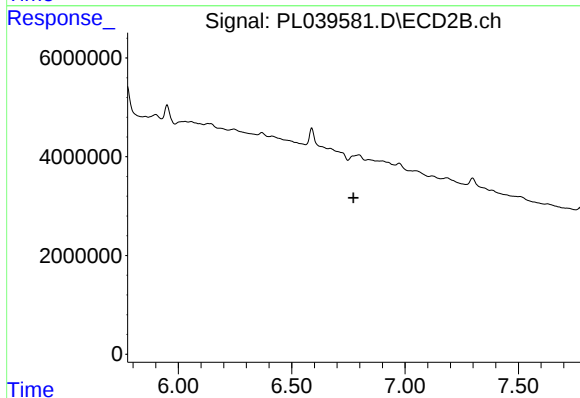


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

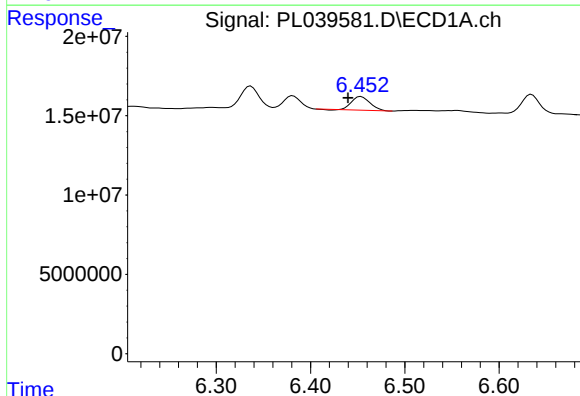


#19 Endosulfan Sulfate

R.T.: 6.454 min
Delta R.T.: 0.014 min
Response: 11489562
Conc: 1.41 ng/ml

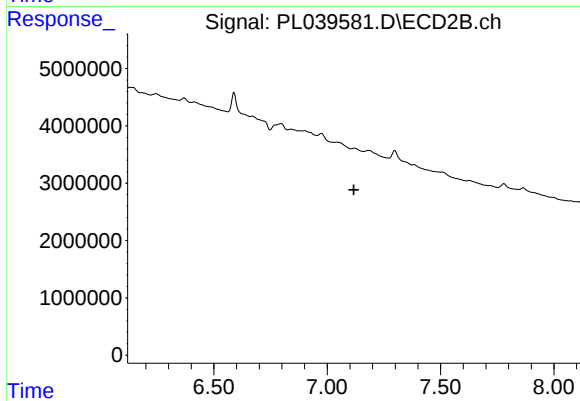

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

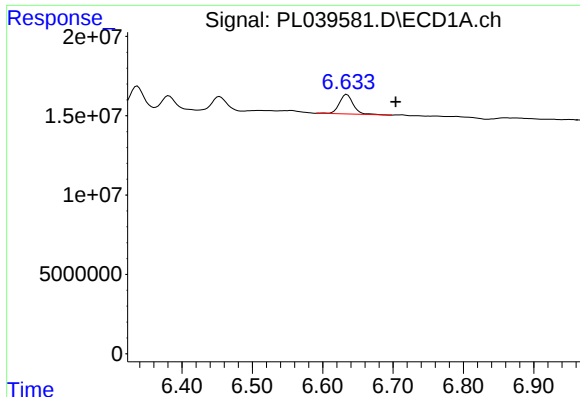

#20 Methoxychlor


R.T.: 6.634 min
Delta R.T.: -0.069 min
Response: 17007717
Conc: 4.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

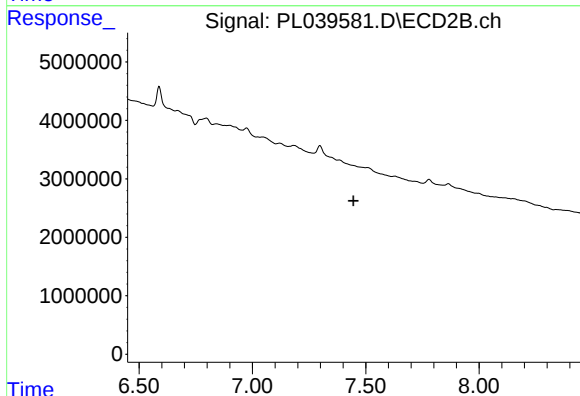


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

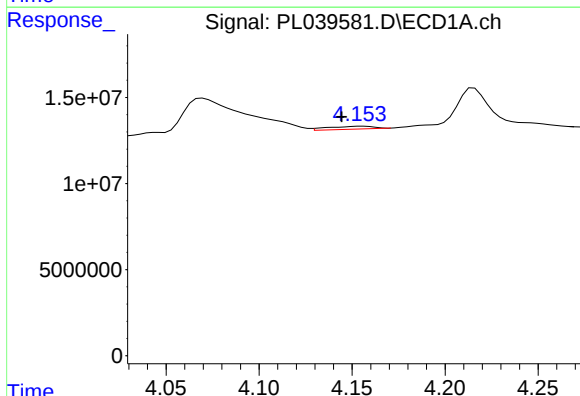


#23 Chlordane-1

R.T.: 4.155 min
Delta R.T.: 0.011 min
Response: 2950790
Conc: 9.32 ng/ml

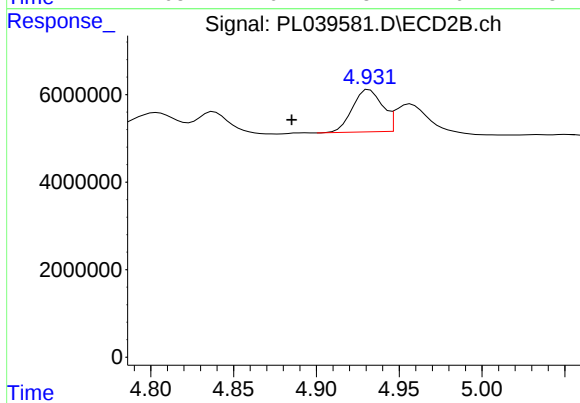

#23 Chlordane-1


R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 12110066
Conc: 96.93 ng/ml

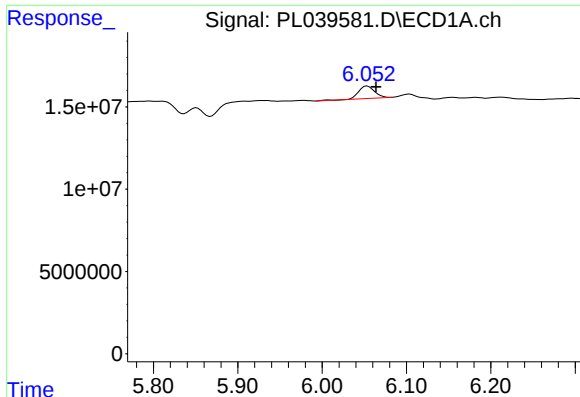

#27 Chlordane-5


R.T.: 6.054 min
Delta R.T.: -0.010 min
Response: 9934707
Conc: 30.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

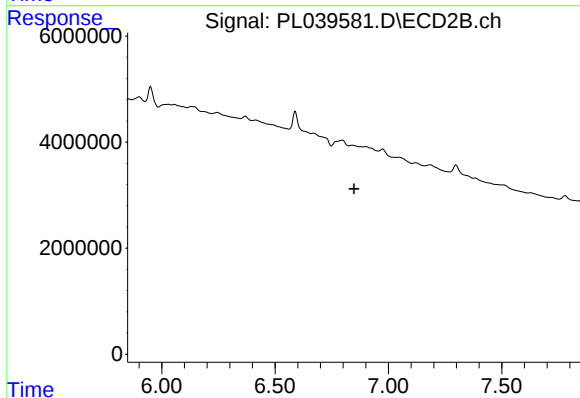


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

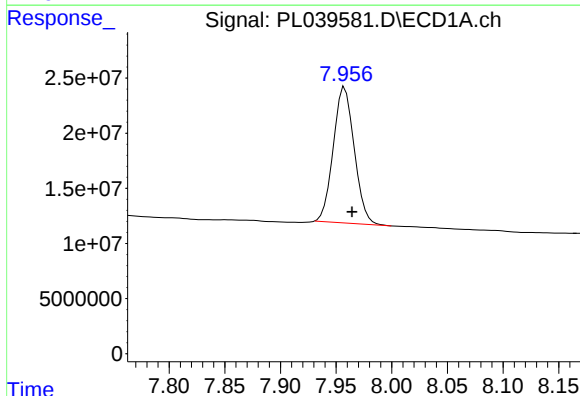

#28 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 161372942
Conc: 22.98 ng/ml

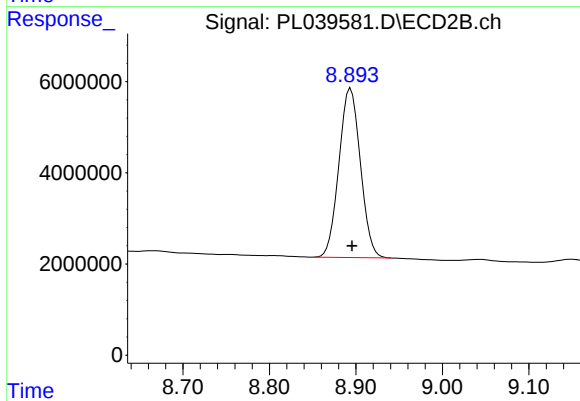

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 63643179
Conc: 27.43 ng/ml