

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2018 10:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 11:58:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.904	126.8E6	53548954	18.137	19.974
28)	SA Decachlor...	7.970	8.896	139.1E6	50855098	19.810	21.915
Target Compounds							
4)	MA Heptachlor	4.227f	0.000	2585157	0	0.246	N.D. #
6)	B beta-BHC	4.227f	0.000	2585157	0	0.556	N.D. #
8)	B Heptachlo...	4.919f	0.000	2661140	0	0.279	N.D. #
14)	MA Endrin	5.813	0.000	5709138	0	0.638	N.D. #
17)	MA 4,4'-DDT	6.133	0.000	23644082	0	3.119	N.D. #
18)	B Endrin al...	6.218	0.000	6716503	0	0.991	N.D. #
20)	A Methoxychlor	6.689	0.000	25345863	0	6.194	N.D. #
23)	Chlordane-1	4.126	0.000	2257777	0	7.132	N.D. #
27)	Chlordane-5	6.133	0.000	23644082	0	72.901	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2018 10:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 11:58:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

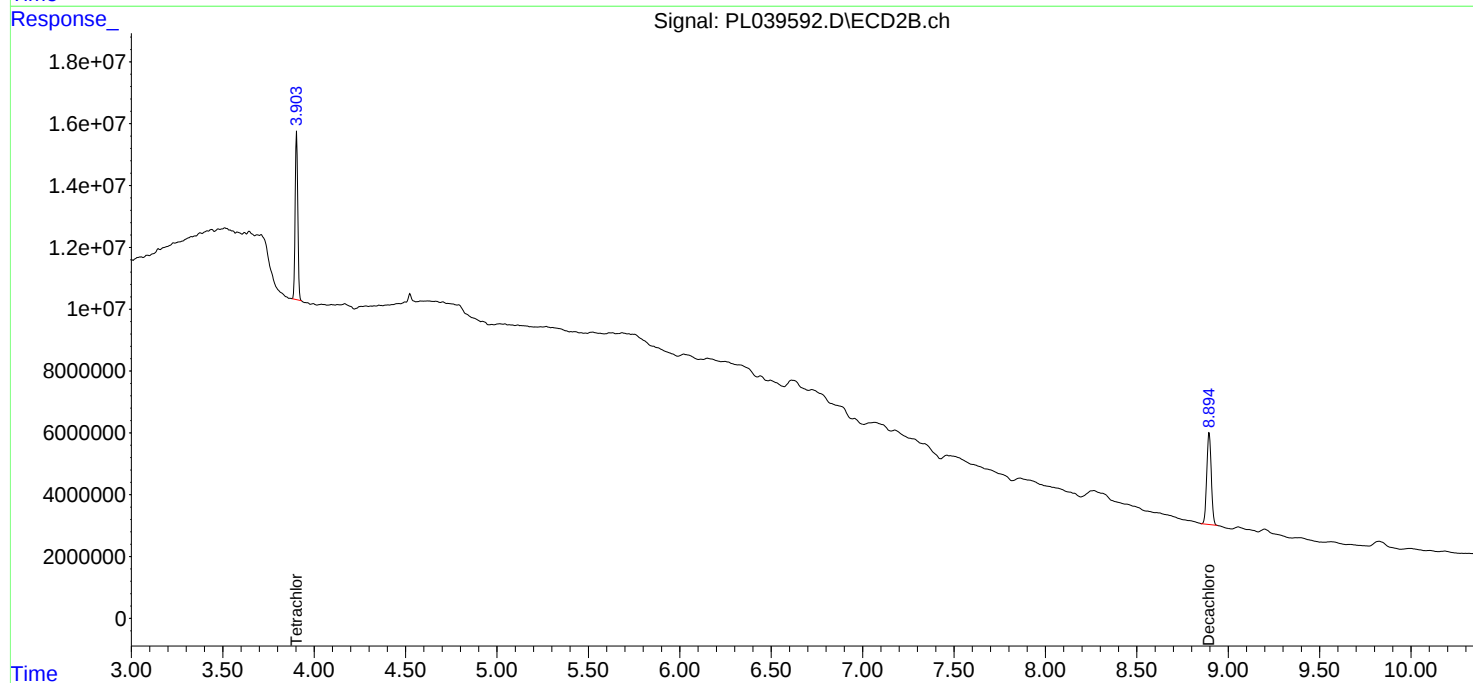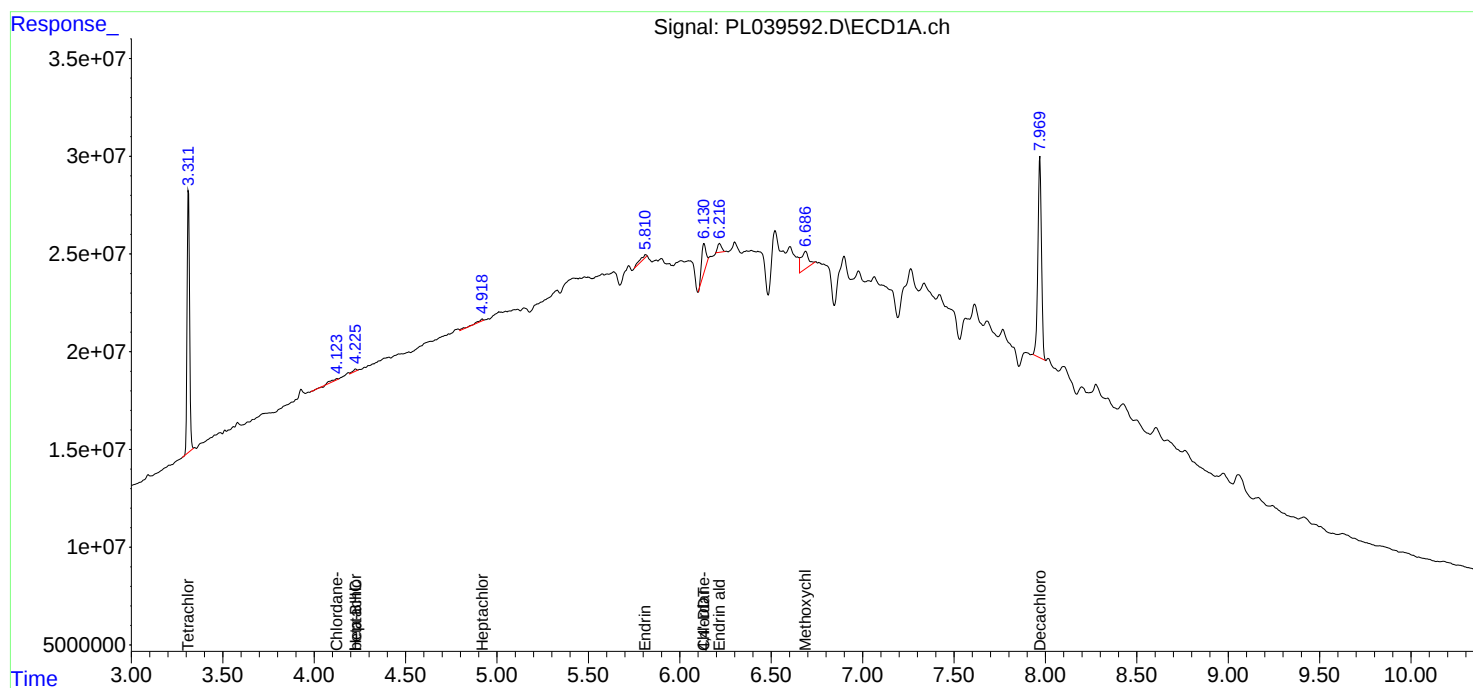


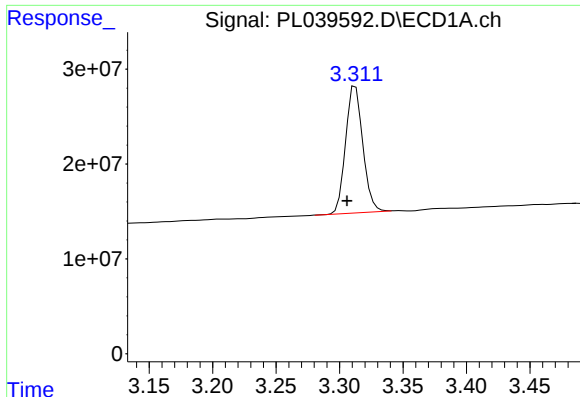

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.007 min
Response: 126786256
Conc: 18.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

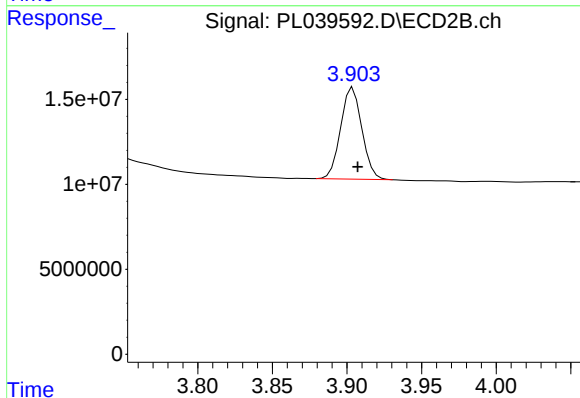


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: -0.003 min
Response: 53548954
Conc: 19.97 ng/ml

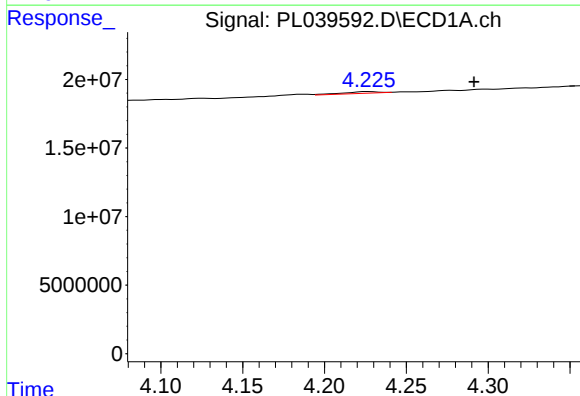


#4 Heptachlor

R.T.: 4.227 min
Delta R.T.: -0.065 min
Response: 2585157
Conc: 0.25 ng/ml

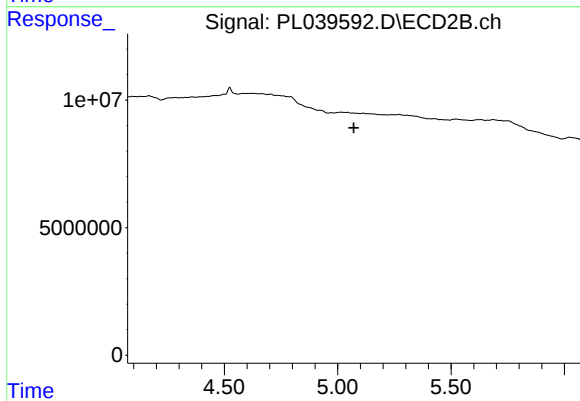

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

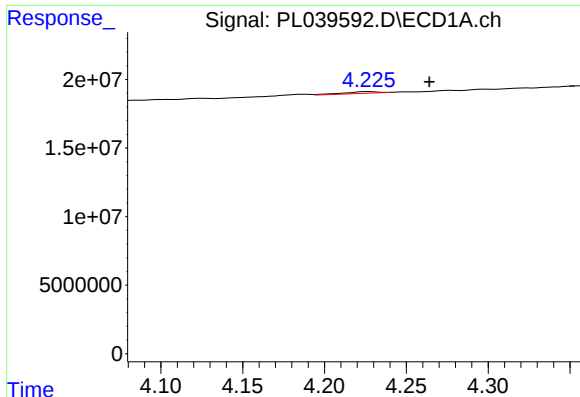

#6 beta-BHC


R.T.: 4.227 min
Delta R.T.: -0.037 min
Response: 2585157
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

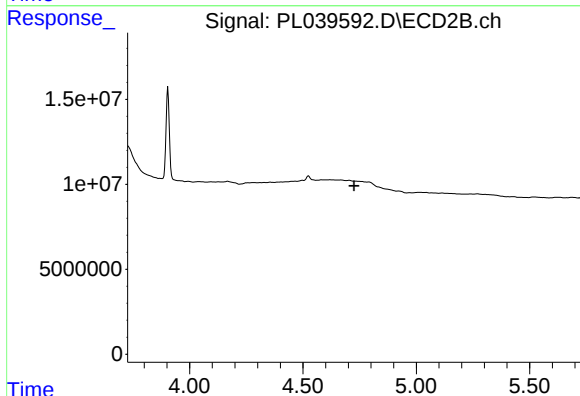


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

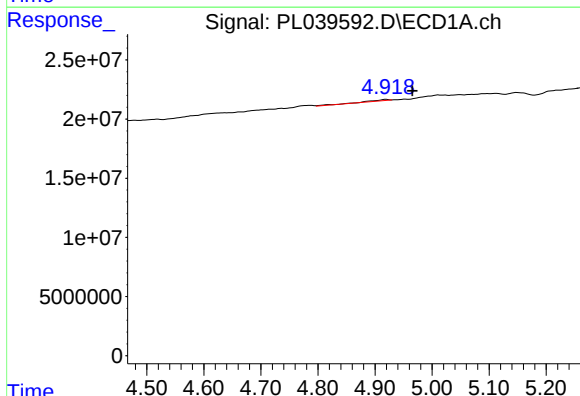


#8 Heptachlor epoxide

R.T.: 4.919 min
Delta R.T.: -0.046 min
Response: 2661140
Conc: 0.28 ng/ml

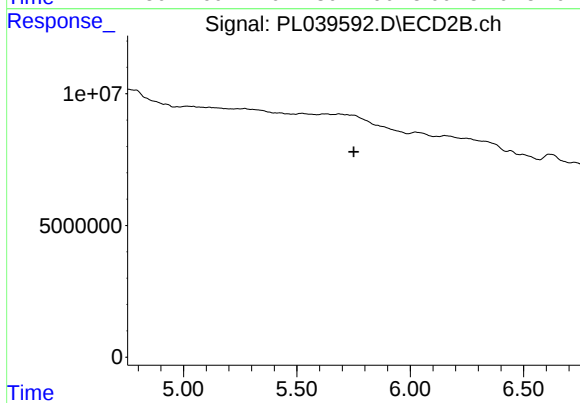

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

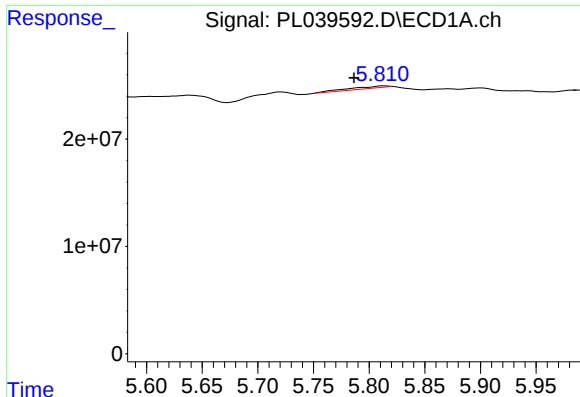

#14 Endrin


R.T.: 5.813 min
Delta R.T.: 0.027 min
Response: 5709138
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

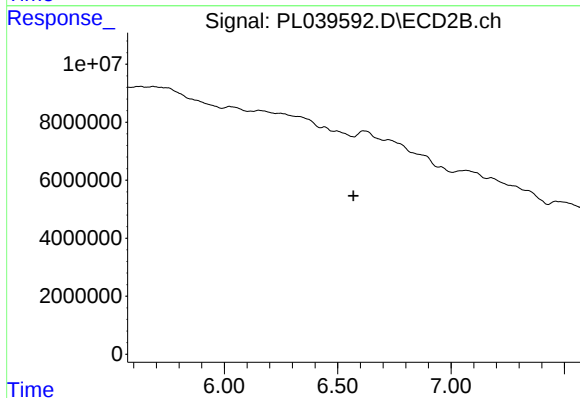


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

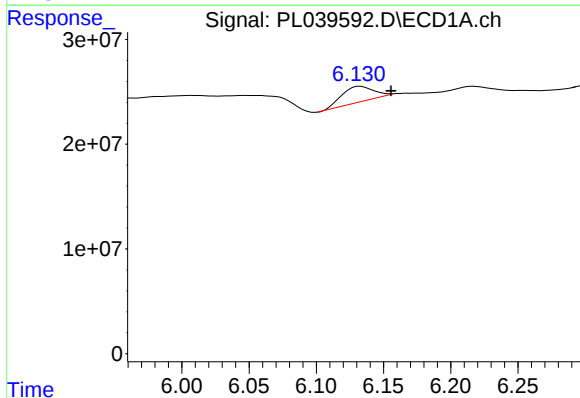


#17 4,4'-DDT

R.T.: 6.133 min
Delta R.T.: -0.023 min
Response: 23644082
Conc: 3.12 ng/ml

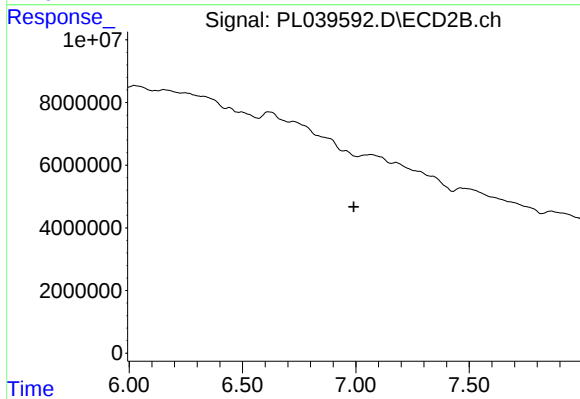

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

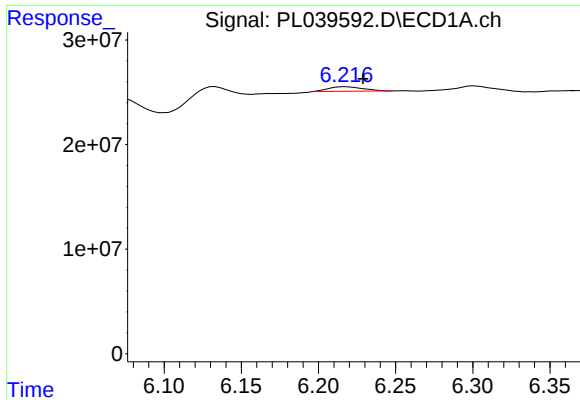

#18 Endrin aldehyde


R.T.: 6.218 min
Delta R.T.: -0.011 min
Response: 6716503
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

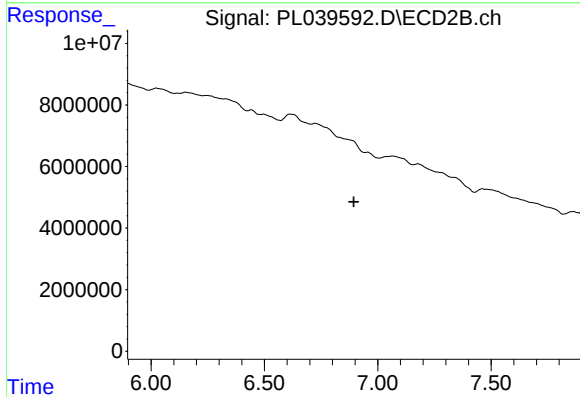


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

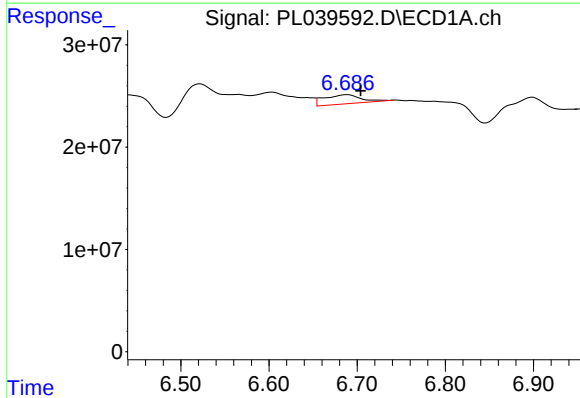


#20 Methoxychlor

R.T.: 6.689 min
Delta R.T.: -0.015 min
Response: 25345863
Conc: 6.19 ng/ml

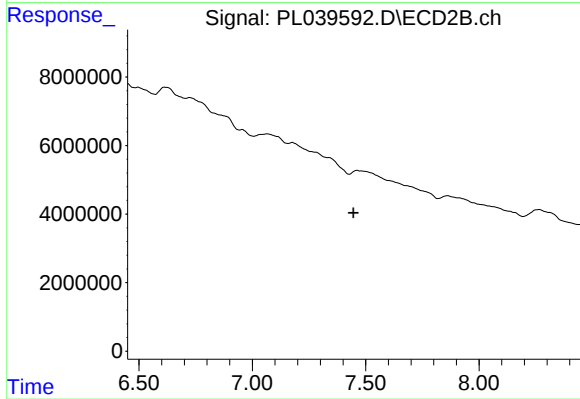

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

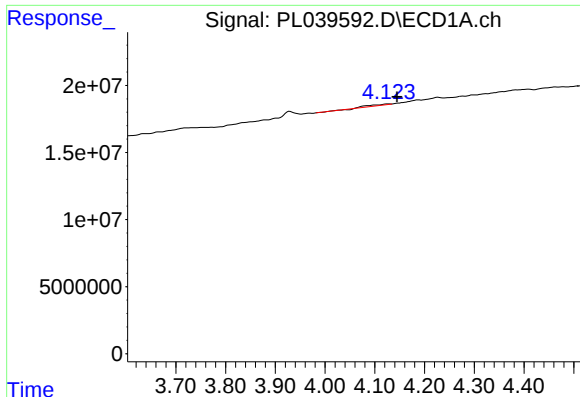

#23 Chlordane-1


R.T.: 4.126 min
Delta R.T.: -0.018 min
Response: 2257777
Conc: 7.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

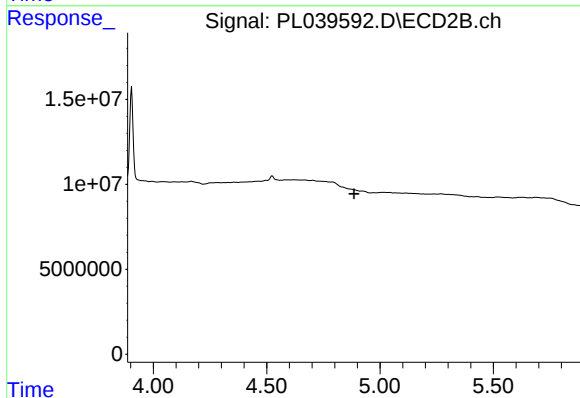


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

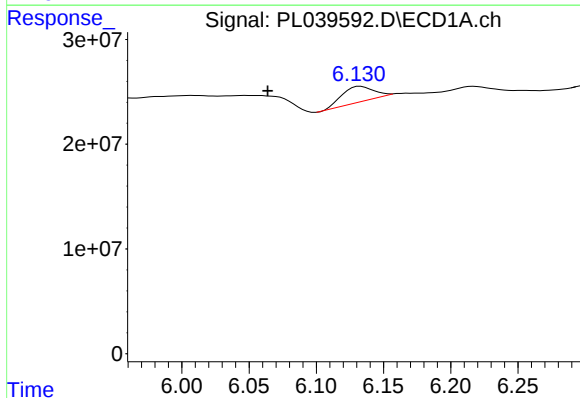


#27 Chlordane-5

R.T.: 6.133 min
Delta R.T.: 0.069 min
Response: 23644082
Conc: 72.90 ng/ml

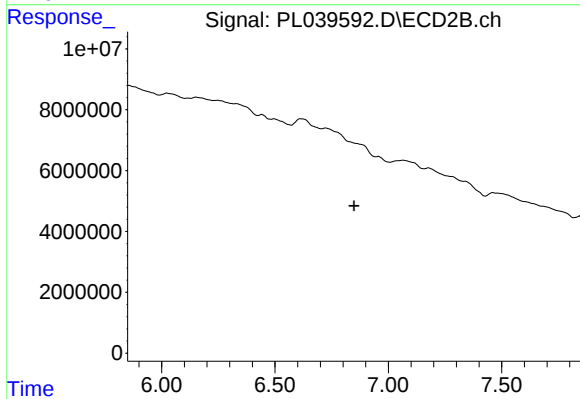

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

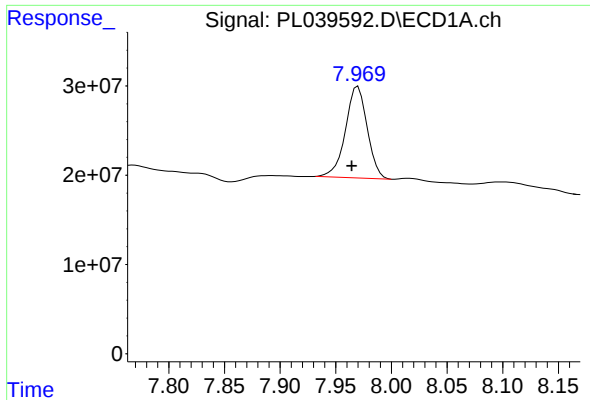

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: 0.006 min
Response: 139130333
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

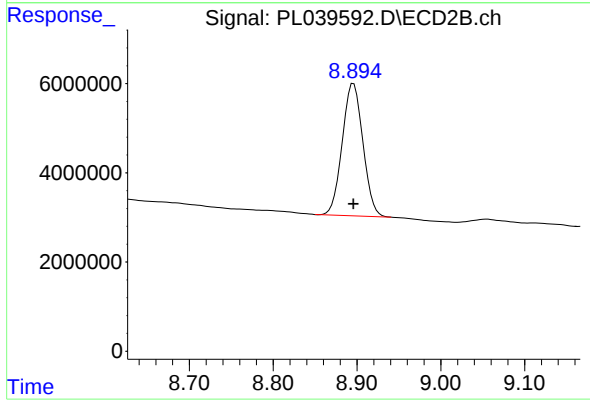

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 50855098
Conc: 21.91 ng/ml