

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2018 12:00
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 12:16:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.310	3.904	152.5E6	66725656	21.817	24.889
28)	SA Decachlor...	7.966	8.894	148.9E6	53368465	21.198	22.998
Target Compounds							
4)	MA Heptachlor	4.221f	0.000	6035320	0	0.573	N.D. #
6)	B beta-BHC	4.221f	0.000	6035320	0	1.299	N.D. #
23)	Chlordane-1	4.130	0.000	6379043	0	20.149	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2018 12:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 12:16:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

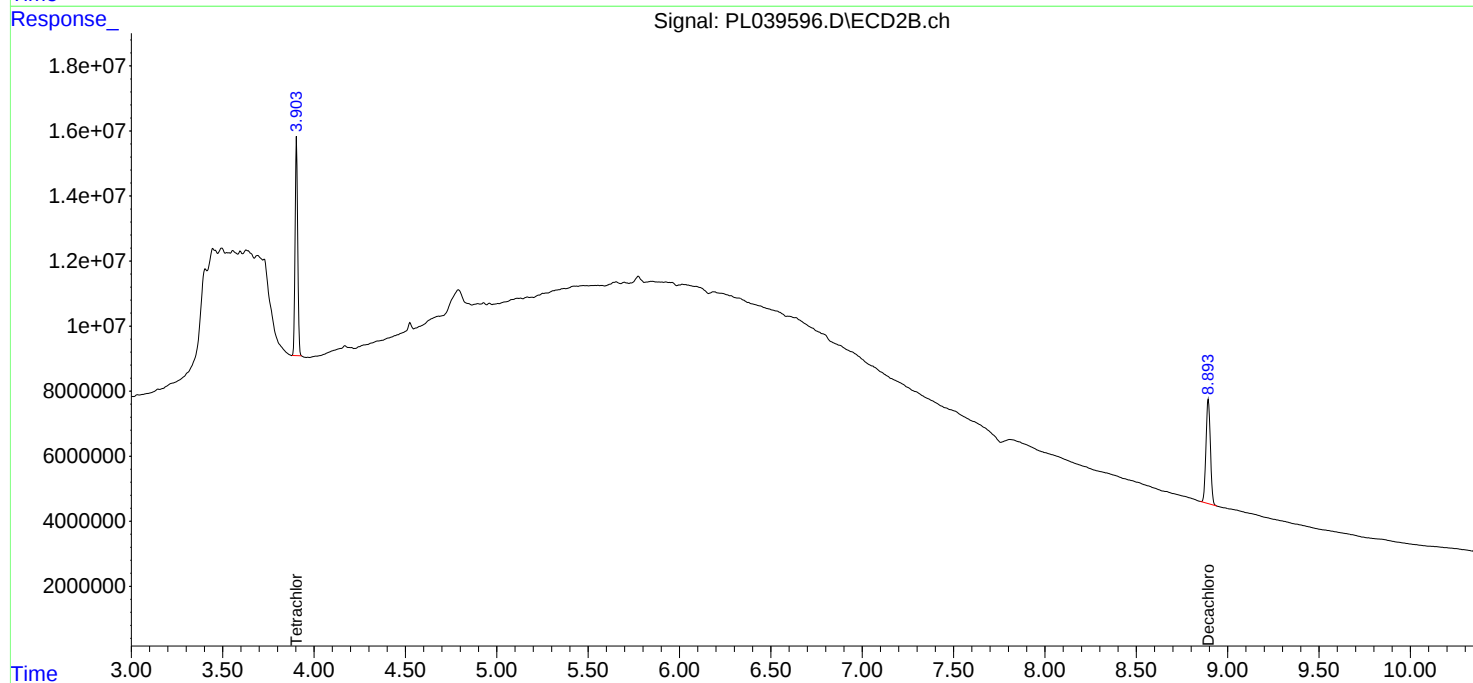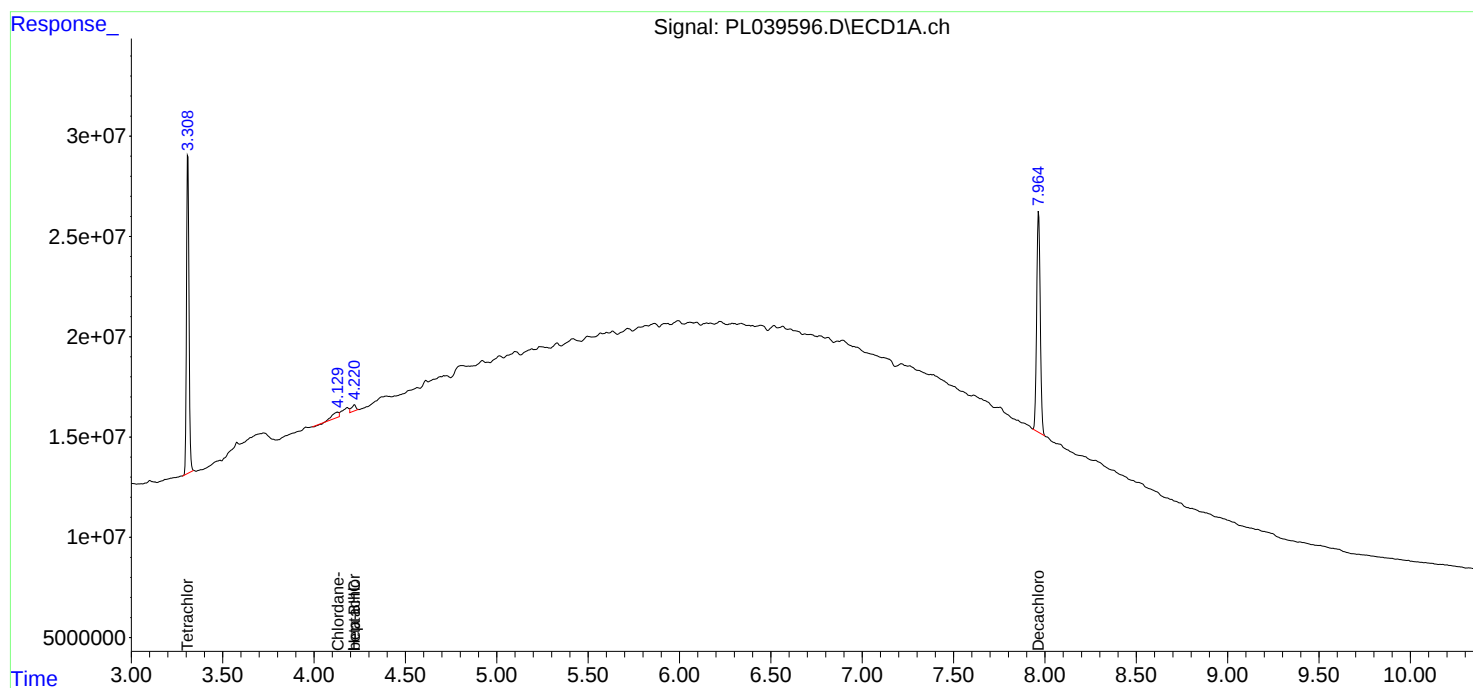


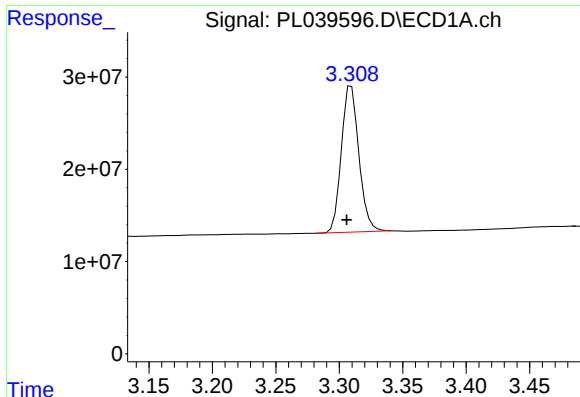

#1 Tetrachloro-m-xylene


R.T.: 3.310 min
Delta R.T.: 0.004 min
Response: 152512961
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

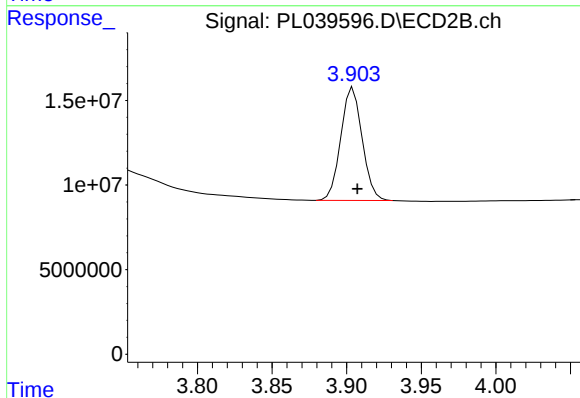


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: -0.003 min
Response: 66725656
Conc: 24.89 ng/ml

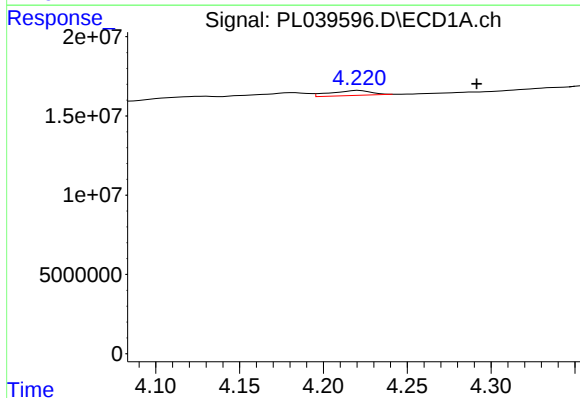


#4 Heptachlor

R.T.: 4.221 min
Delta R.T.: -0.070 min
Response: 6035320
Conc: 0.57 ng/ml

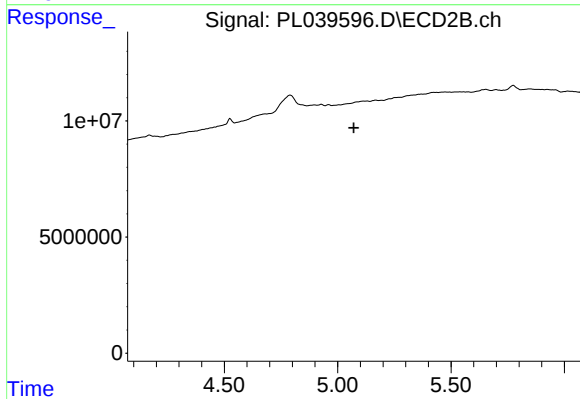

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

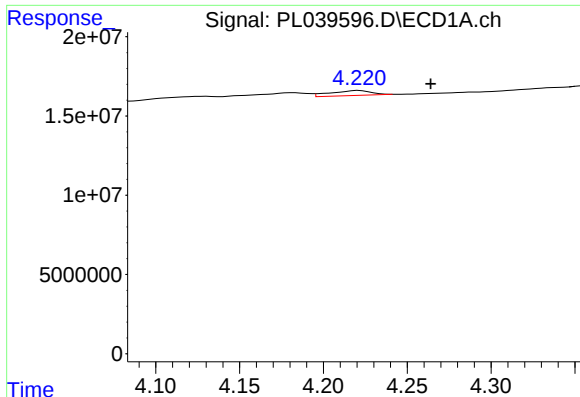

#6 beta-BHC


R.T.: 4.221 min
Delta R.T.: -0.043 min
Response: 6035320
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

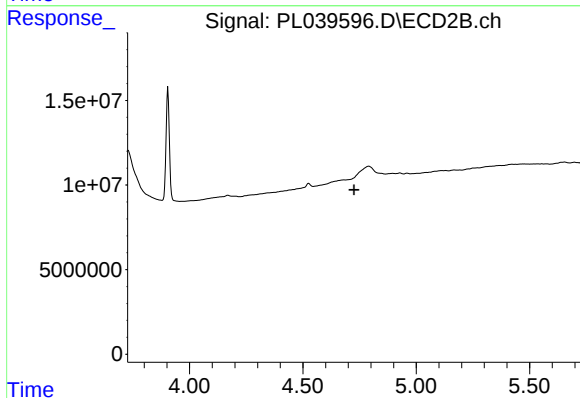


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

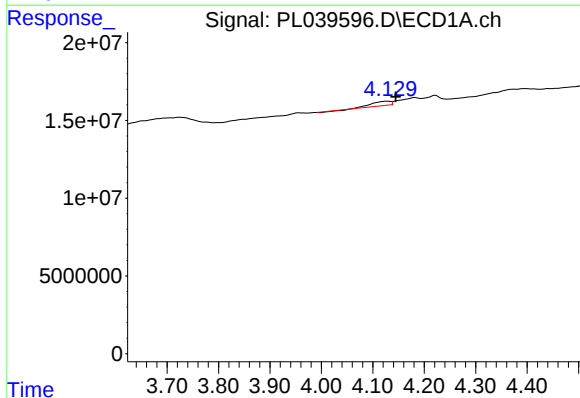


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: -0.015 min
Response: 6379043
Conc: 20.15 ng/ml

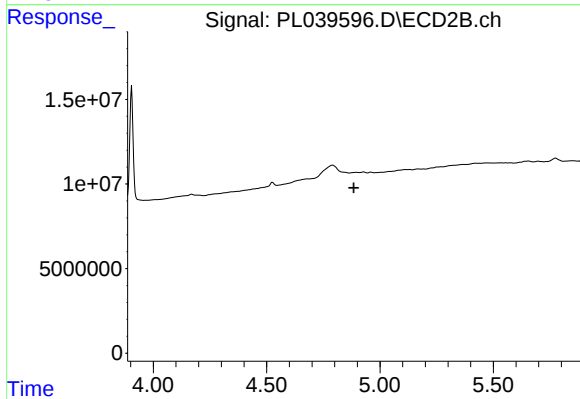

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

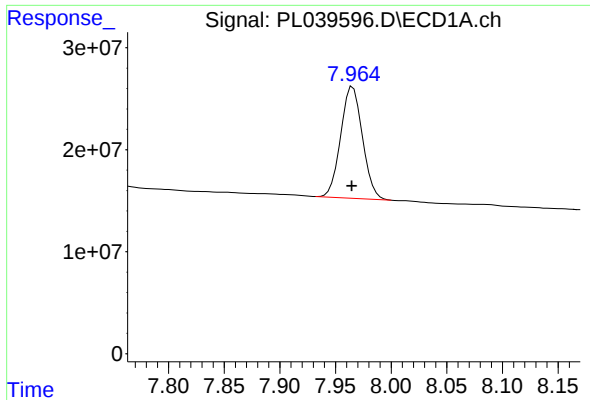

#28 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.001 min
Response: 148883455
Conc: 21.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

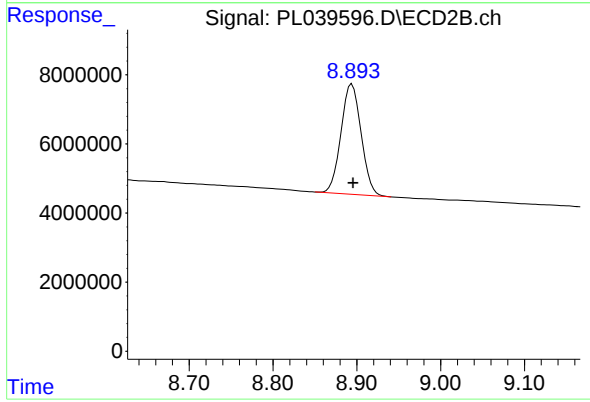

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.001 min
Response: 53368465
Conc: 23.00 ng/ml