

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 17:12
 Operator : AJ\SJ
 Sample : J4671-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TL-SPEEDY-DRY

Manual Integrations
 APPROVED

Sohil
 8/29/2018 1:39:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:55:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.904	116.2E6	40725552	16.622	15.191m
28)	SA Decachlor...	7.960	8.895	104.4E6	42082596	14.866	18.134

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 17:12
Operator : AJ\SJ
Sample : J4671-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TL-SPEEDY-DRY


Manual Integrations
APPROVED

Sohil
8/29/2018 1:39:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:55:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

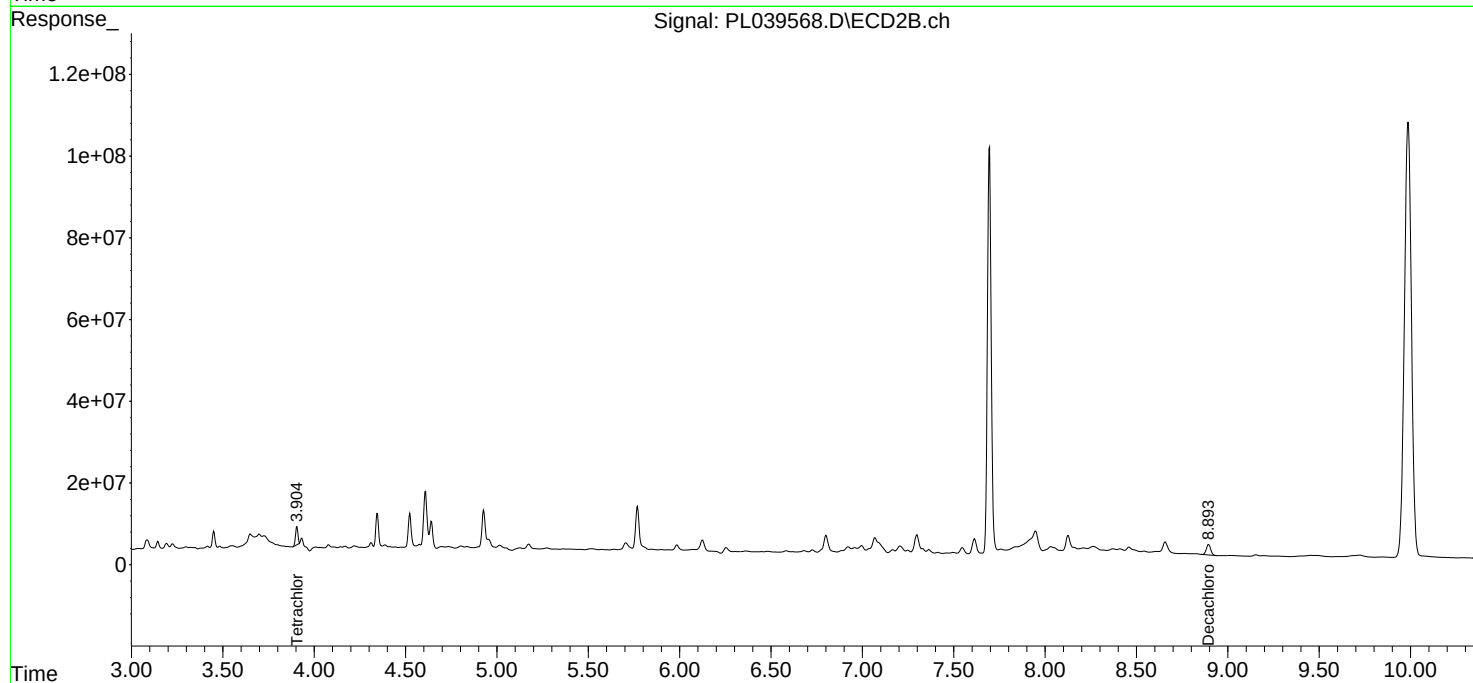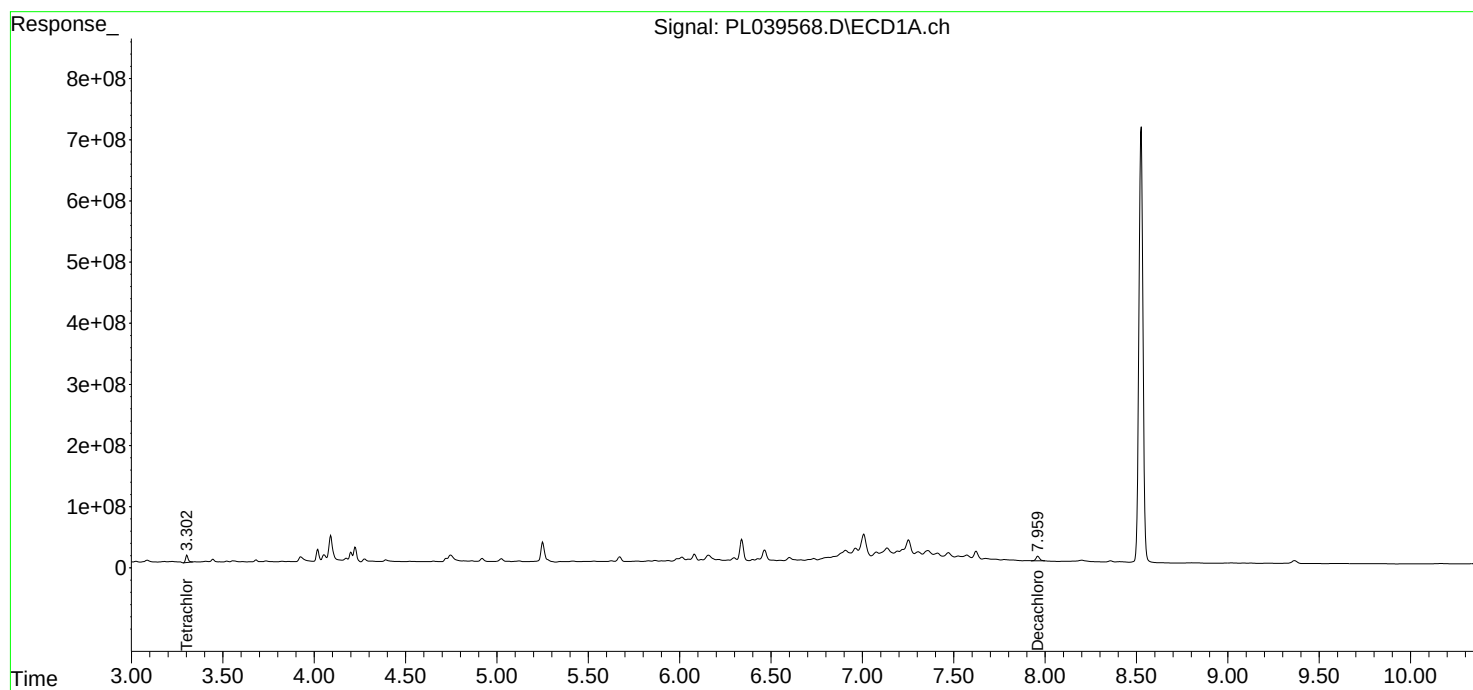

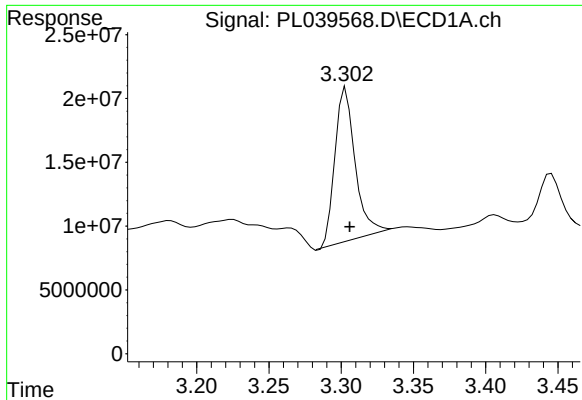


#1 Tetrachloro-m-xylene

R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 116192452
Conc: 16.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TL-SPEEDY-DRY


Manual Integrations
APPROVED

Sohil
8/29/2018 1:39:52 PM

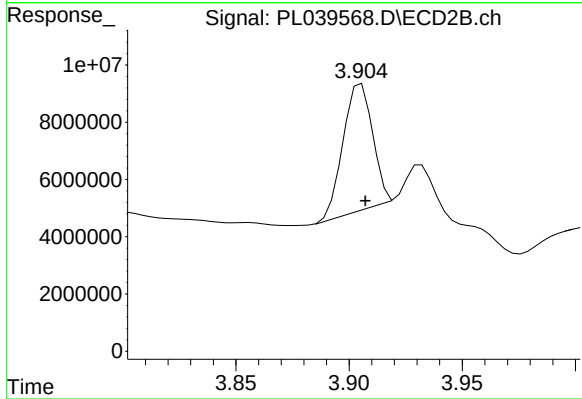


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: -0.003 min
Response: 40725552
Conc: 15.19 ng/ml m

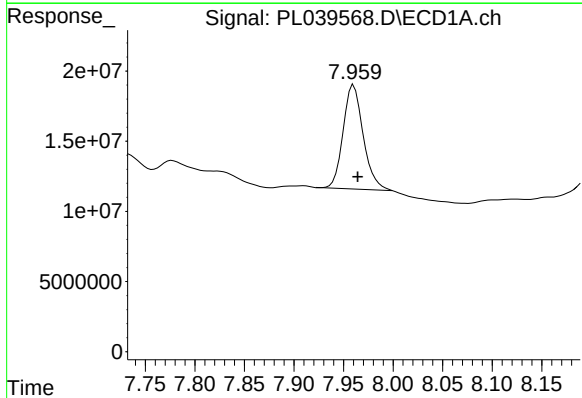

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 104412262
Conc: 14.87 ng/ml

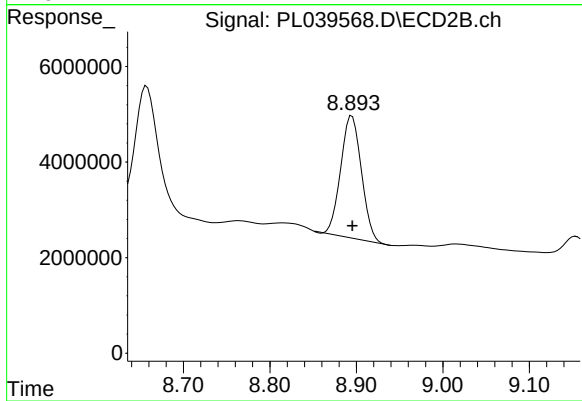

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 42082596
Conc: 18.13 ng/ml