

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 17:20
 Operator : SG\AJ
 Sample : PB122626BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122626BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 00:58:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.925	161.5E6	33752158	18.867	15.449
28)	SA Decachlor...	7.973	8.952	244.9E6	60361403	20.180	19.830
Target Compounds							
4)	MA Heptachlor	0.000	5.103	0	661110	N.D.	0.189 #
8)	B Heptachlo...	0.000	5.781	0	390619	N.D.	0.116 #
9)	A Endosulfan I	5.335f	0.000	2069984	0	0.154	N.D. #
10)	B gamma-Chl...	0.000	6.004f	0	1051669	N.D.	0.288 #
11)	B alpha-Chl...	0.000	6.099	0	1479050	N.D.	0.429 #
13)	MA Dieldrin	5.546	0.000	2615906	0	0.172	N.D. #
15)	B Endosulfa...	0.000	6.848f	0	1960912	N.D.	0.595 #
18)	B Endrin al...	0.000	6.973f	0	1861477	N.D.	0.659 #
25)	Chlordane-3	0.000	6.004f	0	1051669	N.D.	2.360 #
26)	Chlordane-4	0.000	6.099	0	1479050	N.D.	2.723 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 17:20
Operator : SG\AJ
Sample : PB122626BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB122626BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 00:58:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

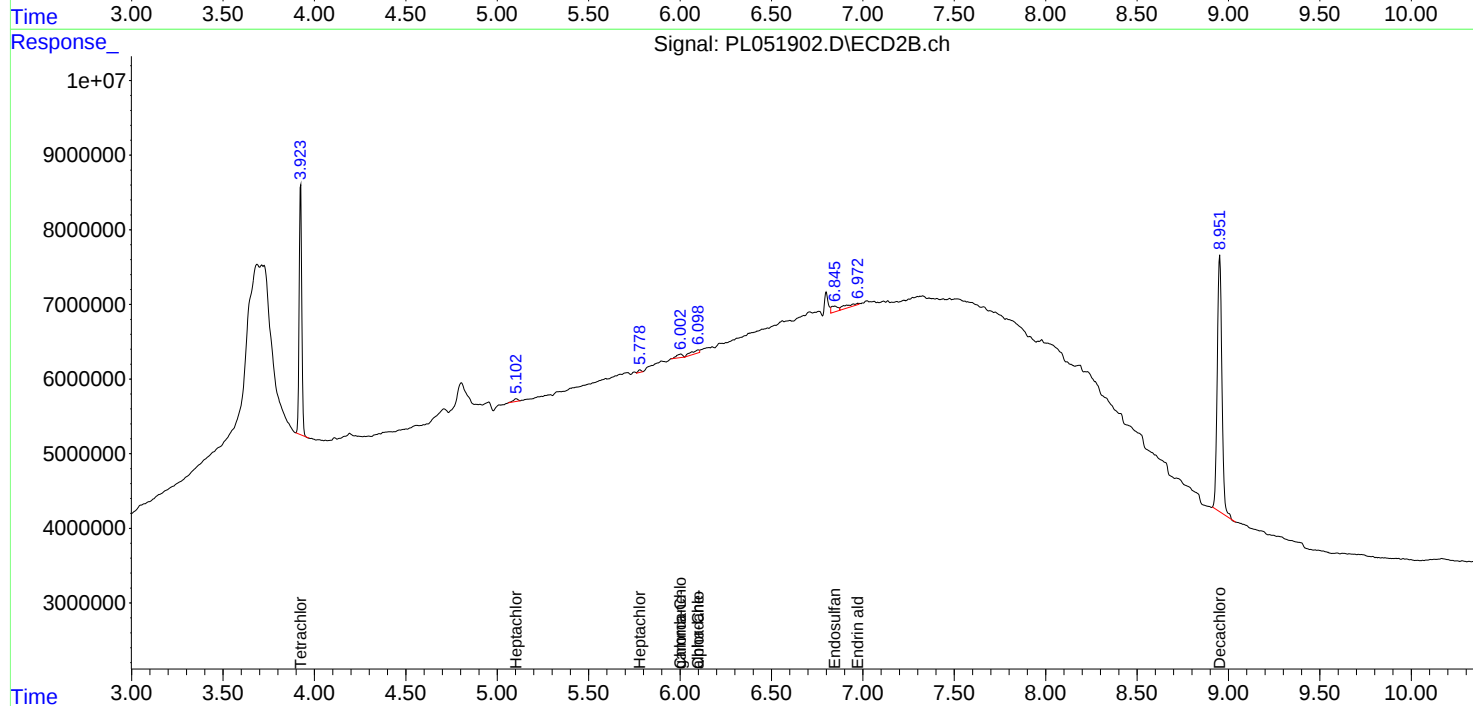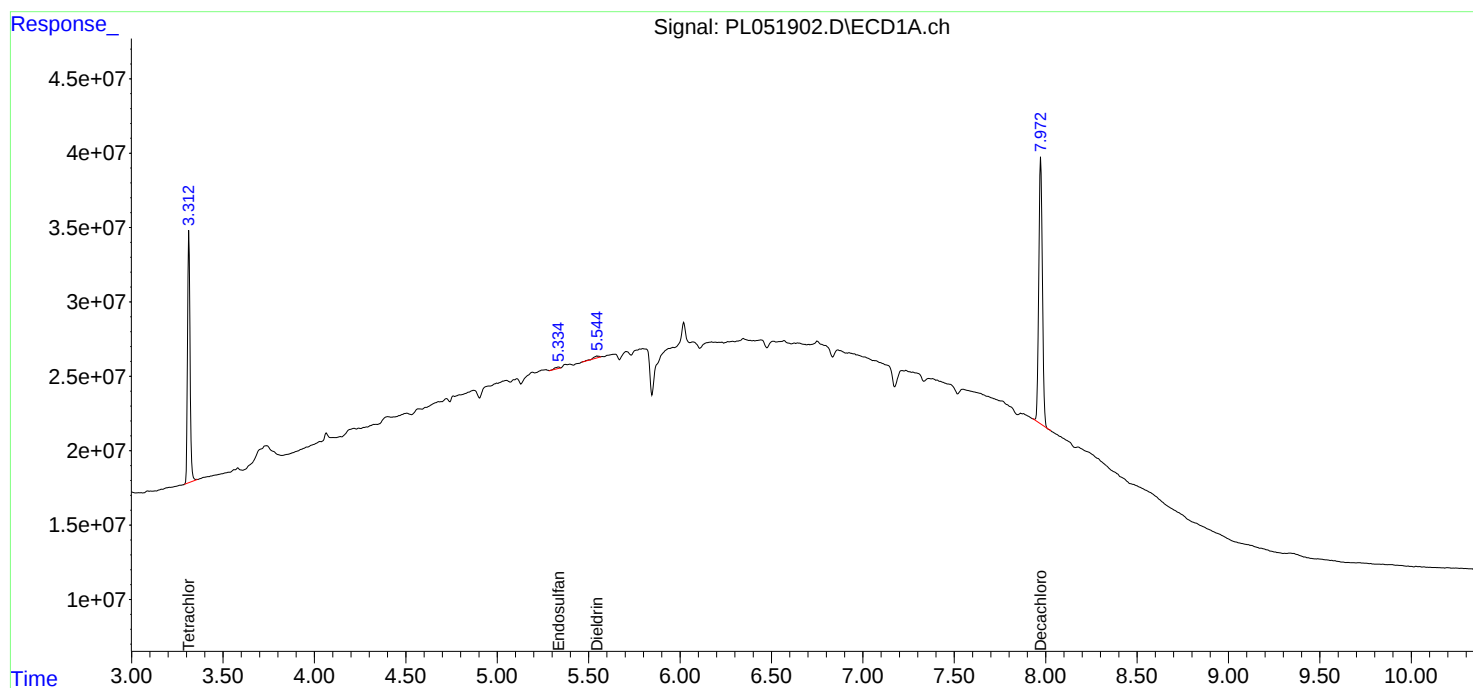


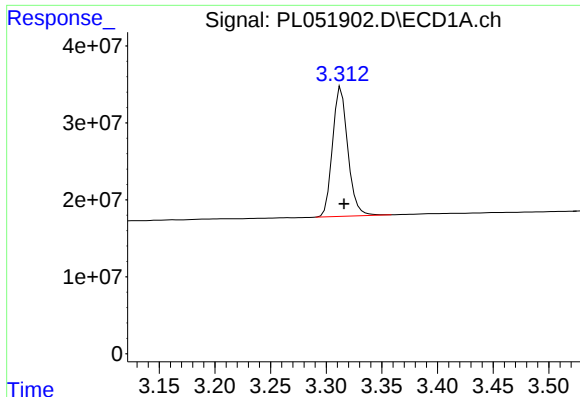

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 161471611
Conc: 18.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122626BL

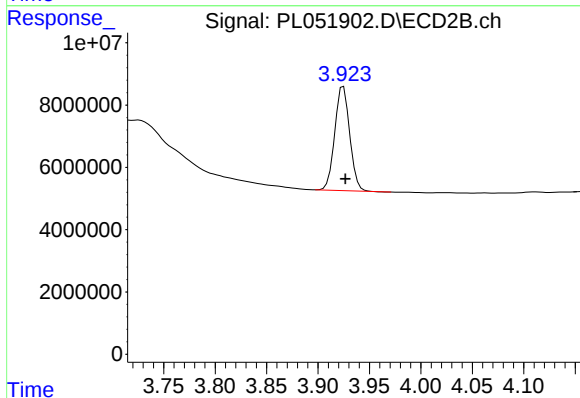


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 33752158
Conc: 15.45 ng/ml

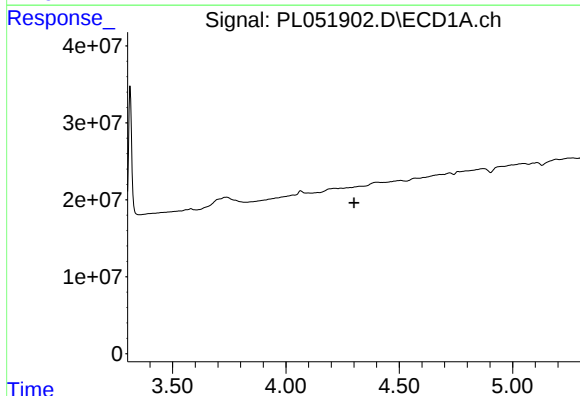


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

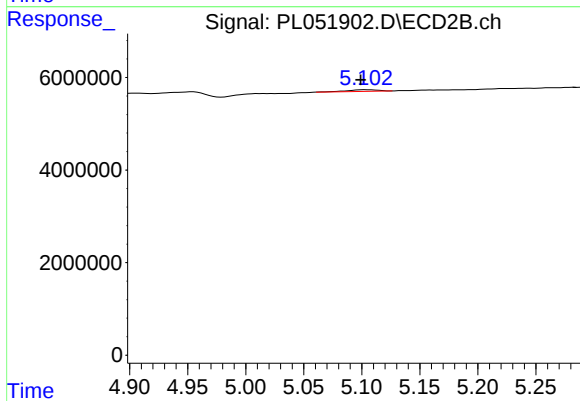

#4 Heptachlor


R.T.: 5.103 min
Delta R.T.: 0.004 min
Response: 661110
Conc: 0.19 ng/ml

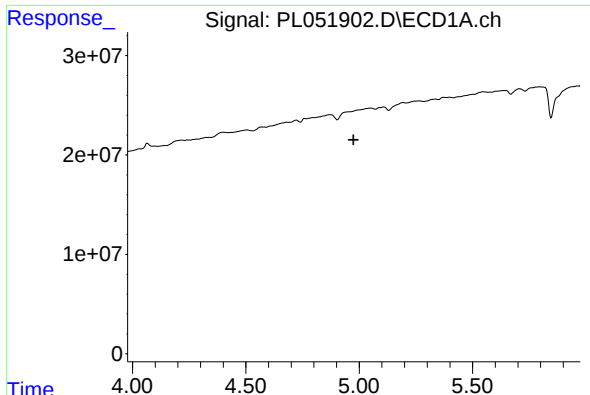

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122626BL

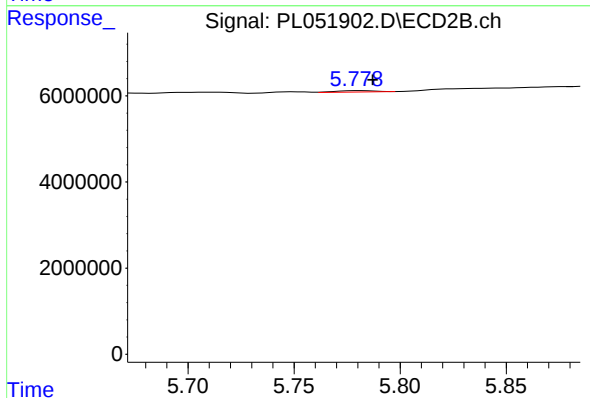


#8 Heptachlor epoxide

R.T.: 5.781 min
Delta R.T.: -0.006 min
Response: 390619
Conc: 0.12 ng/ml

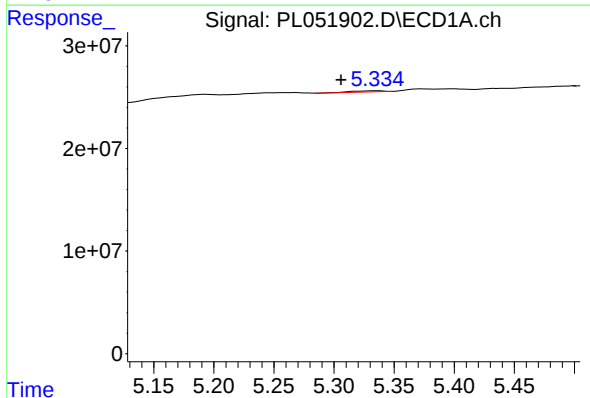


#9 Endosulfan I

R.T.: 5.335 min
Delta R.T.: 0.030 min
Response: 2069984
Conc: 0.15 ng/ml

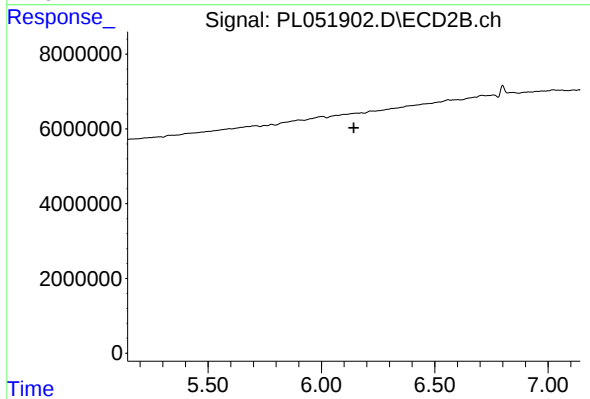

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

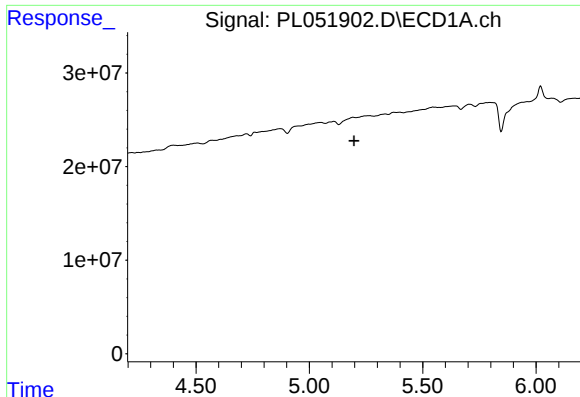

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122626BL

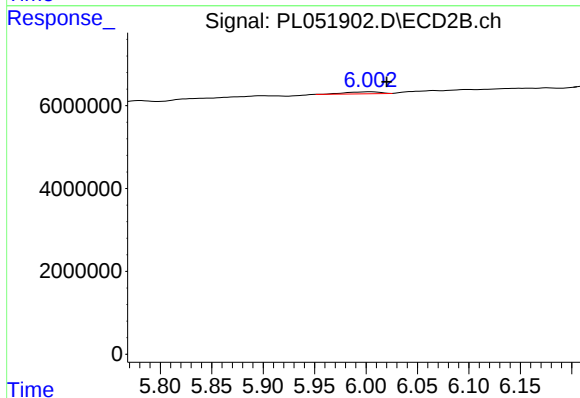


#10 gamma-Chlordane

R.T.: 6.004 min
Delta R.T.: -0.016 min
Response: 1051669
Conc: 0.29 ng/ml

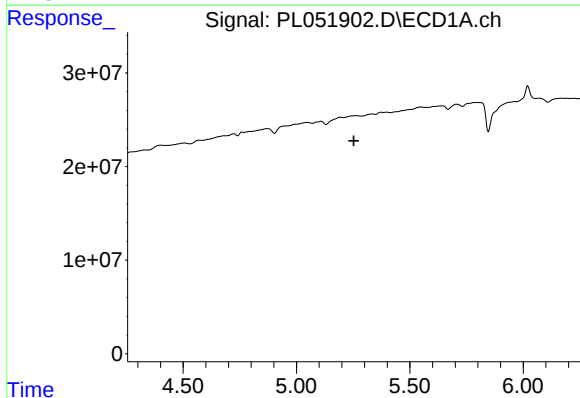


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

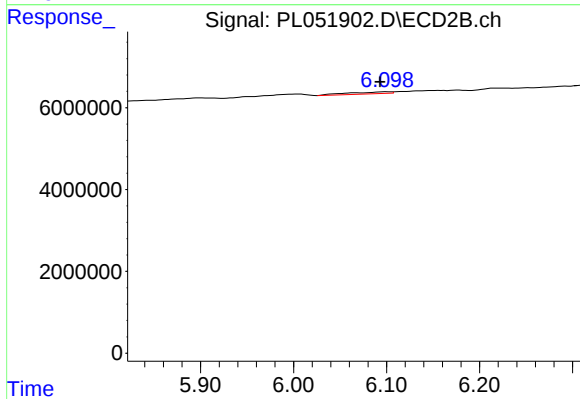

#11 alpha-Chlordane


R.T.: 6.099 min
Delta R.T.: 0.006 min
Response: 1479050
Conc: 0.43 ng/ml

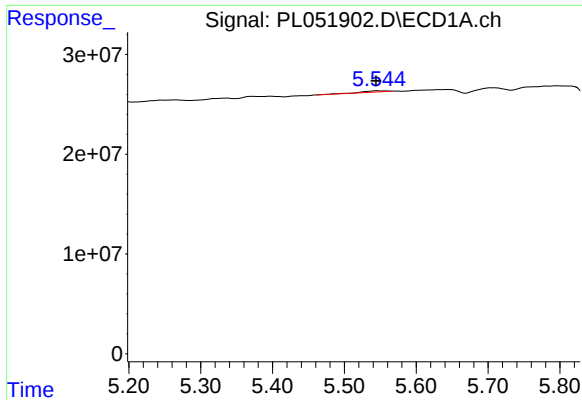

#13 Dieldrin


R.T.: 5.546 min
Delta R.T.: 0.002 min
Response: 2615906
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122626BL

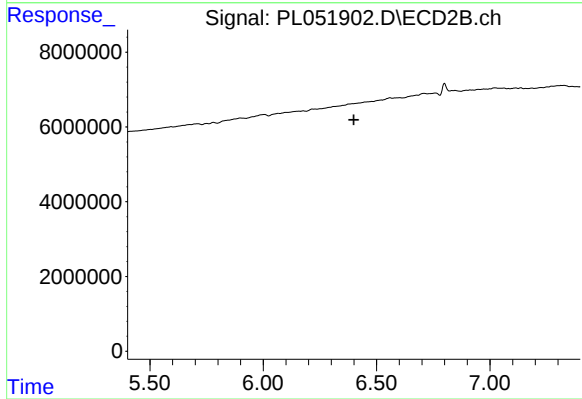


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

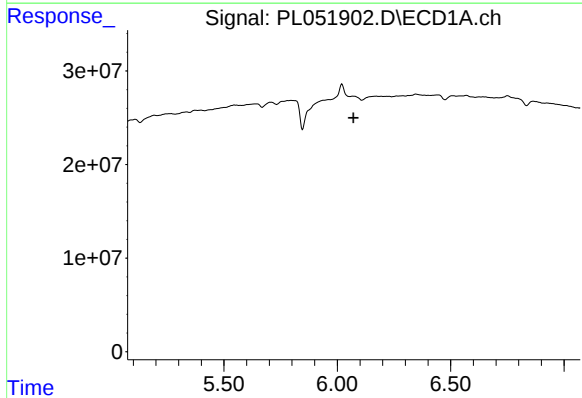


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

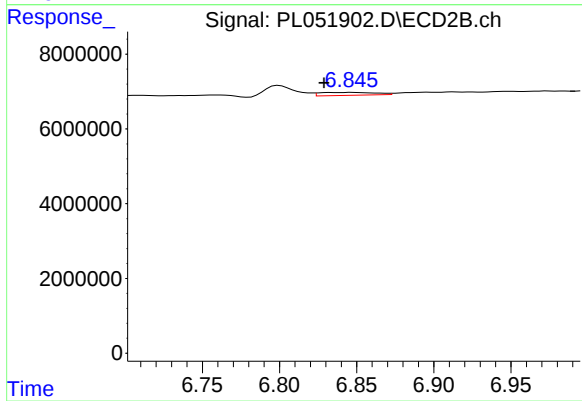

#15 Endosulfan II


R.T.: 6.848 min
Delta R.T.: 0.019 min
Response: 1960912
Conc: 0.59 ng/ml

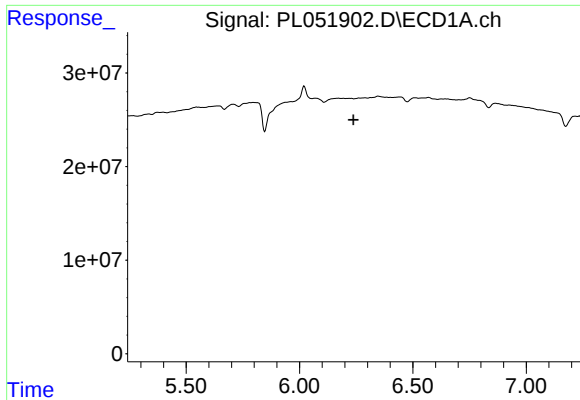

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122626BL

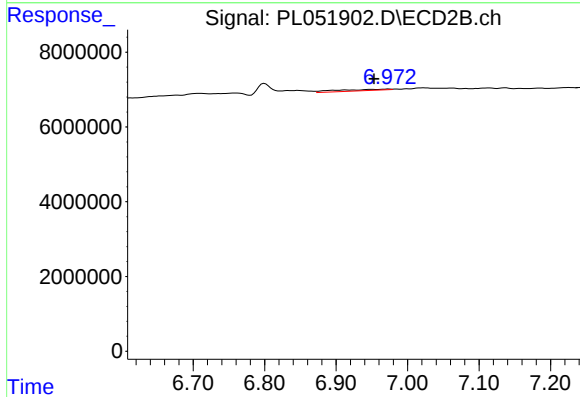


#18 Endrin aldehyde

R.T.: 6.973 min
Delta R.T.: 0.020 min
Response: 1861477
Conc: 0.66 ng/ml

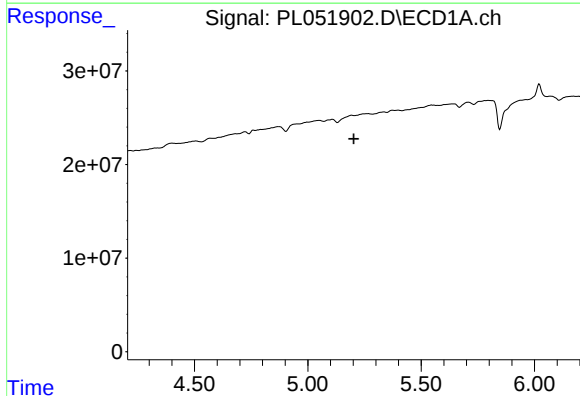


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

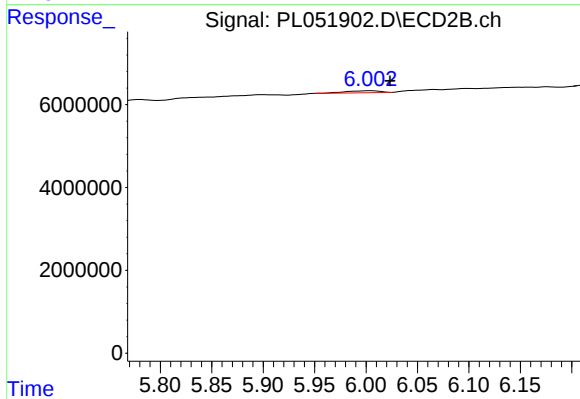

#25 Chlordane-3


R.T.: 6.004 min
Delta R.T.: -0.019 min
Response: 1051669
Conc: 2.36 ng/ml

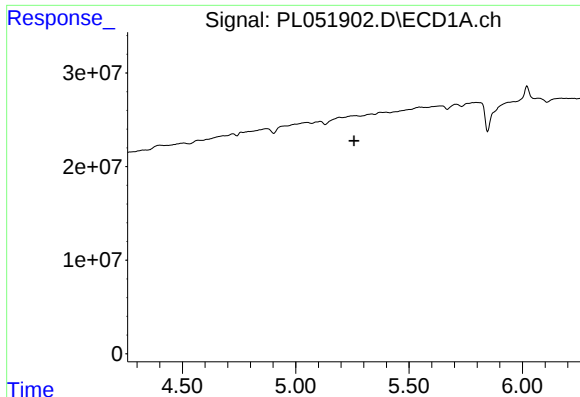

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122626BL

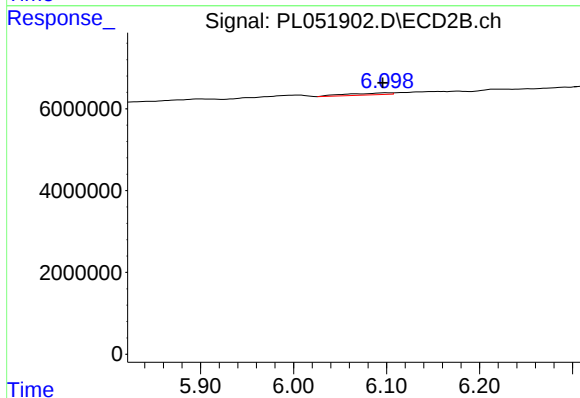


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.003 min
Response: 1479050
Conc: 2.72 ng/ml

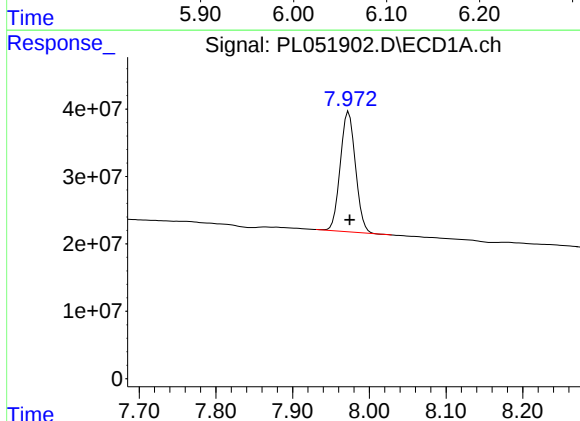

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 244939727
Conc: 20.18 ng/ml

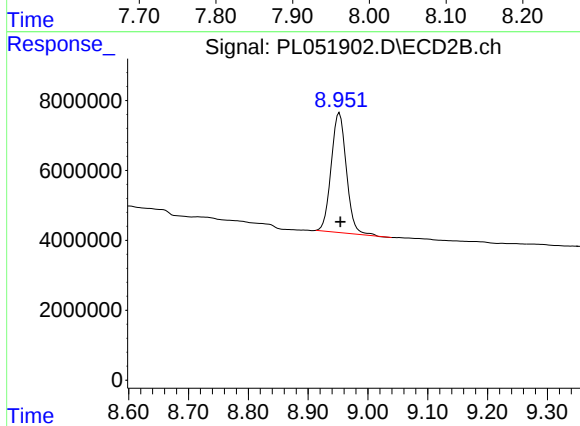

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 60361403
Conc: 19.83 ng/ml