

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 22:04
 Operator : SG\AJ
 Sample : K4567-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:04:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.925	99856194	21858038	11.667	10.005
28)	SA Decachlor...	7.972	8.952	166.0E6	39911617	13.672	13.112
Target Compounds							
4)	MA Heptachlor	0.000	5.104	0	706428	N.D.	0.201 #
6)	B beta-BHC	0.000	4.803f	0	603784	N.D.	0.414 #
9)	A Endosulfan I	0.000	6.152	0	283320	N.D.	0.088 #
10)	B gamma-Chl...	0.000	6.010	0	908650	N.D.	0.249 #
11)	B alpha-Chl...	0.000	6.101	0	619469	N.D.	0.180 #
15)	B Endosulfa...	0.000	6.843	0	539995	N.D.	0.164 #
25)	Chlordane-3	0.000	6.010	0	908650	N.D.	2.039 #
26)	Chlordane-4	0.000	6.101	0	619469	N.D.	1.141 #
27)	Chlordane-5	0.000	6.902	0	146752	N.D.	1.489 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 22:04
Operator : SG\AJ
Sample : K4567-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:04:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

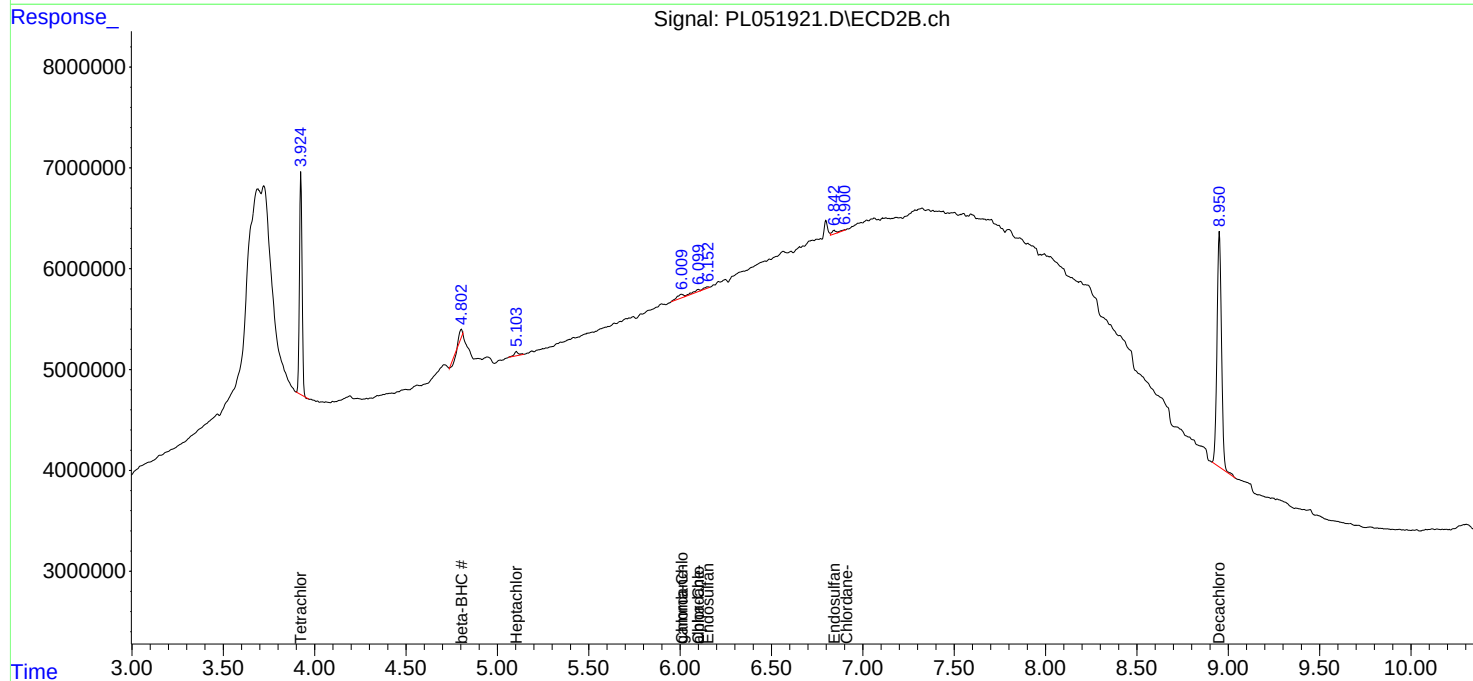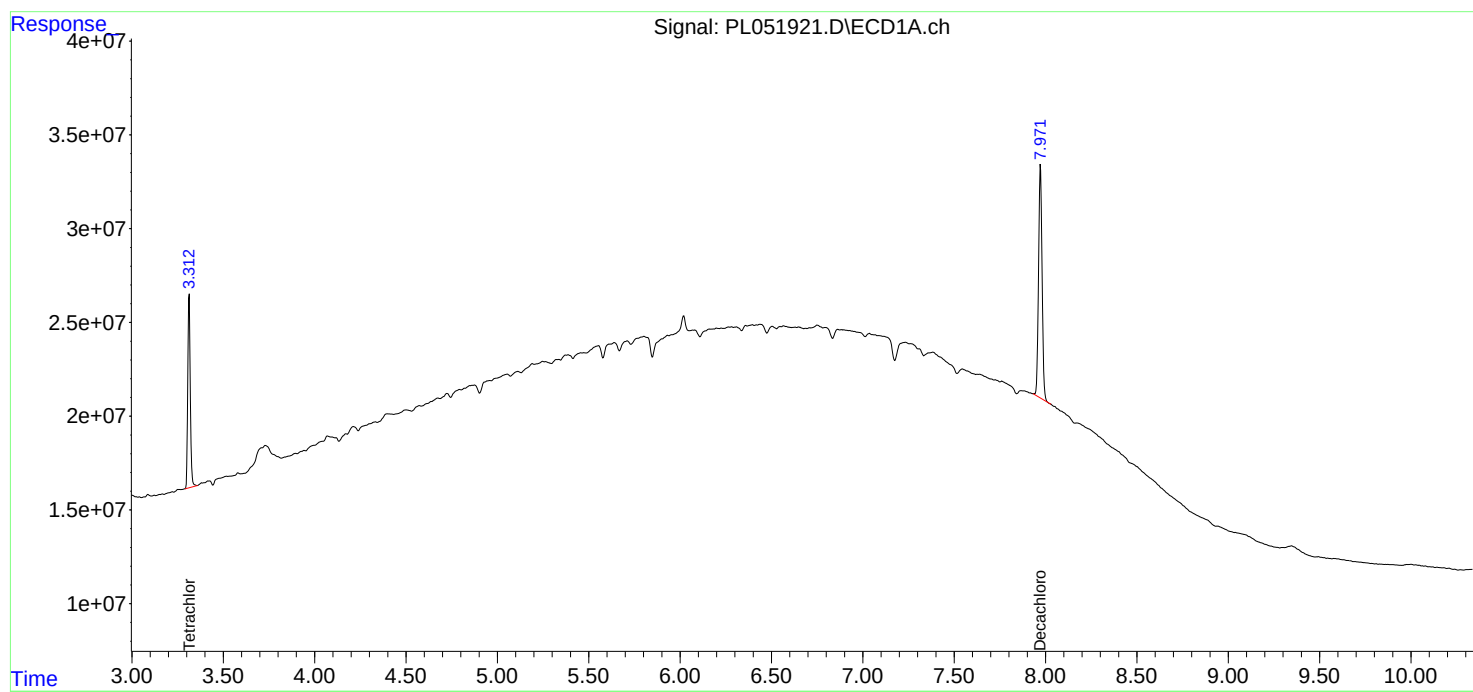


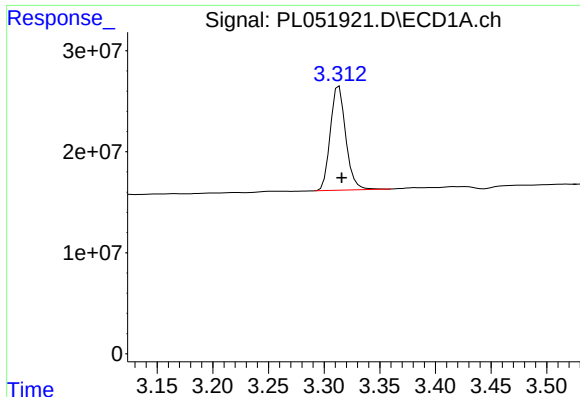

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 99856194
Conc: 11.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-D

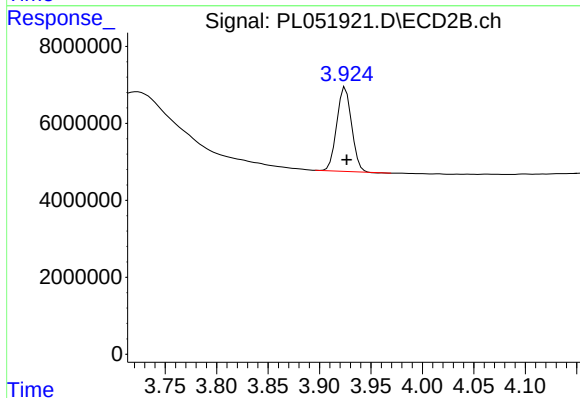


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 21858038
Conc: 10.00 ng/ml

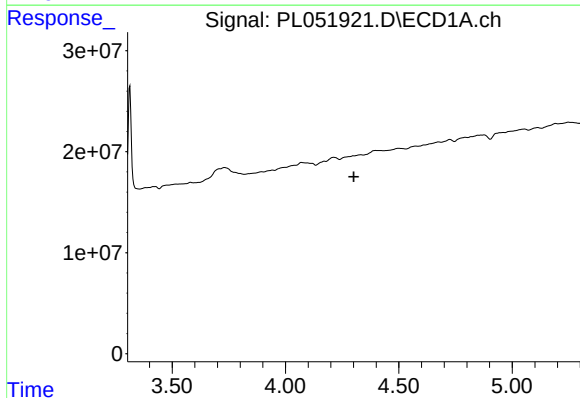


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

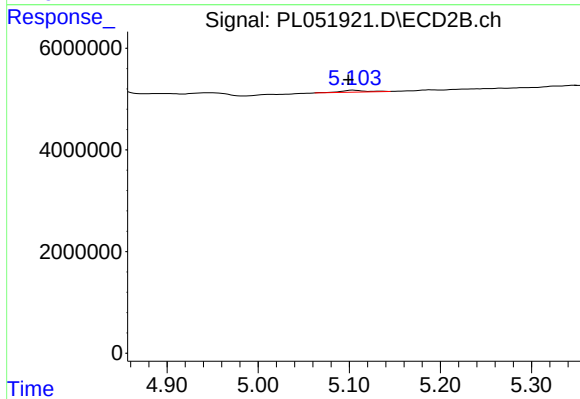

#4 Heptachlor


R.T.: 5.104 min
Delta R.T.: 0.005 min
Response: 706428
Conc: 0.20 ng/ml

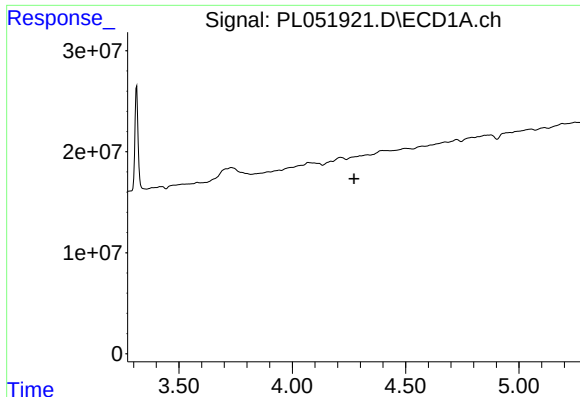

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-D

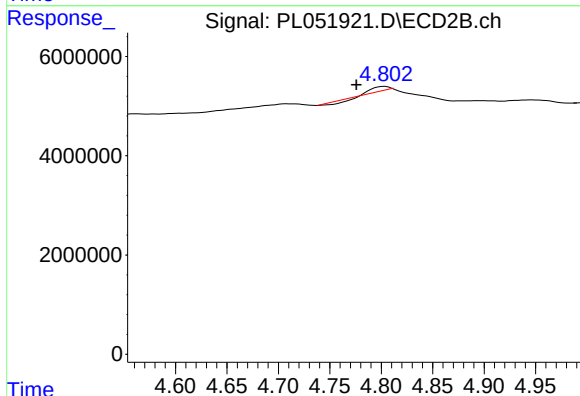


#6 beta-BHC

R.T.: 4.803 min
Delta R.T.: 0.028 min
Response: 603784
Conc: 0.41 ng/ml

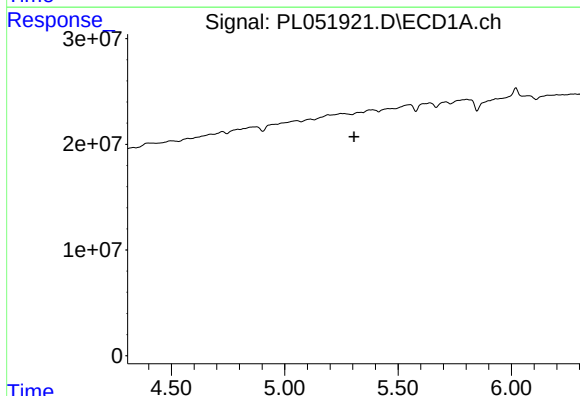


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

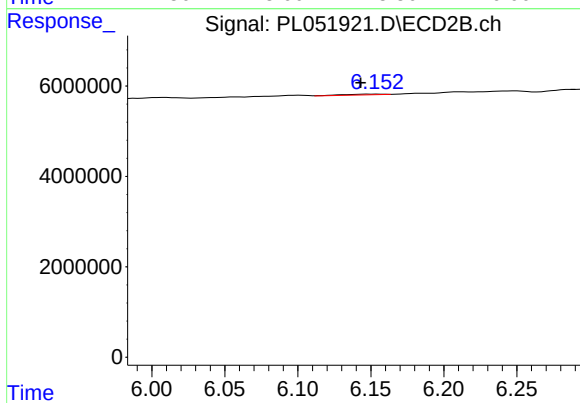

#9 Endosulfan I


R.T.: 6.152 min
Delta R.T.: 0.009 min
Response: 283320
Conc: 0.09 ng/ml

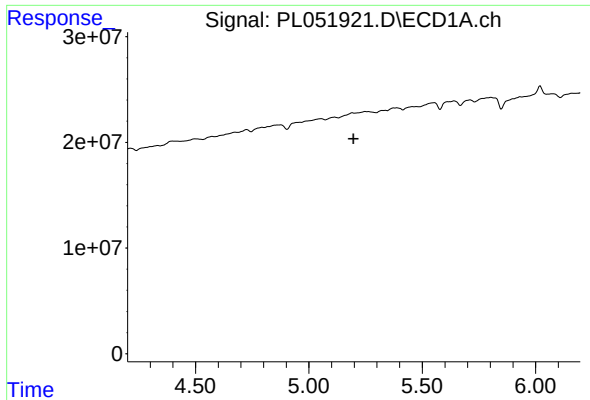

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-D

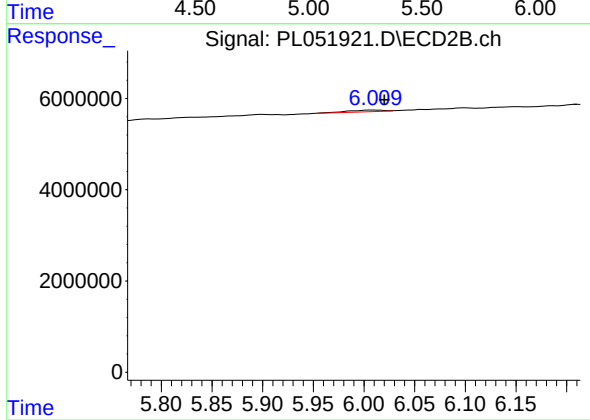


#10 gamma-Chlordane

R.T.: 6.010 min
Delta R.T.: -0.010 min
Response: 908650
Conc: 0.25 ng/ml

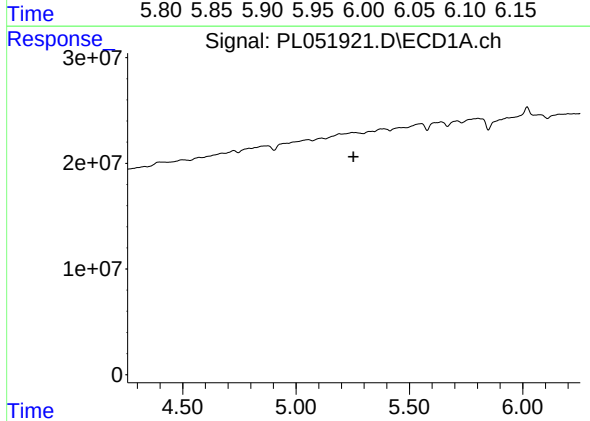


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

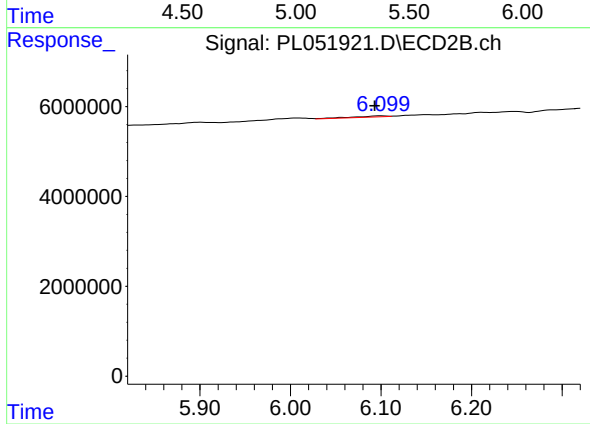

#11 alpha-Chlordane


R.T.: 6.101 min
Delta R.T.: 0.007 min
Response: 619469
Conc: 0.18 ng/ml

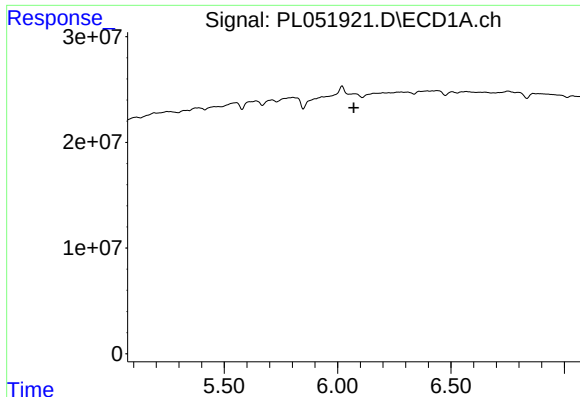

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-D

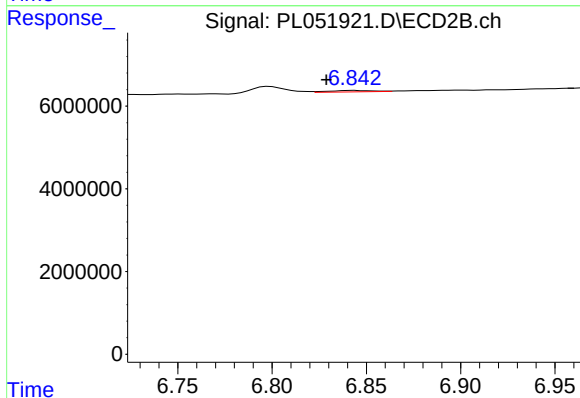


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 539995
Conc: 0.16 ng/ml

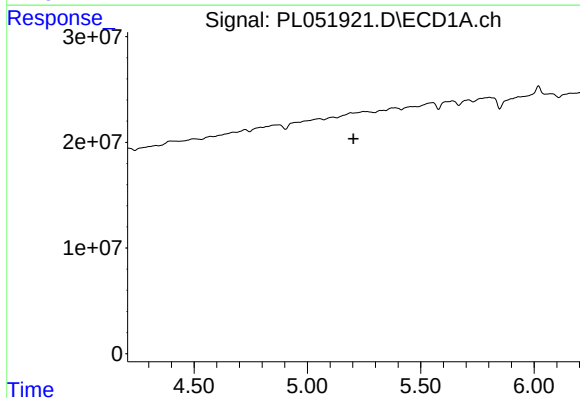


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

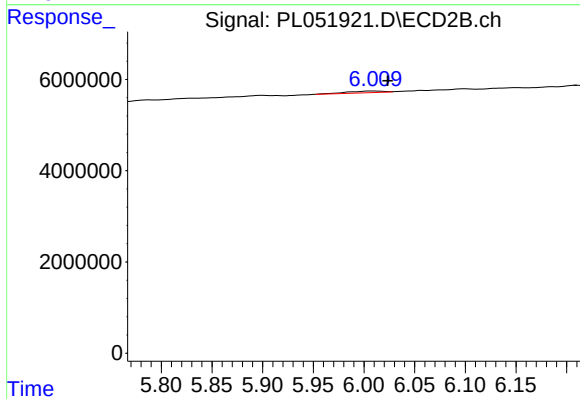

#25 Chlordane-3


R.T.: 6.010 min
Delta R.T.: -0.014 min
Response: 908650
Conc: 2.04 ng/ml

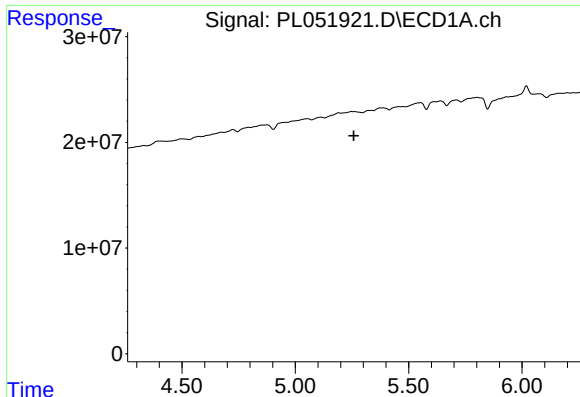

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-D

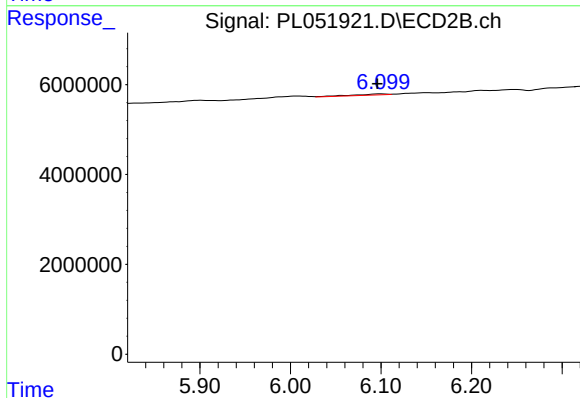


#26 Chlordane-4

R.T.: 6.101 min
Delta R.T.: 0.005 min
Response: 619469
Conc: 1.14 ng/ml

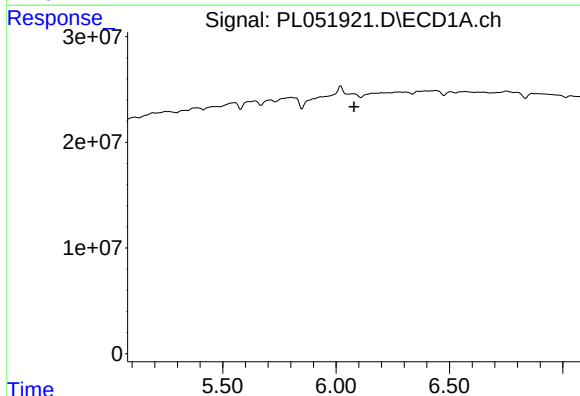


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

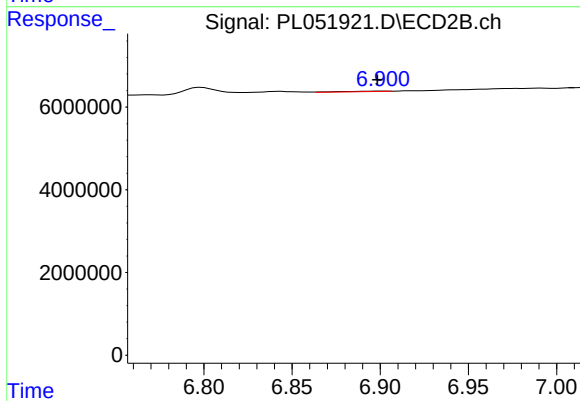

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.003 min
Response: 146752
Conc: 1.49 ng/ml

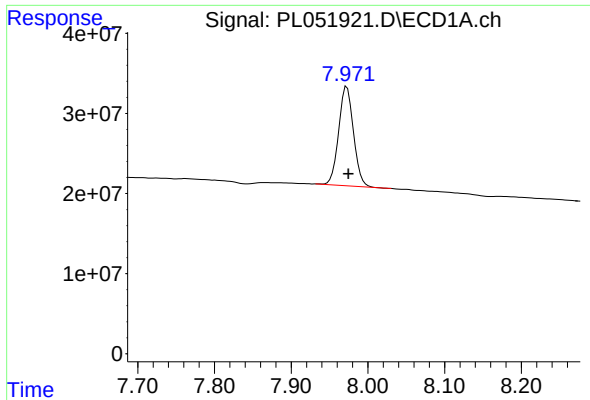

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 165952788
Conc: 13.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-D

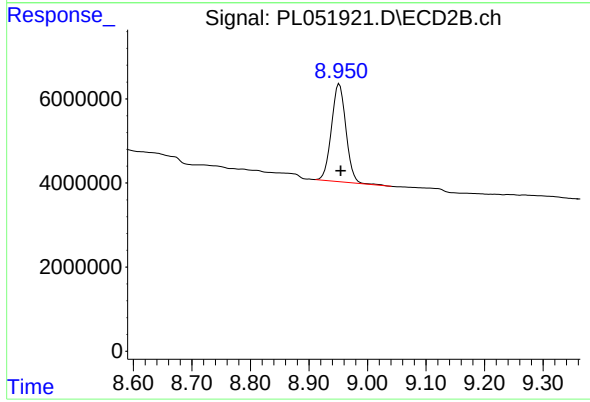

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 39911617
Conc: 13.11 ng/ml