

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 00:54
 Operator : SG\AJ
 Sample : K4527-34
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T9-12-13-O-(0-1.9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 03:31:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	192.6E6	42057315	22.504	19.250
28)	SA Decachlor...	7.973	8.951	281.1E6	67278237	23.156	22.103
Target Compounds							
3)	MA gamma-BHC...	0.000	4.573f	0	672447	N.D.	0.214 #
8)	B Heptachlo...	0.000	5.779	0	475051	N.D.	0.141 #
10)	B gamma-Chl...	0.000	6.000f	0	968807	N.D.	0.265 #
11)	B alpha-Chl...	0.000	6.105	0	367212	N.D.	0.106 #
15)	B Endosulfa...	0.000	6.844f	0	5868985	N.D.	1.781 #
18)	B Endrin al...	0.000	6.949	0	4114626	N.D.	1.456 #
25)	Chlordane-3	0.000	6.000f	0	968807	N.D.	2.174 #
26)	Chlordane-4	0.000	6.105	0	367212	N.D.	0.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 00:54
Operator : SG\AJ
Sample : K4527-34
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 03:31:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

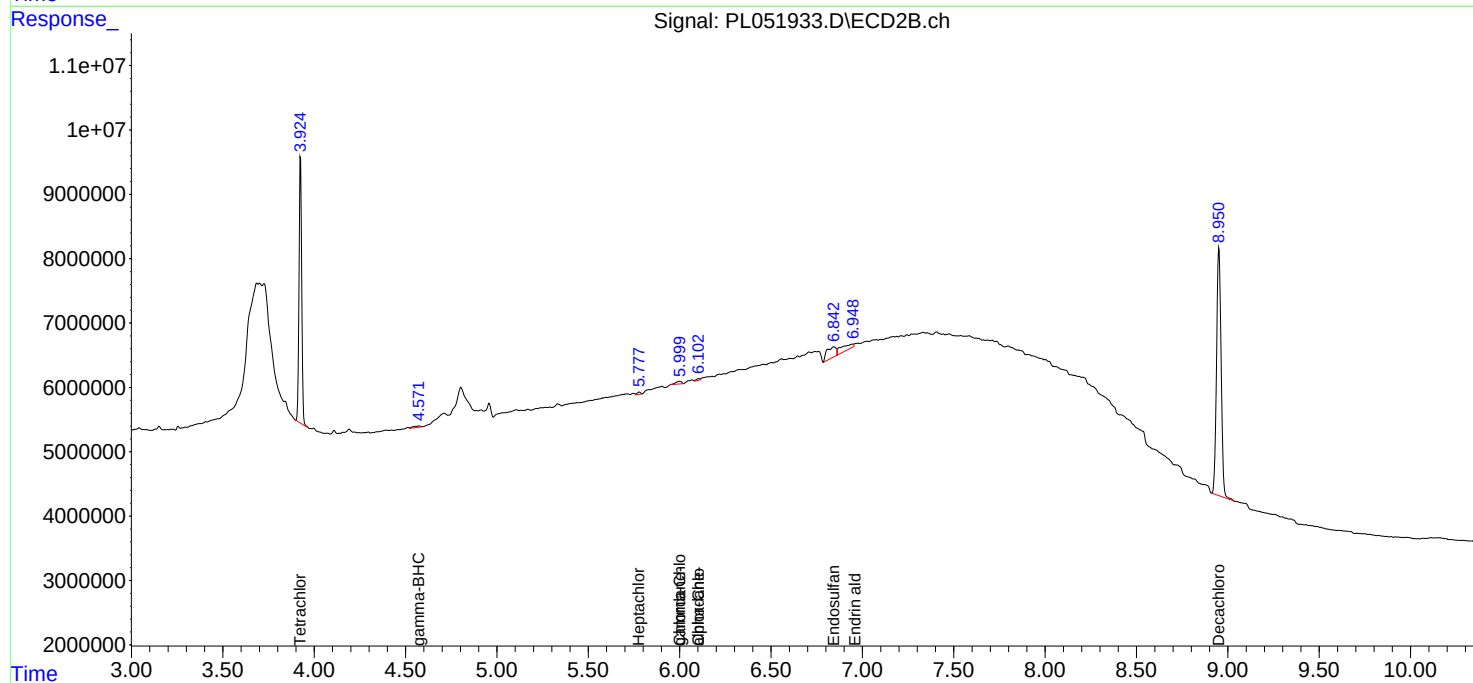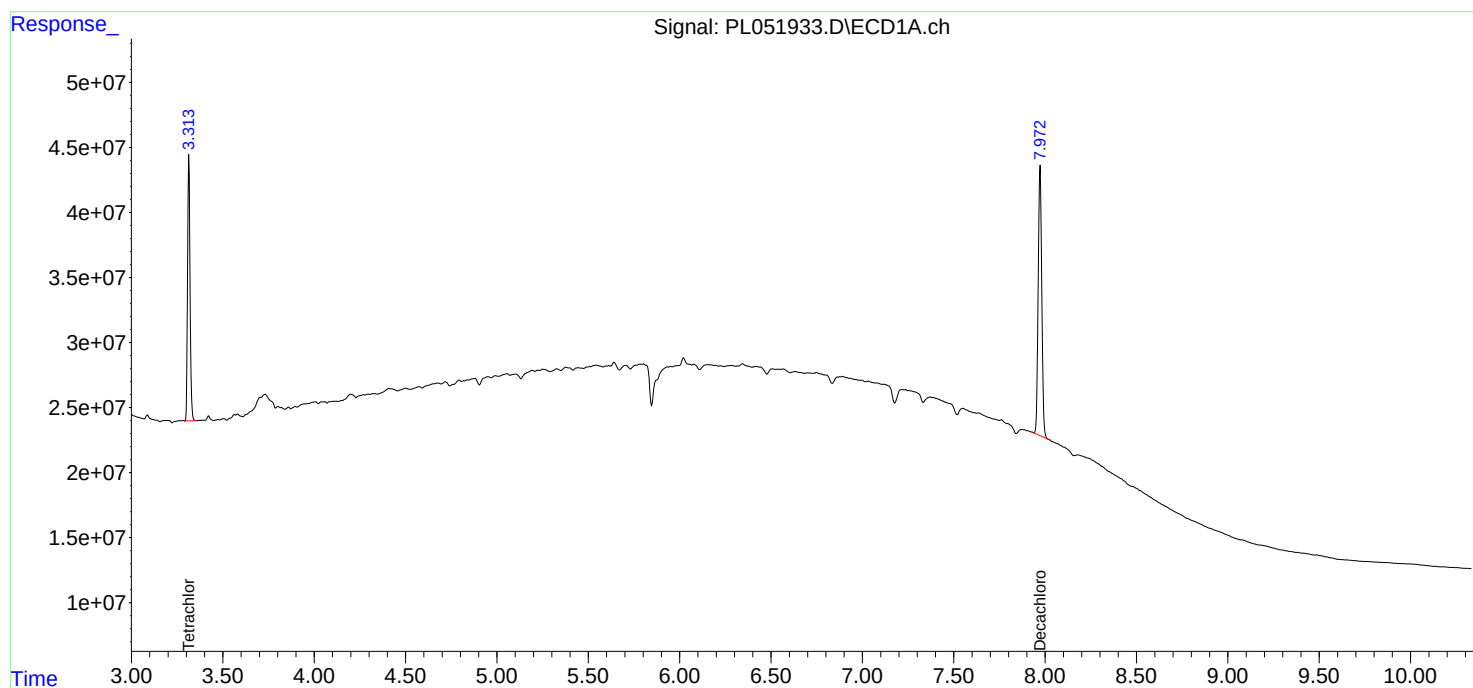


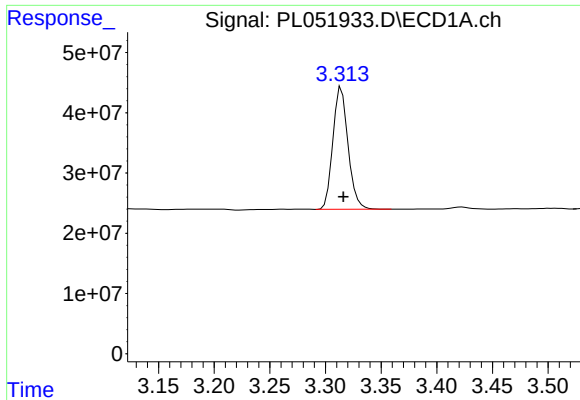

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 192600733
Conc: 22.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

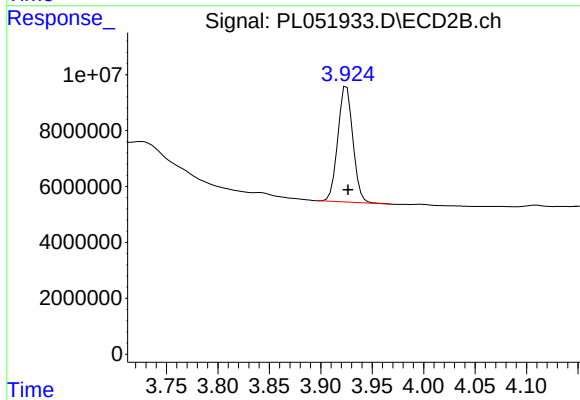


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 42057315
Conc: 19.25 ng/ml

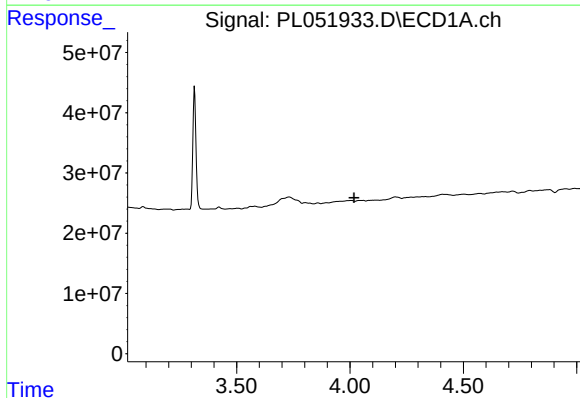


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

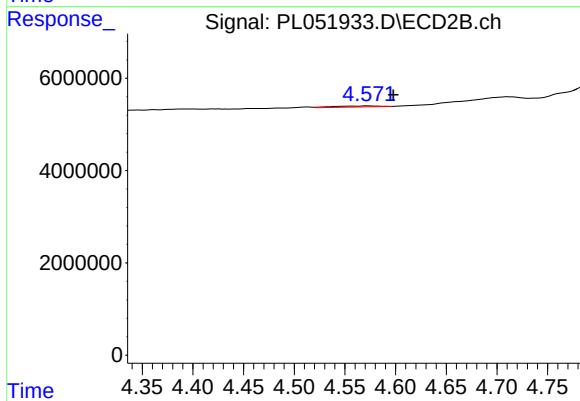

#3 gamma-BHC (Lindane)


R.T.: 4.573 min
Delta R.T.: -0.025 min
Response: 672447
Conc: 0.21 ng/ml

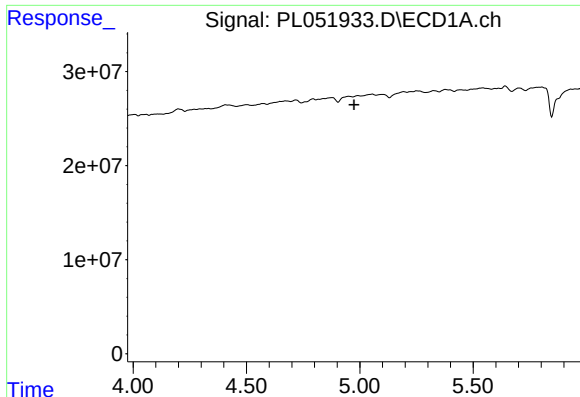

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

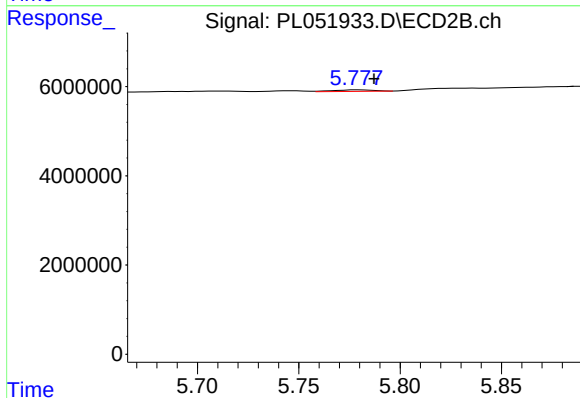


#8 Heptachlor epoxide

R.T.: 5.779 min
Delta R.T.: -0.008 min
Response: 475051
Conc: 0.14 ng/ml

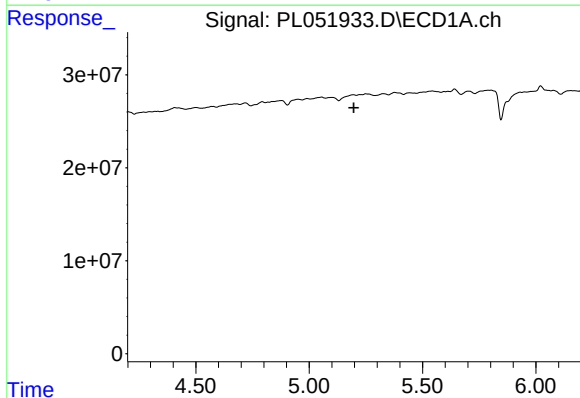


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

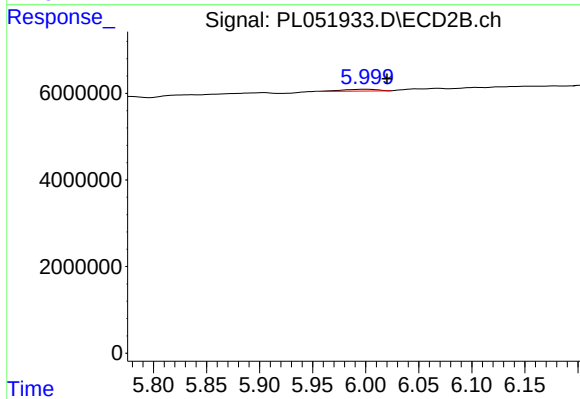

#10 gamma-Chlordane


R.T.: 6.000 min
Delta R.T.: -0.020 min
Response: 968807
Conc: 0.27 ng/ml

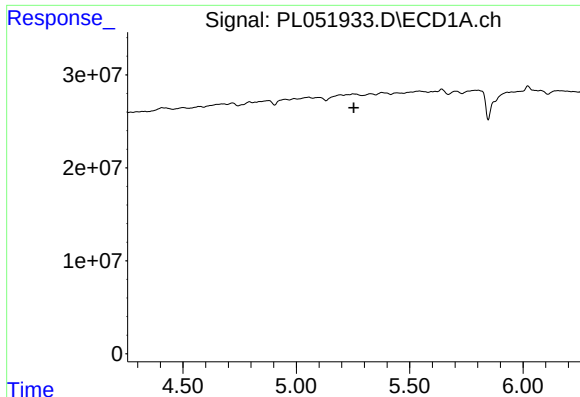

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

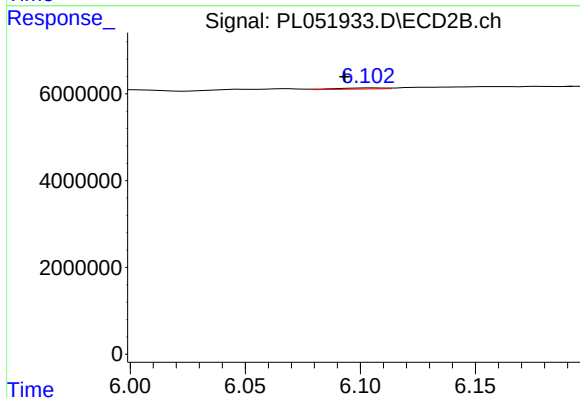


#11 alpha-Chlordane

R.T.: 6.105 min
Delta R.T.: 0.012 min
Response: 367212
Conc: 0.11 ng/ml

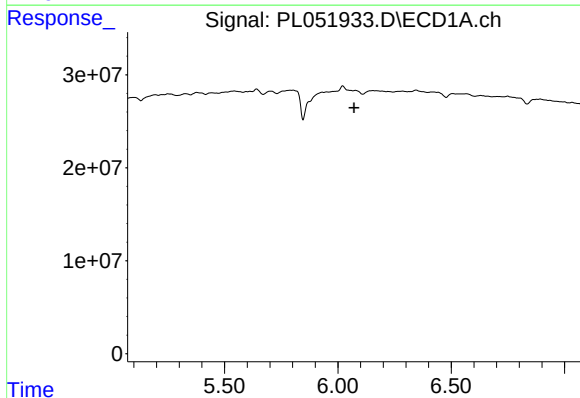


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

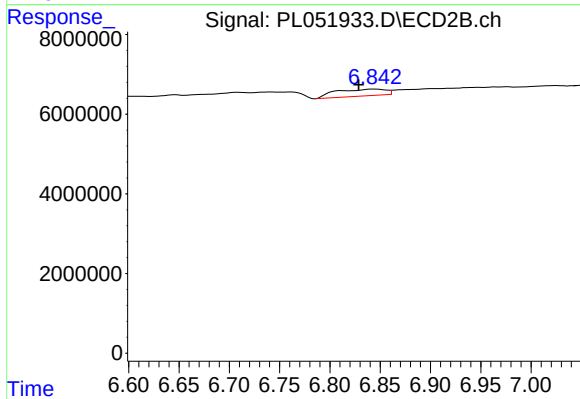

#15 Endosulfan II


R.T.: 6.844 min
Delta R.T.: 0.015 min
Response: 5868985
Conc: 1.78 ng/ml

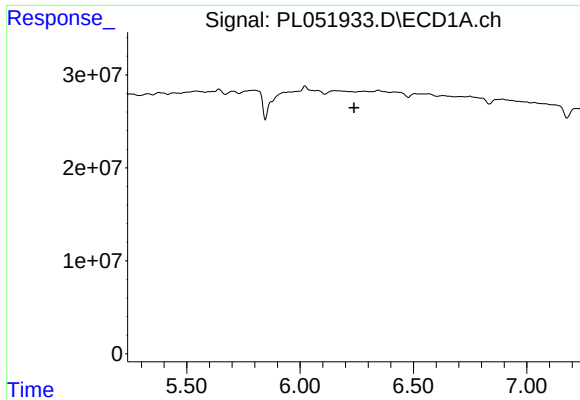

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

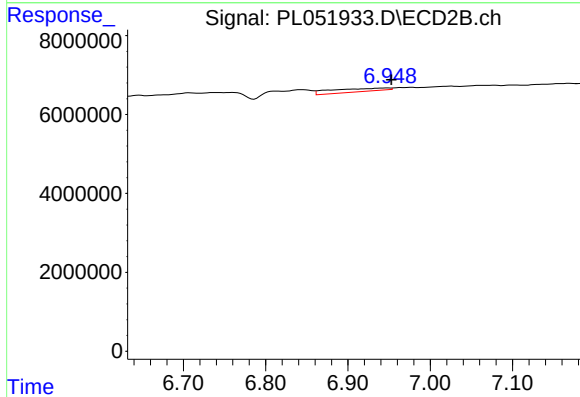


#18 Endrin aldehyde

R.T.: 6.949 min
Delta R.T.: -0.004 min
Response: 4114626
Conc: 1.46 ng/ml

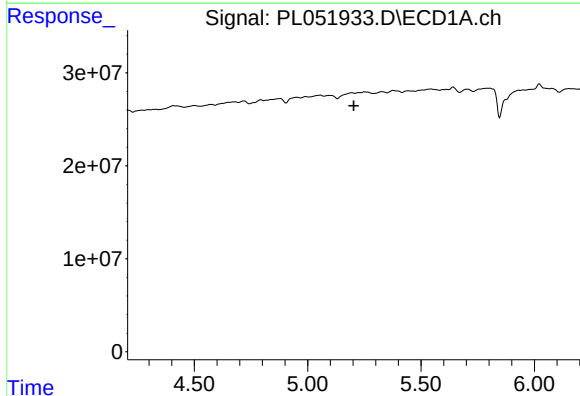


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

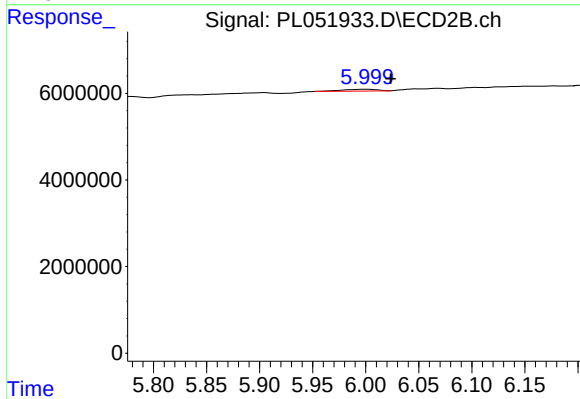

#25 Chlordane-3


R.T.: 6.000 min
Delta R.T.: -0.023 min
Response: 968807
Conc: 2.17 ng/ml

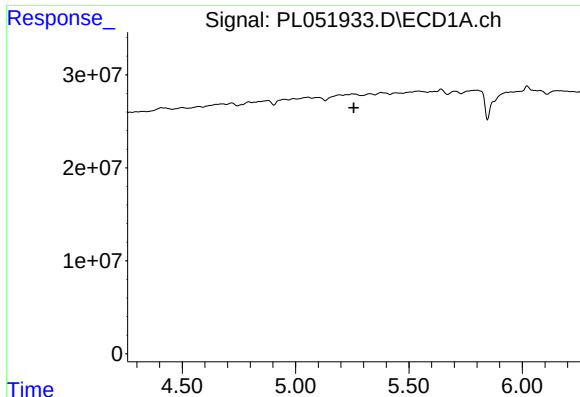

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T9-12-13-O-(0-1.9)

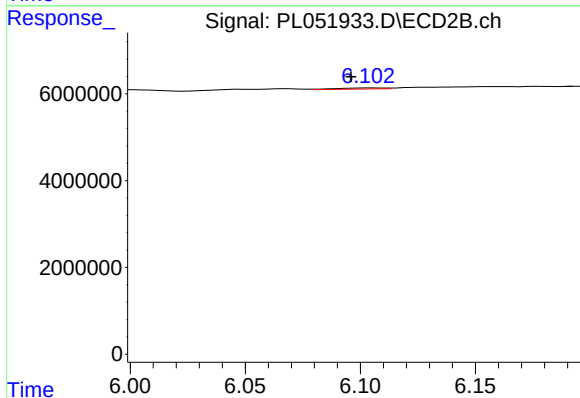


#26 Chlorodane-4

R.T.: 6.105 min
Delta R.T.: 0.009 min
Response: 367212
Conc: 0.68 ng/ml

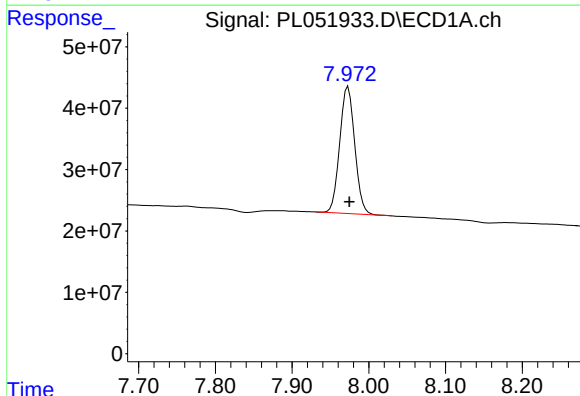

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 281061501
Conc: 23.16 ng/ml

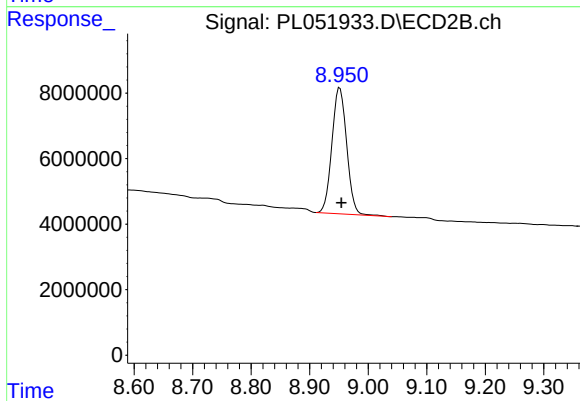

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 67278237
Conc: 22.10 ng/ml