

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 01:22
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 03:32:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	186.2E6	39961698	21.752	18.291
28)	SA Decachlor...	7.973	8.952	278.0E6	63570833	22.904	20.885
Target Compounds							
5)	MB Aldrin	4.564f	0.000	44724018	0	3.095	N.D. #
6)	B beta-BHC	0.000	4.803f	0	291420	N.D.	0.200 #
8)	B Heptachlo...	0.000	5.785	0	7610230	N.D.	2.255 #
9)	A Endosulfan I	5.325f	6.160f	16628851	440467	1.237	0.136 #
10)	B gamma-Chl...	0.000	6.016	0	864118	N.D.	0.237 #
11)	B alpha-Chl...	0.000	6.105	0	333571	N.D.	0.097 #
13)	MA Dieldrin	5.537	6.410	1599217	1624256	0.105	0.474 #
15)	B Endosulfa...	0.000	6.845f	0	619794	N.D.	0.188 #
18)	B Endrin al...	0.000	6.979f	0	1722970	N.D.	0.610 #
25)	Chlordane-3	0.000	6.016	0	864118	N.D.	1.939 #
26)	Chlordane-4	0.000	6.105	0	333571	N.D.	0.614 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 01:22
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 03:32:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

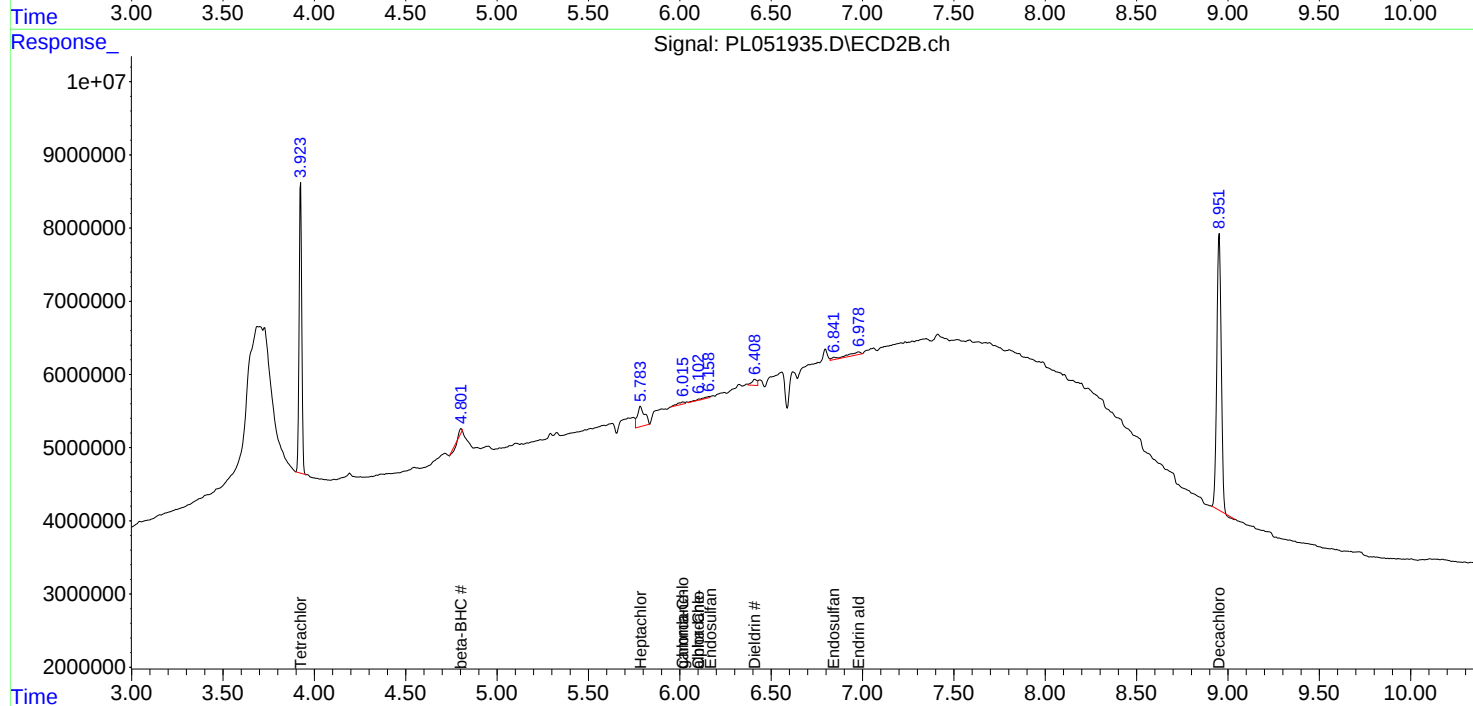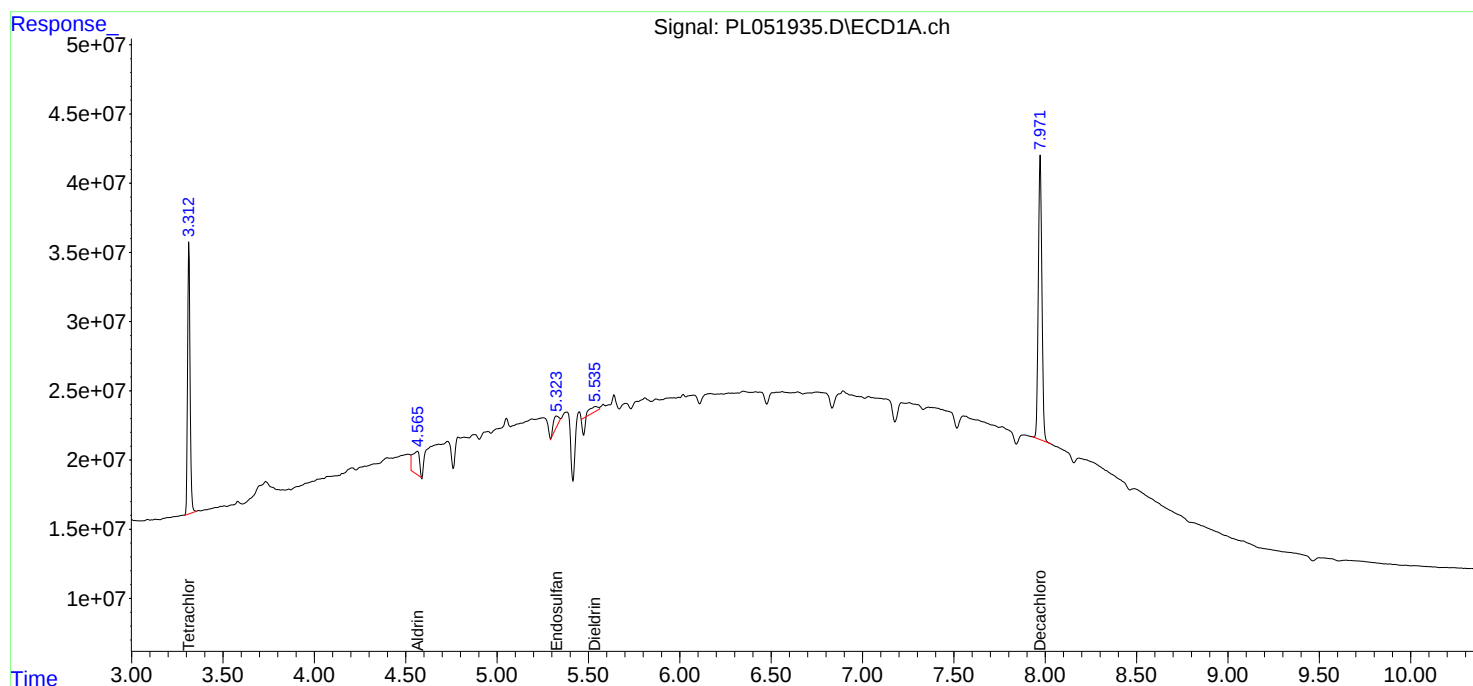


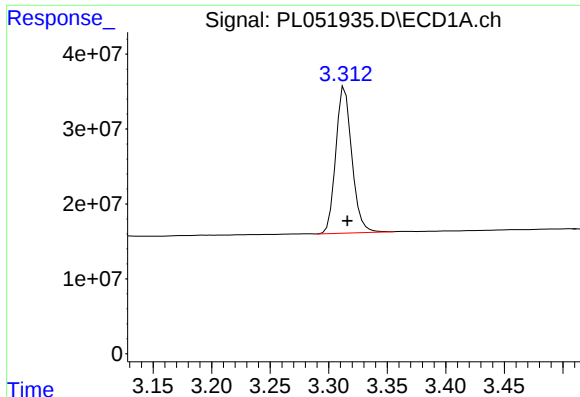

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 186165742
Conc: 21.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

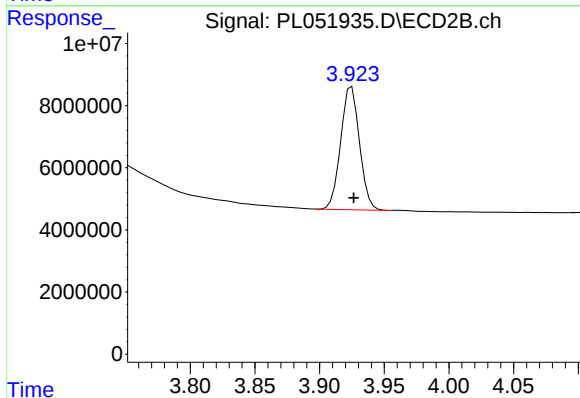


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 39961698
Conc: 18.29 ng/ml

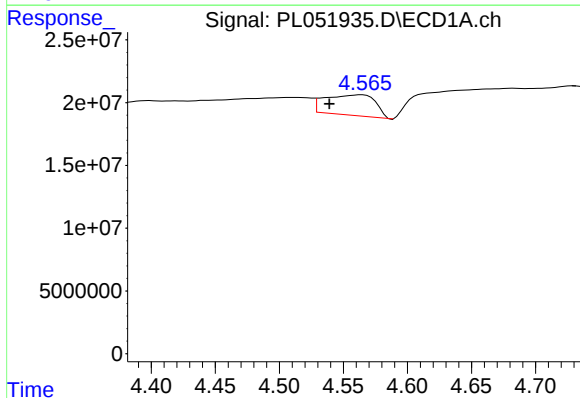


#5 Aldrin

R.T.: 4.564 min
Delta R.T.: 0.025 min
Response: 44724018
Conc: 3.09 ng/ml

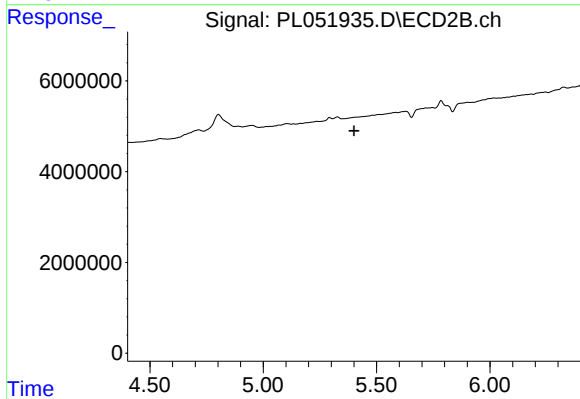

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

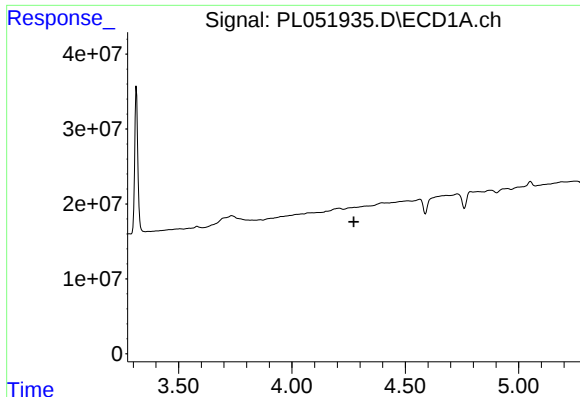

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

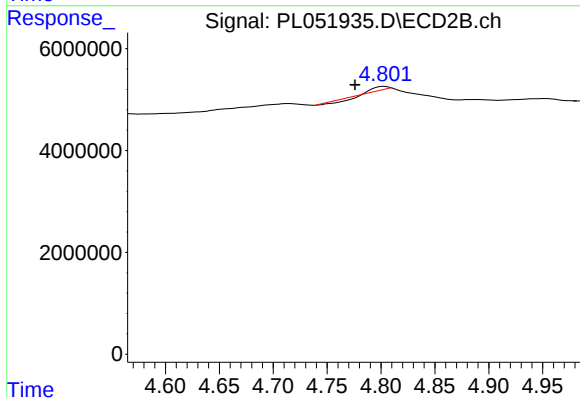


#6 beta-BHC

R.T.: 4.803 min
Delta R.T.: 0.027 min
Response: 291420
Conc: 0.20 ng/ml

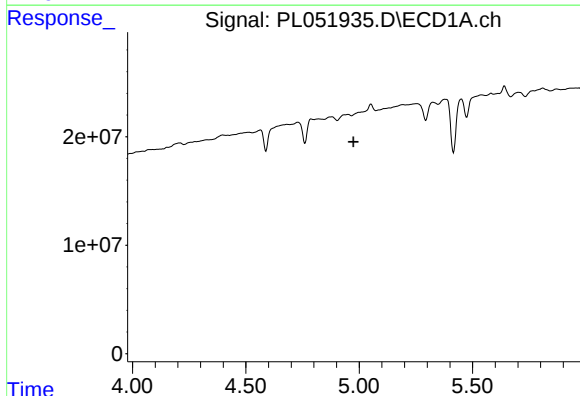


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

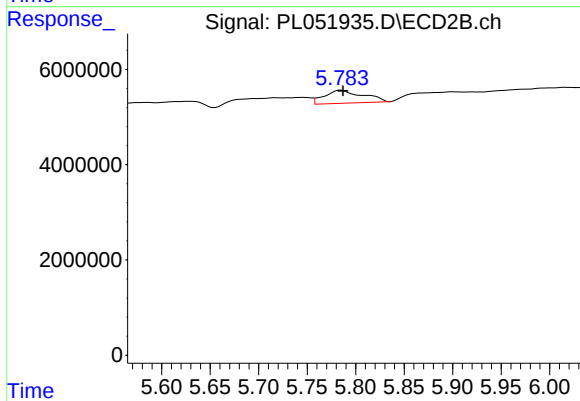

#8 Heptachlor epoxide


R.T.: 5.785 min
Delta R.T.: -0.002 min
Response: 7610230
Conc: 2.26 ng/ml

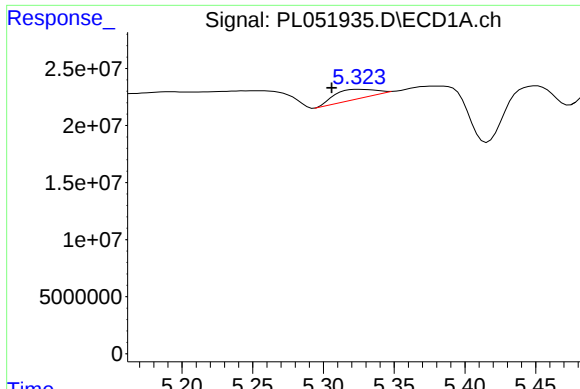

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.019 min
Response: 16628851
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

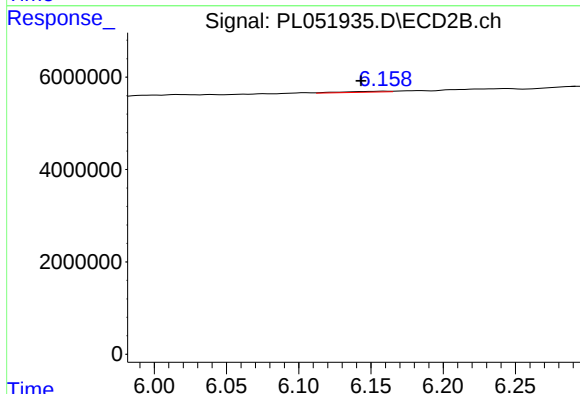


#9 Endosulfan I

R.T.: 6.160 min
Delta R.T.: 0.017 min
Response: 440467
Conc: 0.14 ng/ml

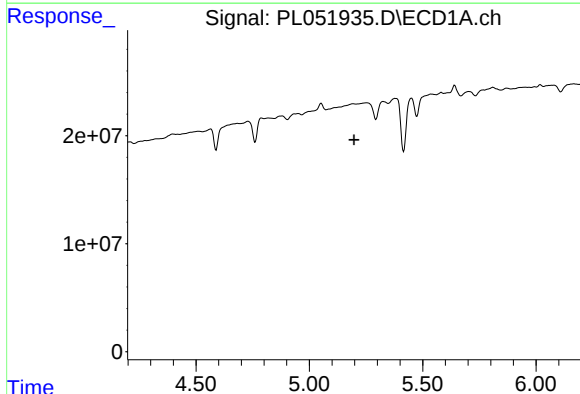


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

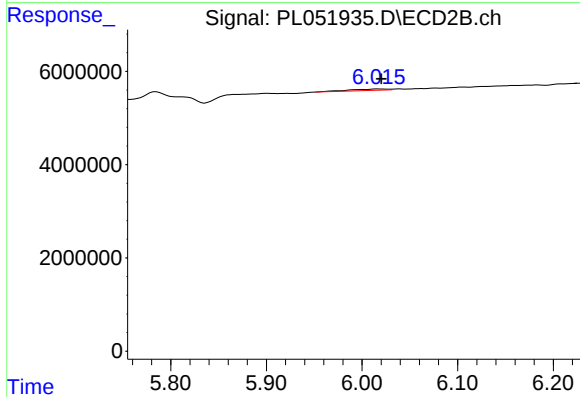

#10 gamma-Chlordane


R.T.: 6.016 min
Delta R.T.: -0.004 min
Response: 864118
Conc: 0.24 ng/ml

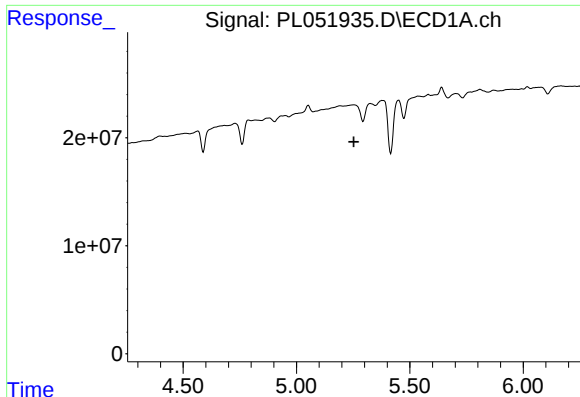

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

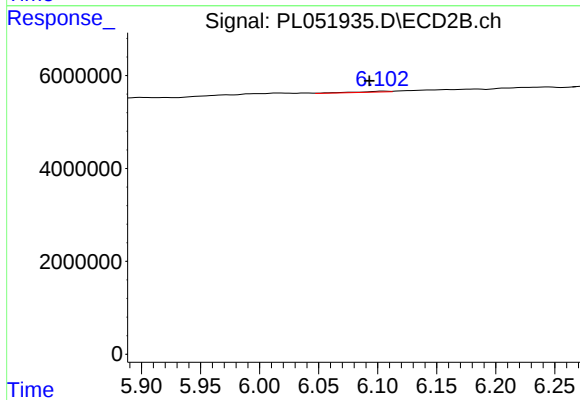


#11 alpha-Chlordane

R.T.: 6.105 min
Delta R.T.: 0.012 min
Response: 333571
Conc: 0.10 ng/ml

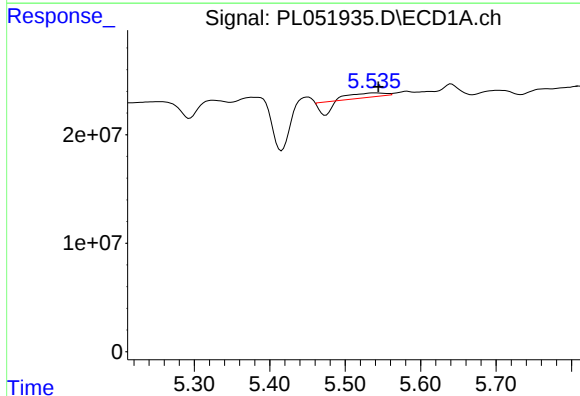


#13 Dieldrin

R.T.: 5.537 min
Delta R.T.: -0.007 min
Response: 1599217
Conc: 0.11 ng/ml

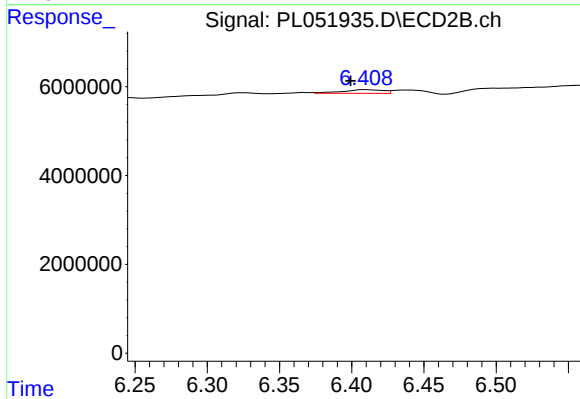

#13 Dieldrin


R.T.: 6.410 min
Delta R.T.: 0.010 min
Response: 1624256
Conc: 0.47 ng/ml

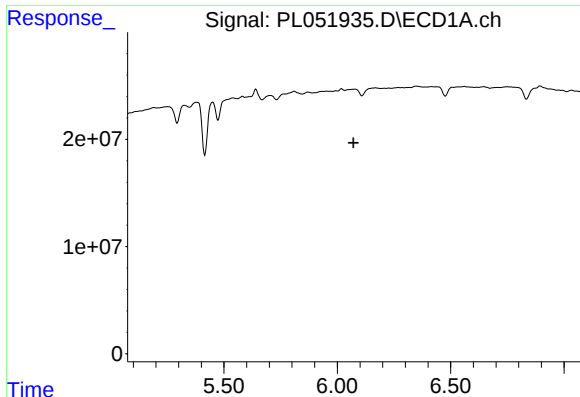

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

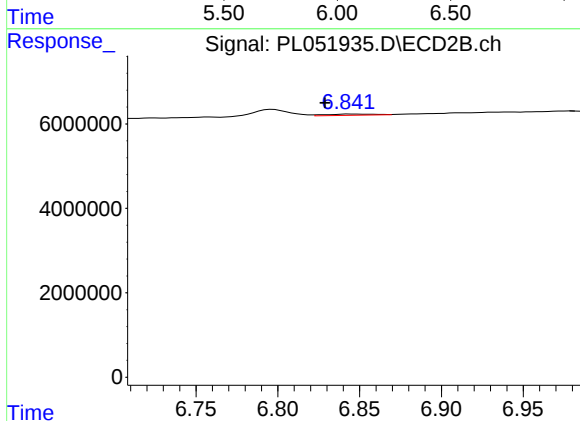


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.016 min
Response: 619794
Conc: 0.19 ng/ml

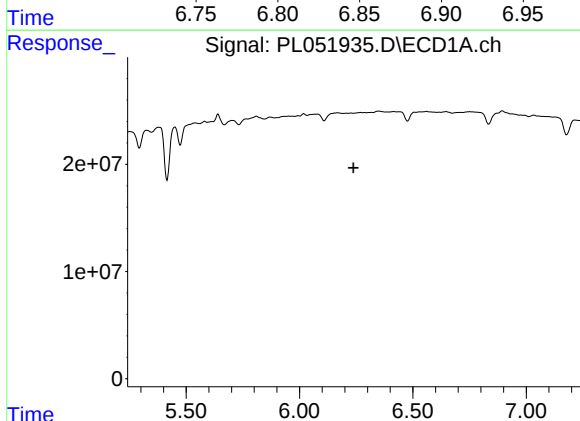


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

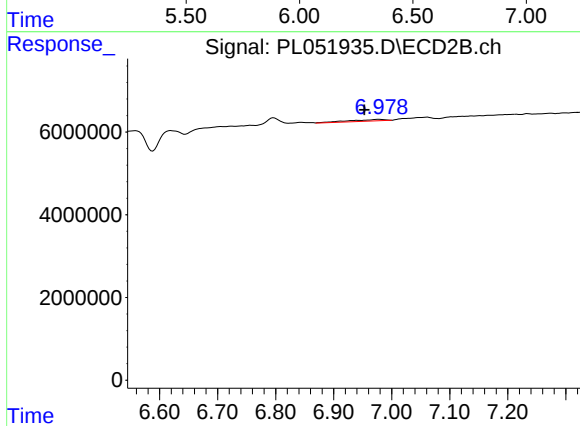

#18 Endrin aldehyde


R.T.: 6.979 min
Delta R.T.: 0.026 min
Response: 1722970
Conc: 0.61 ng/ml

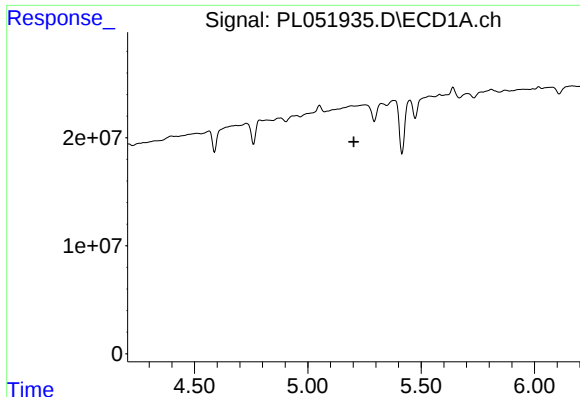

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

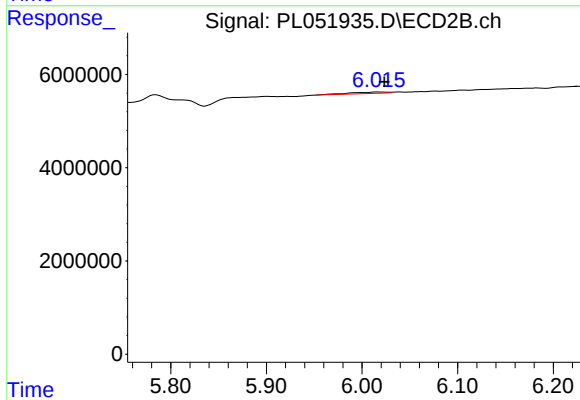


#25 Chlordane-3

R.T.: 6.016 min
Delta R.T.: -0.007 min
Response: 864118
Conc: 1.94 ng/ml

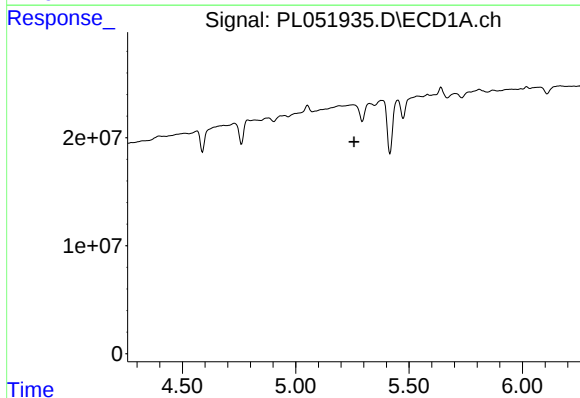


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

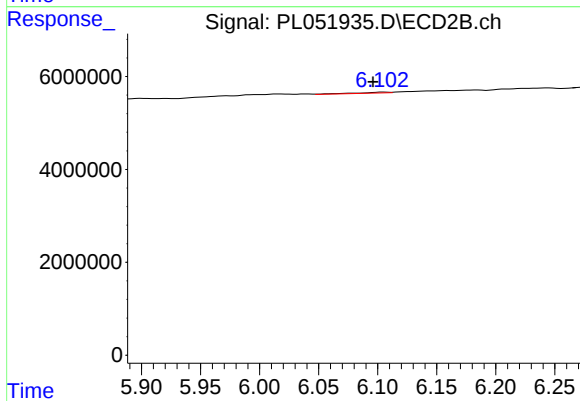

#26 Chlordane-4


R.T.: 6.105 min
Delta R.T.: 0.009 min
Response: 333571
Conc: 0.61 ng/ml

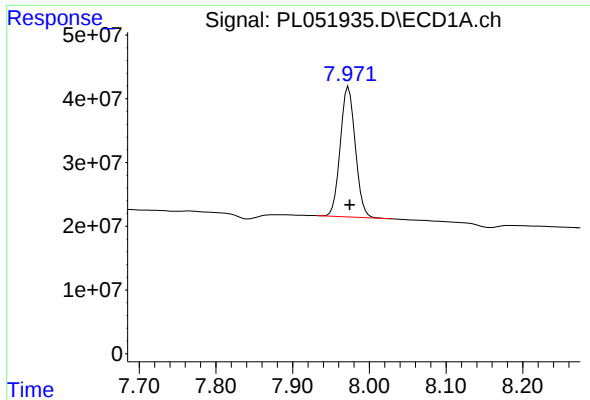

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 278009380
Conc: 22.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

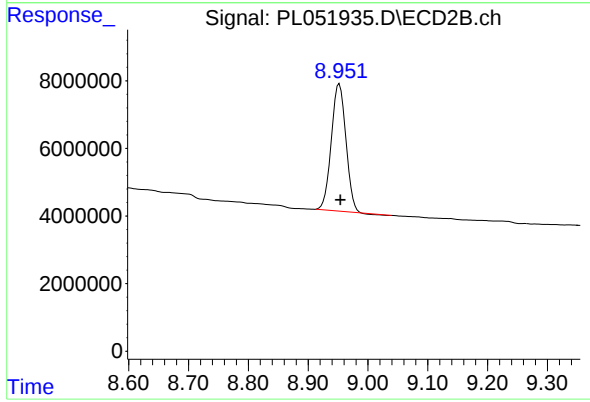

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 63570833
Conc: 20.88 ng/ml