

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 03:30
 Operator : SG\AJ
 Sample : K4548-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T8-S-G1-G4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 04:16:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	166.8E6	36811150	19.488	16.849
28)	SA Decachlor...	7.973	8.952	245.7E6	59541035	20.243	19.561
Target Compounds							
8)	B Heptachlo...	4.994f	0.000	3046301	0	0.218	N.D. #
9)	A Endosulfan I	0.000	6.145	0	262525	N.D.	0.081 #
15)	B Endosulfa...	0.000	6.845f	0	6332089	N.D.	1.921 #
17)	MA 4,4'-DDT	6.162	0.000	16870586	0	1.323	N.D. #
18)	B Endrin al...	0.000	6.934f	0	1222982	N.D.	0.433 #
24)	Chlordane-2	4.673f	0.000	26047843	0	63.731	N.D. #
27)	Chlordane-5	0.000	6.908	0	826440	N.D.	8.383 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 03:30
Operator : SG\AJ
Sample : K4548-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 04:16:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

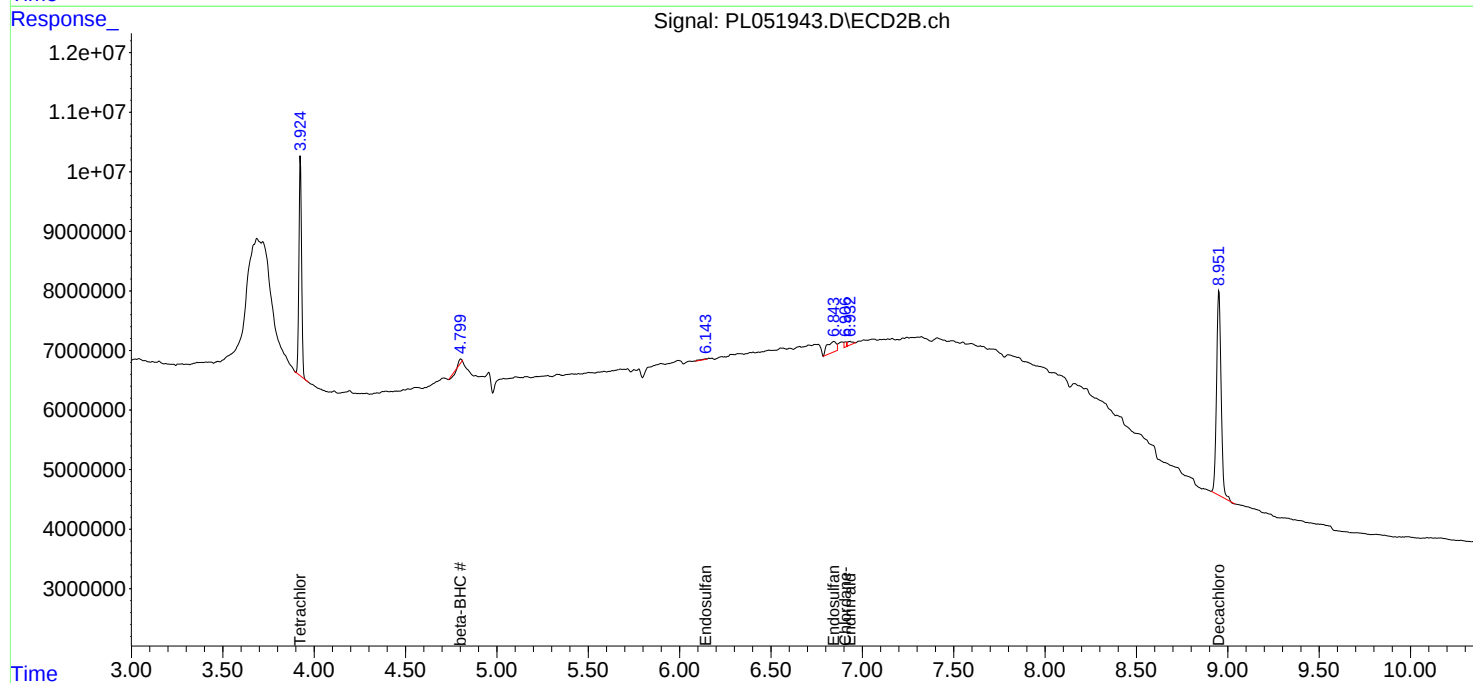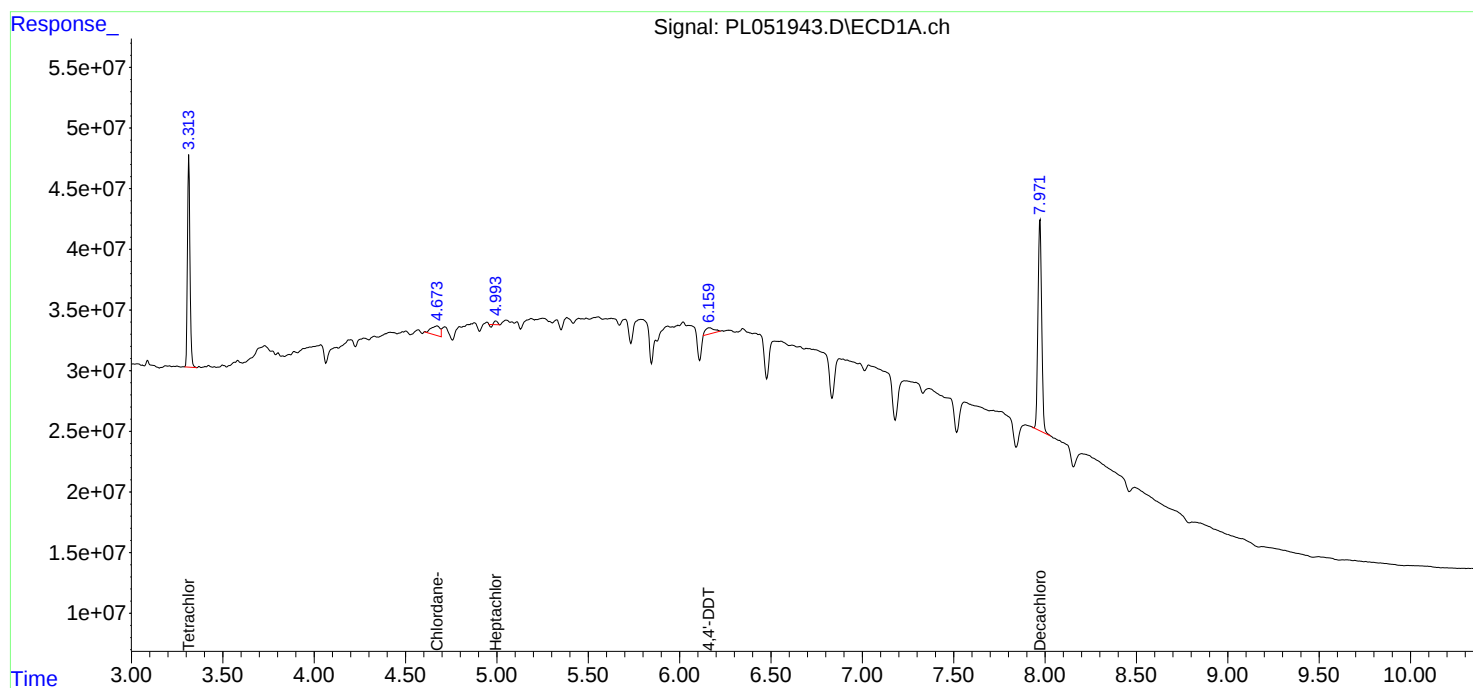


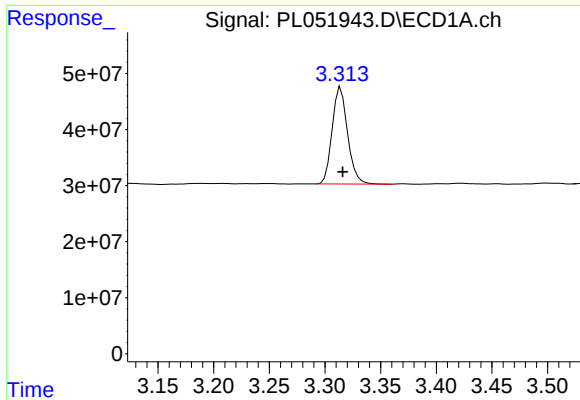

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 166787245
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

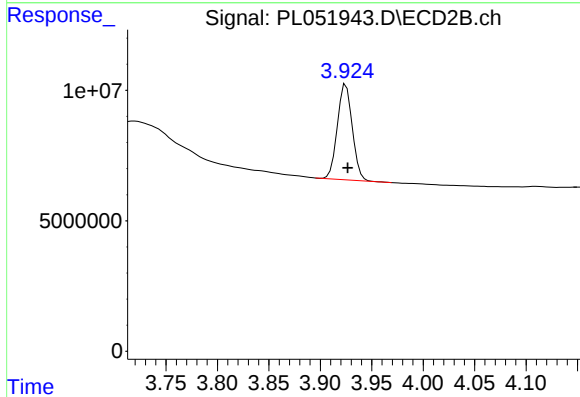


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 36811150
Conc: 16.85 ng/ml

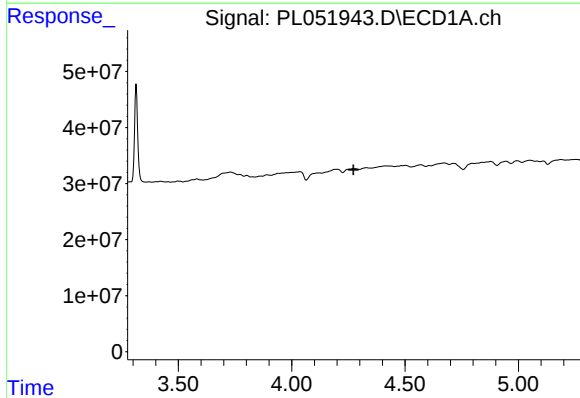


#6 beta-BHC

R.T.: 4.272 min
Delta R.T.: -0.001 min
Response: -1594611
Conc: N.D.

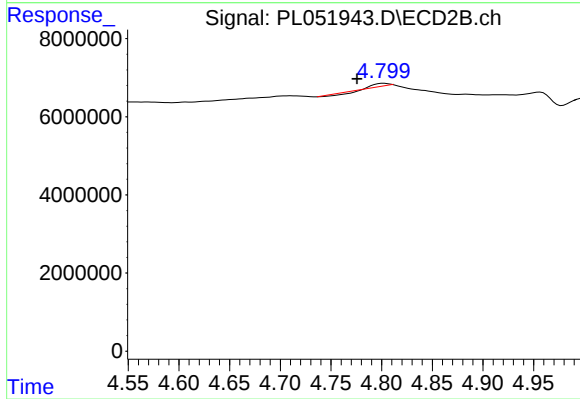

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 255953
Conc: 0.18 ng/ml

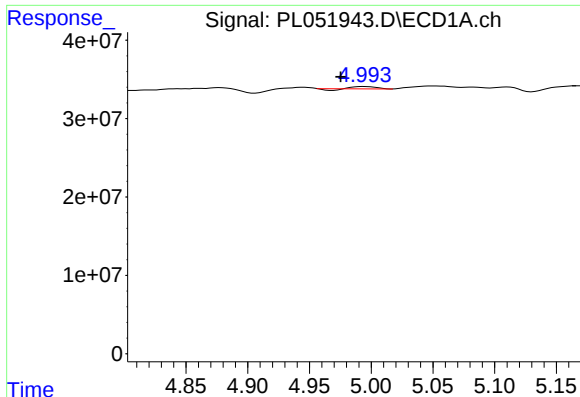

#8 Heptachlor epoxide


R.T.: 4.994 min
Delta R.T.: 0.018 min
Response: 3046301
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

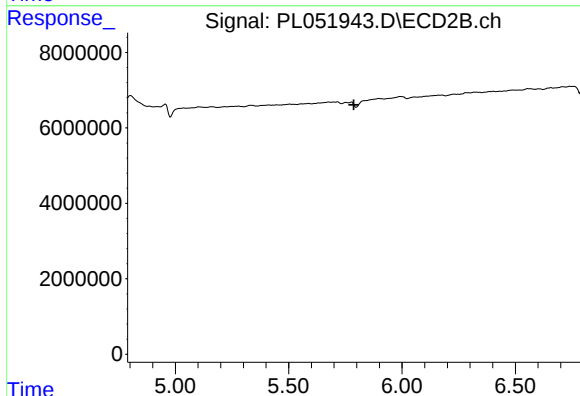


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

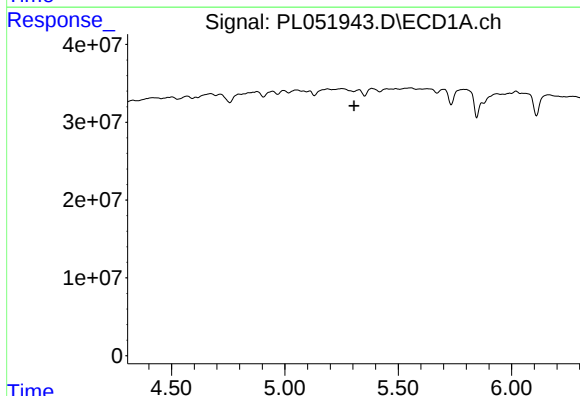


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

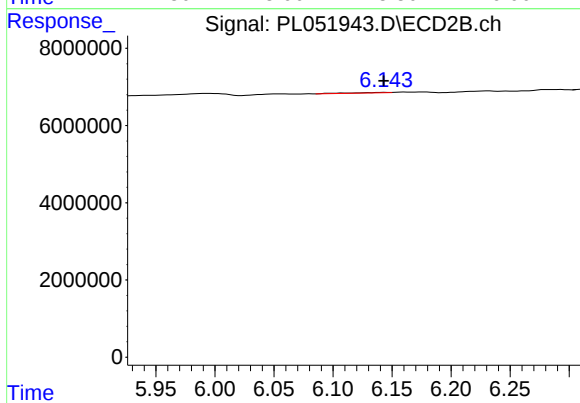

#9 Endosulfan I


R.T.: 6.145 min
Delta R.T.: 0.002 min
Response: 262525
Conc: 0.08 ng/ml

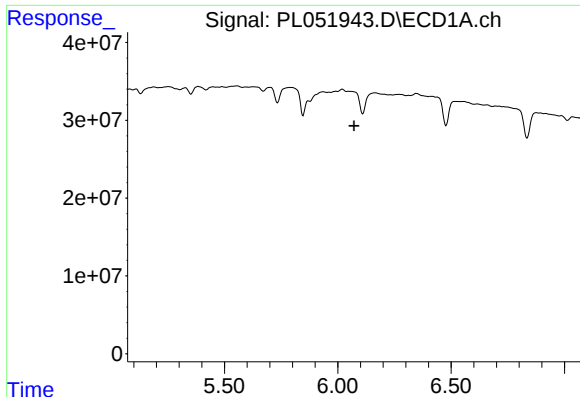

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

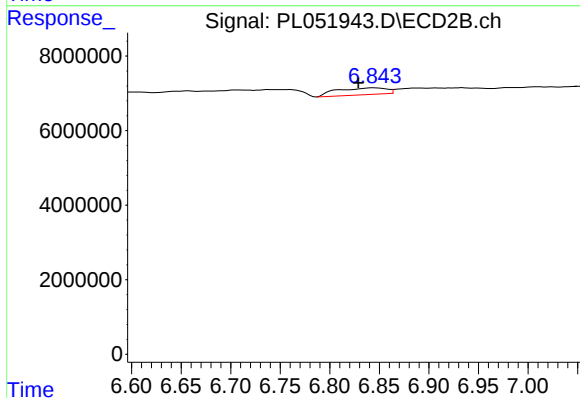


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.016 min
Response: 6332089
Conc: 1.92 ng/ml

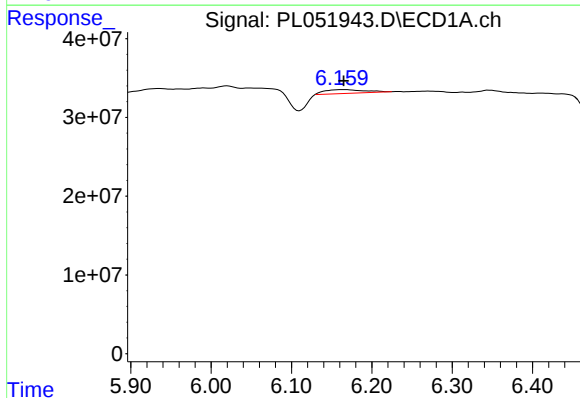


#17 4,4'-DDT

R.T.: 6.162 min
Delta R.T.: -0.003 min
Response: 16870586
Conc: 1.32 ng/ml

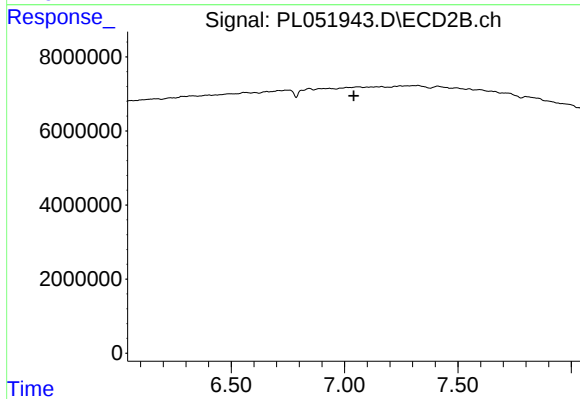

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

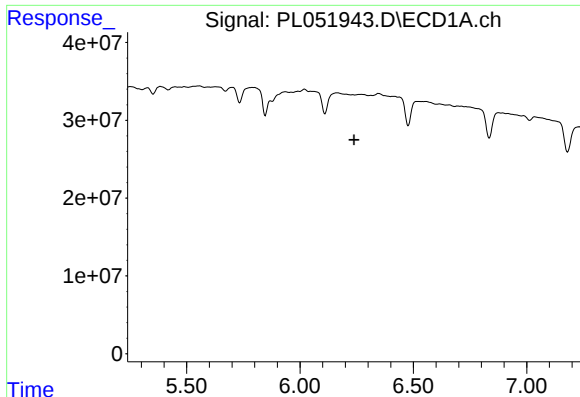

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

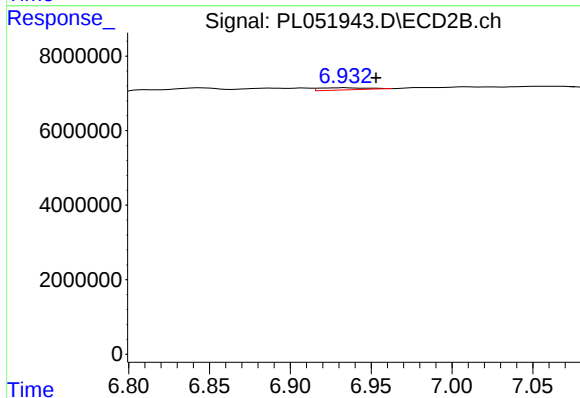


#18 Endrin aldehyde

R.T.: 6.934 min
Delta R.T.: -0.019 min
Response: 1222982
Conc: 0.43 ng/ml

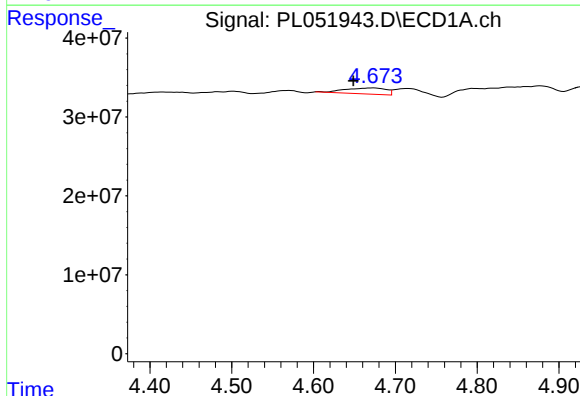


#24 Chlordane-2

R.T.: 4.673 min
Delta R.T.: 0.025 min
Response: 26047843
Conc: 63.73 ng/ml

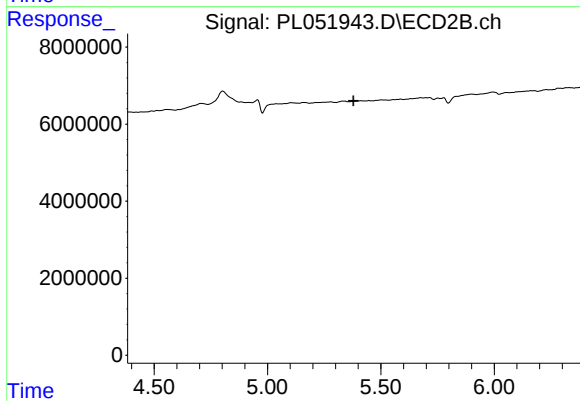

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

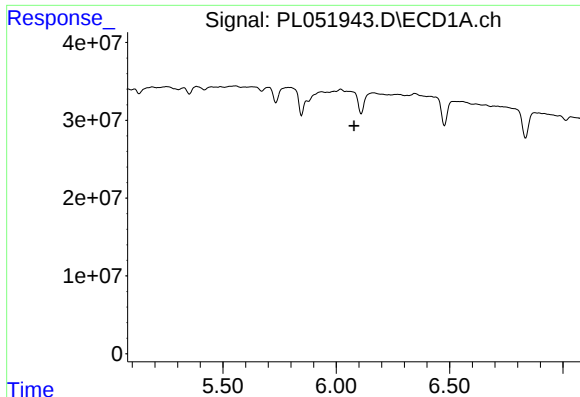

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T8-S-G1-G4

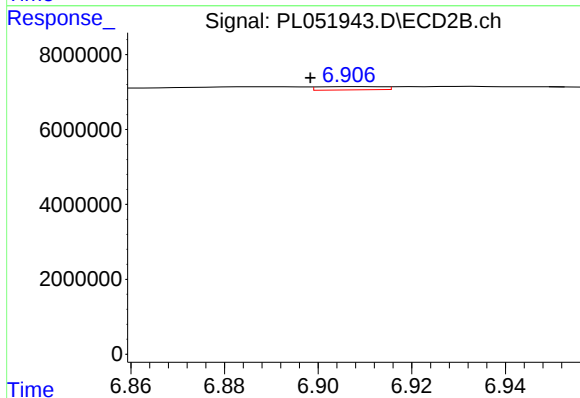


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.010 min
Response: 826440
Conc: 8.38 ng/ml

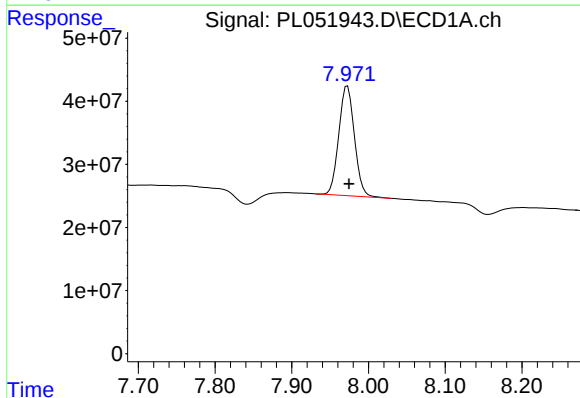

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 245710297
Conc: 20.24 ng/ml

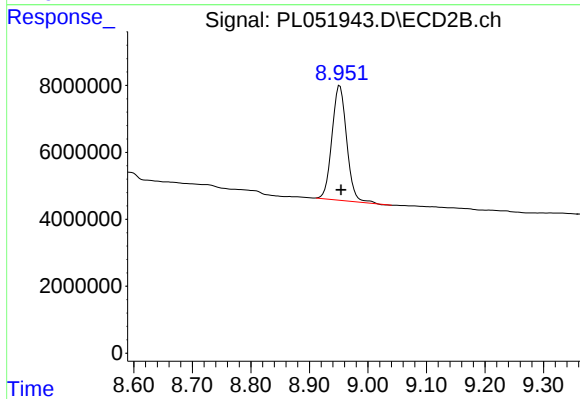

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 59541035
Conc: 19.56 ng/ml