

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 21:49
 Operator : SG\AJ
 Sample : K4567-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:03:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.314	3.925	173.8E6	37620513	20.306	17.219
28) SA Decachlor...	7.972	8.952	227.3E6	53554019	18.724	17.594
Target Compounds						
17) MA 4,4'-DDT	6.162	7.039	14436442	2995788	1.132	1.023



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 21:49
Operator : SG\AJ
Sample : K4567-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:03:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

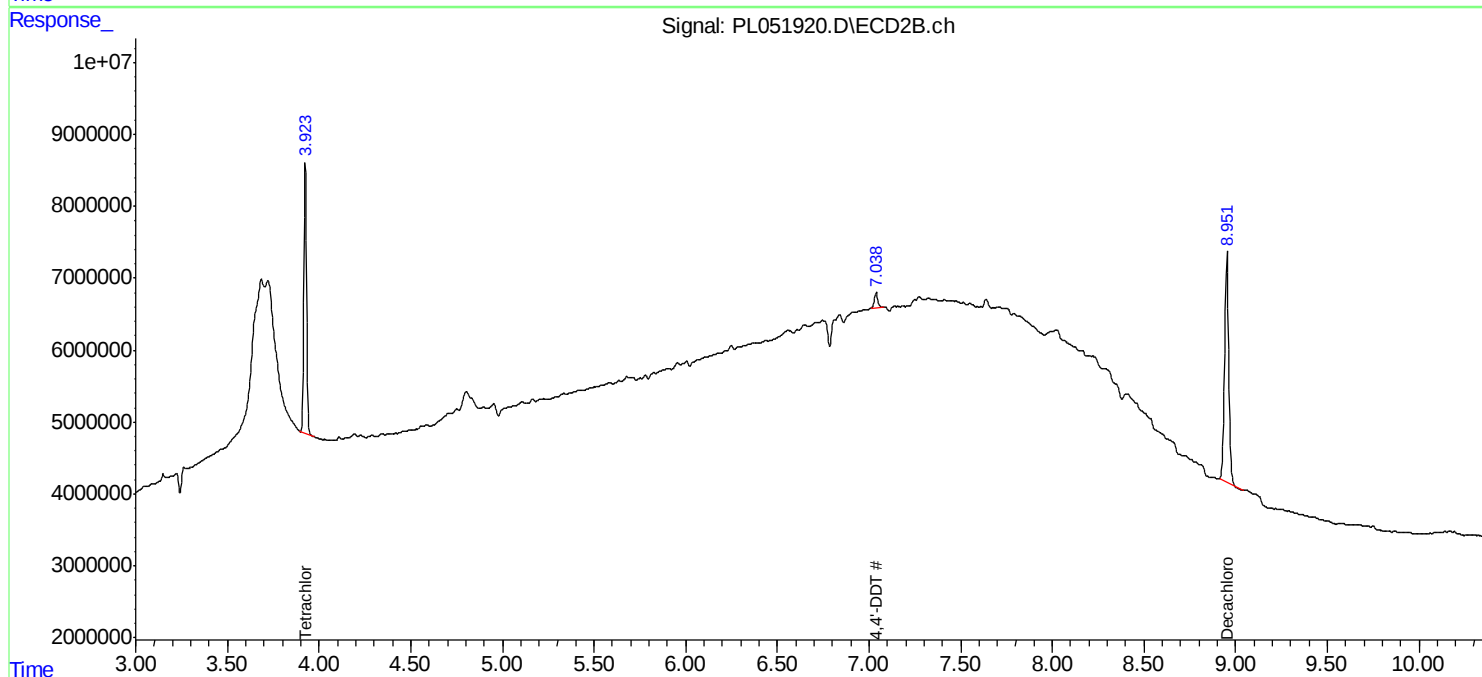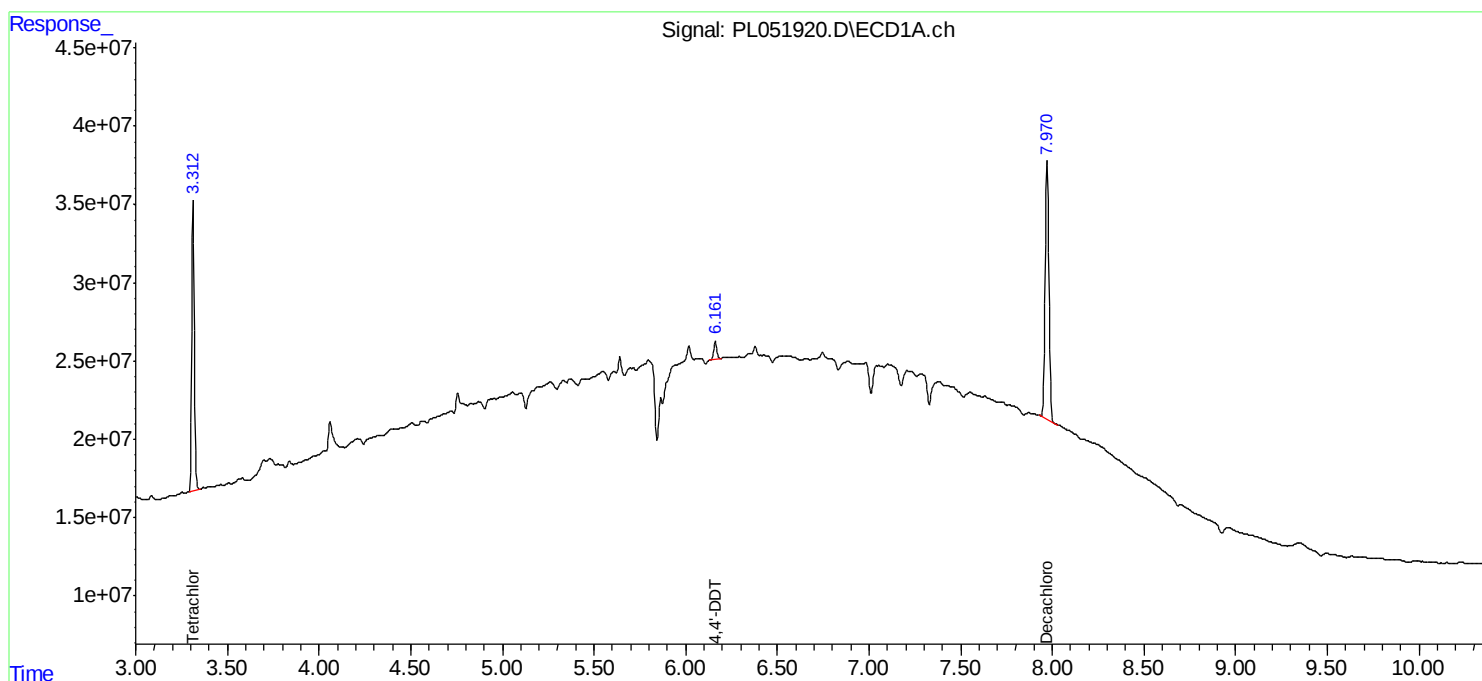


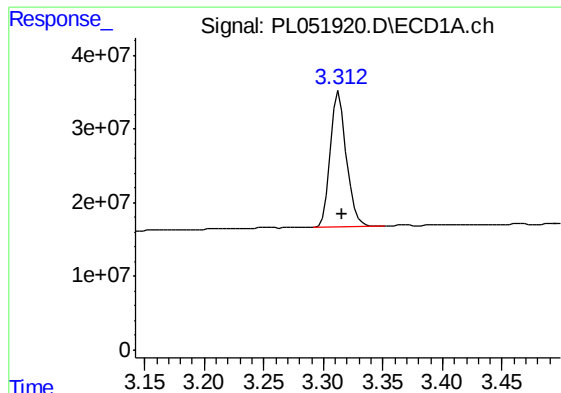

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 173794345
Conc: 20.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

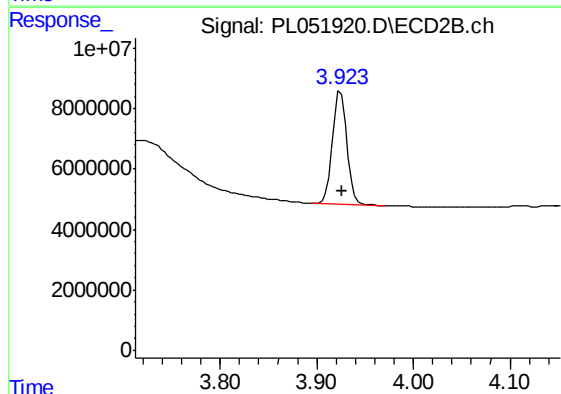


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 37620513
Conc: 17.22 ng/ml

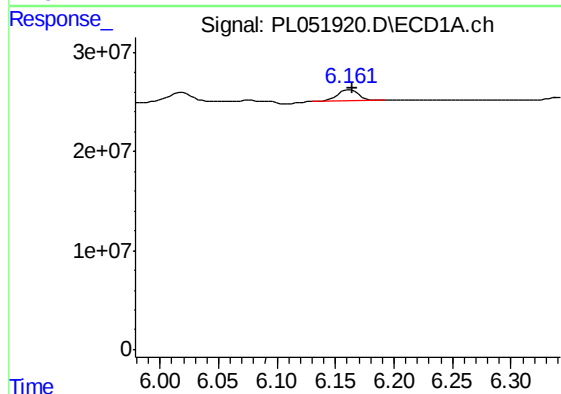


#17 4,4'-DDT

R.T.: 6.162 min
Delta R.T.: -0.003 min
Response: 14436442
Conc: 1.13 ng/ml

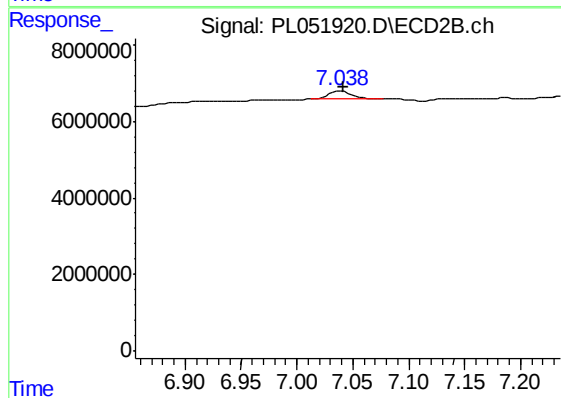

#17 4,4'-DDT


R.T.: 7.039 min
Delta R.T.: -0.002 min
Response: 2995788
Conc: 1.02 ng/ml

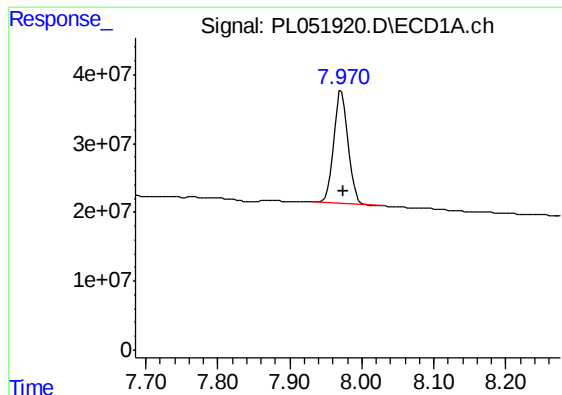

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 227267083
Conc: 18.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

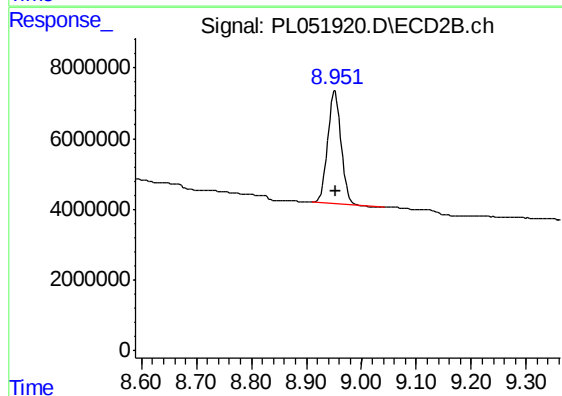

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 53554019
Conc: 17.59 ng/ml