

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
 Data File : PL051923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 22:32
 Operator : SG\AJ
 Sample : K4567-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-8-D

Manual Integrations
 APPROVED

Ankita
 8/29/2019 1:44:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:04:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.313	3.924	93354644	20352067	10.908	9.315
28) SA Decachlor...	7.972	8.952	134.0E6	30730404	11.038	10.096
Target Compounds						
17) MA 4,4'-DDT	6.160	7.040	6666761	1095768	0.523m	0.374 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082819\
Data File : PL051923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 22:32
Operator : SG\AJ
Sample : K4567-19
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-8-D


Manual Integrations
APPROVED

Ankita
8/29/2019 1:44:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:04:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

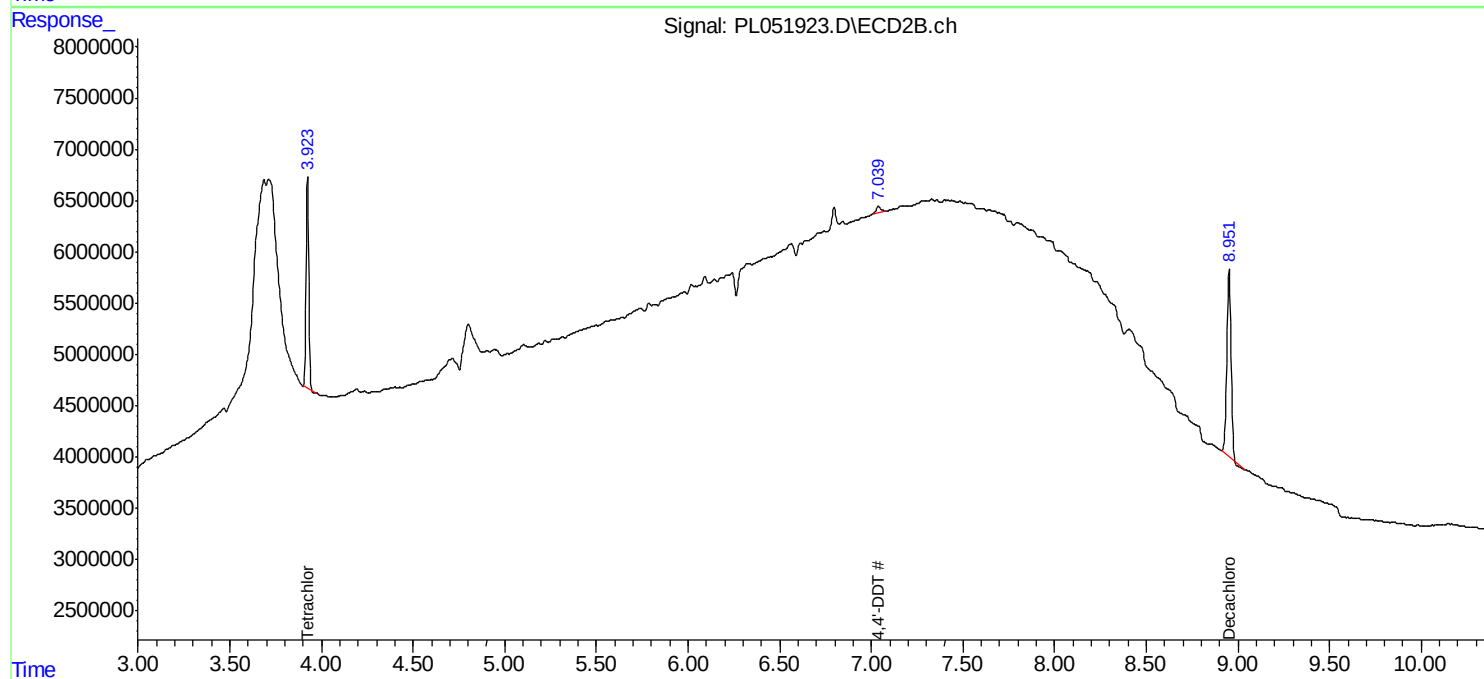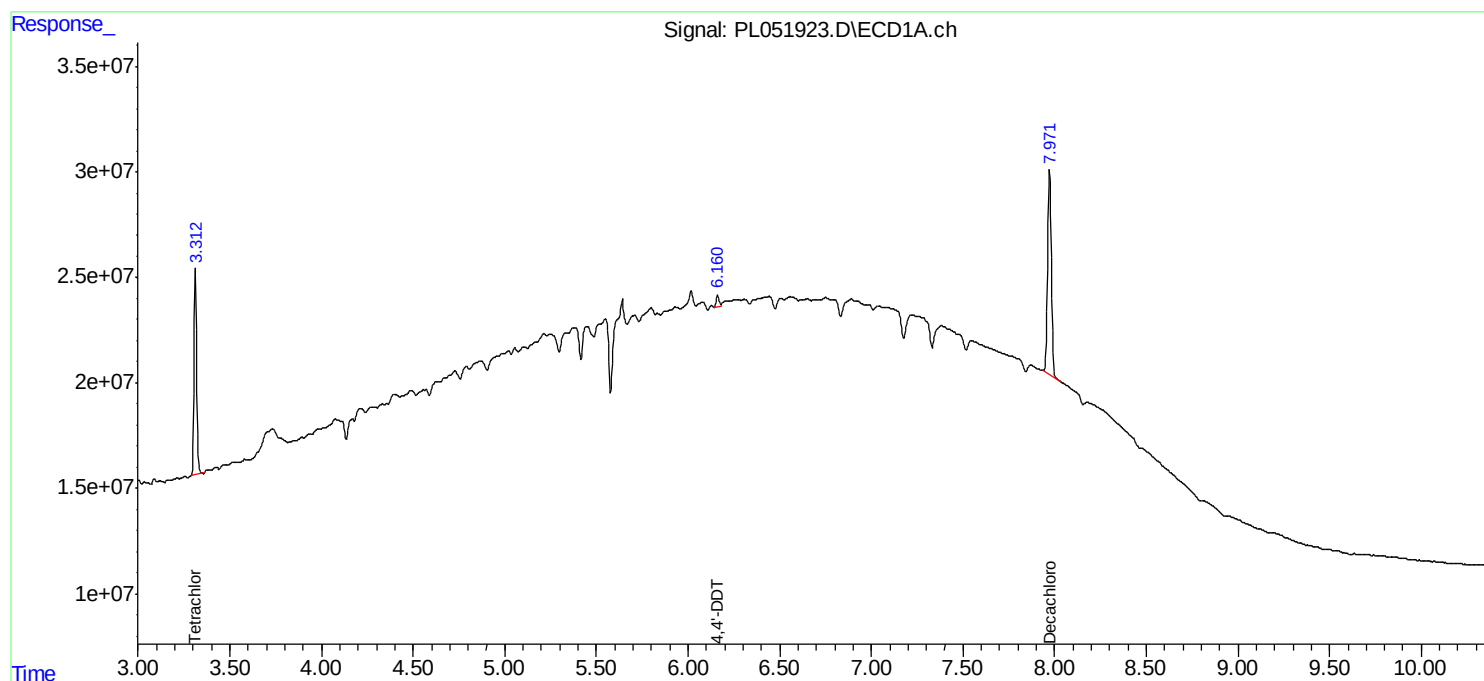

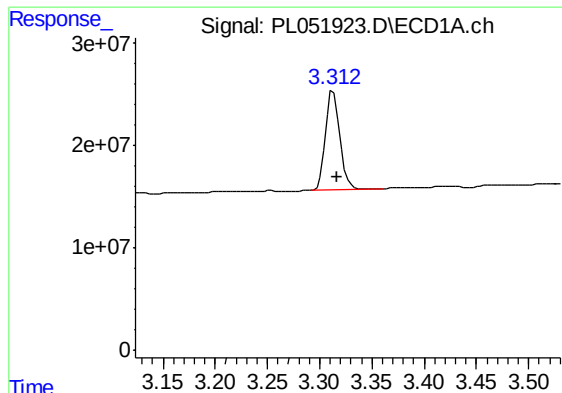


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 93354644
Conc: 10.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-D


Manual Integrations
APPROVED

Ankita
8/29/2019 1:44:47 PM

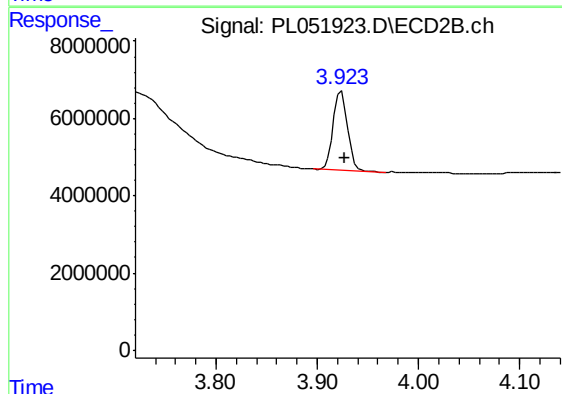


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 20352067
Conc: 9.32 ng/ml

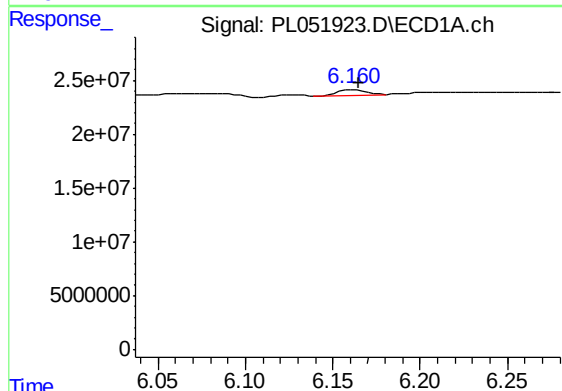


#17 4,4'-DDT

R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 6666761
Conc: 0.52 ng/ml m

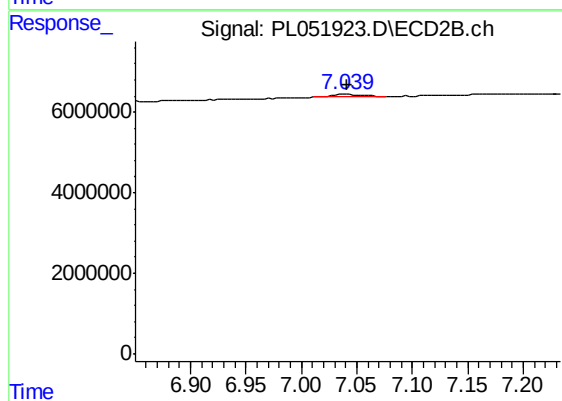

#17 4,4'-DDT

R.T.: 7.040 min
Delta R.T.: 0.000 min
Response: 1095768
Conc: 0.37 ng/ml

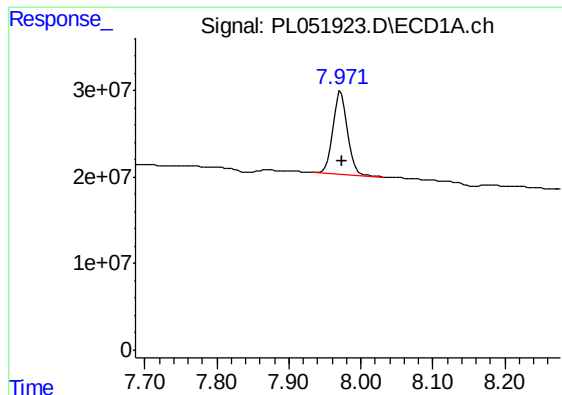


#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 133977200
Conc: 11.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-D

Manual Integrations
APPROVED

Ankita
8/29/2019 1:44:47 PM

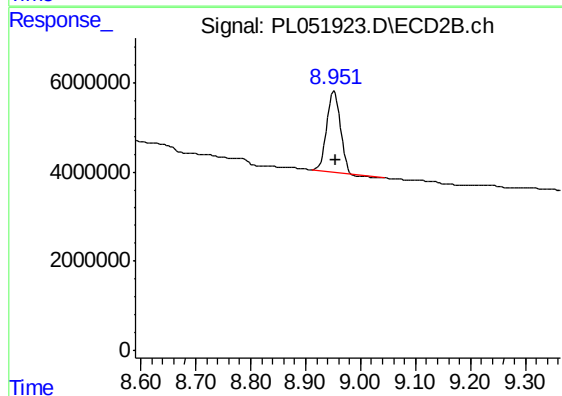

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 30730404
Conc: 10.10 ng/ml