

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
 Data File : PL061067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2020 16:59
 Operator : DD\AJ
 Sample : L3712-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 18:17:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	37239103	49380853	20.180	19.000
28)	SA Decachlor...	8.215	9.098	35337682	47743539	20.977	22.627
Target Compounds							
5)	MB Aldrin	0.000	5.492	0	2633331	N.D.	0.781 #
8)	B Heptachlo...	0.000	5.884	0	2271695	N.D.	0.868 #
9)	A Endosulfan I	5.489f	6.227f	5457178	15864895	3.003	5.518 #
10)	B gamma-Chl...	0.000	6.108f	0	2063340	N.D.	0.664 #
11)	B alpha-Chl...	5.459	6.197	-537374	6310594	N.D.	2.030
15)	B Endosulfa...	0.000	6.934	0	3406178	N.D.	1.324 #
24)	Chlordane-2	0.000	5.492f	0	2633331	N.D.	25.588 #
25)	Chlordane-3	0.000	6.108f	0	2063340	N.D.	5.162 #
26)	Chlordane-4	5.459	6.197	-537374	6310594	N.D.	13.127



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
Data File : PL061067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2020 16:59
Operator : DD\AJ
Sample : L3712-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 18:17:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

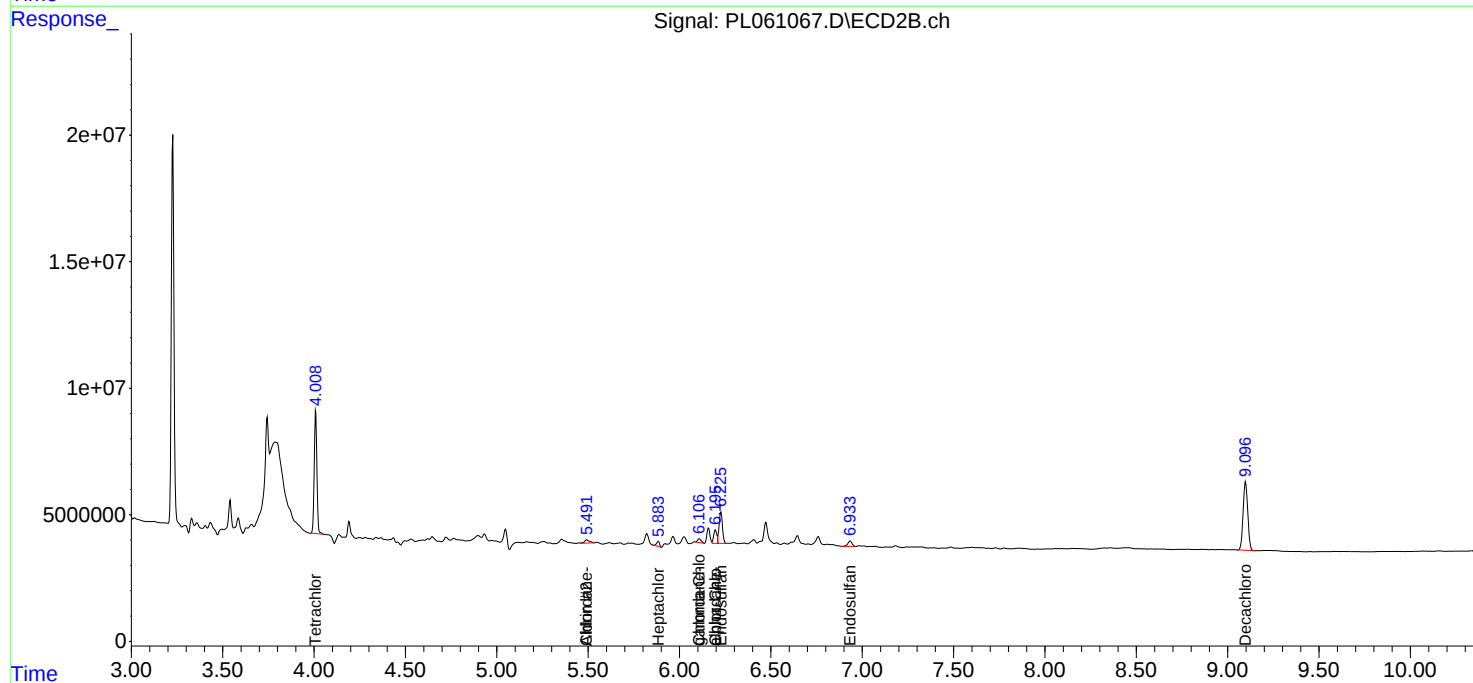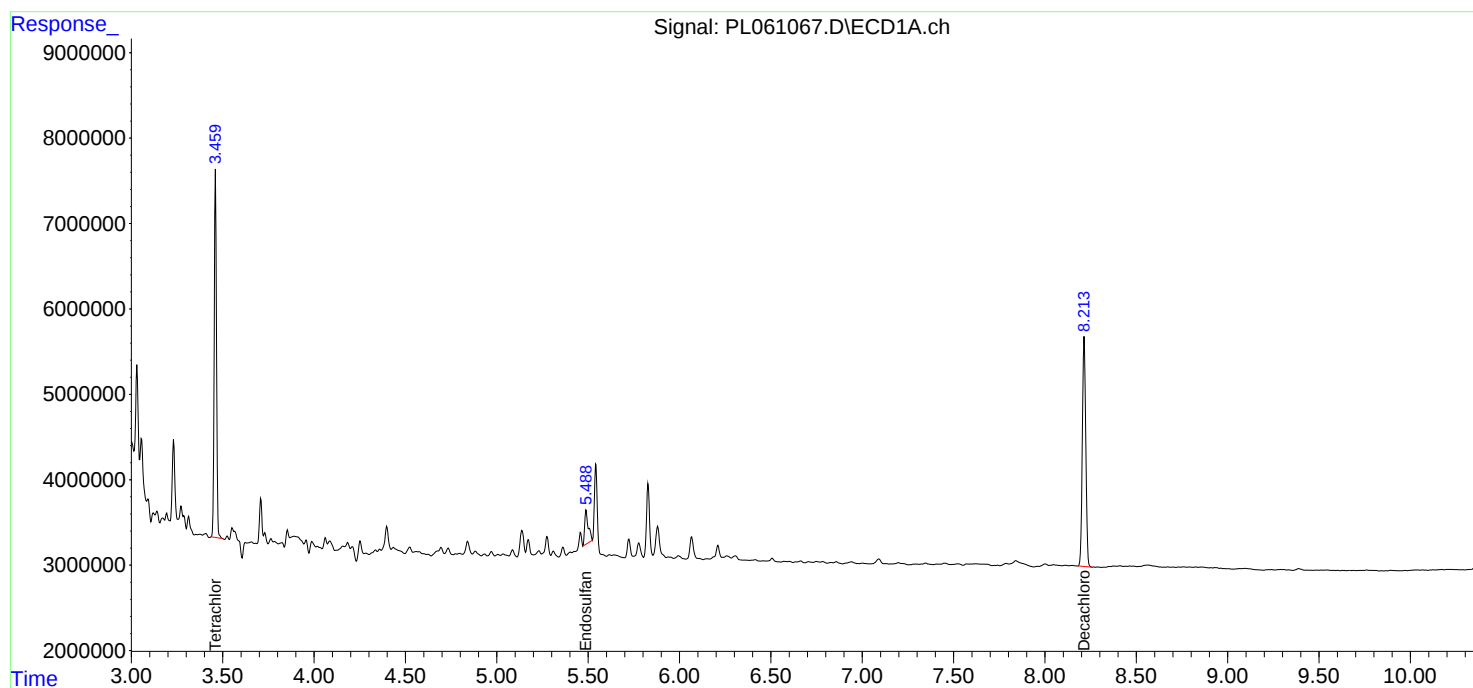


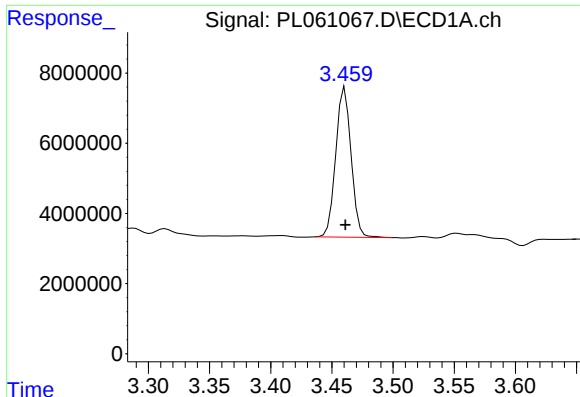

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 37239103
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

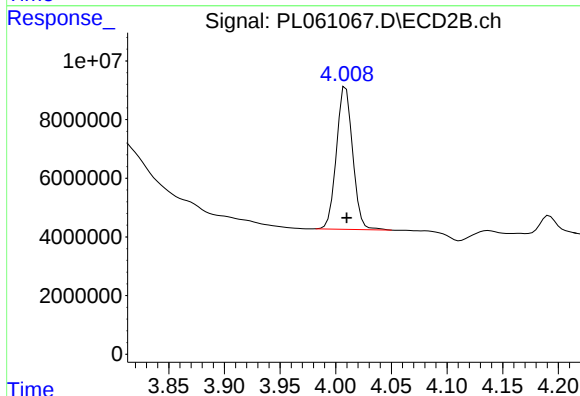


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 49380853
Conc: 19.00 ng/ml

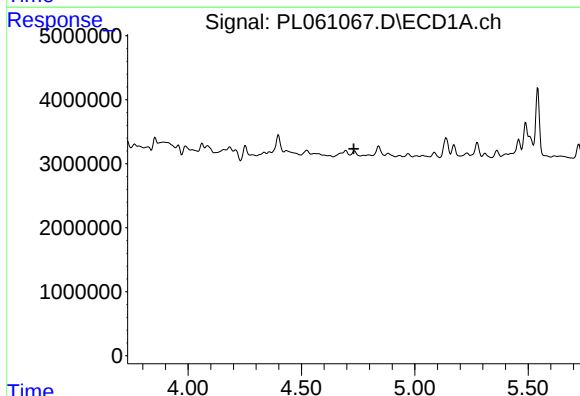


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

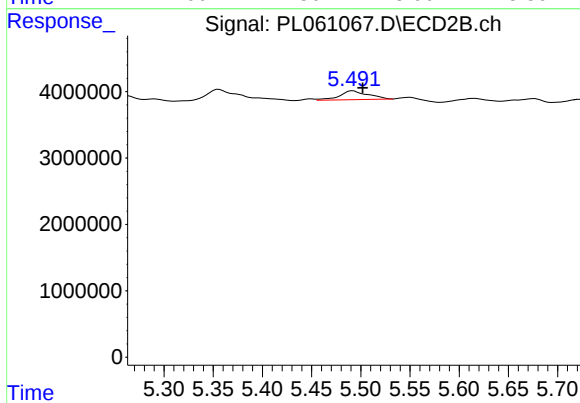

#5 Aldrin


R.T.: 5.492 min
Delta R.T.: -0.010 min
Response: 2633331
Conc: 0.78 ng/ml

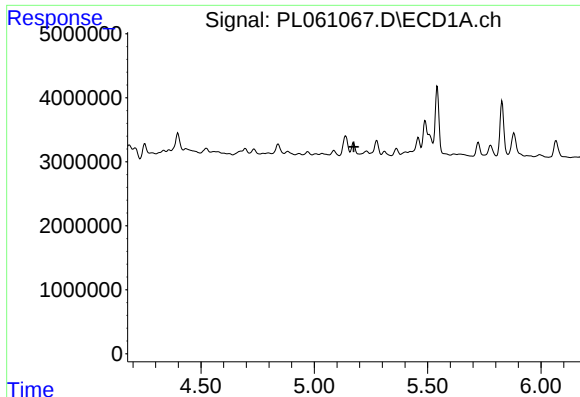

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

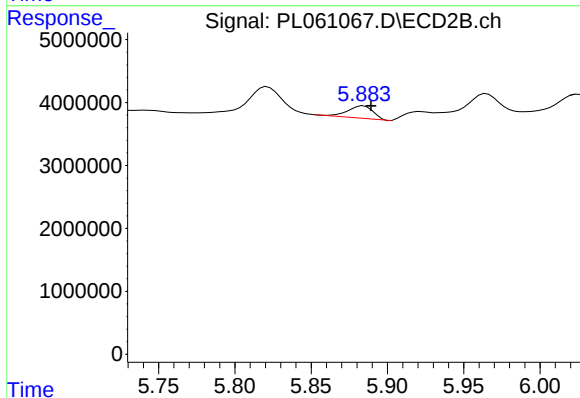


#8 Heptachlor epoxide

R.T.: 5.884 min
Delta R.T.: -0.005 min
Response: 2271695
Conc: 0.87 ng/ml

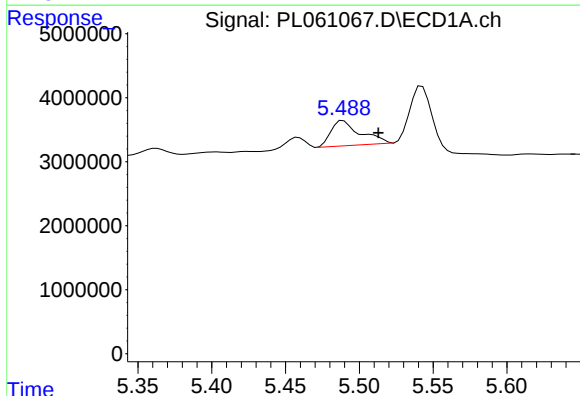


#9 Endosulfan I

R.T.: 5.489 min
Delta R.T.: -0.024 min
Response: 5457178
Conc: 3.00 ng/ml

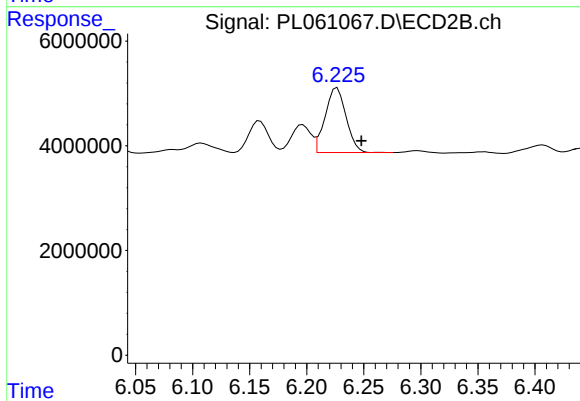

#9 Endosulfan I


R.T.: 6.227 min
Delta R.T.: -0.021 min
Response: 15864895
Conc: 5.52 ng/ml

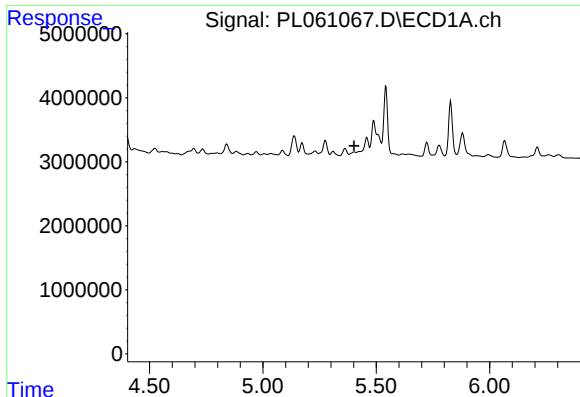

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

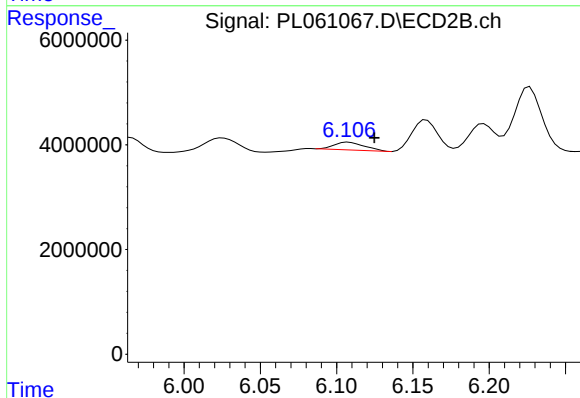


#10 gamma-Chlordane

R.T.: 6.108 min
Delta R.T.: -0.017 min
Response: 2063340
Conc: 0.66 ng/ml

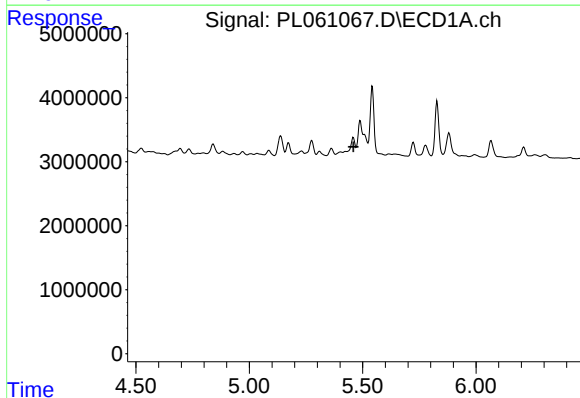


#11 alpha-Chlordane

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: -537374
Conc: N.D.

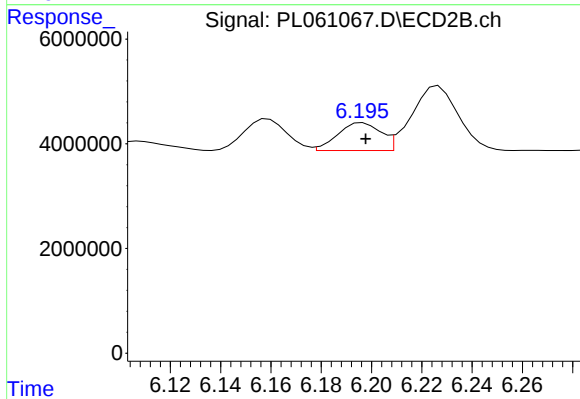

#11 alpha-Chlordane


R.T.: 6.197 min
Delta R.T.: -0.001 min
Response: 6310594
Conc: 2.03 ng/ml

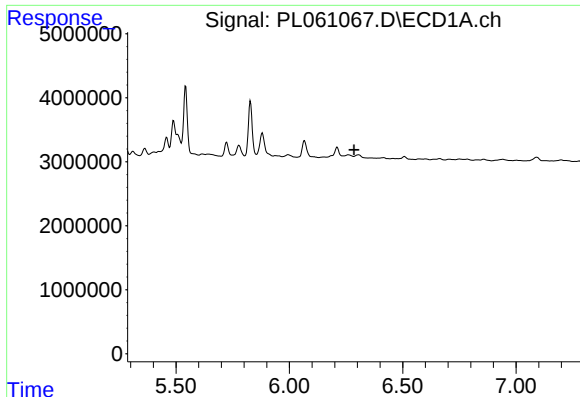

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

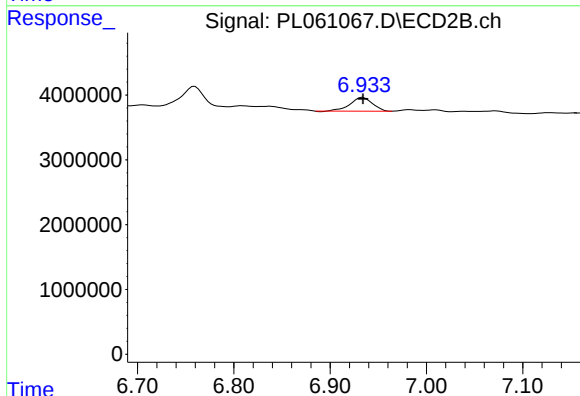


#15 Endosulfan II

R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 3406178
Conc: 1.32 ng/ml

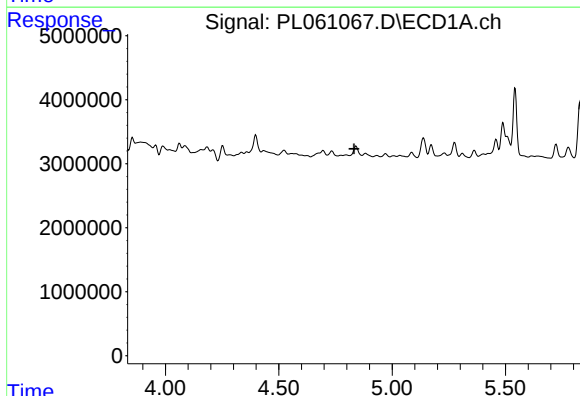


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.833 min
Response: 0
Conc: N.D.

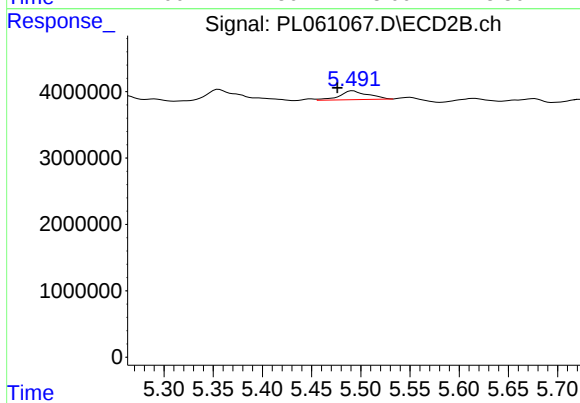

#24 Chlordane-2


R.T.: 5.492 min
Delta R.T.: 0.016 min
Response: 2633331
Conc: 25.59 ng/ml

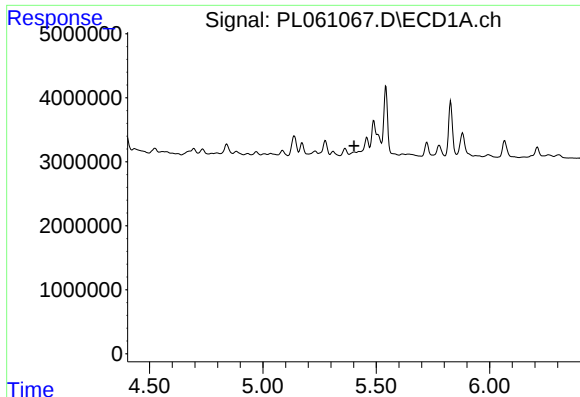

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

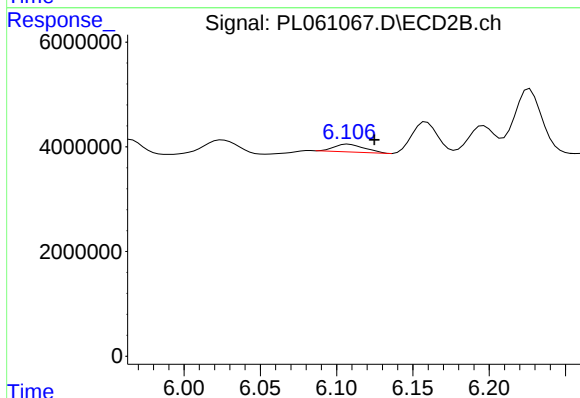


#25 Chlordane-3

R.T.: 6.108 min
Delta R.T.: -0.017 min
Response: 2063340
Conc: 5.16 ng/ml

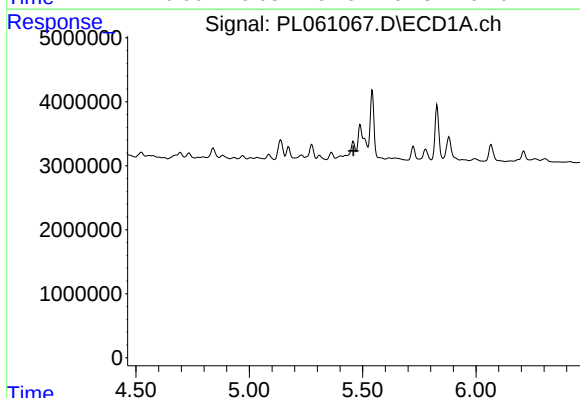


#26 Chlordane-4

R.T.: 5.459 min
Delta R.T.: -0.002 min
Response: -537374
Conc: N.D.

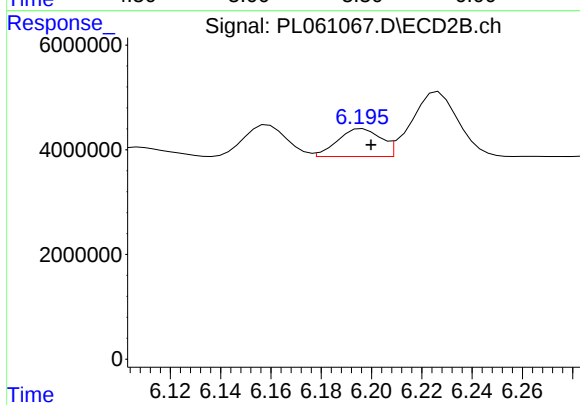

#26 Chlordane-4


R.T.: 6.197 min
Delta R.T.: -0.003 min
Response: 6310594
Conc: 13.13 ng/ml

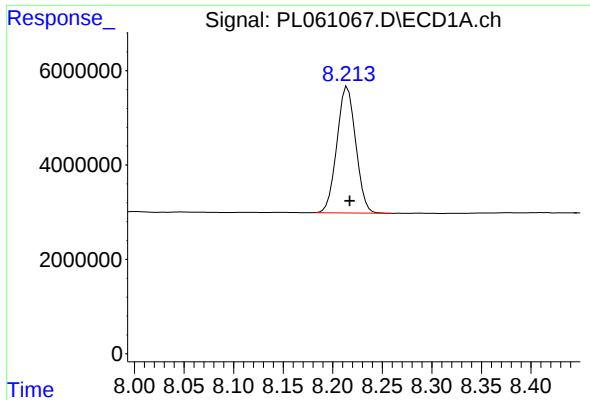

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 35337682
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

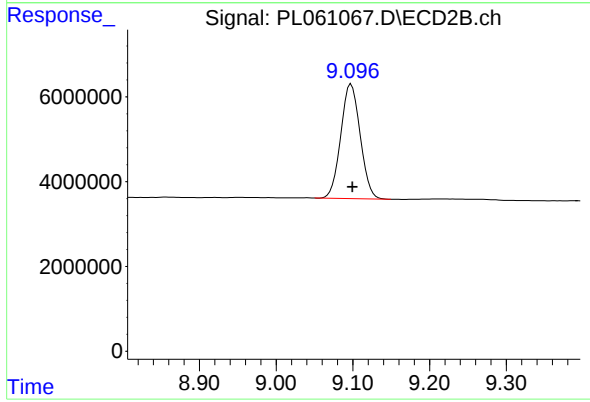

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.002 min
Response: 47743539
Conc: 22.63 ng/ml