

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
 Data File : PL061067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2020 16:59
 Operator : DD\AJ
 Sample : L3712-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-27137

Manual Integrations
 APPROVED

Ankita
 8/31/2020 3:26:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 02:01:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	37239103	49380853	20.180	19.000
28)	SA Decachlor...	8.215	9.098	35337682	47743539	20.977	22.627
Target Compounds							
11)	B alpha-Chl...	5.457	6.197	2264298	6310594	1.160m	2.030 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
Data File : PL061067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2020 16:59
Operator : DD\AJ
Sample : L3712-17
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-27137


Manual Integrations
APPROVED

Ankita
8/31/2020 3:26:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 02:01:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

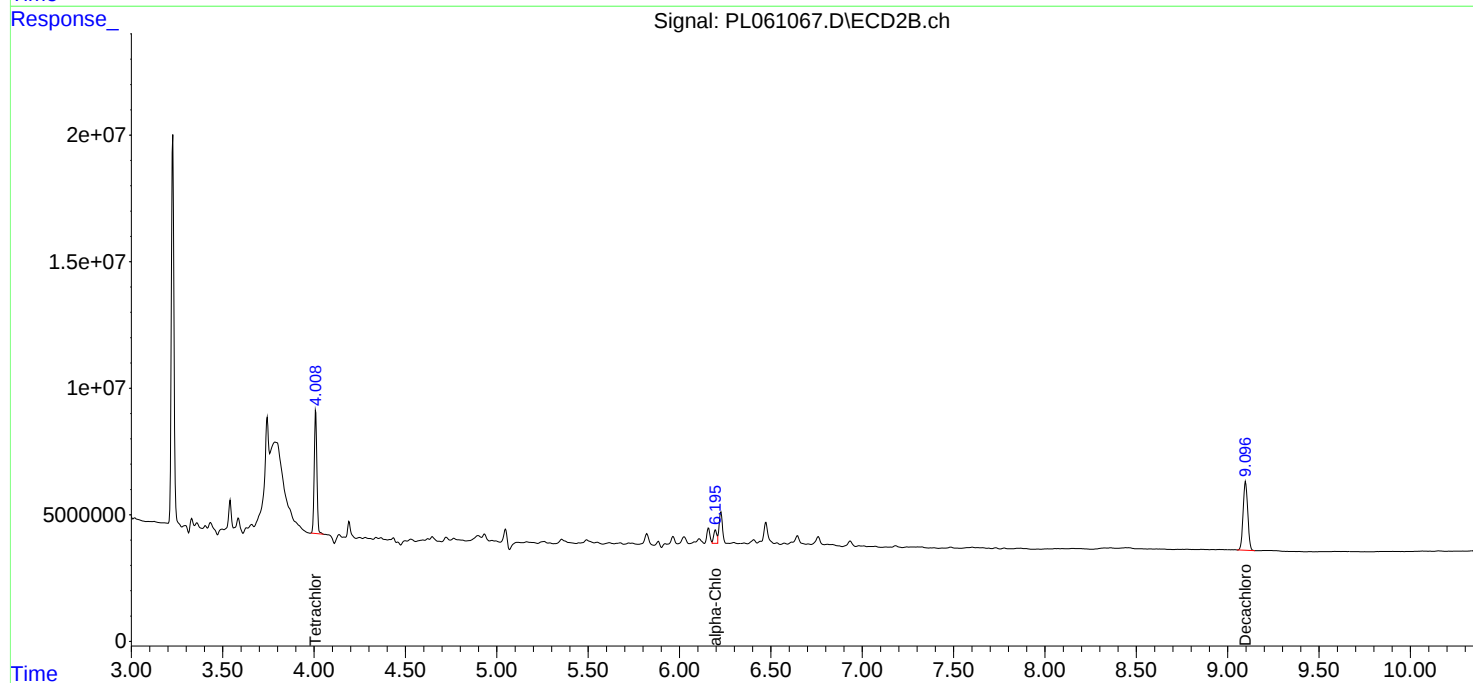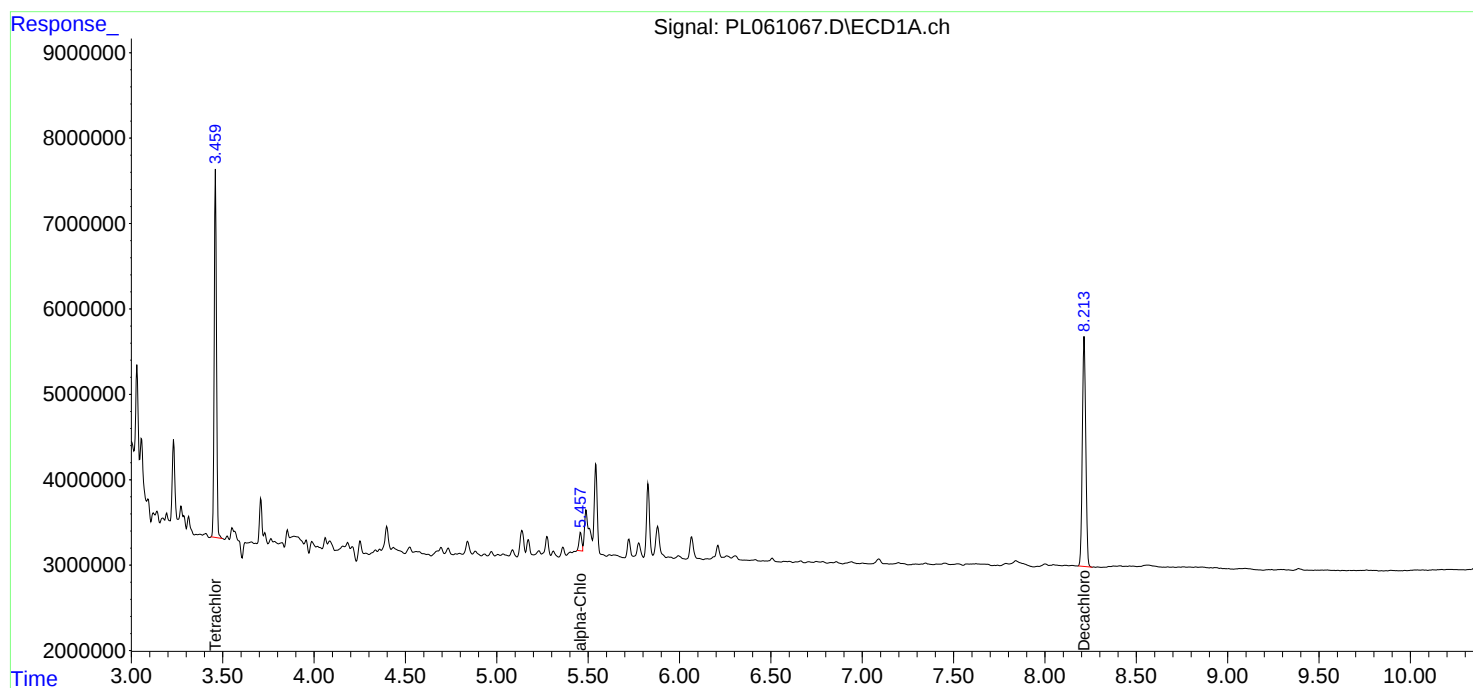

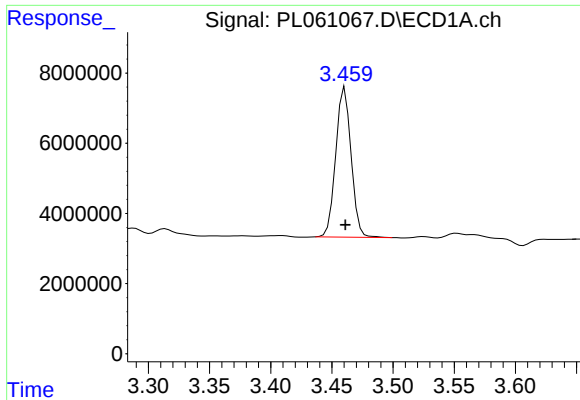


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 37239103
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-27137


Manual Integrations
APPROVED

Ankita
8/31/2020 3:26:11 PM

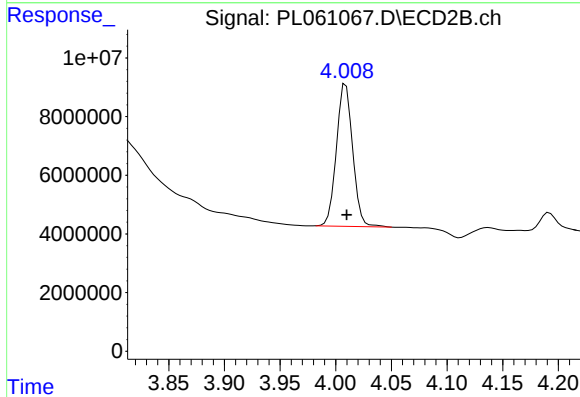


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 49380853
Conc: 19.00 ng/ml

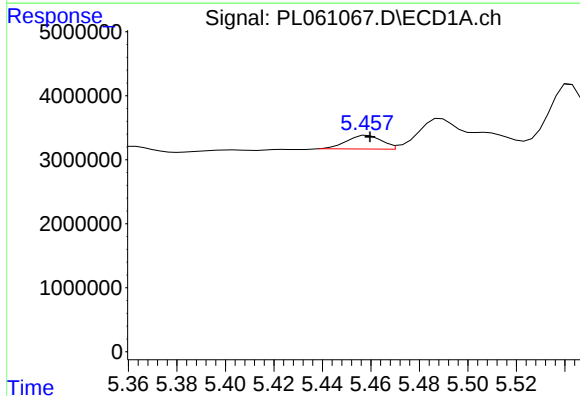


#11 alpha-Chlordane

R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 2264298
Conc: 1.16 ng/ml m

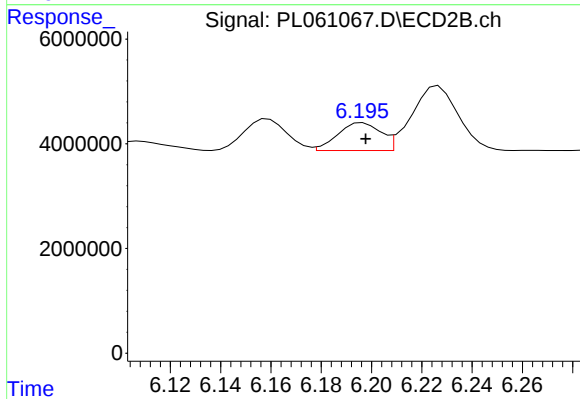

#11 alpha-Chlordane

R.T.: 6.197 min
Delta R.T.: -0.001 min
Response: 6310594
Conc: 2.03 ng/ml

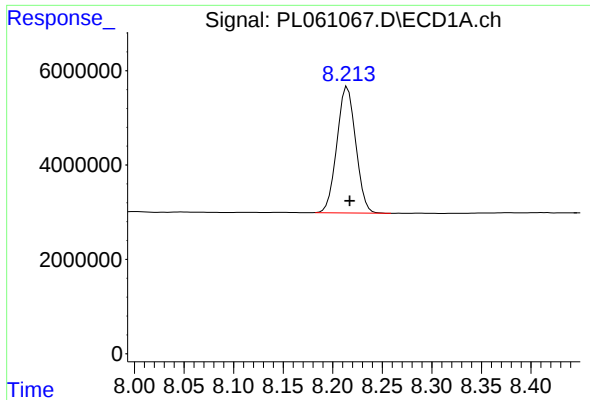


#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 35337682
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-27137

Manual Integrations
APPROVED

Ankita
8/31/2020 3:26:11 PM

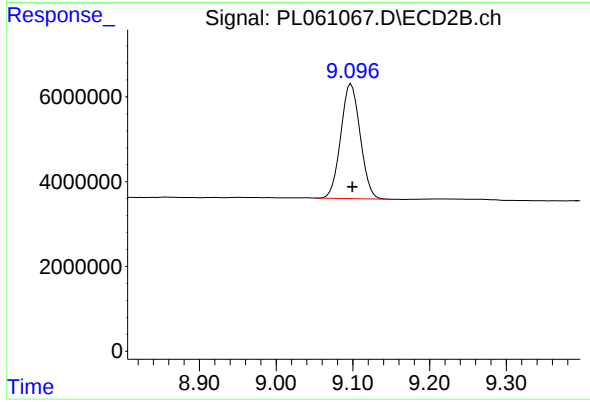

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.002 min
Response: 47743539
Conc: 22.63 ng/ml