

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
 Data File : PL061069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2020 17:27
 Operator : DD\AJ
 Sample : L3712-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VB-25860

Manual Integrations
 APPROVED

Ankita
 8/31/2020 3:26:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 18:17:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.009	30042693	39920934	16.280m	15.360
28) SA Decachlor...	8.216	9.099	32773209	45668076	19.454	21.643

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082820\
Data File : PL061069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2020 17:27
Operator : DD\AJ
Sample : L3712-19
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VB-25860


Manual Integrations
APPROVED

Ankita
8/31/2020 3:26:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 18:17:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

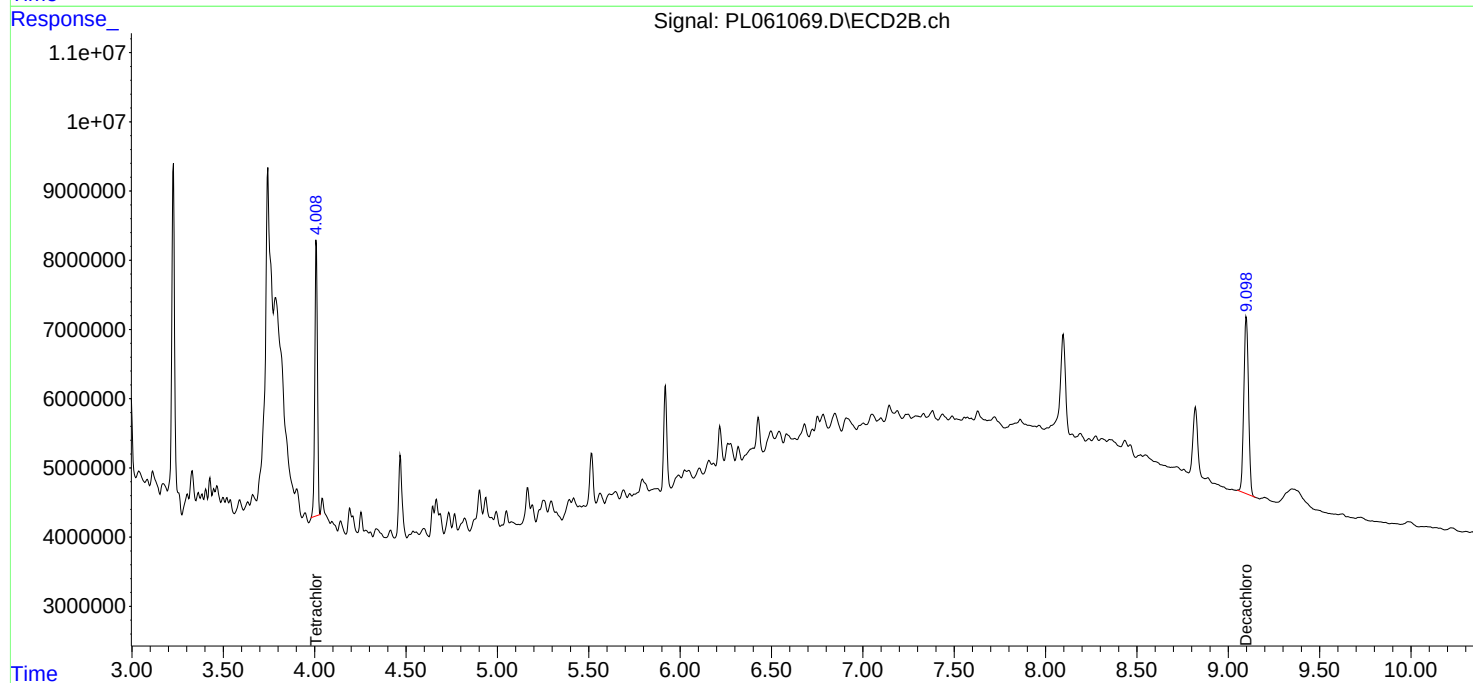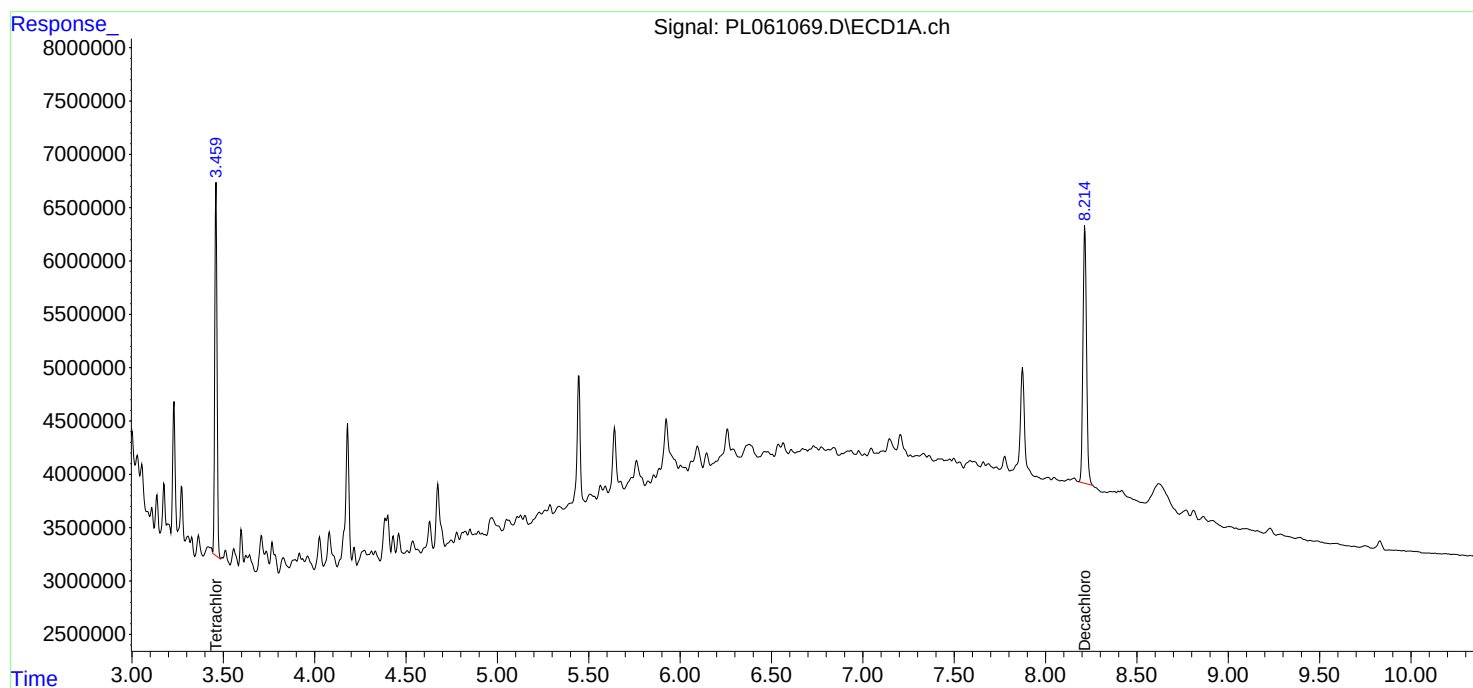

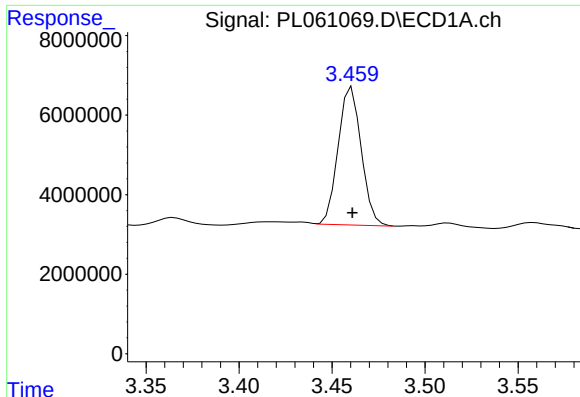


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 30042693
Conc: 16.28 ng/ml m

Instrument :
ECD_L
ClientSampleId :
VB-25860


Manual Integrations
APPROVED

Ankita
8/31/2020 3:26:13 PM

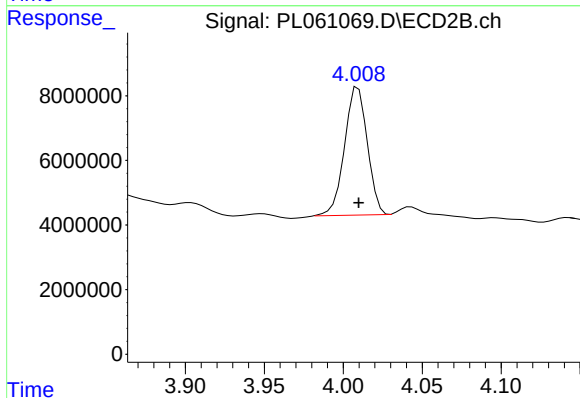


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 39920934
Conc: 15.36 ng/ml

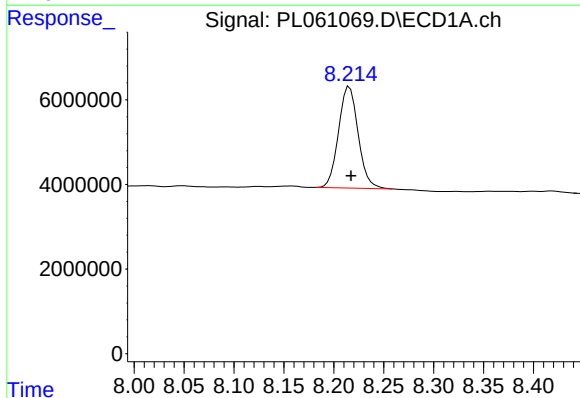

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.002 min
Response: 32773209
Conc: 19.45 ng/ml

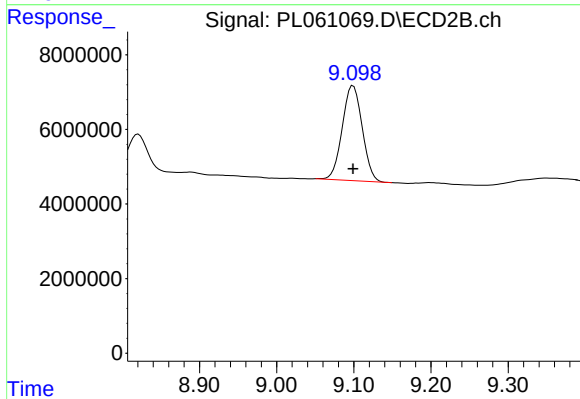

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 45668076
Conc: 21.64 ng/ml