

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 12:33
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:44:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	199.6E6	47292655	23.323	21.646
28)	SA Decachlor...	7.972	8.950	279.0E6	62533539	22.989	20.544
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	581901	N.D.	0.399 #
8)	B Heptachlo...	0.000	5.785	0	7348974	N.D.	2.178 #
9)	A Endosulfan I	5.327f	0.000	12417395	0	0.924	N.D. #
10)	B gamma-Chl...	0.000	6.020	0	964271	N.D.	0.264 #
13)	MA Dieldrin	5.541	6.411	2530888	2091918	0.166	0.611 #
18)	B Endrin al...	0.000	6.980f	0	825896	N.D.	0.292 #
20)	A Methoxychlor	0.000	7.505	0	438313	N.D.	0.261 #
25)	Chlordane-3	0.000	6.020	0	964271	N.D.	2.164 #
27)	Chlordane-5	0.000	6.922f	0	1214806	N.D.	12.323 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 12:33
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:44:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

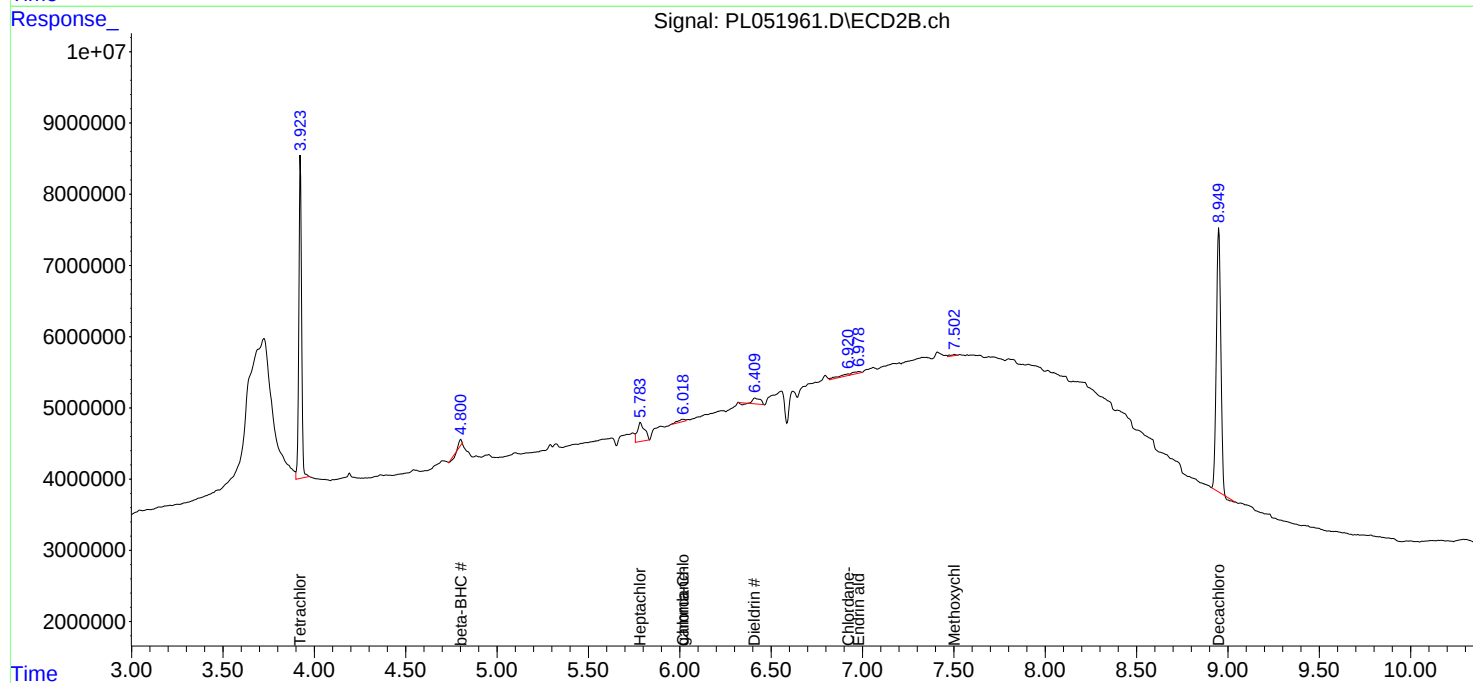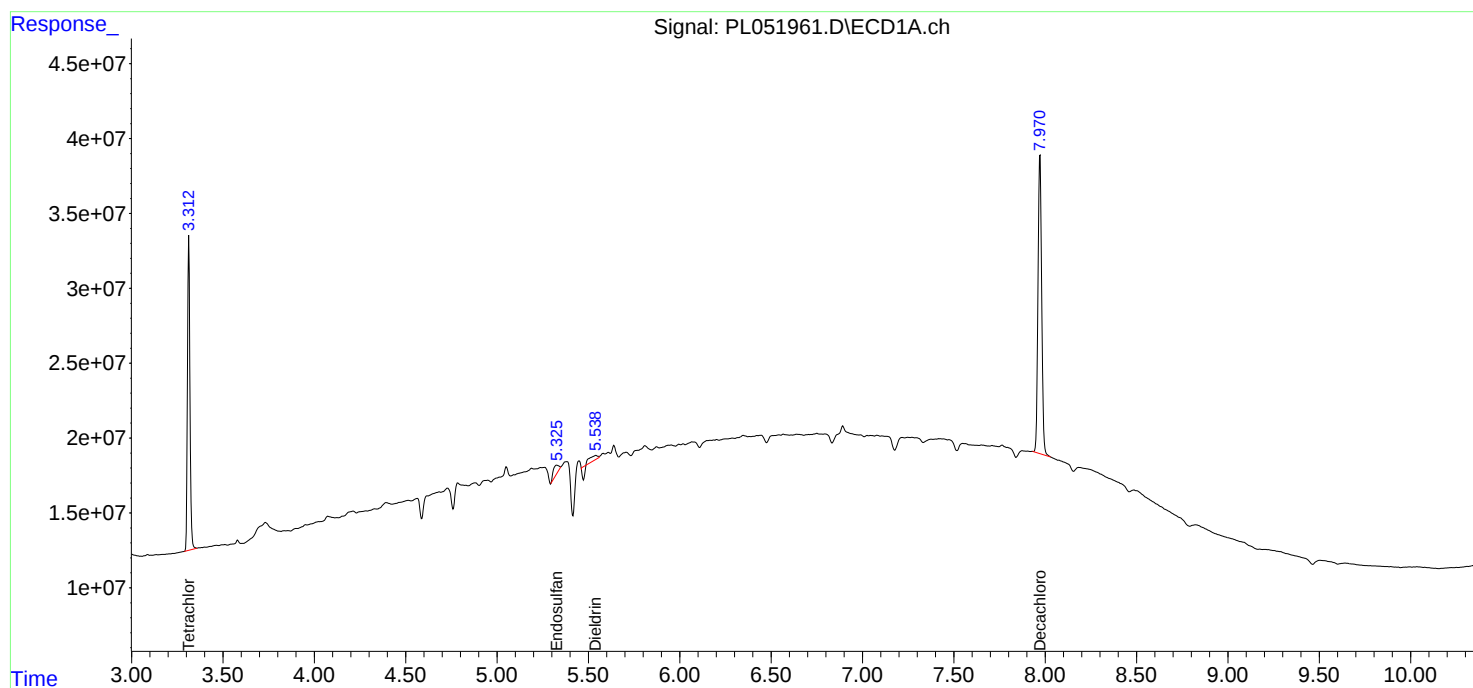


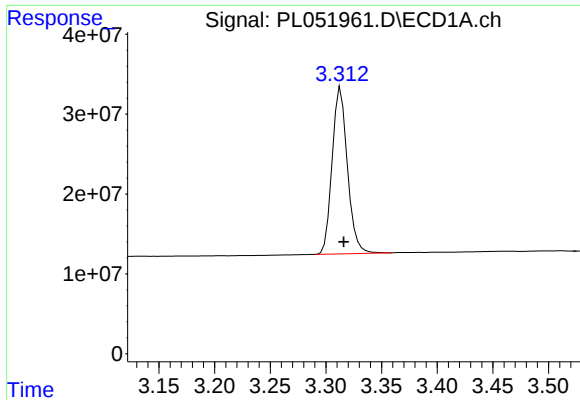

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 199609007
Conc: 23.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

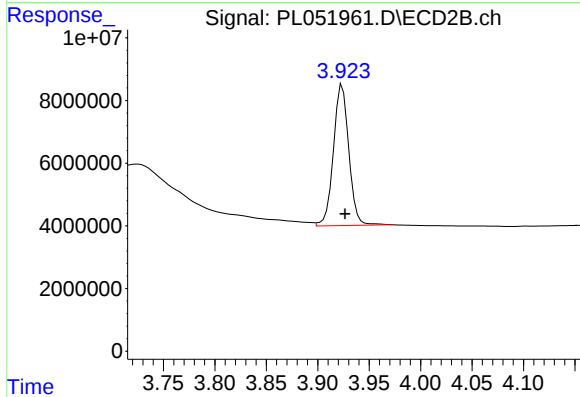


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 47292655
Conc: 21.65 ng/ml

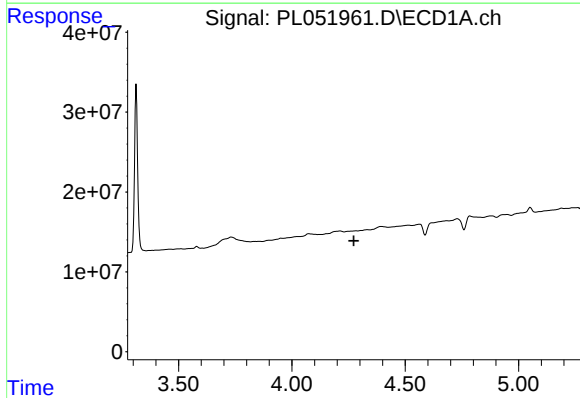


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

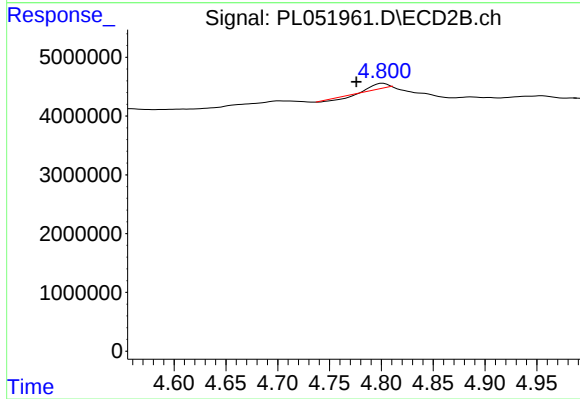

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 581901
Conc: 0.40 ng/ml

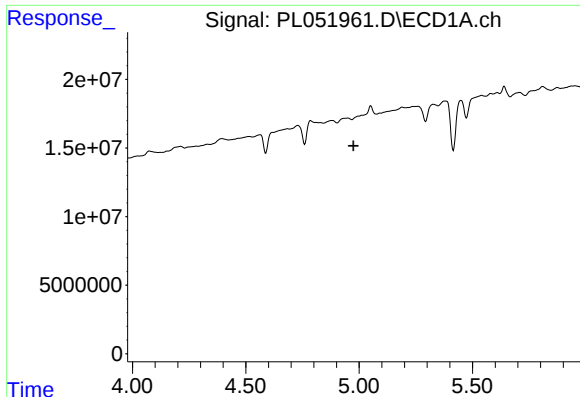

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

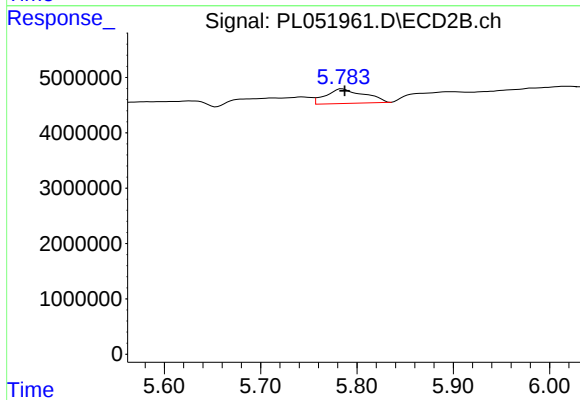


#8 Heptachlor epoxide

R.T.: 5.785 min
Delta R.T.: -0.002 min
Response: 7348974
Conc: 2.18 ng/ml

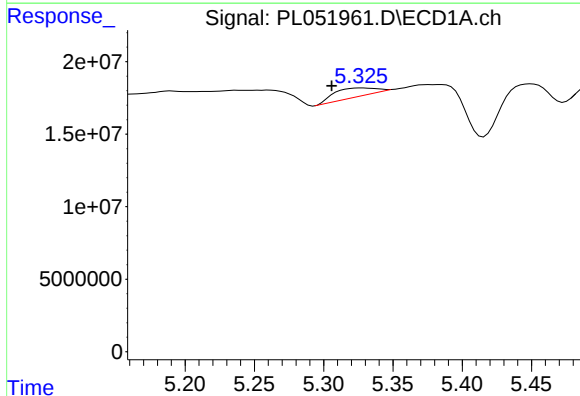


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.021 min
Response: 12417395
Conc: 0.92 ng/ml

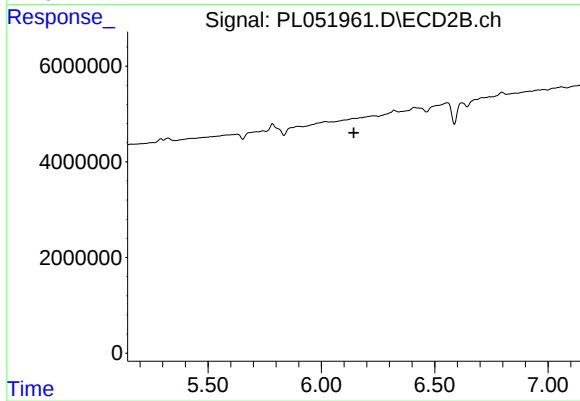

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

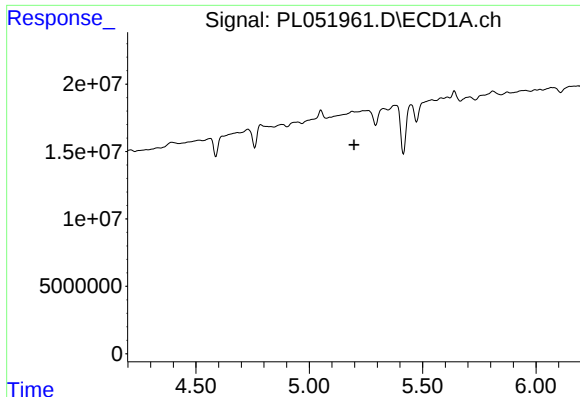

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

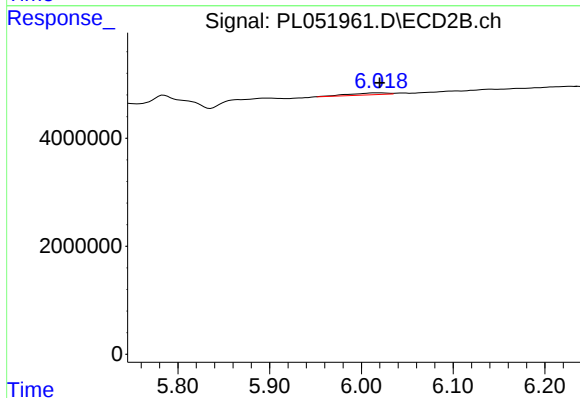


#10 gamma-Chlordane

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 964271
Conc: 0.26 ng/ml

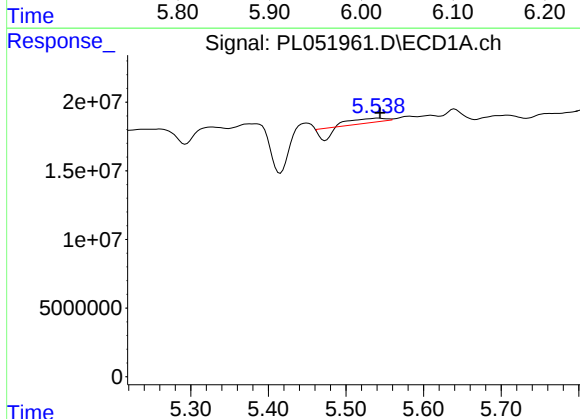


#13 Dieldrin

R.T.: 5.541 min
Delta R.T.: -0.003 min
Response: 2530888
Conc: 0.17 ng/ml

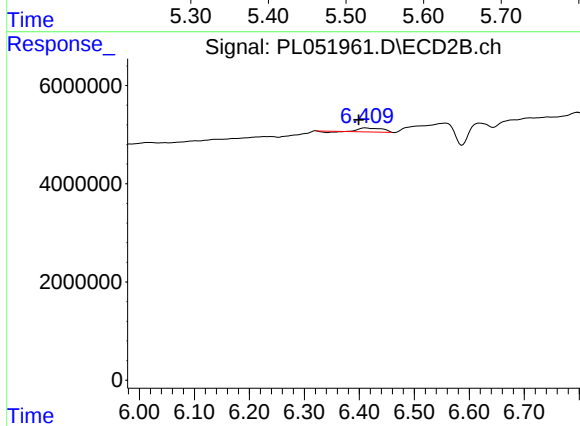

#13 Dieldrin


R.T.: 6.411 min
Delta R.T.: 0.012 min
Response: 2091918
Conc: 0.61 ng/ml

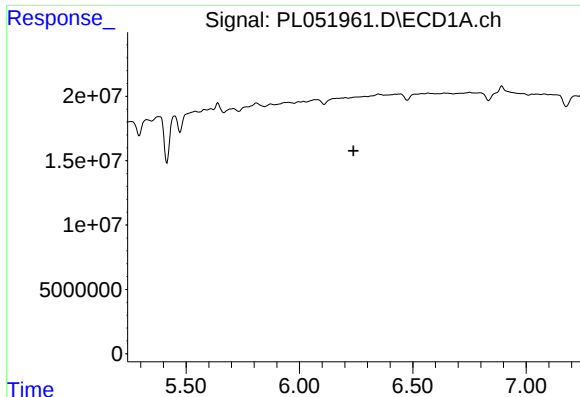

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

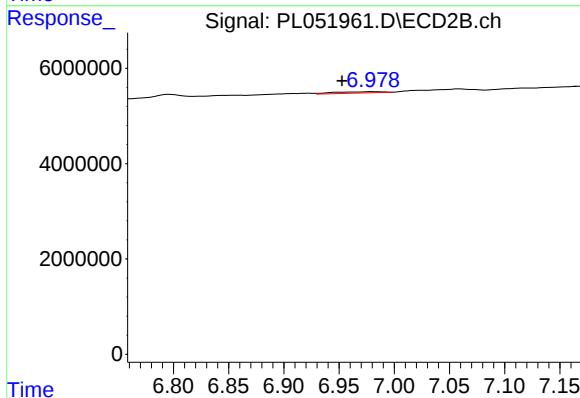


#18 Endrin aldehyde

R.T.: 6.980 min
Delta R.T.: 0.027 min
Response: 825896
Conc: 0.29 ng/ml

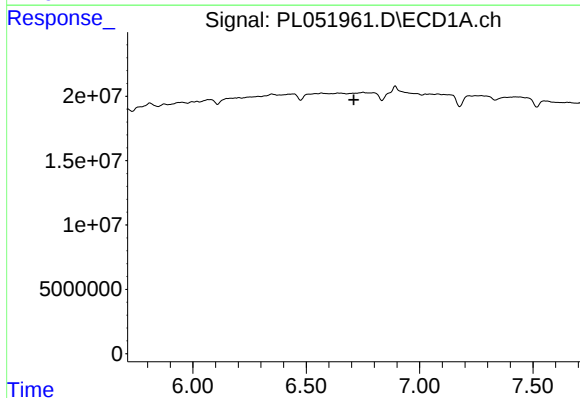


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

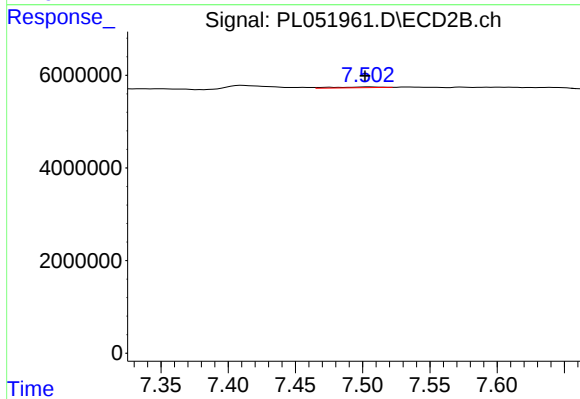

#20 Methoxychlor


R.T.: 7.505 min
Delta R.T.: 0.003 min
Response: 438313
Conc: 0.26 ng/ml

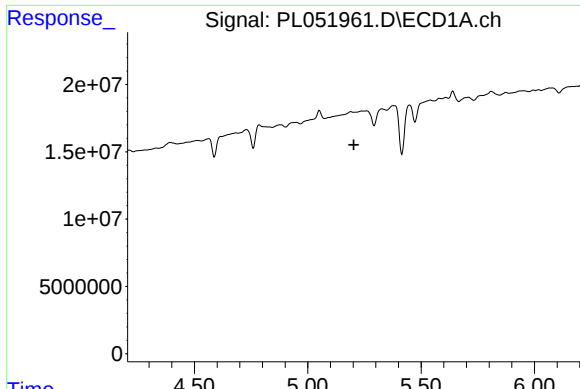

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

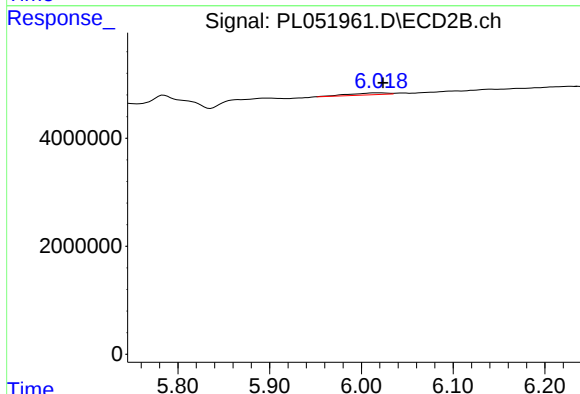


#25 Chlordane-3

R.T.: 6.020 min
Delta R.T.: -0.003 min
Response: 964271
Conc: 2.16 ng/ml

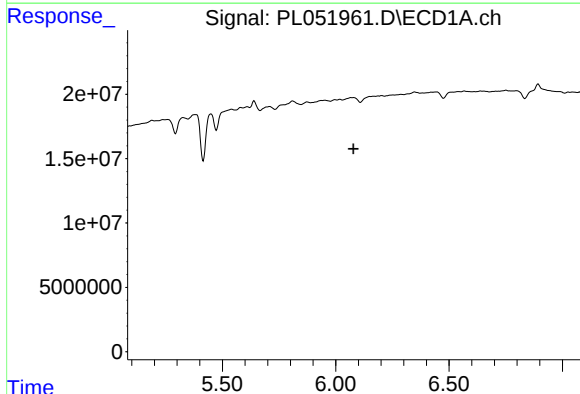


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

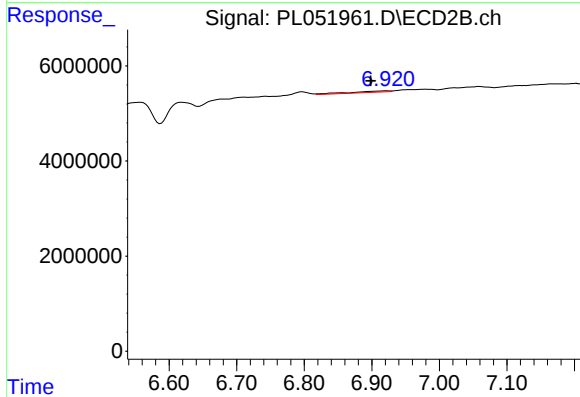

#27 Chlordane-5


R.T.: 6.922 min
Delta R.T.: 0.023 min
Response: 1214806
Conc: 12.32 ng/ml

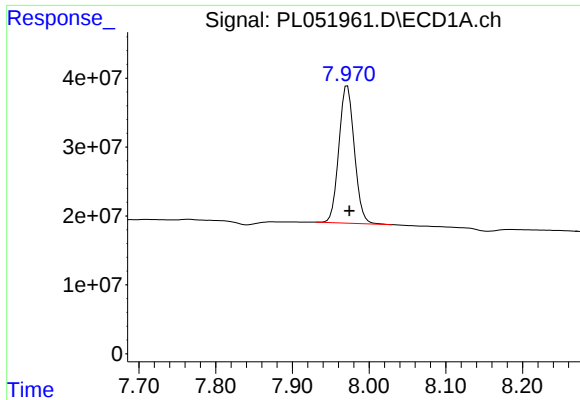

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 279038118
Conc: 22.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

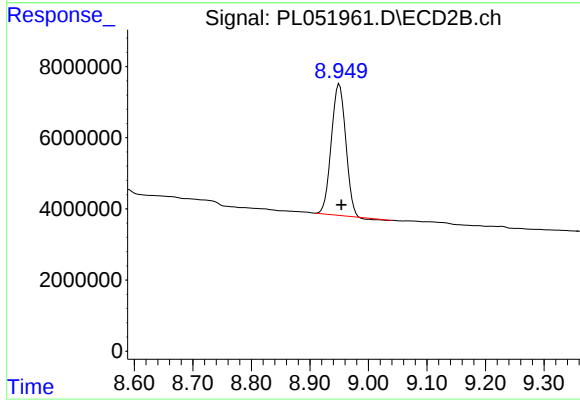

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 62533539
Conc: 20.54 ng/ml