

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 13:23
 Operator : SG\AJ
 Sample : PB122646BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122646BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:45:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.925	153.0E6	34257767	17.872	15.680
28)	SA Decachlor...	7.974	8.952	237.0E6	55215106	19.527	18.140
Target Compounds							
6)	B beta-BHC	0.000	4.796f	0	2127549	N.D.	1.460 #
8)	B Heptachlo...	0.000	5.803f	0	1589122	N.D.	0.471 #
9)	A Endosulfan I	0.000	6.153	0	1151770	N.D.	0.356 #
11)	B alpha-Chl...	5.263	0.000	10471392	0	0.724	N.D. #
14)	MA Endrin	5.811	0.000	10358501	0	0.710	N.D. #
15)	B Endosulfa...	0.000	6.842	0	1657047	N.D.	0.503 #
17)	MA 4,4'-DDT	0.000	7.058f	0	751197	N.D.	0.257 #
18)	B Endrin al...	0.000	6.937f	0	2517171	N.D.	0.891 #
20)	A Methoxychlor	0.000	7.483f	0	1417024	N.D.	0.845 #
24)	Chlordane-2	4.674f	0.000	5636641	0	13.791	N.D. #
26)	Chlordane-4	5.263	0.000	10471392	0	8.588	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 13:23
Operator : SG\AJ
Sample : PB122646BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB122646BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:45:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

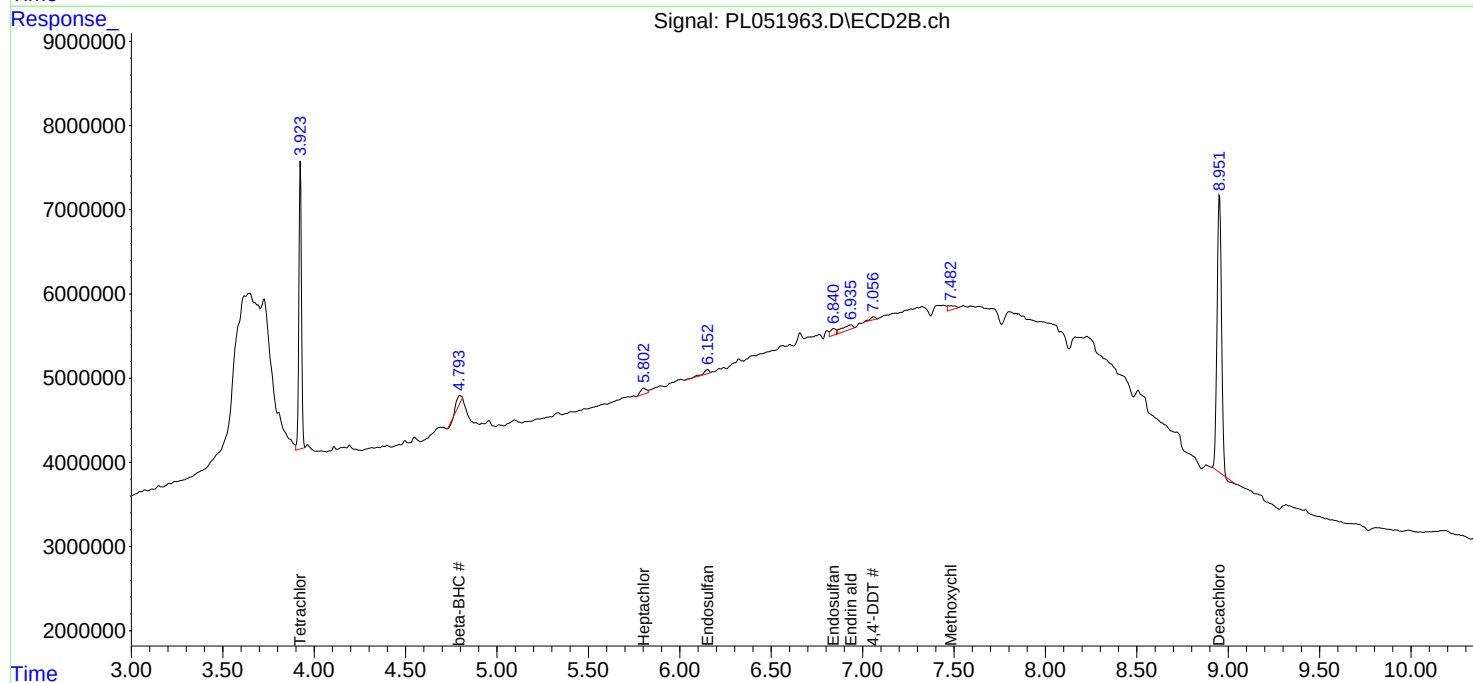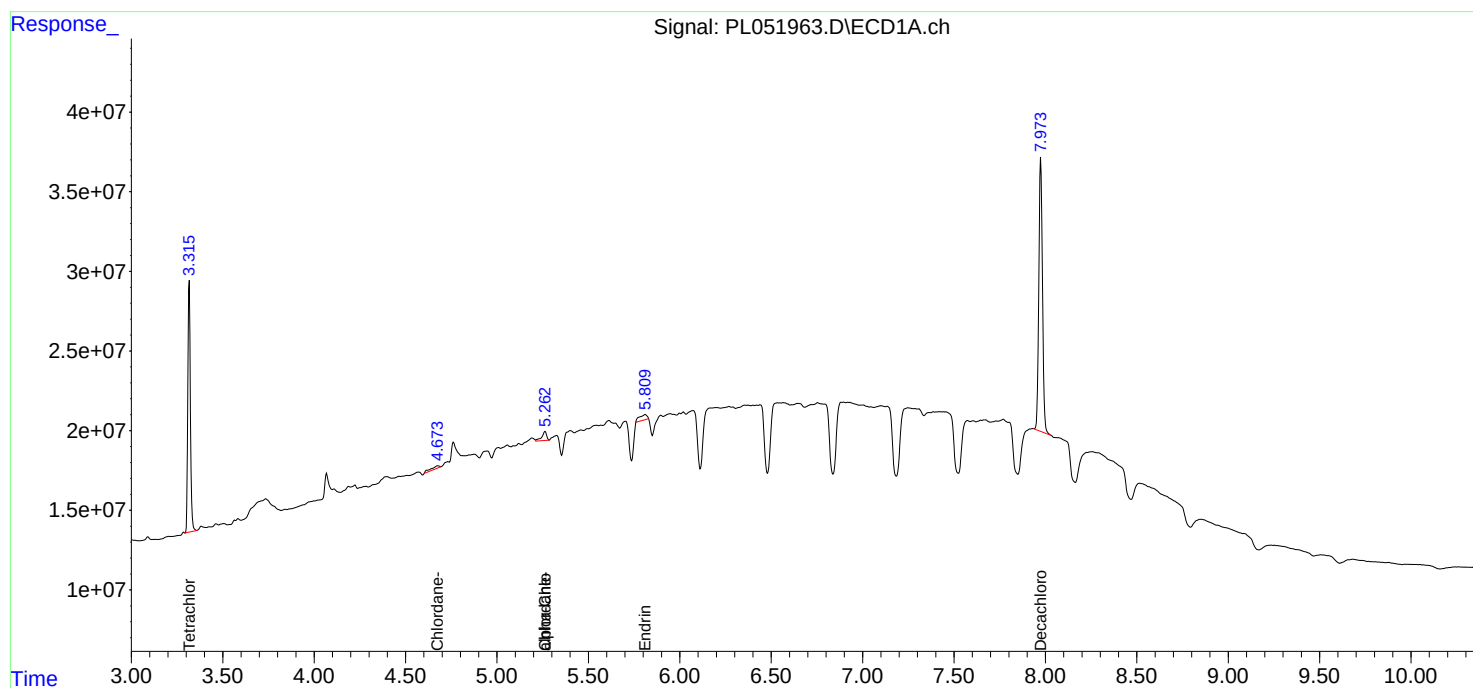


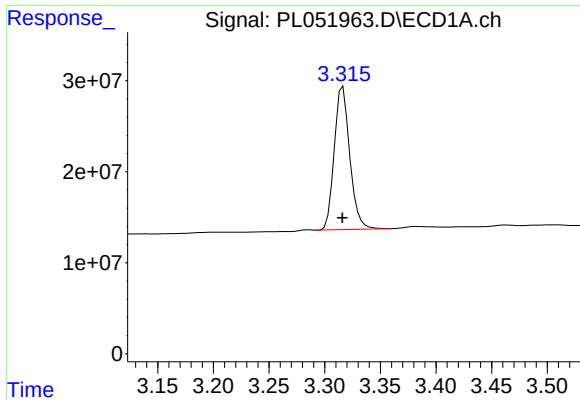

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: 0.000 min
Response: 152958269
Conc: 17.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122646BL

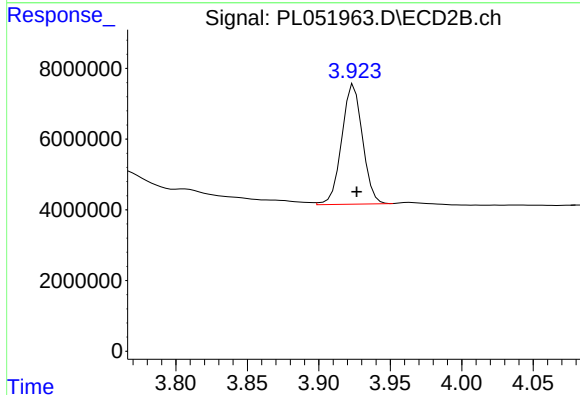


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 34257767
Conc: 15.68 ng/ml

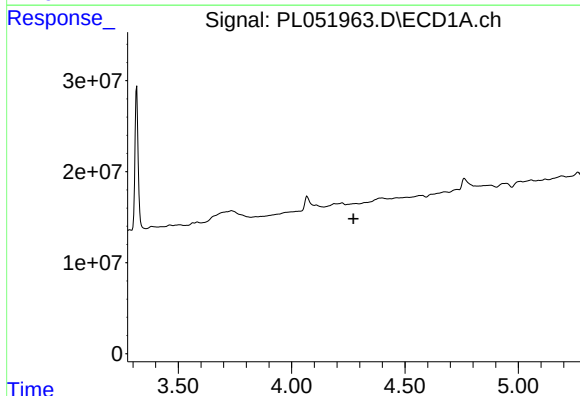


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

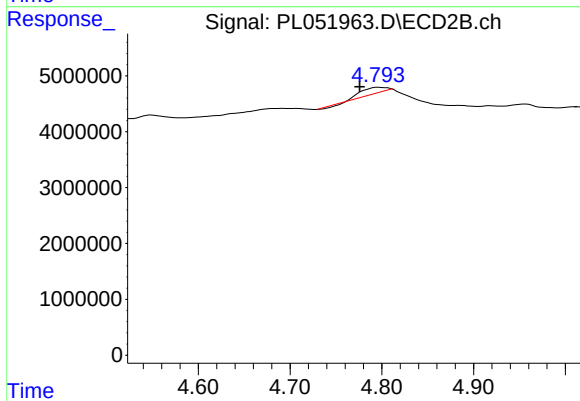

#6 beta-BHC


R.T.: 4.796 min
Delta R.T.: 0.020 min
Response: 2127549
Conc: 1.46 ng/ml

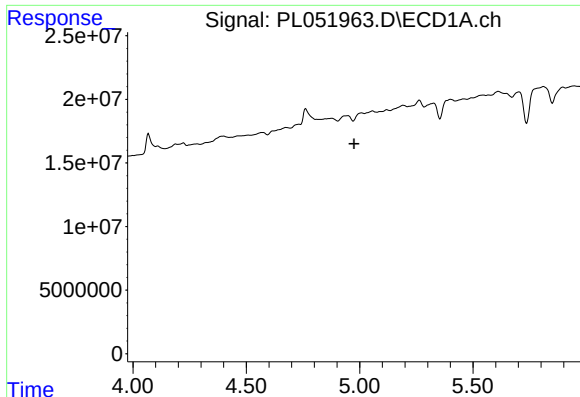

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122646BL

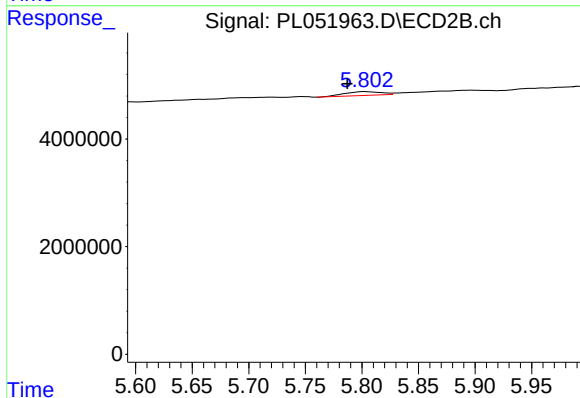


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: 0.016 min
Response: 1589122
Conc: 0.47 ng/ml

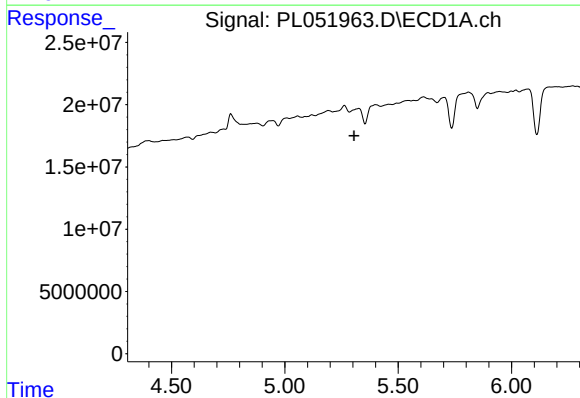


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

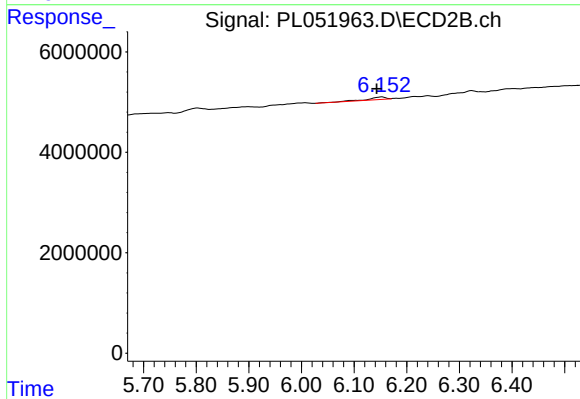

#9 Endosulfan I


R.T.: 6.153 min
Delta R.T.: 0.010 min
Response: 1151770
Conc: 0.36 ng/ml

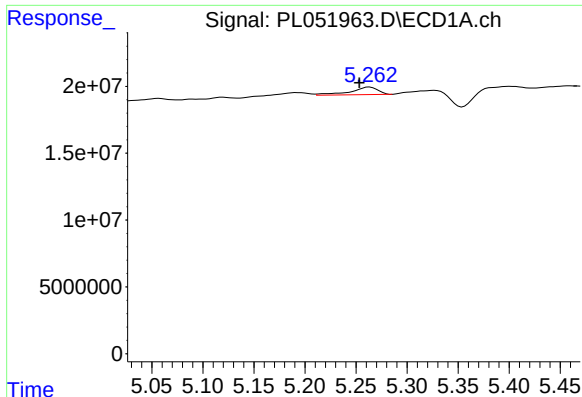

#11 alpha-Chlordane


R.T.: 5.263 min
Delta R.T.: 0.010 min
Response: 10471392
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122646BL

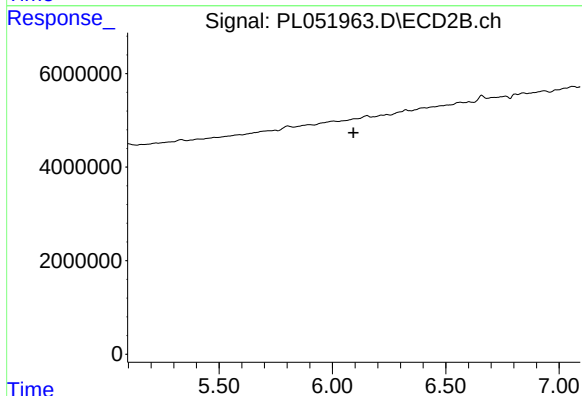


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

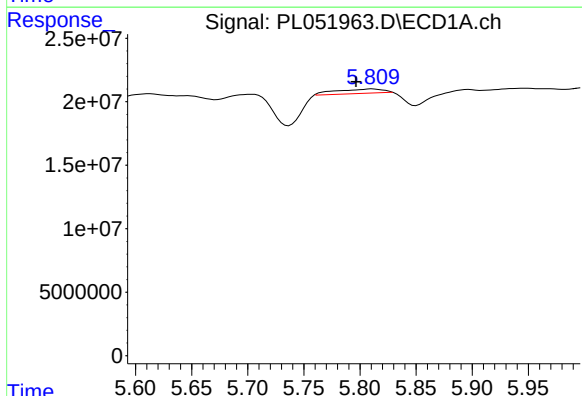


#14 Endrin

R.T.: 5.811 min
Delta R.T.: 0.014 min
Response: 10358501
Conc: 0.71 ng/ml

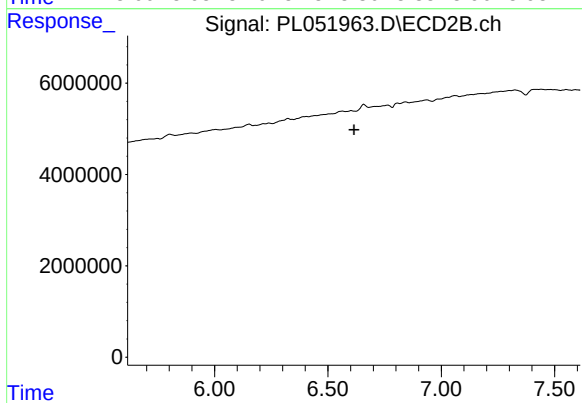

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.616 min
Response: 0
Conc: N.D.

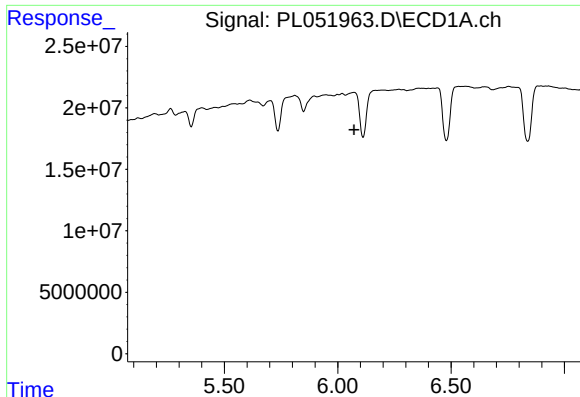

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122646BL

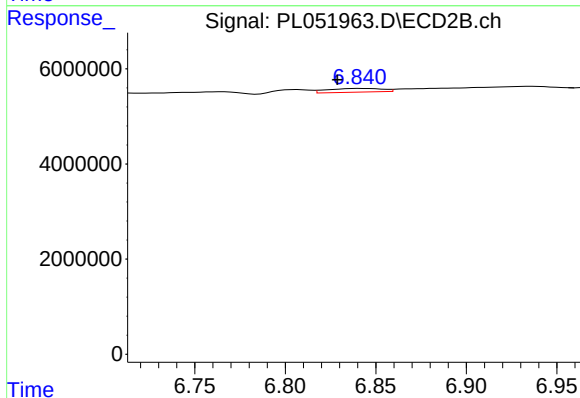


#15 Endosulfan II

R.T.: 6.842 min
Delta R.T.: 0.013 min
Response: 1657047
Conc: 0.50 ng/ml

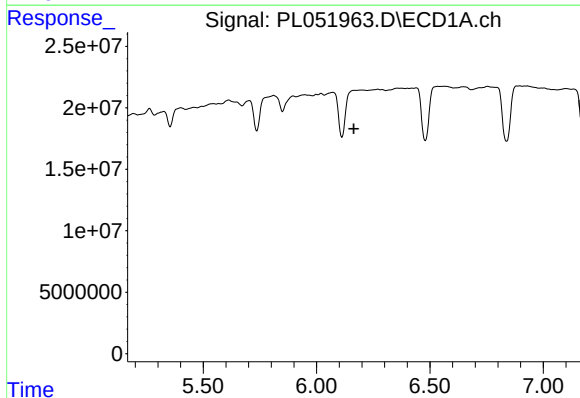


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.165 min
Response: 0
Conc: N.D.

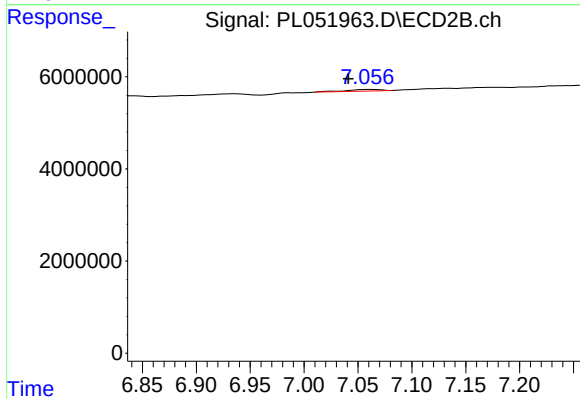

#17 4,4'-DDT


R.T.: 7.058 min
Delta R.T.: 0.017 min
Response: 751197
Conc: 0.26 ng/ml

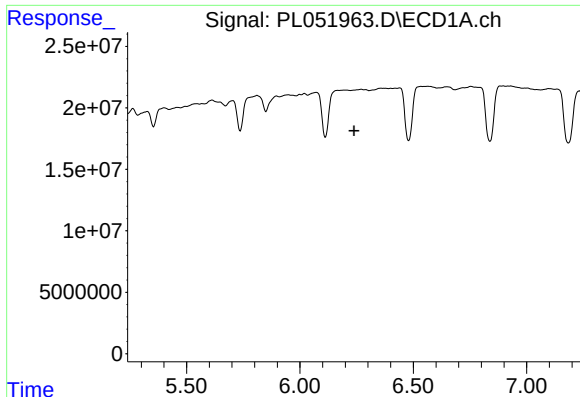

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122646BL

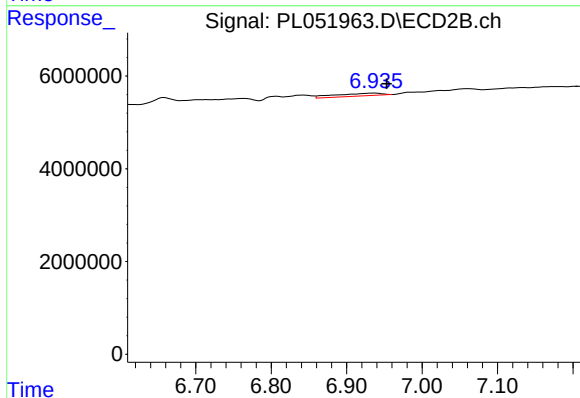


#18 Endrin aldehyde

R.T.: 6.937 min
Delta R.T.: -0.016 min
Response: 2517171
Conc: 0.89 ng/ml

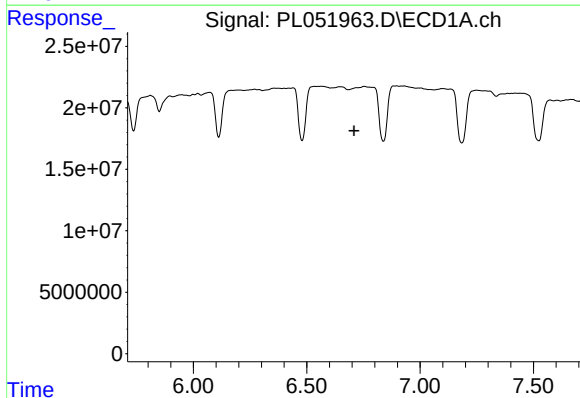


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

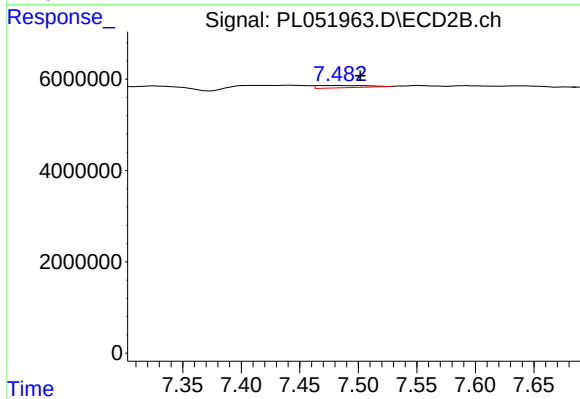

#20 Methoxychlor


R.T.: 7.483 min
Delta R.T.: -0.019 min
Response: 1417024
Conc: 0.84 ng/ml

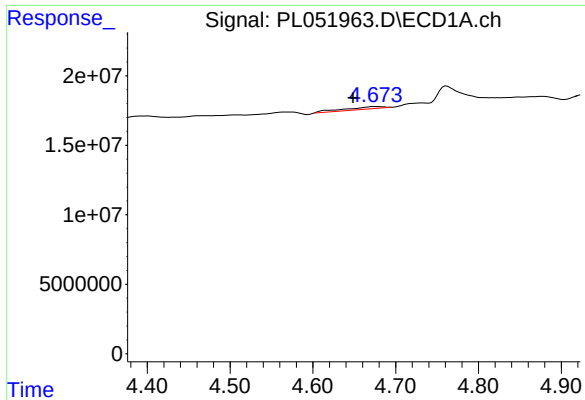

#24 Chlordane-2


R.T.: 4.674 min
Delta R.T.: 0.026 min
Response: 5636641
Conc: 13.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122646BL

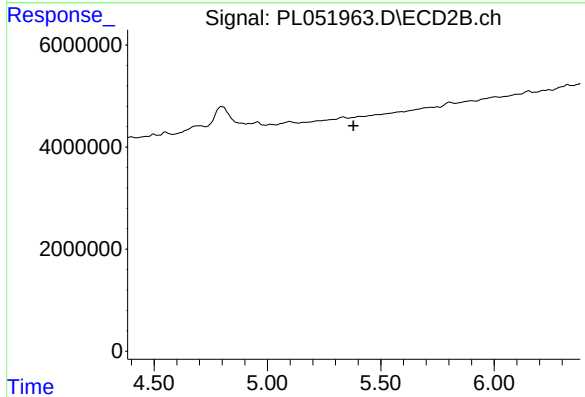


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.380 min
Response: 0
Conc: N.D.

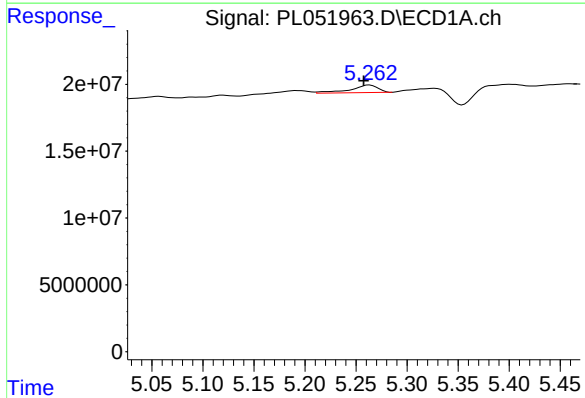


#26 Chlordane-4

R.T.: 5.263 min
Delta R.T.: 0.006 min
Response: 10471392
Conc: 8.59 ng/ml

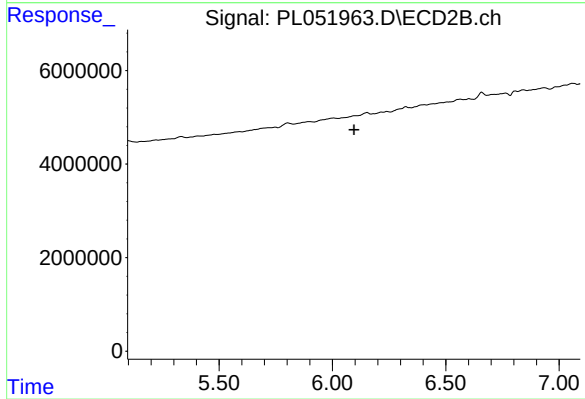

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

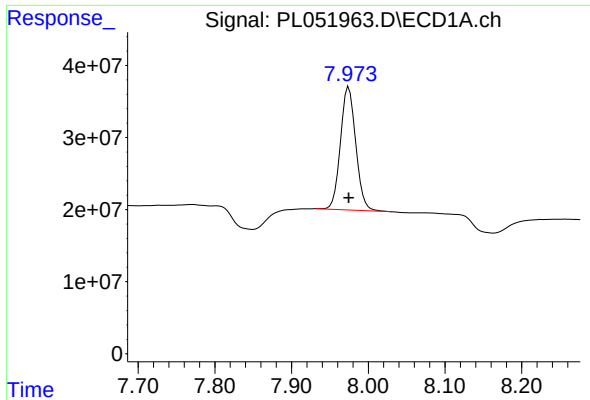

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 237015381
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122646BL

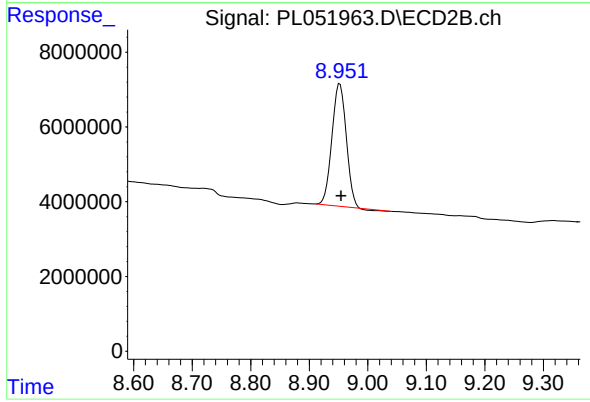

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 55215106
Conc: 18.14 ng/ml