

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 14:20
 Operator : SG\AJ
 Sample : K4439-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-1-(1-3)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:45:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.923	86891290	22589750	10.152	10.339
28)	SA Decachlor...	7.973	8.950	133.1E6	34088348	10.964	11.199
Target Compounds							
5)	MB Aldrin	4.527	5.383f	18225660	335820	1.261	0.102 #
6)	B beta-BHC	0.000	4.800f	0	2711623	N.D.	1.861 #
9)	A Endosulfan I	0.000	6.167f	0	1714051	N.D.	0.530 #
12)	B 4,4'-DDE	0.000	6.246	0	2848526	N.D.	0.809 #
15)	B Endosulfa...	0.000	6.846f	0	1147989	N.D.	0.348 #
22)	Mirex	0.000	8.118f	0	6535068	N.D.	2.686 #
23)	Chlordane-1	4.156	0.000	5883642	0	18.263	N.D. #
24)	Chlordane-2	0.000	5.383	0	335820	N.D.	3.346 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 14:20
Operator : SG\AJ
Sample : K4439-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:45:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

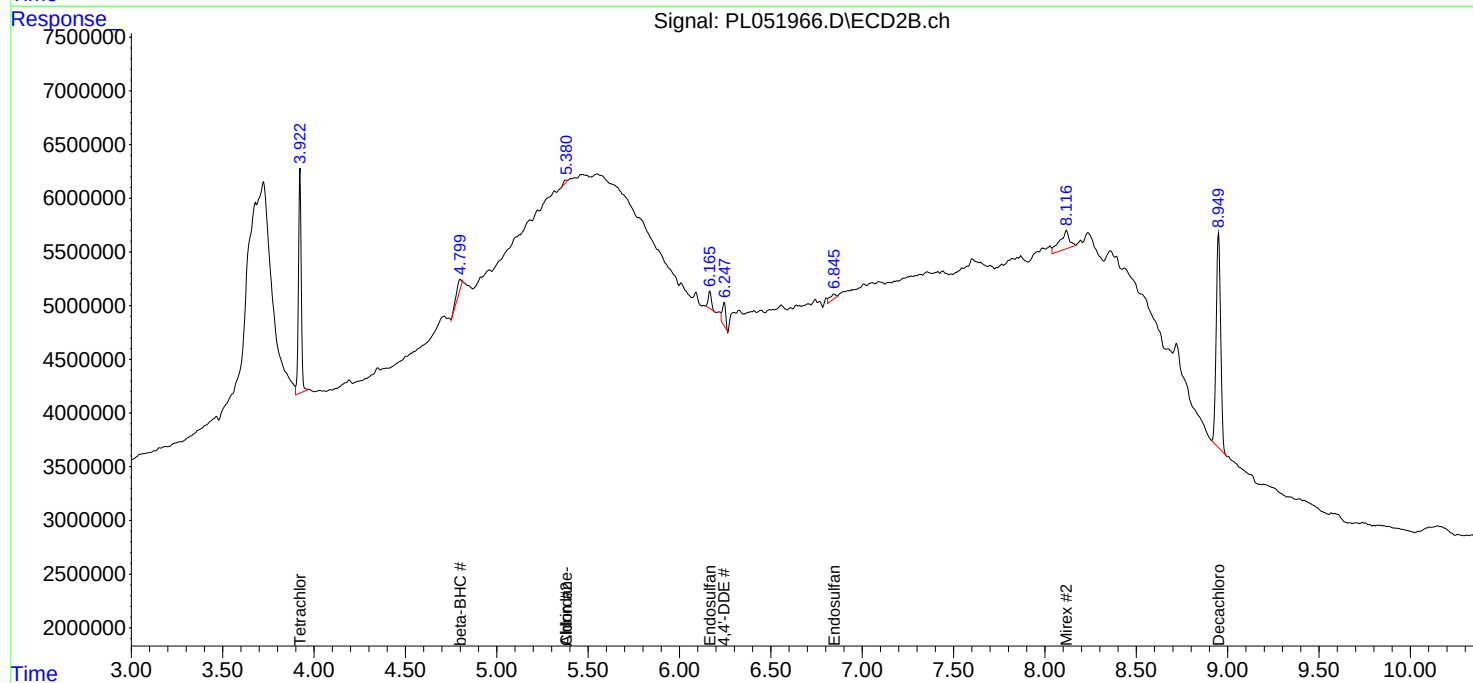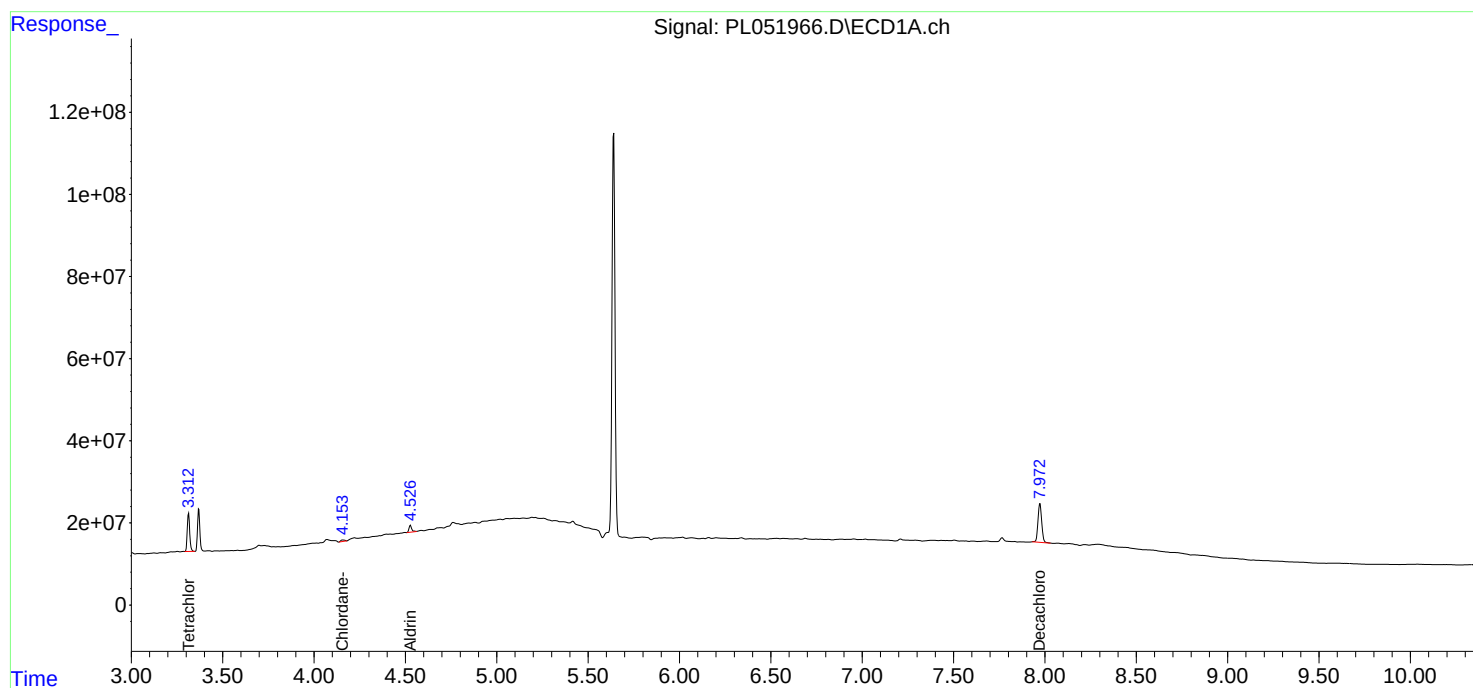


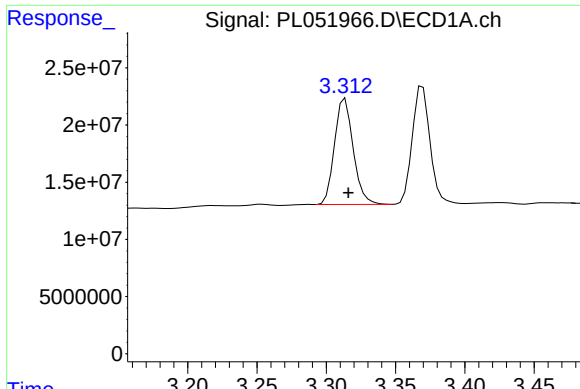

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 86891290
Conc: 10.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

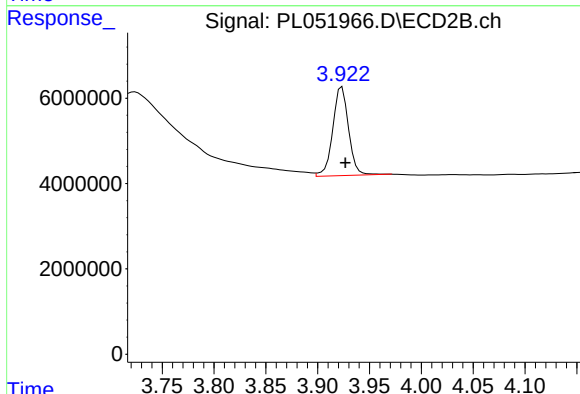


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 22589750
Conc: 10.34 ng/ml

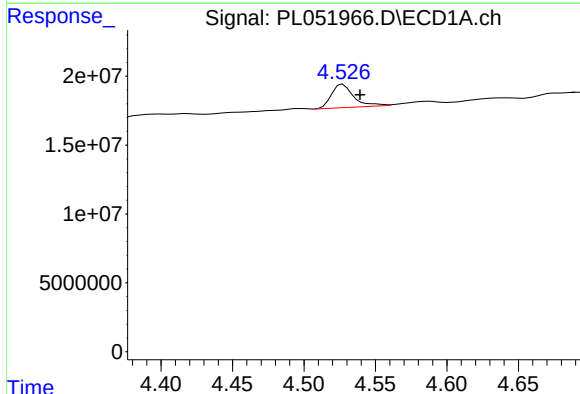


#5 Aldrin

R.T.: 4.527 min
Delta R.T.: -0.012 min
Response: 18225660
Conc: 1.26 ng/ml

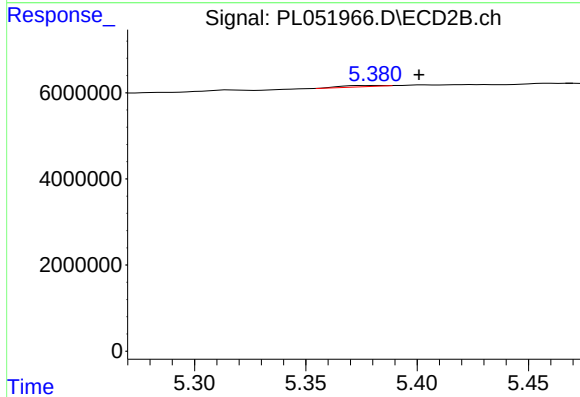

#5 Aldrin


R.T.: 5.383 min
Delta R.T.: -0.018 min
Response: 335820
Conc: 0.10 ng/ml

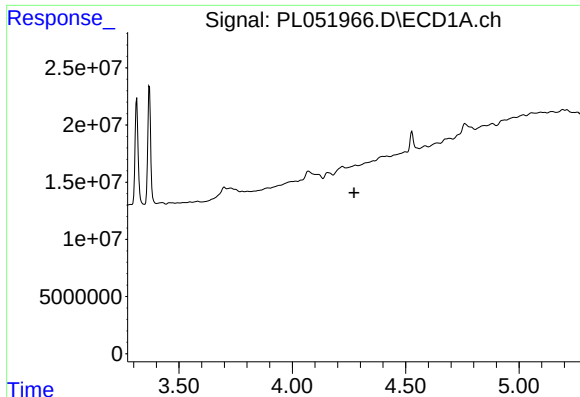

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

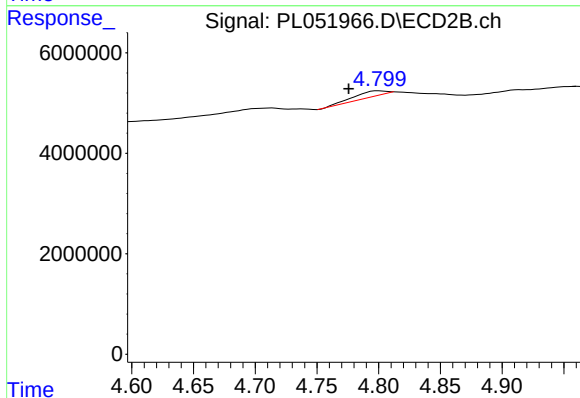


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.024 min
Response: 2711623
Conc: 1.86 ng/ml

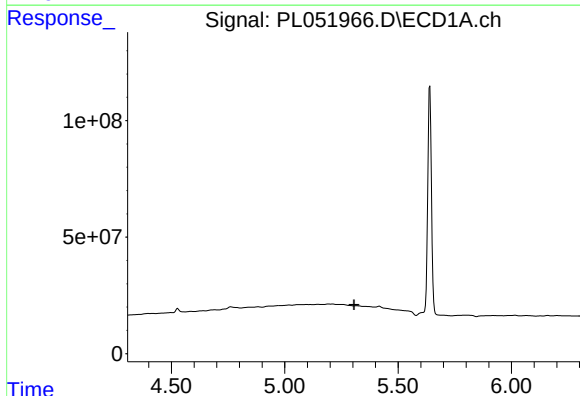


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

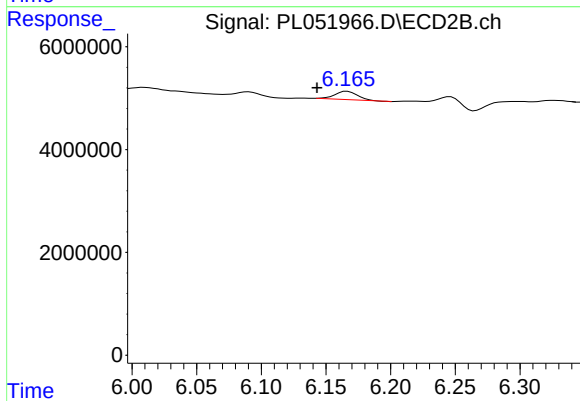

#9 Endosulfan I


R.T.: 6.167 min
Delta R.T.: 0.024 min
Response: 1714051
Conc: 0.53 ng/ml

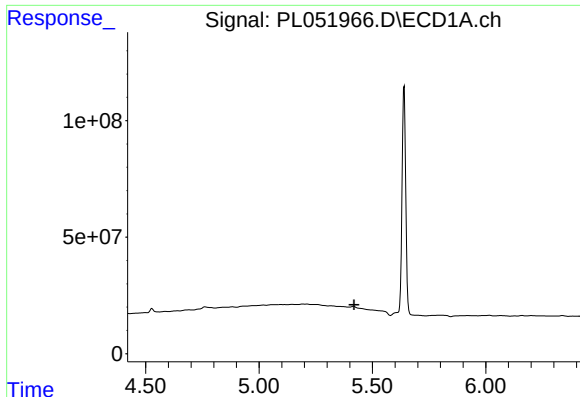

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

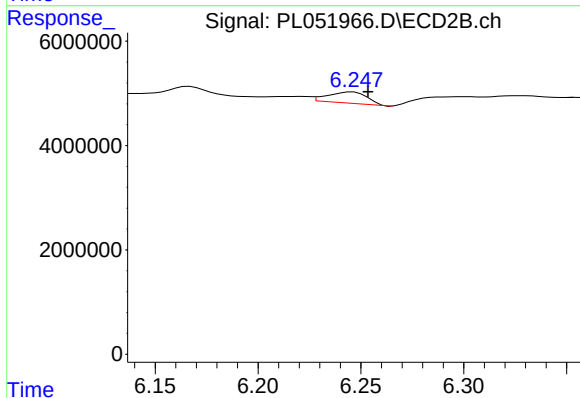


#12 4,4'-DDE

R.T.: 6.246 min
Delta R.T.: -0.007 min
Response: 2848526
Conc: 0.81 ng/ml

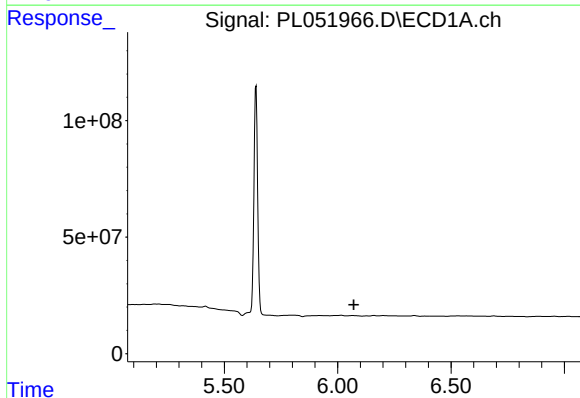


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

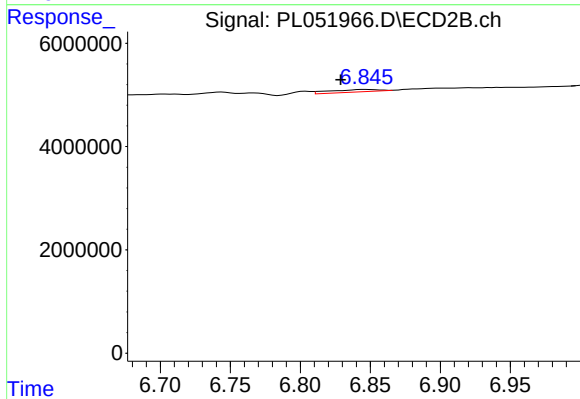

#15 Endosulfan II


R.T.: 6.846 min
Delta R.T.: 0.018 min
Response: 1147989
Conc: 0.35 ng/ml

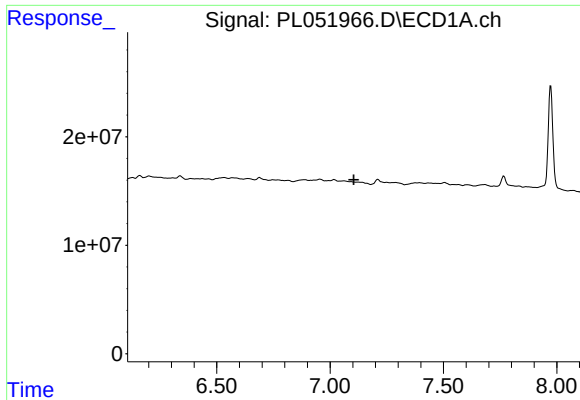

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

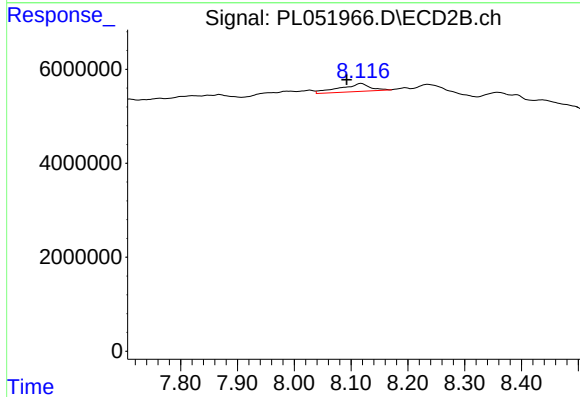


#22 Mirex

R.T.: 8.118 min
Delta R.T.: 0.026 min
Response: 6535068
Conc: 2.69 ng/ml

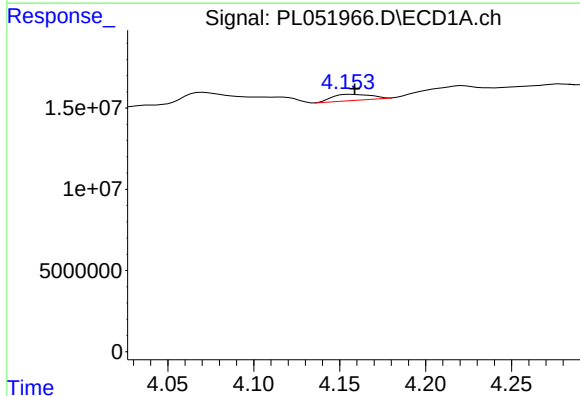


#23 Chlordane-1

R.T.: 4.156 min
Delta R.T.: -0.003 min
Response: 5883642
Conc: 18.26 ng/ml

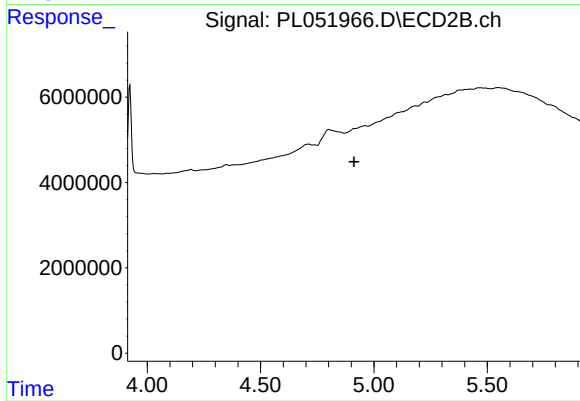

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.913 min
Response: 0
Conc: N.D.

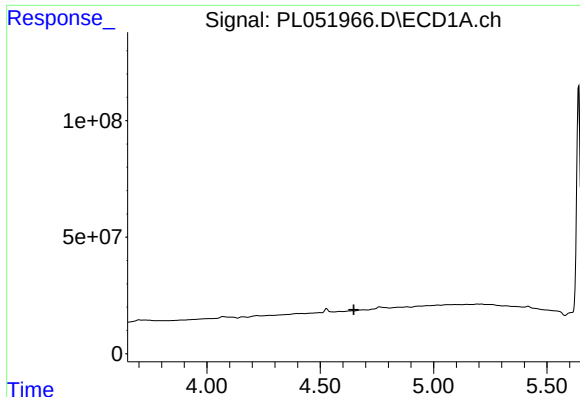

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.649 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-1-(1-3)

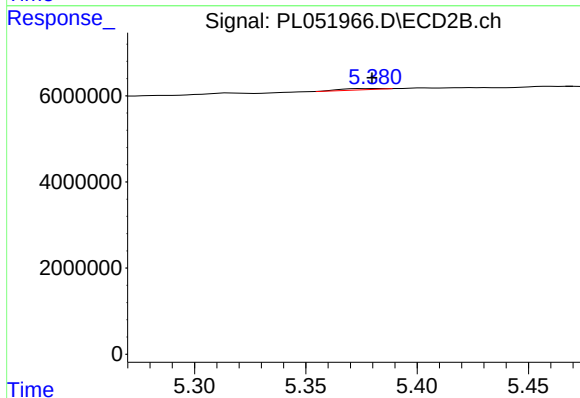


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.003 min
Response: 335820
Conc: 3.35 ng/ml

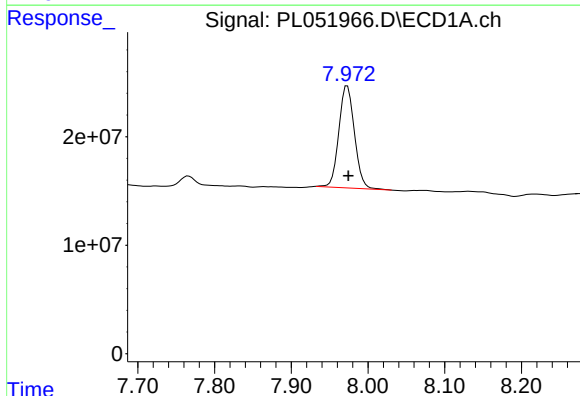

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 133073880
Conc: 10.96 ng/ml

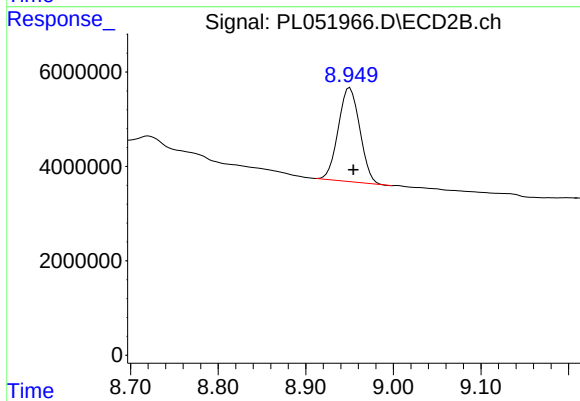

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 34088348
Conc: 11.20 ng/ml