

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 15:59
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:47:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	222.5E6	51746334	25.995	23.685
28)	SA Decachlor...	7.972	8.950	228.7E6	63245581	18.844	20.778
Target Compounds							
8)	B Heptachlo...	0.000	5.785	0	7793439	N.D.	2.309 #
9)	A Endosulfan I	5.324f	0.000	628815	0	0.047	N.D. #
13)	MA Dieldrin	5.528f	6.410	4221131	2112726	0.278	0.617 #
24)	Chlordane-2	4.622f	0.000	7841678	0	19.186	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 15:59
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:47:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

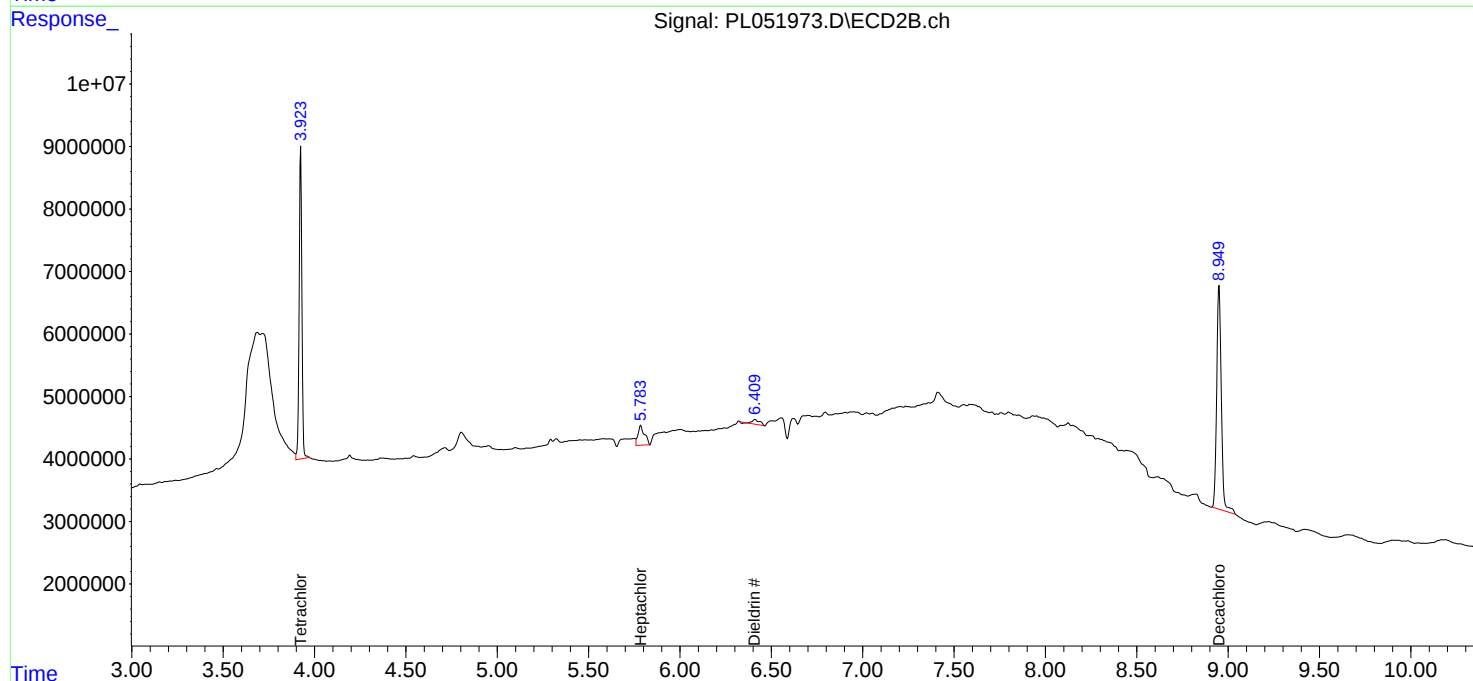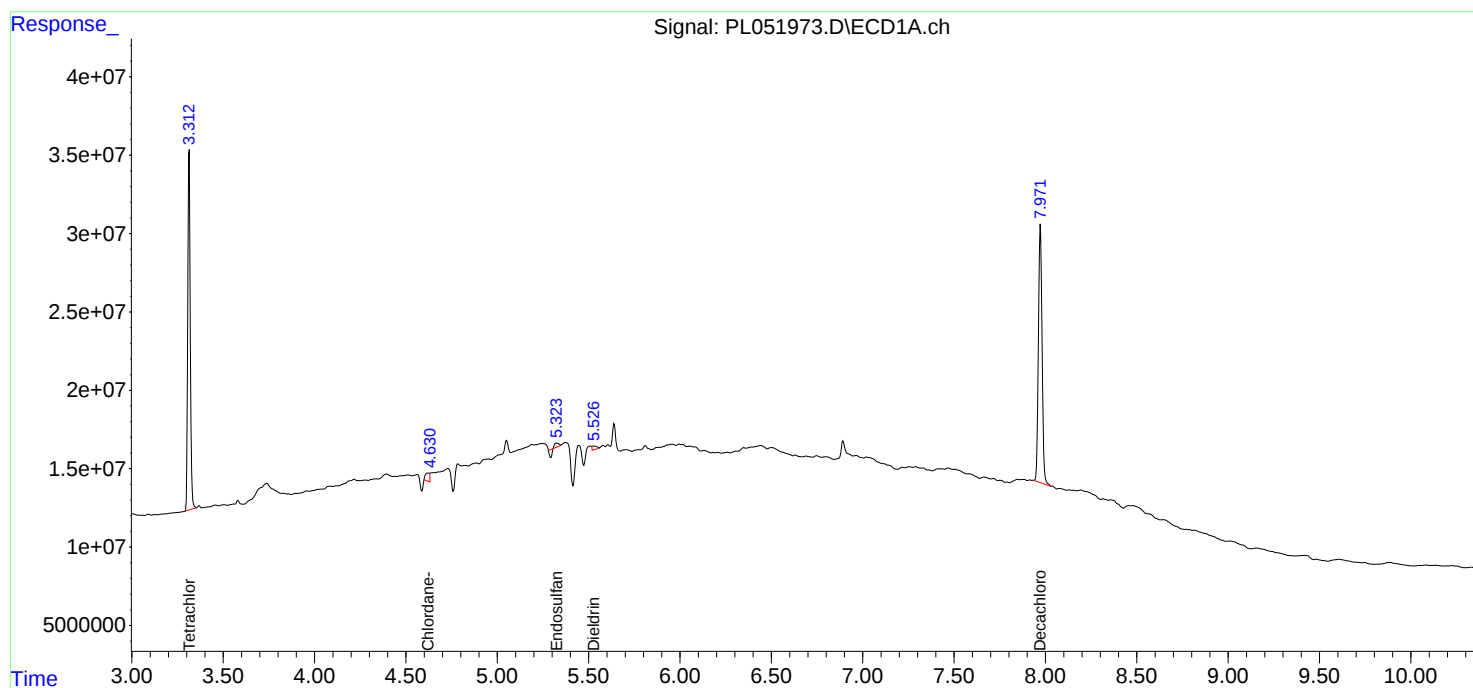


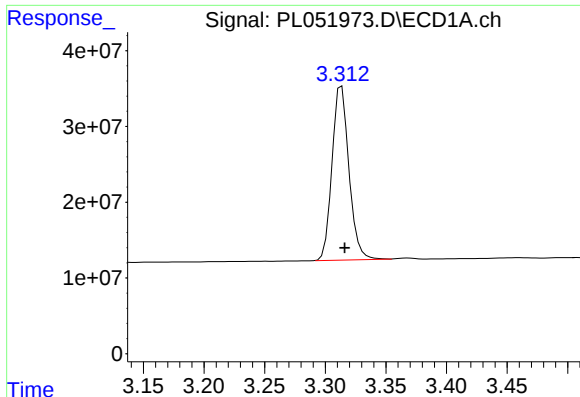

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.002 min
Response: 222477489
Conc: 25.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

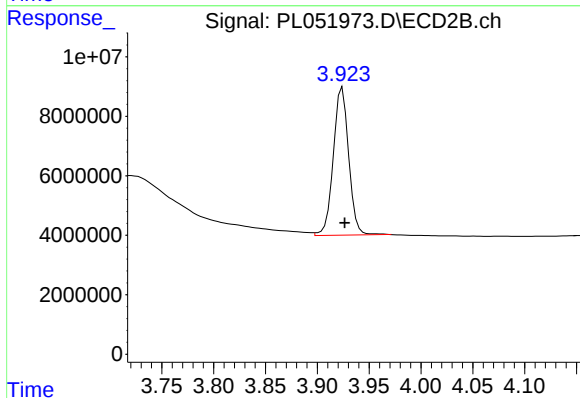


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 51746334
Conc: 23.68 ng/ml

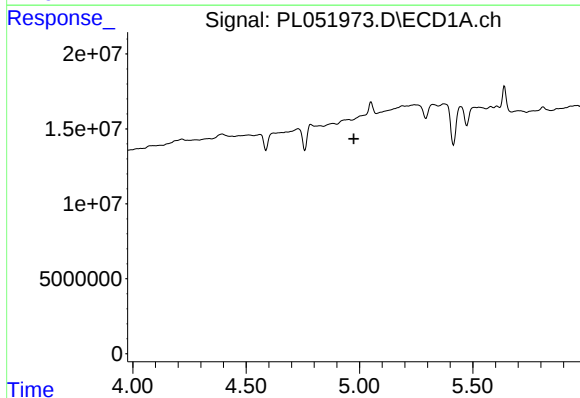


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

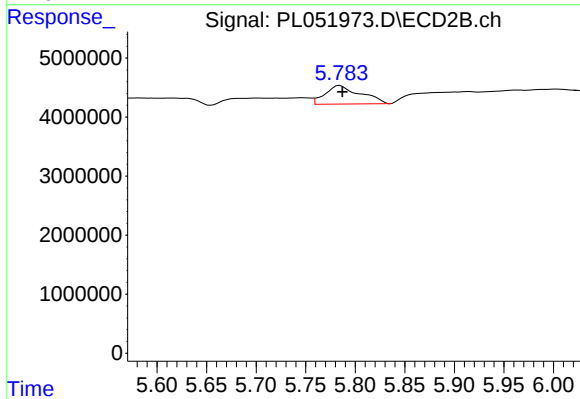

#8 Heptachlor epoxide


R.T.: 5.785 min
Delta R.T.: -0.002 min
Response: 7793439
Conc: 2.31 ng/ml

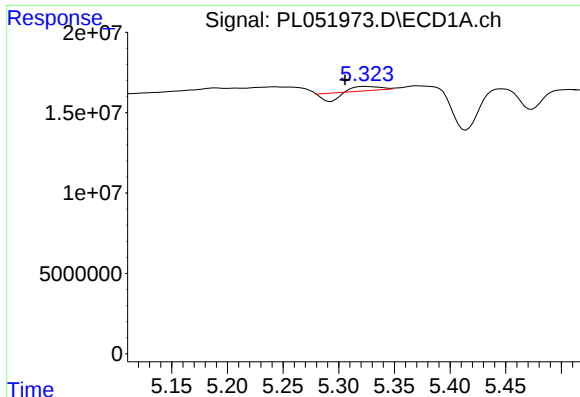

#9 Endosulfan I


R.T.: 5.324 min
Delta R.T.: 0.018 min
Response: 628815
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

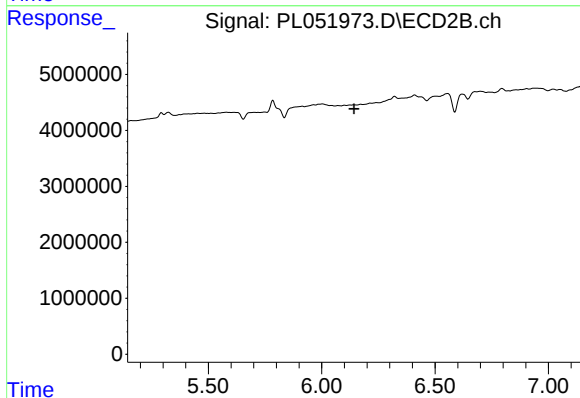


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

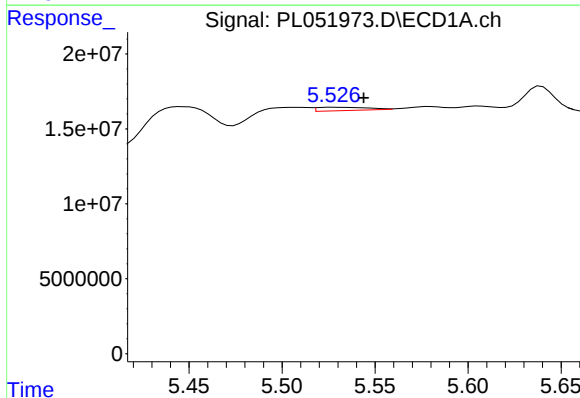


#13 Dieldrin

R.T.: 5.528 min
Delta R.T.: -0.016 min
Response: 4221131
Conc: 0.28 ng/ml

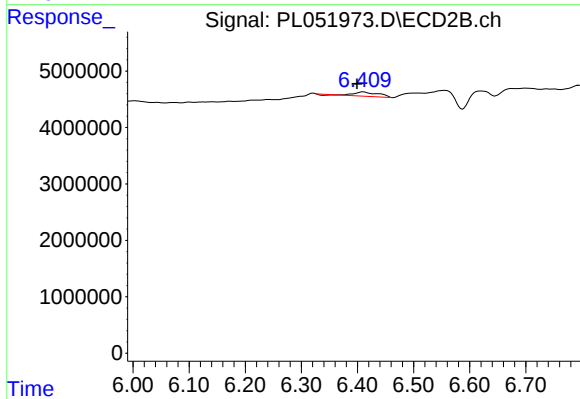

#13 Dieldrin


R.T.: 6.410 min
Delta R.T.: 0.011 min
Response: 2112726
Conc: 0.62 ng/ml

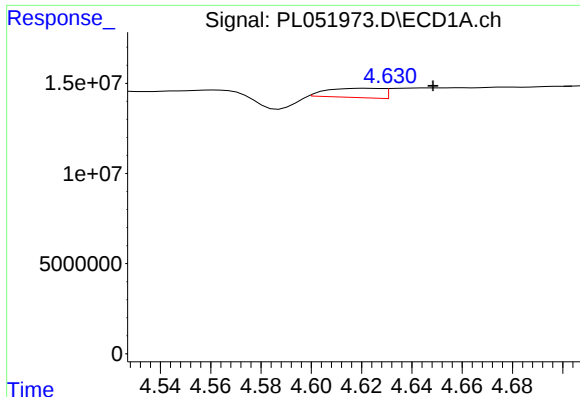

#24 Chlordane-2


R.T.: 4.622 min
Delta R.T.: -0.027 min
Response: 7841678
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

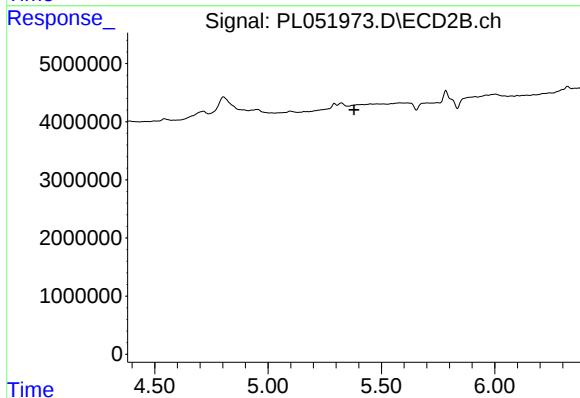


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

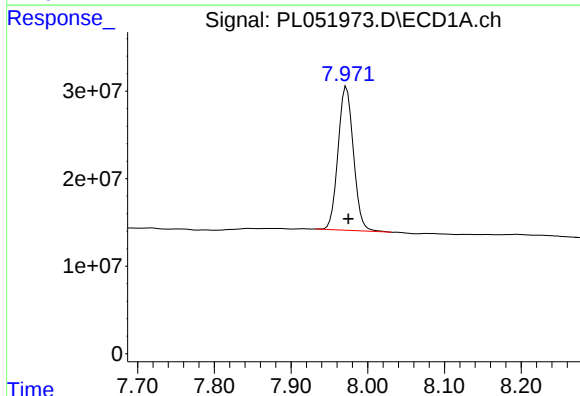

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 228730158
Conc: 18.84 ng/ml

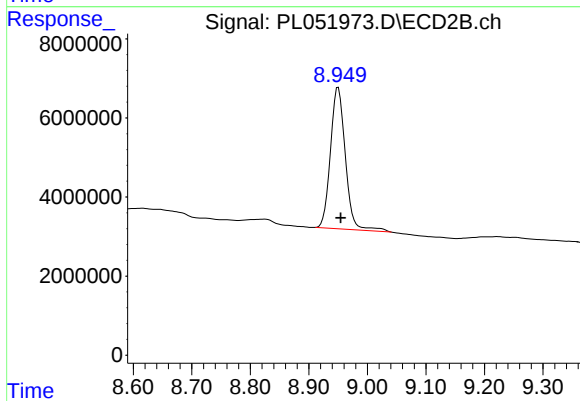

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 63245581
Conc: 20.78 ng/ml