

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 21:27
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:52:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	219.7E6	51495895	25.666	23.570
28)	SA Decachlor...	7.972	8.950	273.9E6	67850818	22.570	22.291
Target Compounds							
3)	MA gamma-BHC...	0.000	4.609	0	42962	N.D.	0.014 #
6)	B beta-BHC	0.000	4.802f	0	739185	N.D.	0.507 #
8)	B Heptachlo...	0.000	5.784	0	10858197	N.D.	3.217 #
9)	A Endosulfan I	5.327f	6.122f	15365752	489032	1.143	0.151 #
11)	B alpha-Chl...	0.000	6.122f	0	489032	N.D.	0.142 #
15)	B Endosulfa...	6.068	6.843	18892200	1067879	1.358	0.324 #
17)	MA 4,4'-DDT	0.000	7.056	0	1088337	N.D.	0.372 #
18)	B Endrin al...	0.000	6.980f	0	2257730	N.D.	0.799 #
26)	Chlordane-4	0.000	6.122f	0	489032	N.D.	0.900 #
27)	Chlordane-5	6.068	0.000	18892200	0	38.499	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 21:27
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:52:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

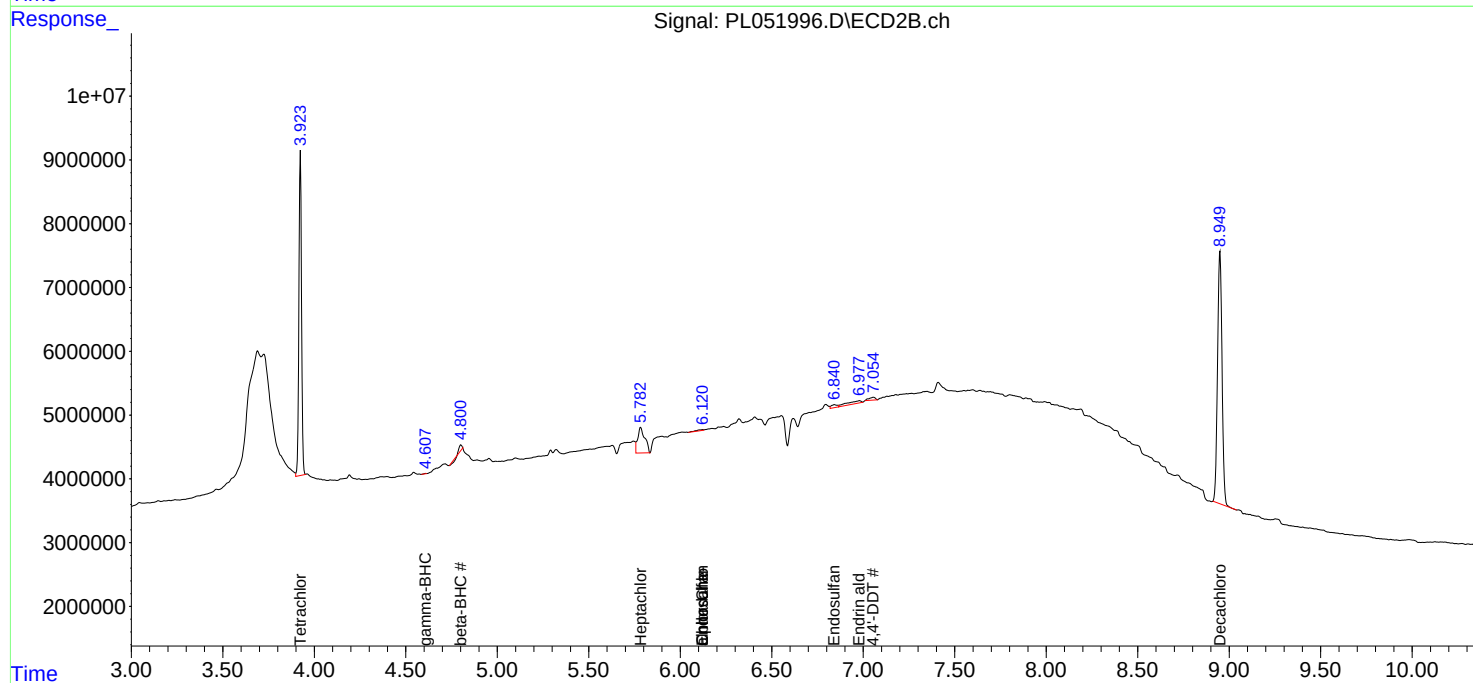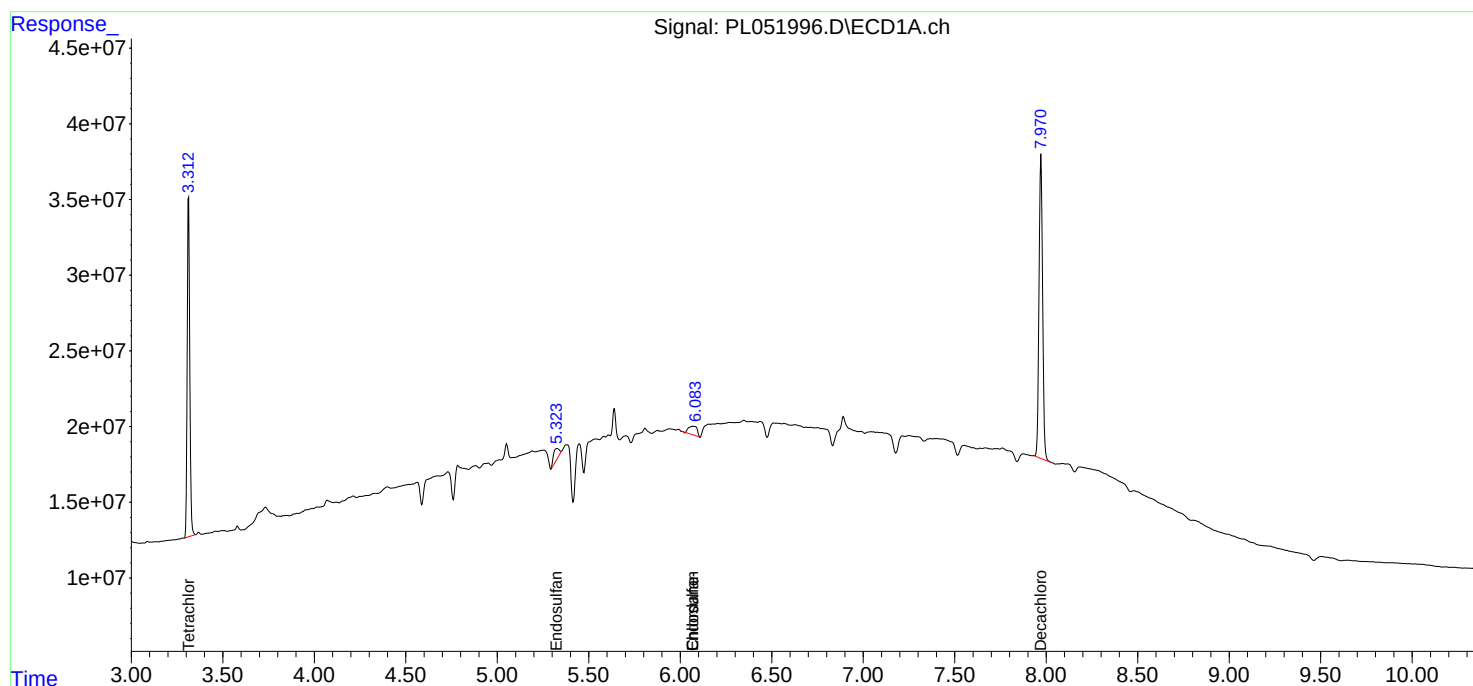


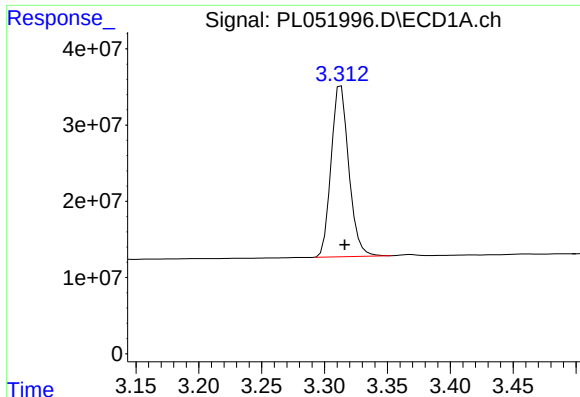

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 21966538
Conc: 25.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

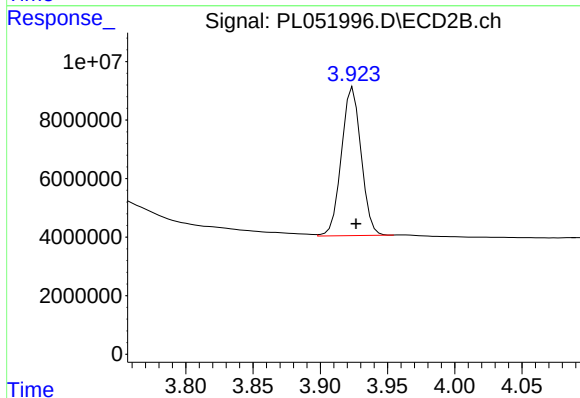


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 51495895
Conc: 23.57 ng/ml

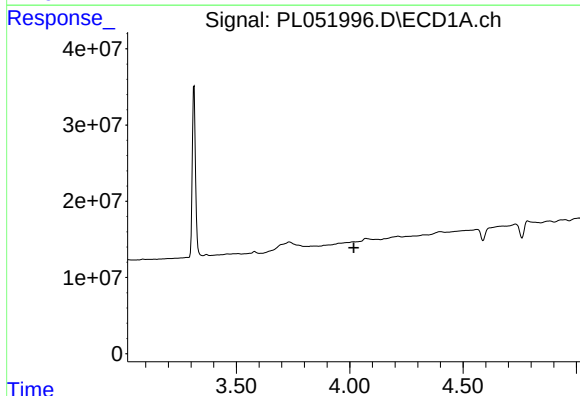


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

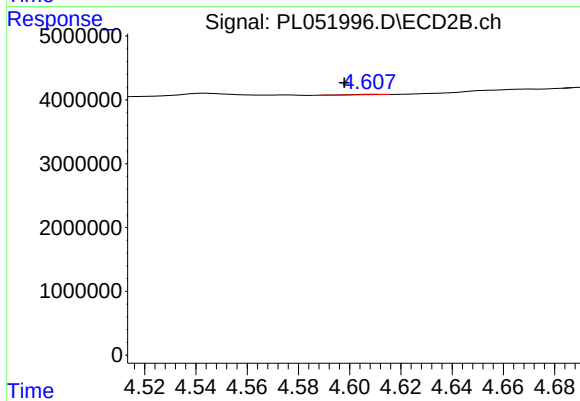

#3 gamma-BHC (Lindane)


R.T.: 4.609 min
Delta R.T.: 0.012 min
Response: 42962
Conc: 0.01 ng/ml

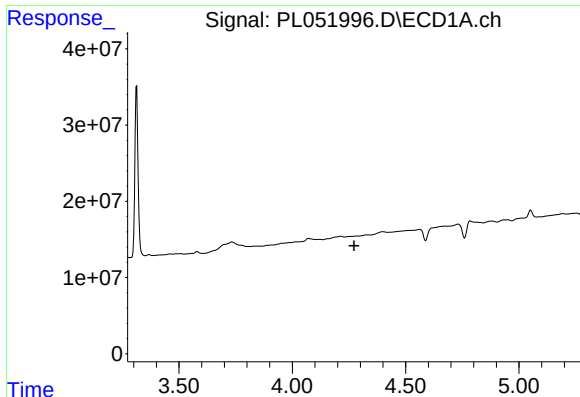

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

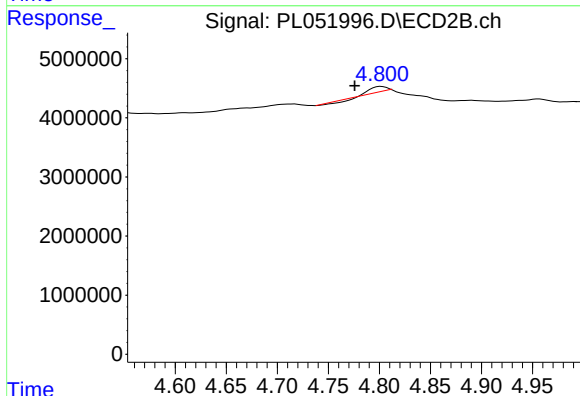


#6 beta-BHC

R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 739185
Conc: 0.51 ng/ml

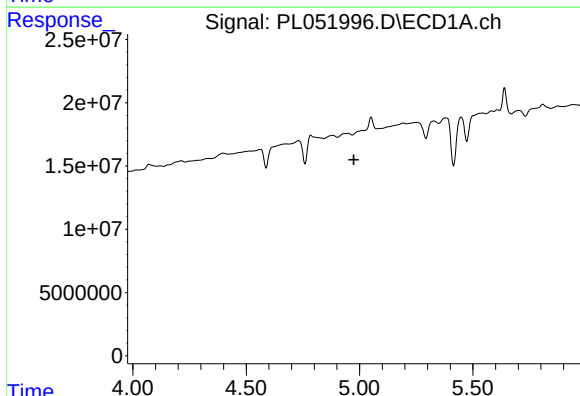


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

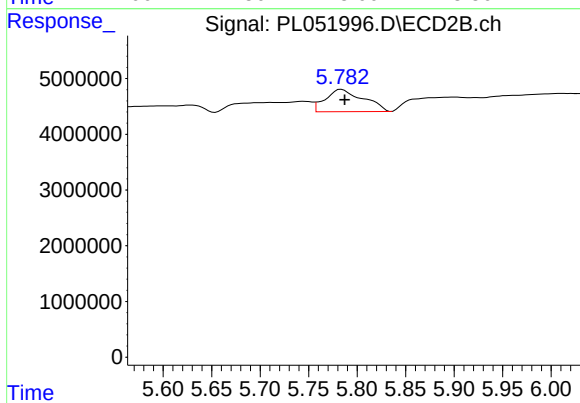

#8 Heptachlor epoxide


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 10858197
Conc: 3.22 ng/ml

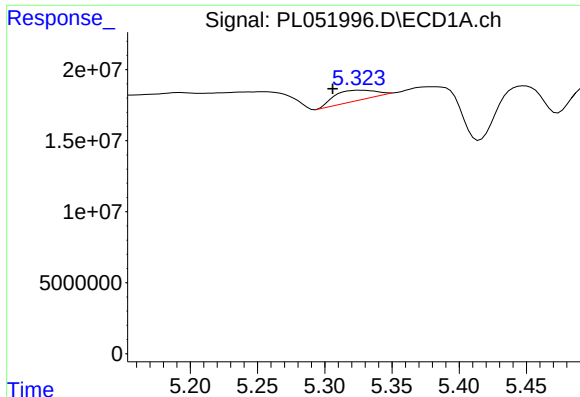

#9 Endosulfan I


R.T.: 5.327 min
Delta R.T.: 0.021 min
Response: 15365752
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

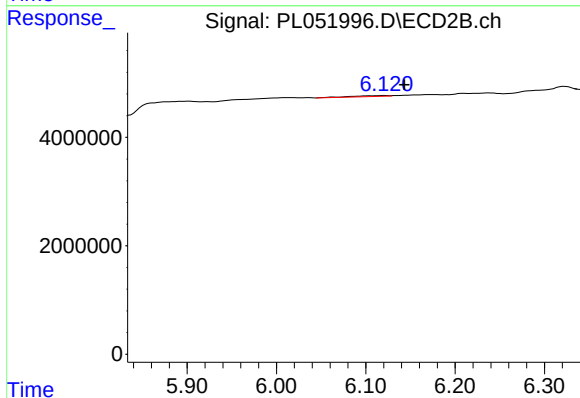


#9 Endosulfan I

R.T.: 6.122 min
Delta R.T.: -0.021 min
Response: 489032
Conc: 0.15 ng/ml

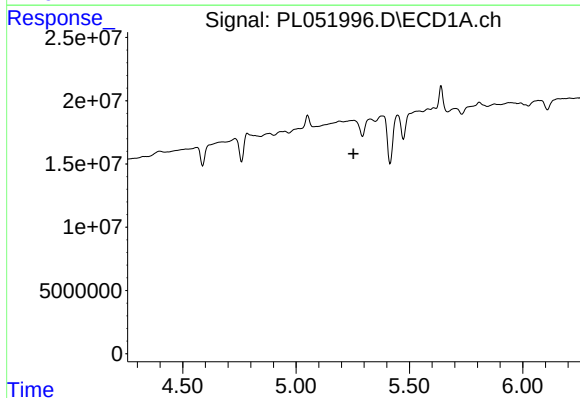


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.253 min
Response: 0
Conc: N.D.

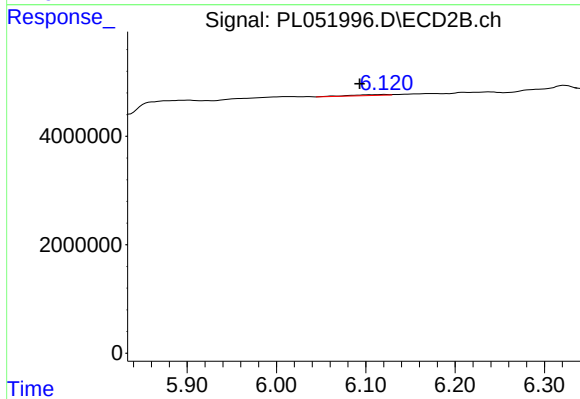

#11 alpha-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.028 min
Response: 489032
Conc: 0.14 ng/ml

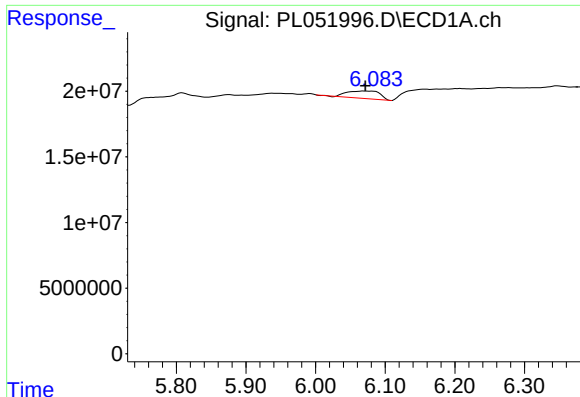

#15 Endosulfan II


R.T.: 6.068 min
Delta R.T.: -0.003 min
Response: 18892200
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

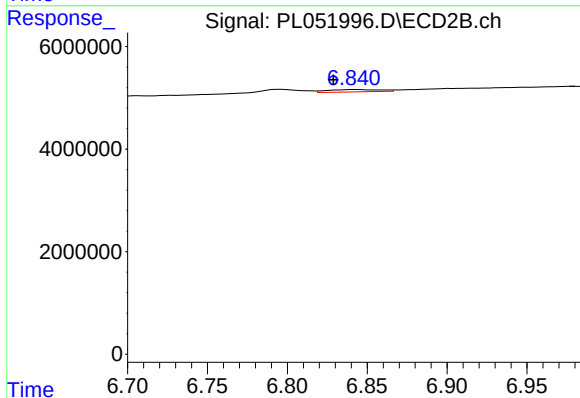


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 1067879
Conc: 0.32 ng/ml

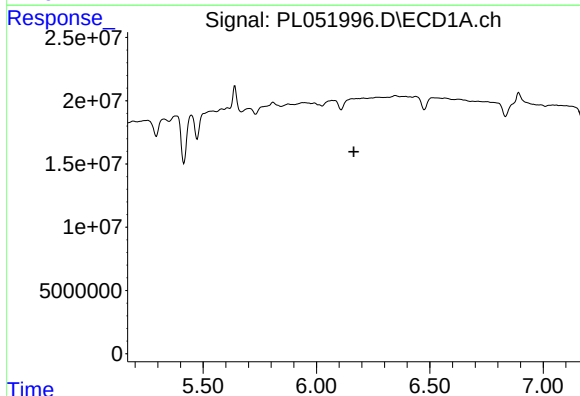


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.165 min
Response: 0
Conc: N.D.

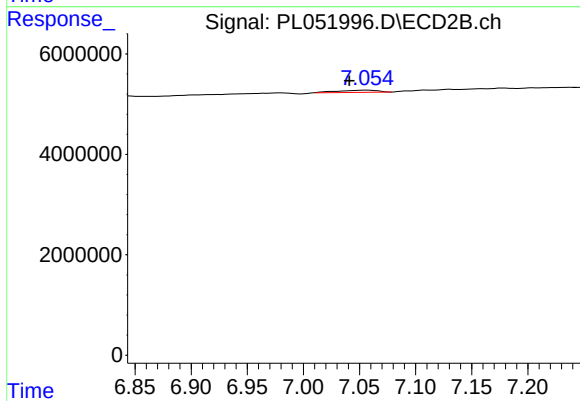

#17 4,4'-DDT


R.T.: 7.056 min
Delta R.T.: 0.015 min
Response: 1088337
Conc: 0.37 ng/ml

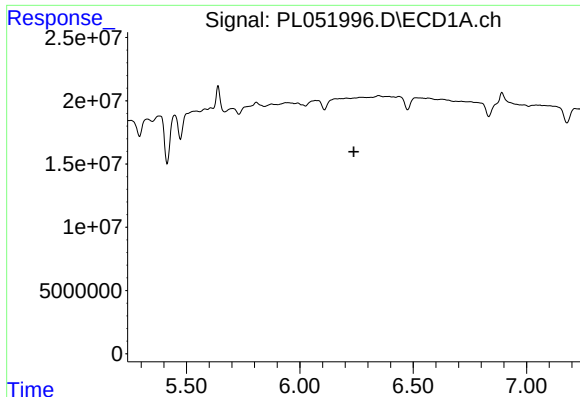

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

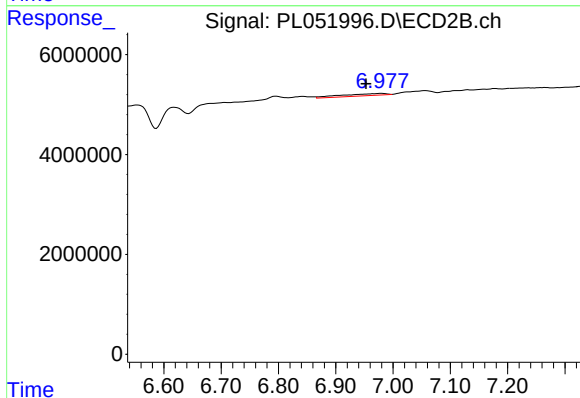


#18 Endrin aldehyde

R.T.: 6.980 min
Delta R.T.: 0.027 min
Response: 2257730
Conc: 0.80 ng/ml

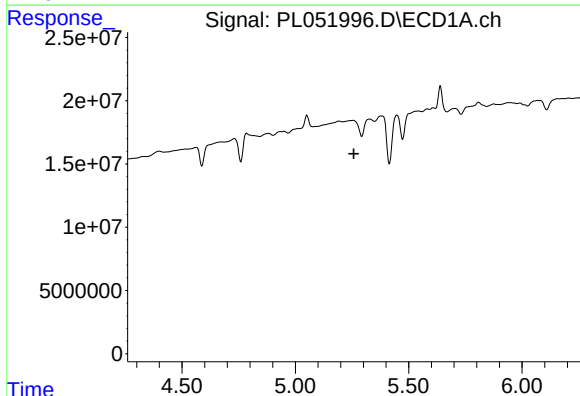


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

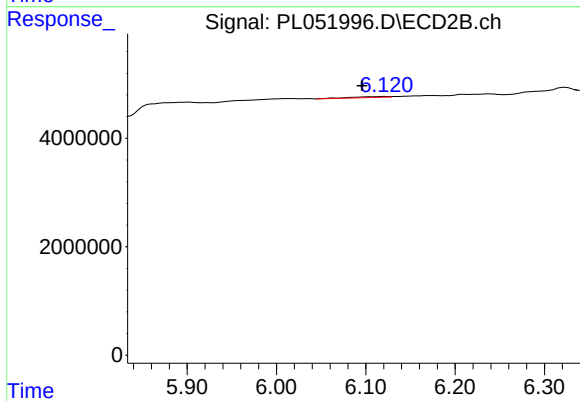

#26 Chlordane-4


R.T.: 6.122 min
Delta R.T.: 0.026 min
Response: 489032
Conc: 0.90 ng/ml

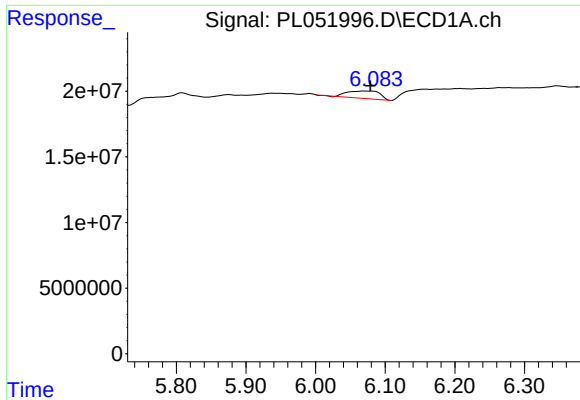

#27 Chlordane-5


R.T.: 6.068 min
Delta R.T.: -0.010 min
Response: 18892200
Conc: 38.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

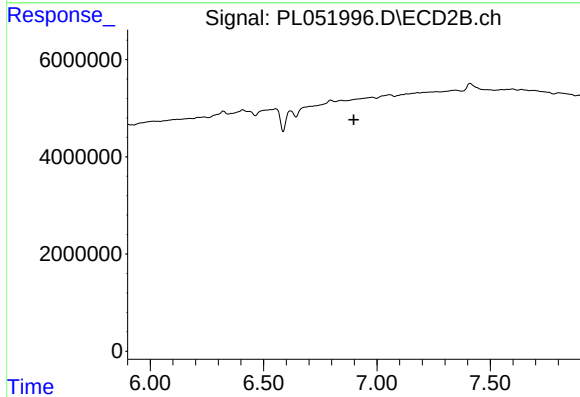


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.898 min
Response: 0
Conc: N.D.

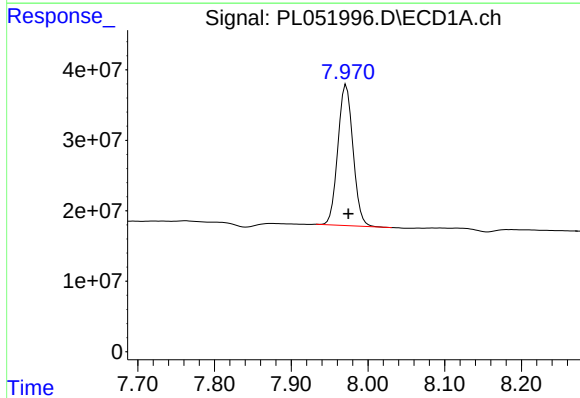

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 273949474
Conc: 22.57 ng/ml

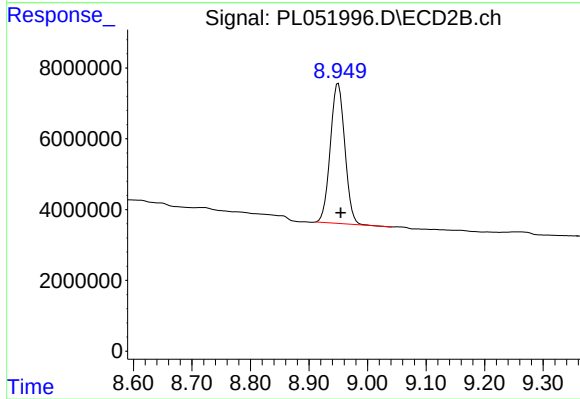

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 67850818
Conc: 22.29 ng/ml