

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL052001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 22:52
 Operator : SG\AJ
 Sample : PB122686BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122686BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:53:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	164.2E6	40767220	19.190	18.659
28)	SA Decachlor...	7.971	8.950	204.2E6	49672315	16.821	16.319
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	434455	N.D.	0.298 #
8)	B Heptachlo...	0.000	5.801	0	893270	N.D.	0.265 #
9)	A Endosulfan I	5.327f	0.000	11912106	0	0.886	N.D. #
10)	B gamma-Chl...	0.000	6.006	0	685883	N.D.	0.188 #
15)	B Endosulfa...	0.000	6.802f	0	794004	N.D.	0.241 #
18)	B Endrin al...	0.000	6.953	0	1070234	N.D.	0.379 #
20)	A Methoxychlor	0.000	7.477f	0	638952	N.D.	0.381 #
21)	B Endrin ke...	0.000	7.657	0	2532138	N.D.	0.791 #
25)	Chlordane-3	0.000	6.006f	0	685883	N.D.	1.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL052001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 22:52
Operator : SG\AJ
Sample : PB122686BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB122686BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:53:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

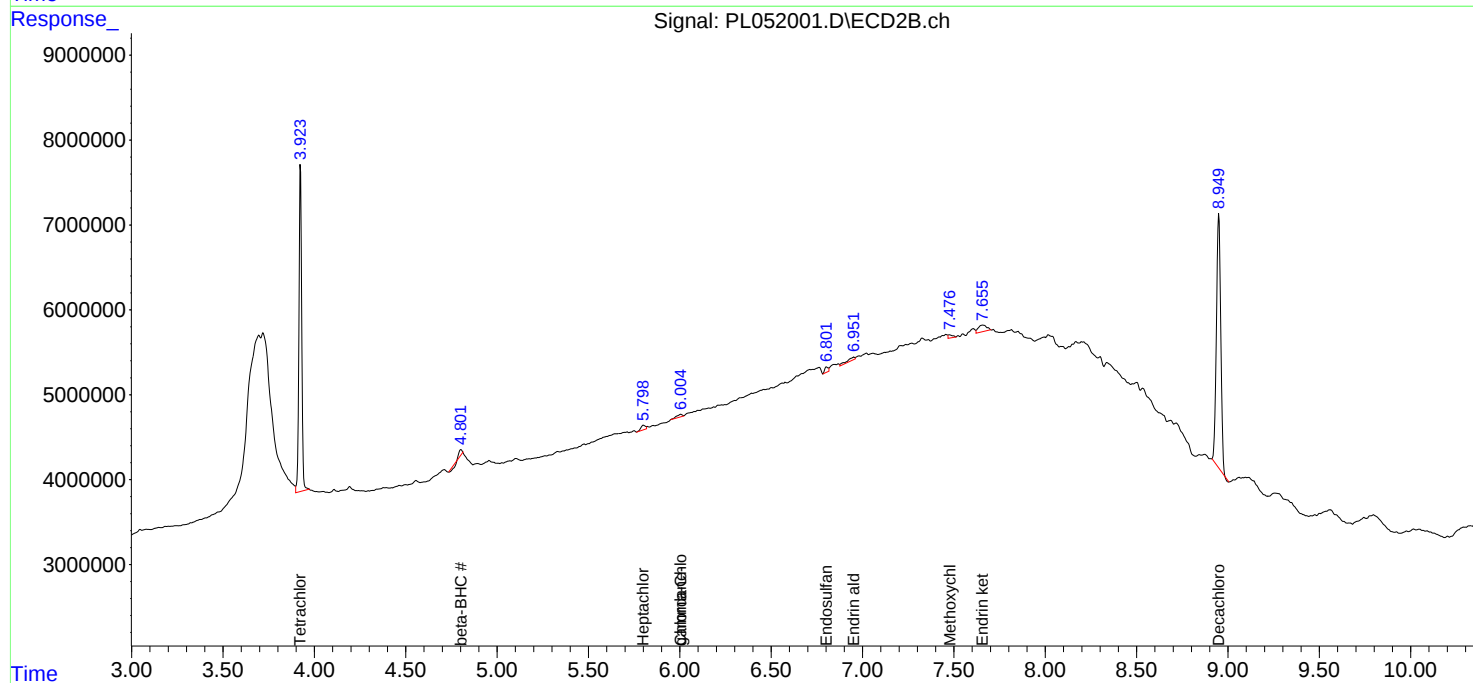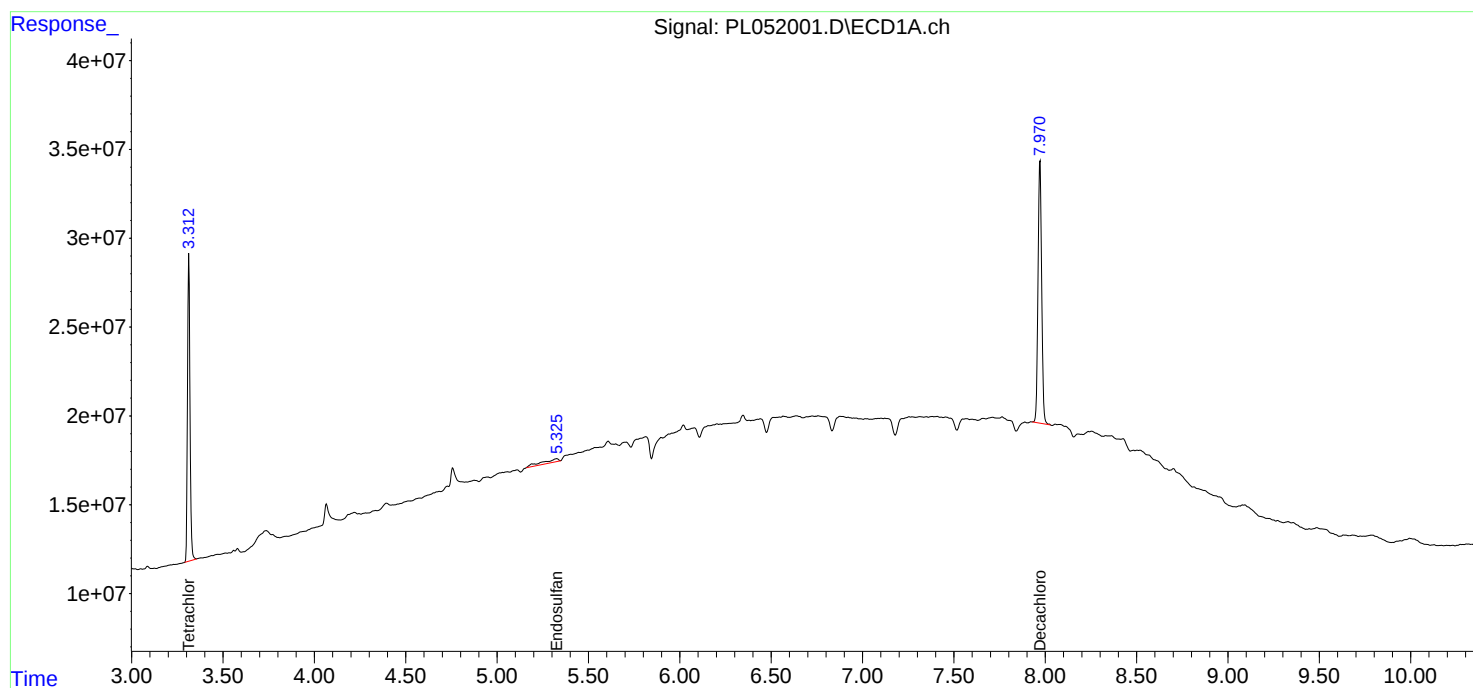


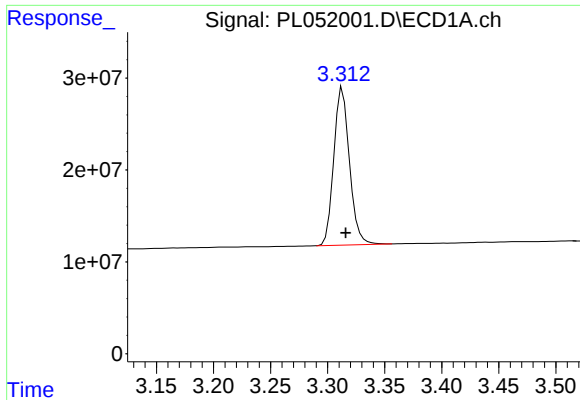

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 164240773
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122686BL

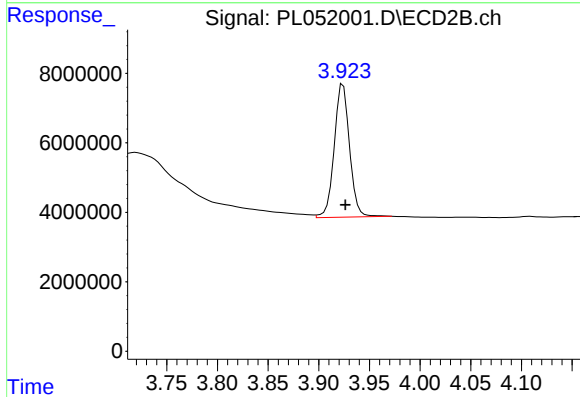


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 40767220
Conc: 18.66 ng/ml

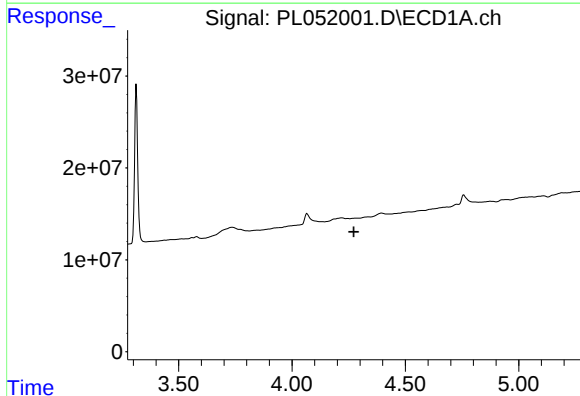


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

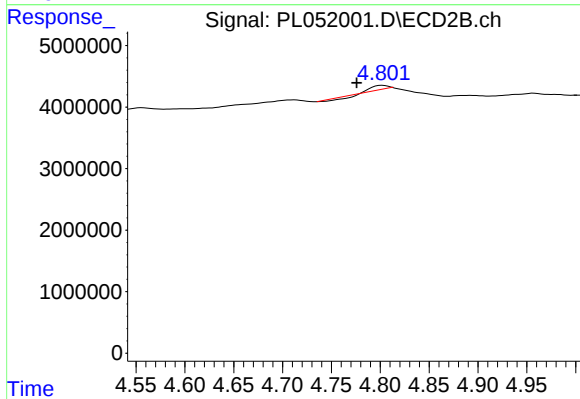

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 434455
Conc: 0.30 ng/ml

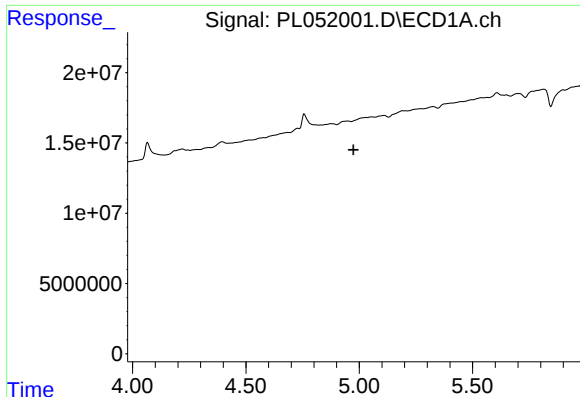

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122686BL

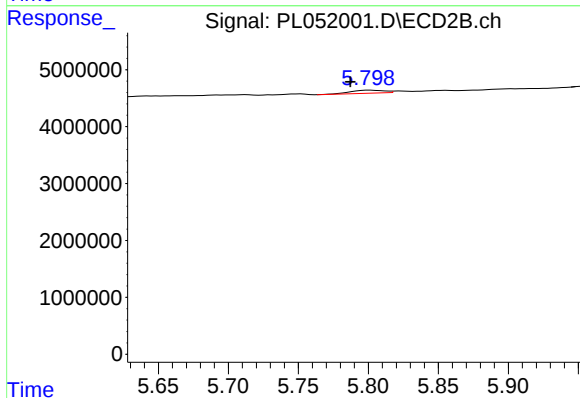


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: 0.014 min
Response: 893270
Conc: 0.26 ng/ml

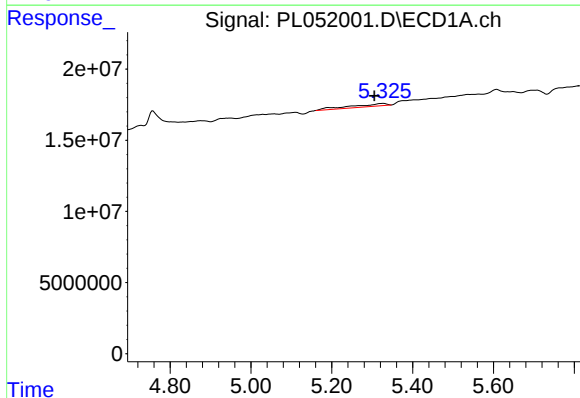


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.022 min
Response: 11912106
Conc: 0.89 ng/ml

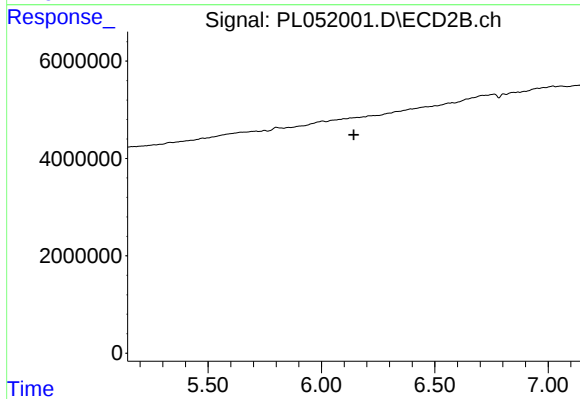

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

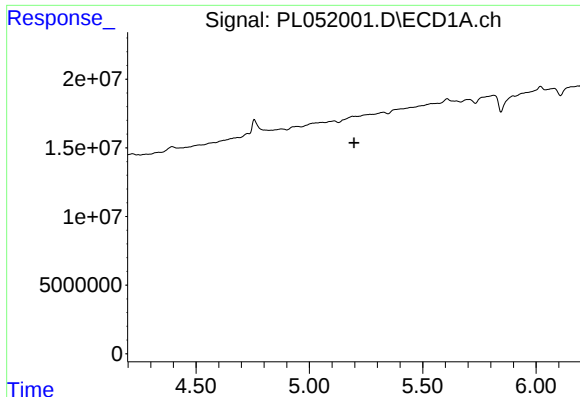

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122686BL

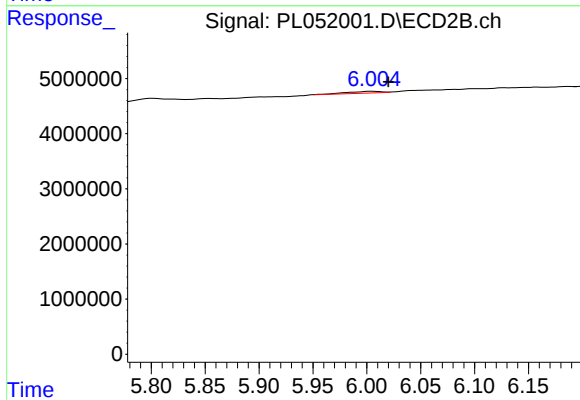


#10 gamma-Chlordane

R.T.: 6.006 min
Delta R.T.: -0.015 min
Response: 685883
Conc: 0.19 ng/ml

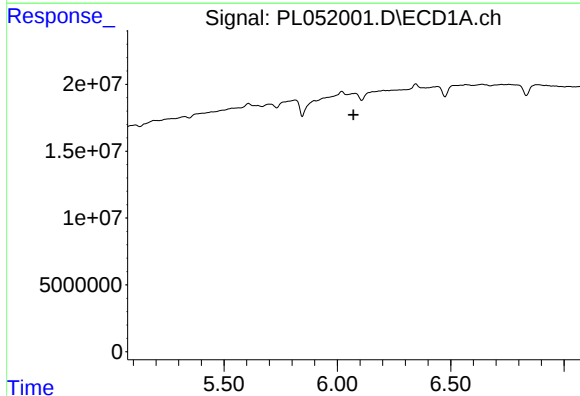


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

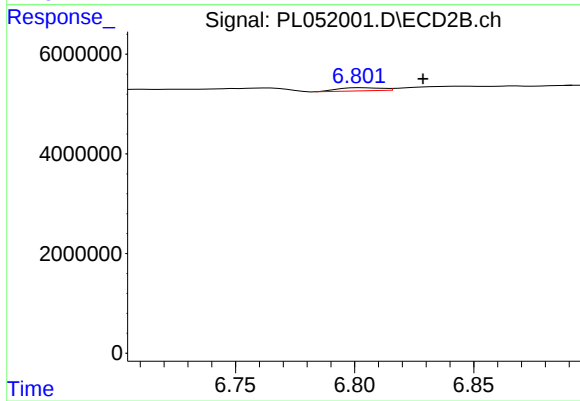

#15 Endosulfan II


R.T.: 6.802 min
Delta R.T.: -0.027 min
Response: 794004
Conc: 0.24 ng/ml

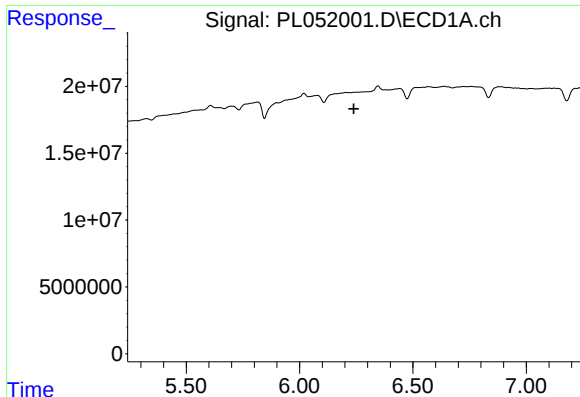

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122686BL

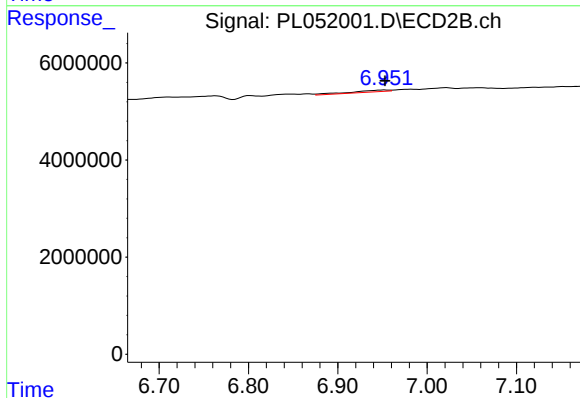


#18 Endrin aldehyde

R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 1070234
Conc: 0.38 ng/ml

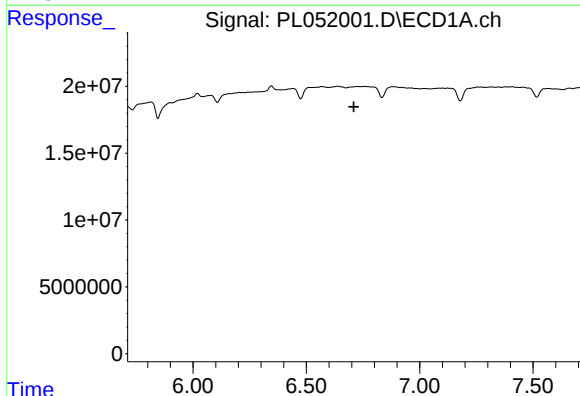


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

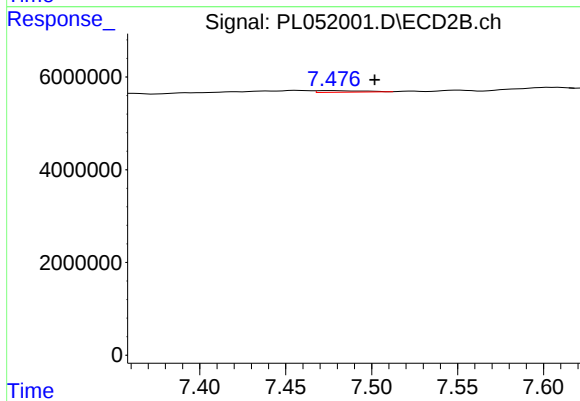

#20 Methoxychlor


R.T.: 7.477 min
Delta R.T.: -0.025 min
Response: 638952
Conc: 0.38 ng/ml

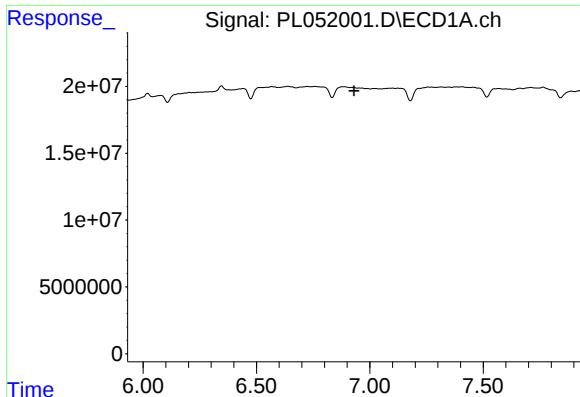

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122686BL

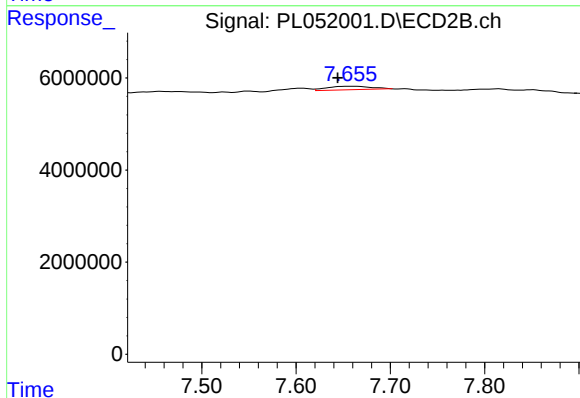


#21 Endrin ketone

R.T.: 7.657 min
Delta R.T.: 0.013 min
Response: 2532138
Conc: 0.79 ng/ml

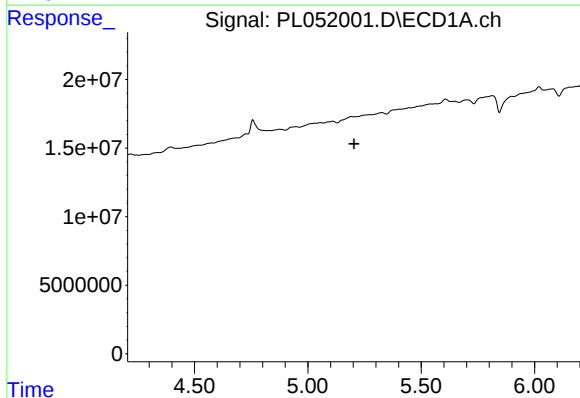


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.204 min
Response: 0
Conc: N.D.

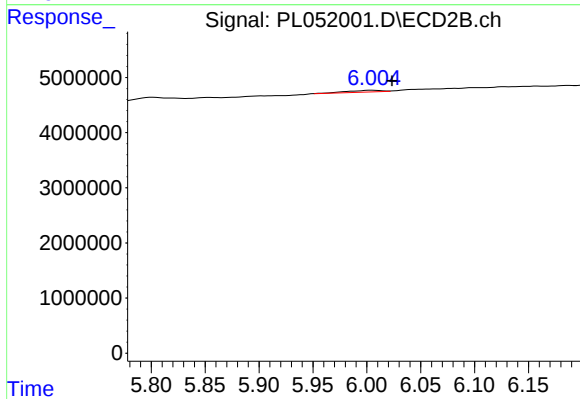

#25 Chlordane-3


R.T.: 6.006 min
Delta R.T.: -0.018 min
Response: 685883
Conc: 1.54 ng/ml

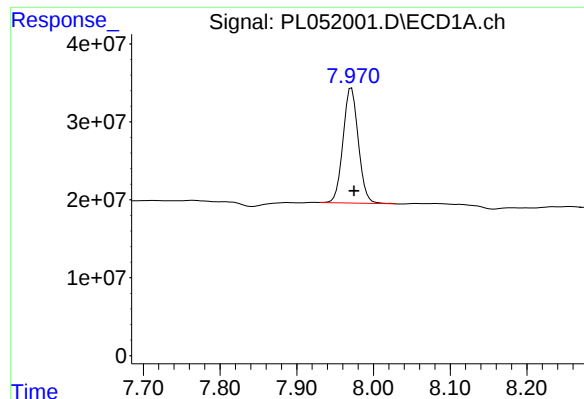

#28 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.003 min
Response: 204168594
Conc: 16.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122686BL

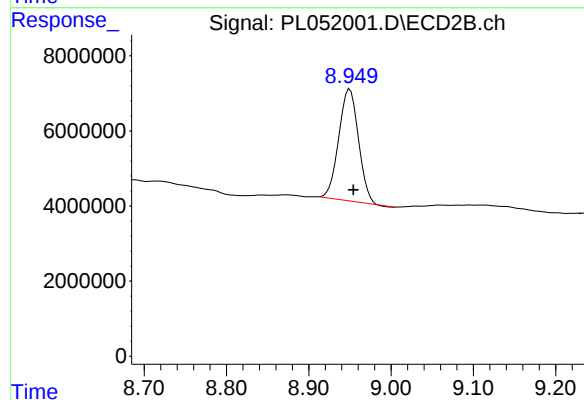

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 49672315
Conc: 16.32 ng/ml