

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL052016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 02:24
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 04:38:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	224.0E6	55307931	26.168	25.315
28)	SA Decachlor...	7.970	8.949	296.7E6	71111049	24.446	23.362
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	512089	N.D.	0.351 #
8)	B Heptachlo...	0.000	5.784	0	14127940	N.D.	4.186 #
9)	A Endosulfan I	5.325f	6.165f	12443756	273290	0.926	0.085 #
14)	MA Endrin	0.000	6.619	0	92246	N.D.	0.030 #
15)	B Endosulfa...	6.076	6.845f	8717068	1012973	0.626	0.307 #
18)	B Endrin al...	0.000	6.976f	0	2409796	N.D.	0.853 #
24)	Chlordane-2	4.676f	0.000	48722279	0	119.208	N.D. #
27)	Chlordane-5	6.076	0.000	8717068	0	17.764	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL052016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 02:24
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 04:38:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

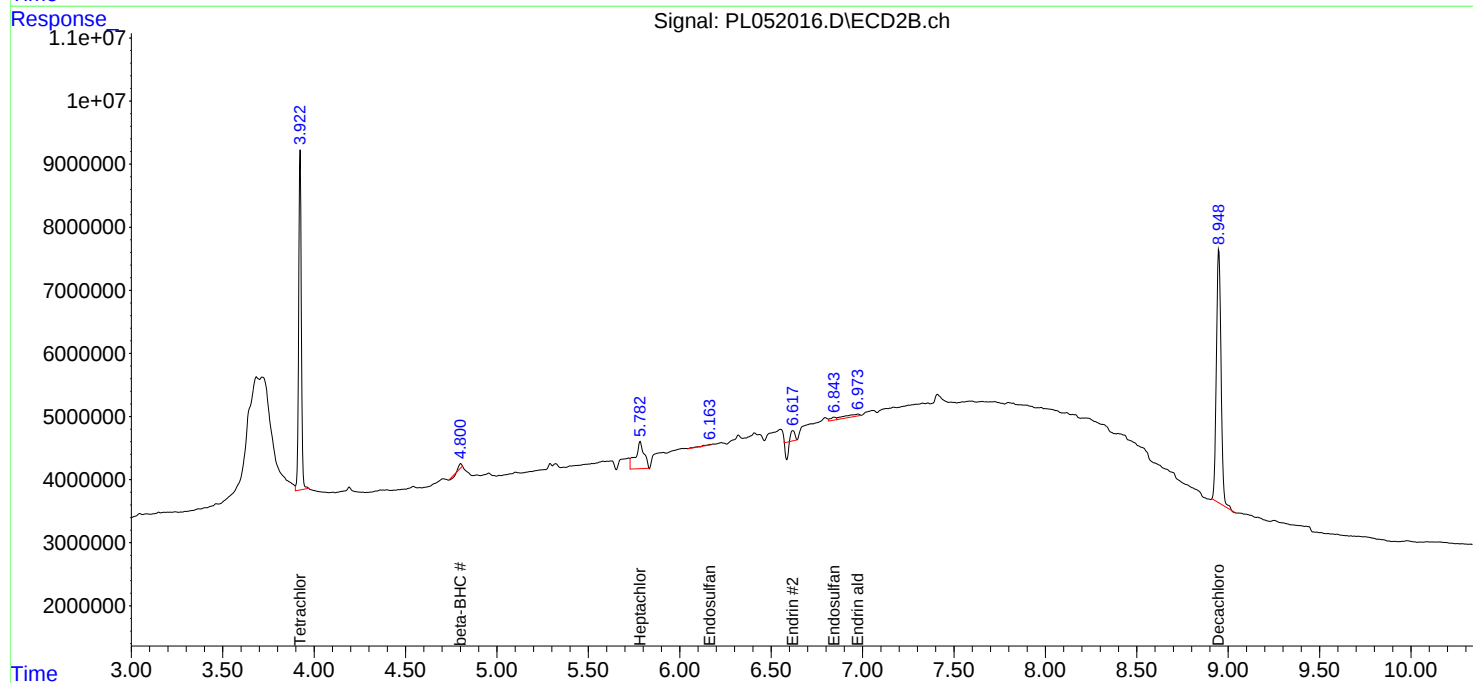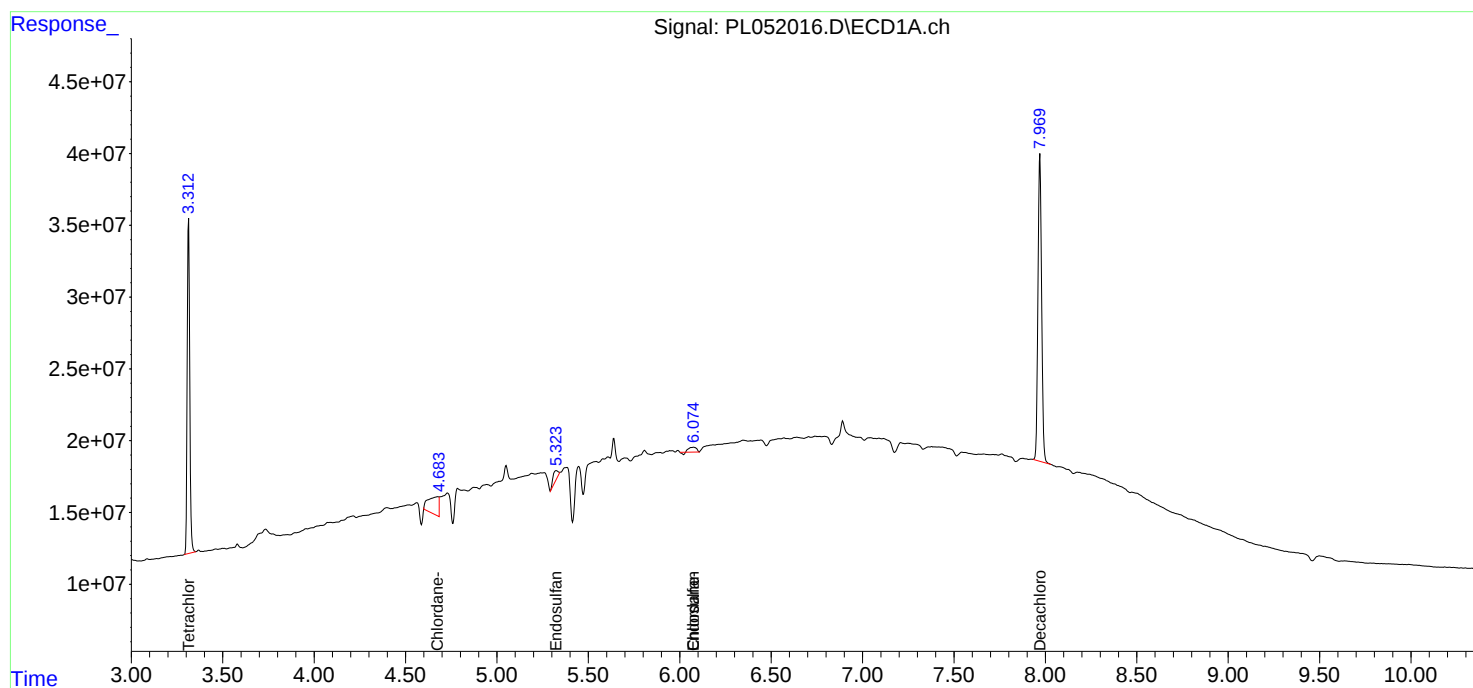


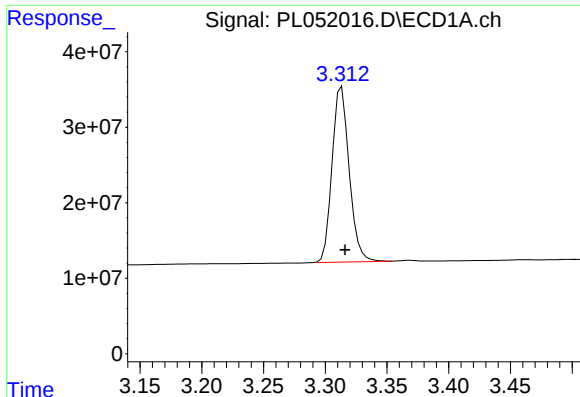

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 223960027
Conc: 26.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

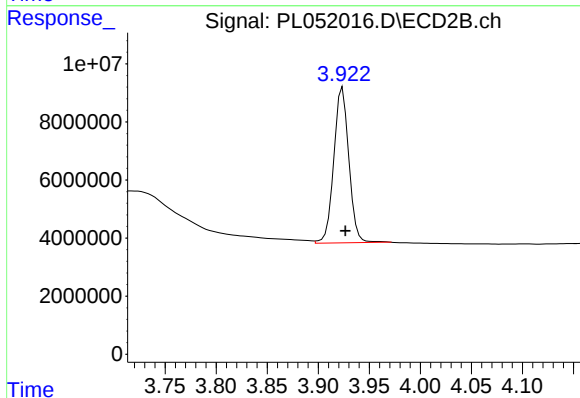


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 55307931
Conc: 25.31 ng/ml

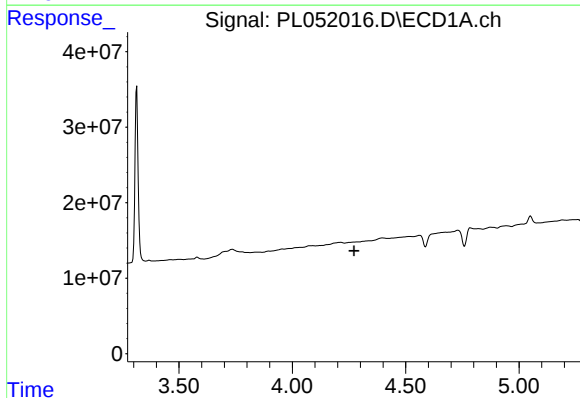


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

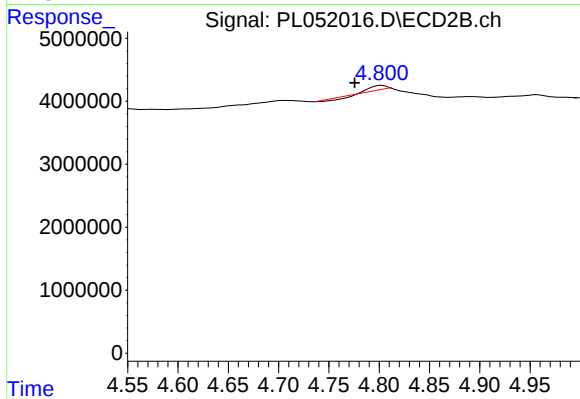

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 512089
Conc: 0.35 ng/ml

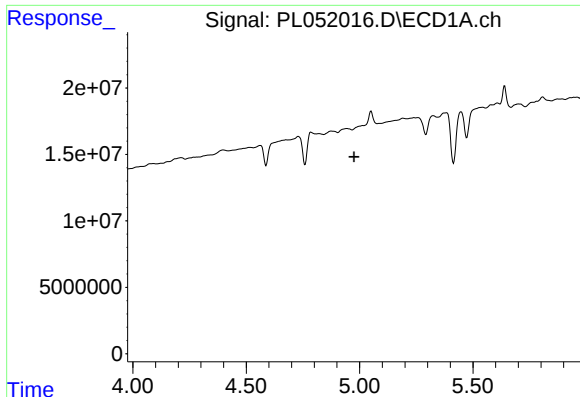

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

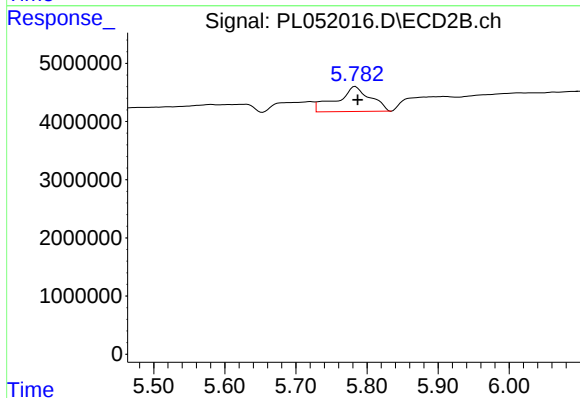


#8 Heptachlor epoxide

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 14127940
Conc: 4.19 ng/ml

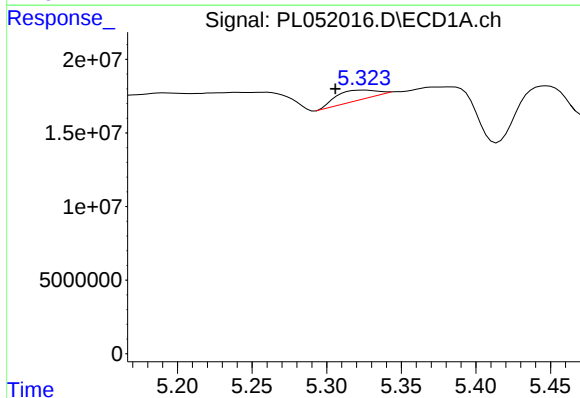


#9 Endosulfan I

R.T.: 5.325 min
Delta R.T.: 0.019 min
Response: 12443756
Conc: 0.93 ng/ml

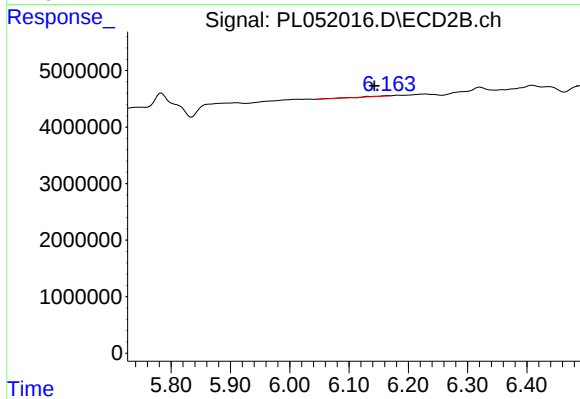

#9 Endosulfan I


R.T.: 6.165 min
Delta R.T.: 0.022 min
Response: 273290
Conc: 0.08 ng/ml

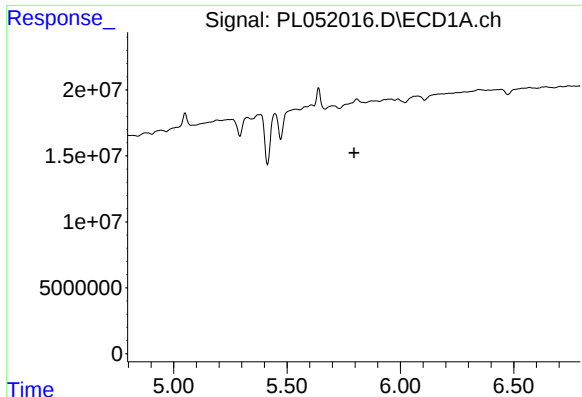

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.796 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

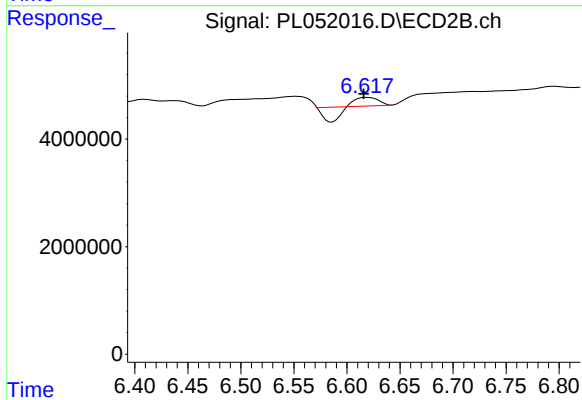


#14 Endrin

R.T.: 6.619 min
Delta R.T.: 0.003 min
Response: 92246
Conc: 0.03 ng/ml

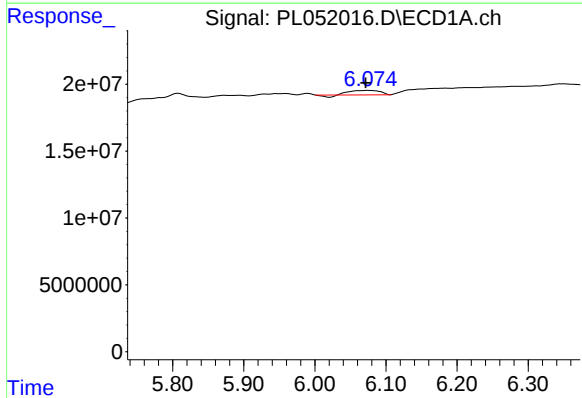


#15 Endosulfan II

R.T.: 6.076 min
Delta R.T.: 0.004 min
Response: 8717068
Conc: 0.63 ng/ml

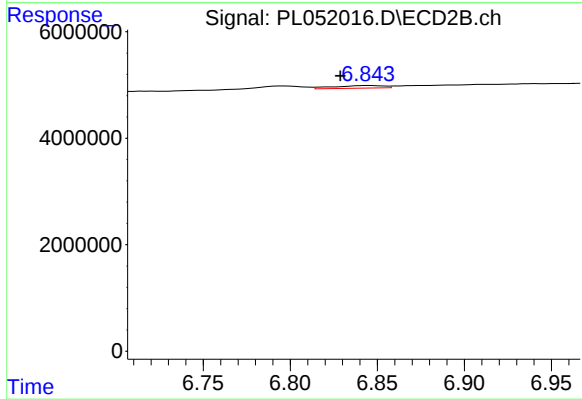

#15 Endosulfan II


R.T.: 6.845 min
Delta R.T.: 0.017 min
Response: 1012973
Conc: 0.31 ng/ml

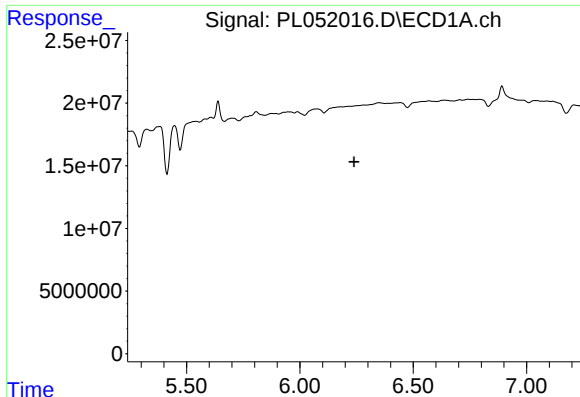

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

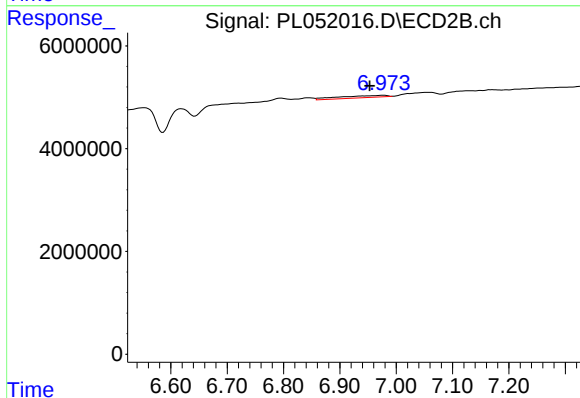


#18 Endrin aldehyde

R.T.: 6.976 min
Delta R.T.: 0.023 min
Response: 2409796
Conc: 0.85 ng/ml

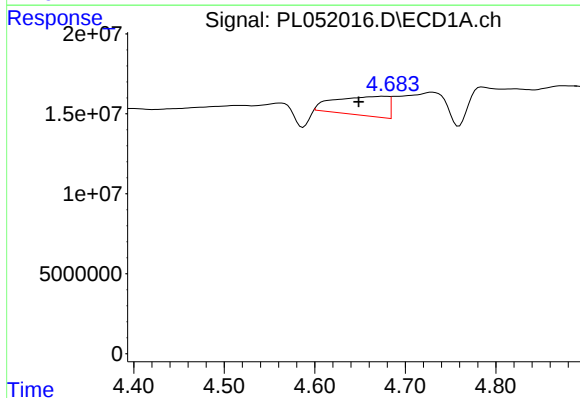


#24 Chlordane-2

R.T.: 4.676 min
Delta R.T.: 0.027 min
Response: 48722279
Conc: 119.21 ng/ml

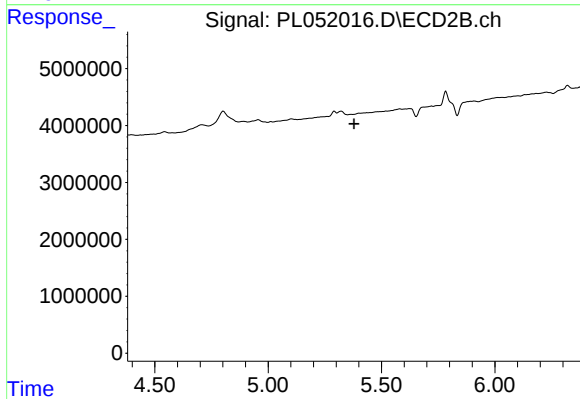

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

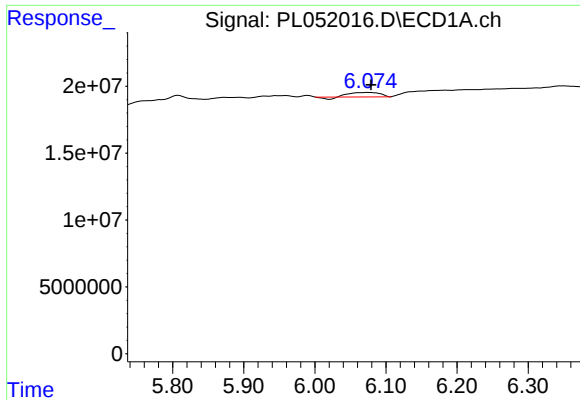

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: -0.003 min
Response: 8717068
Conc: 17.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

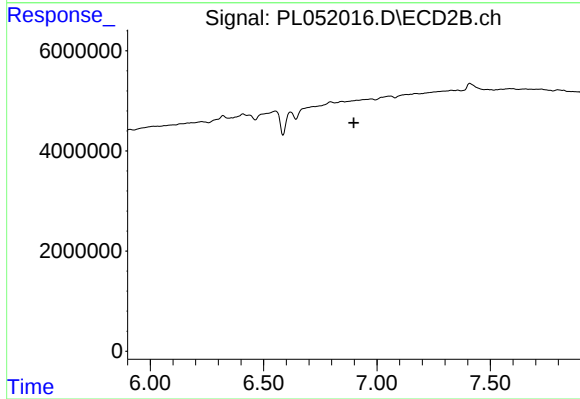


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.898 min
Response: 0
Conc: N.D.

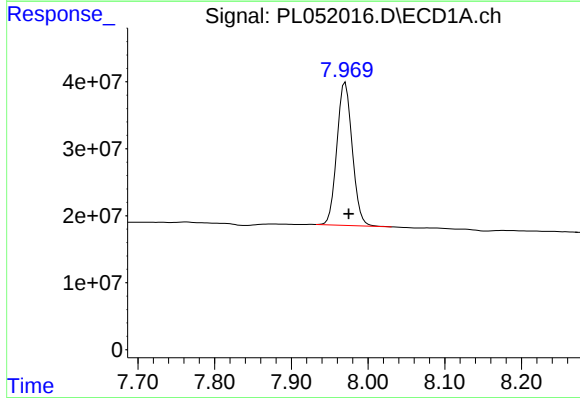

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.004 min
Response: 296724323
Conc: 24.45 ng/ml

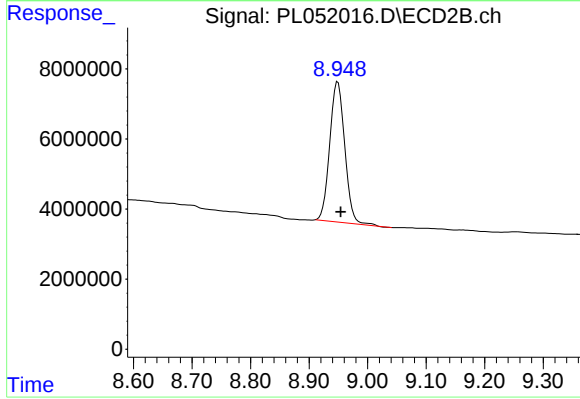

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.005 min
Response: 71111049
Conc: 23.36 ng/ml