

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 10:25
 Operator : SG\AJ
 Sample : K4546-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T3-S-A

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:45:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:42:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	81499627	19799741	9.523	9.062
28)	SA Decachlor...	7.973	8.949	123.7E6	32316455	10.191	10.617m
Target Compounds							
12)	B 4,4'-DDE	5.417	6.249	6119488	1821317	0.447m	0.517m
13)	MA Dieldrin	5.540	6.390	11635469	1877498	0.765m	0.548 #
17)	MA 4,4'-DDT	6.158	7.037	30590607	2706395	2.399m	0.924m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 10:25
Operator : SG\AJ
Sample : K4546-12
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:42:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

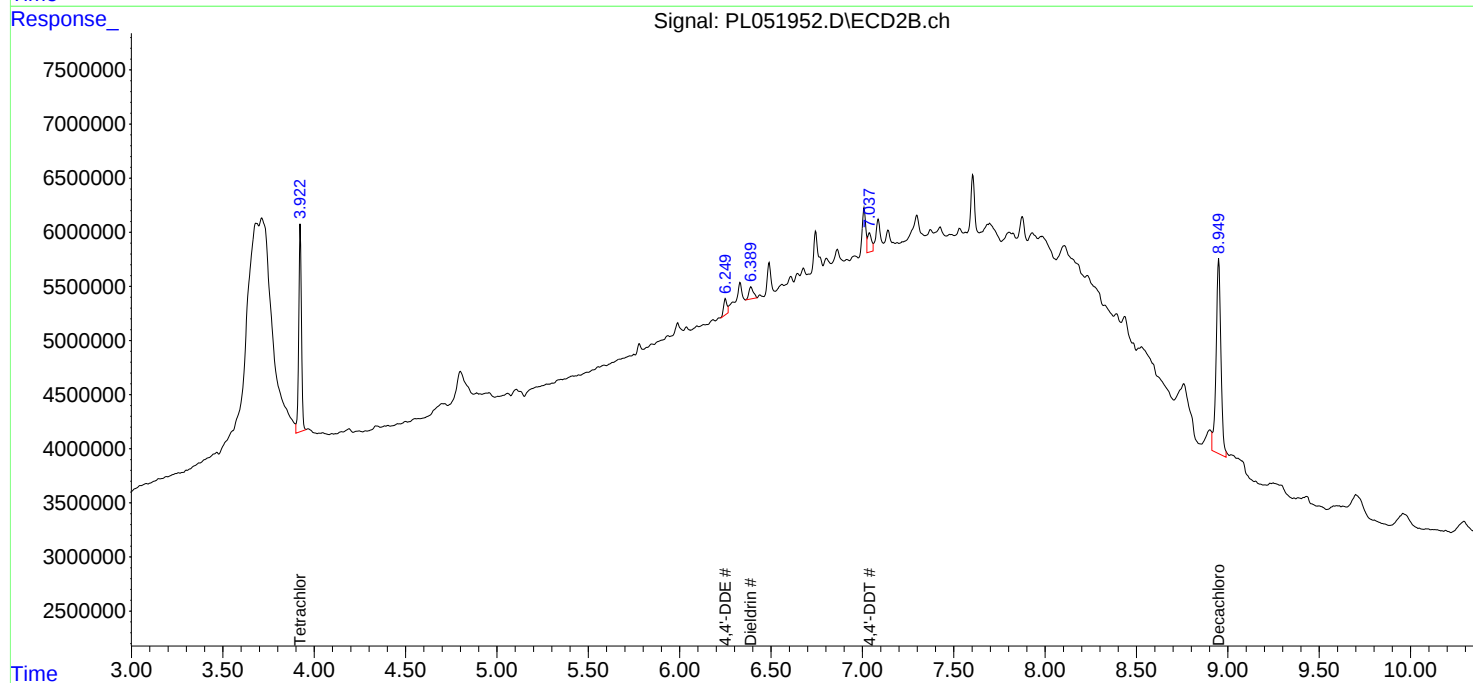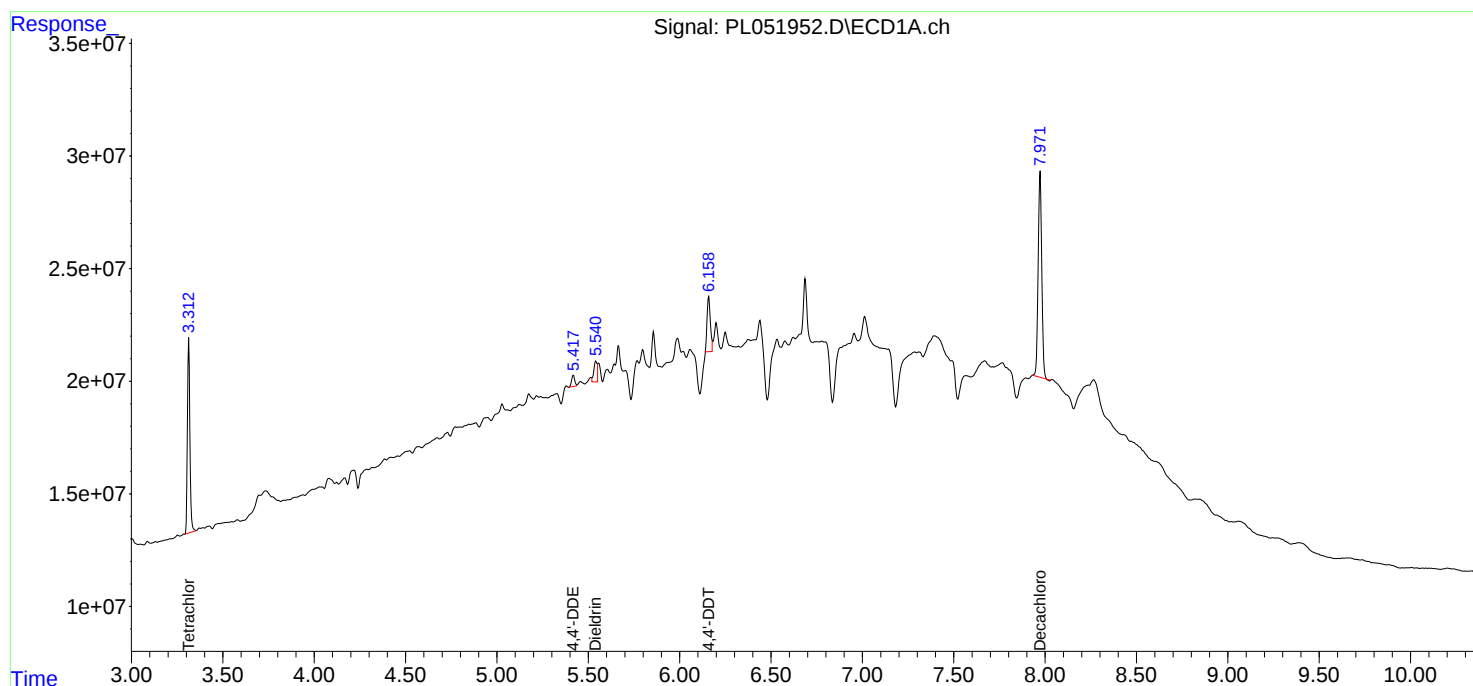

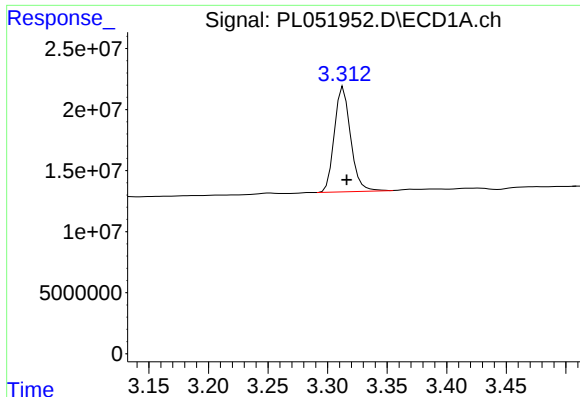


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 81499627
Conc: 9.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:01 PM

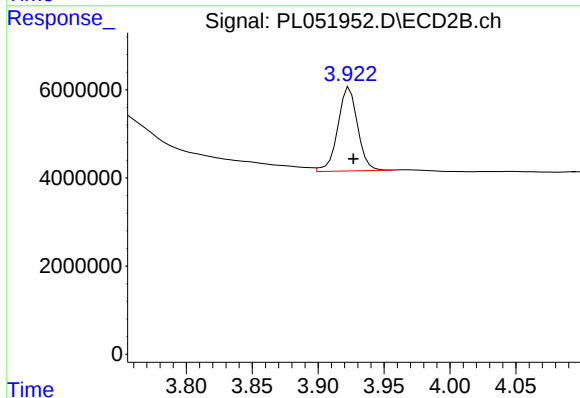


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 19799741
Conc: 9.06 ng/ml

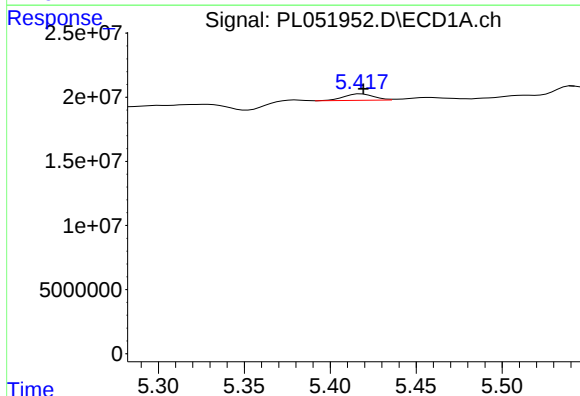


#12 4,4'-DDE

R.T.: 5.417 min
Delta R.T.: -0.003 min
Response: 6119488
Conc: 0.45 ng/ml m

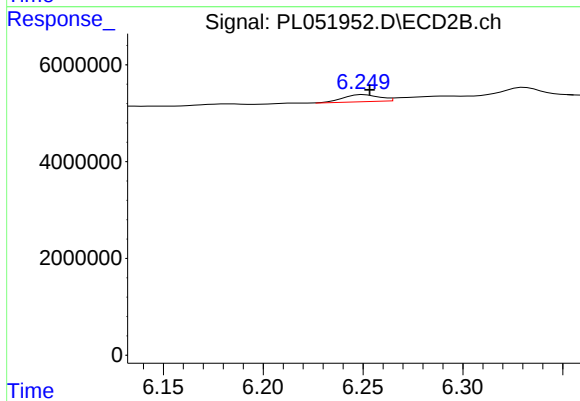

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.005 min
Response: 1821317
Conc: 0.52 ng/ml m

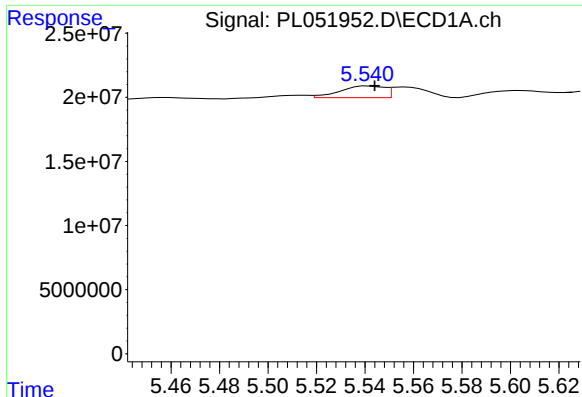


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: -0.004 min
Response: 11635469
Conc: 0.77 ng/ml m

Instrument :
ECD_L
ClientSampleId :
T3-S-A


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:01 PM

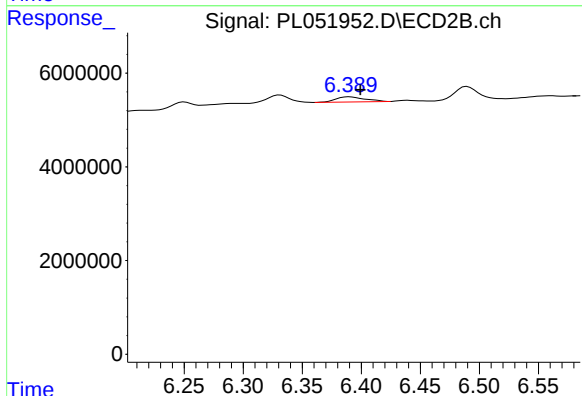


#13 Dieldrin

R.T.: 6.390 min
Delta R.T.: -0.009 min
Response: 1877498
Conc: 0.55 ng/ml

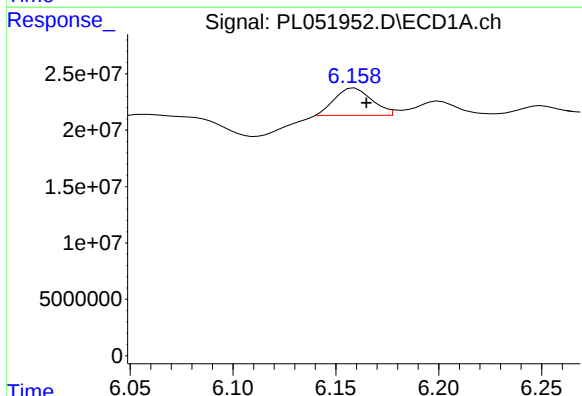


#17 4,4'-DDT

R.T.: 6.158 min
Delta R.T.: -0.007 min
Response: 30590607
Conc: 2.40 ng/ml m

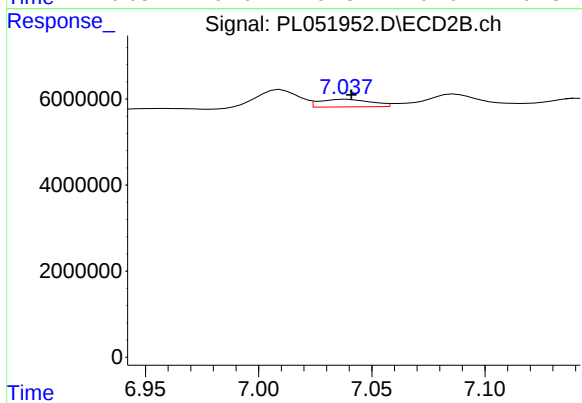

#17 4,4'-DDT

R.T.: 7.037 min
Delta R.T.: -0.004 min
Response: 2706395
Conc: 0.92 ng/ml m

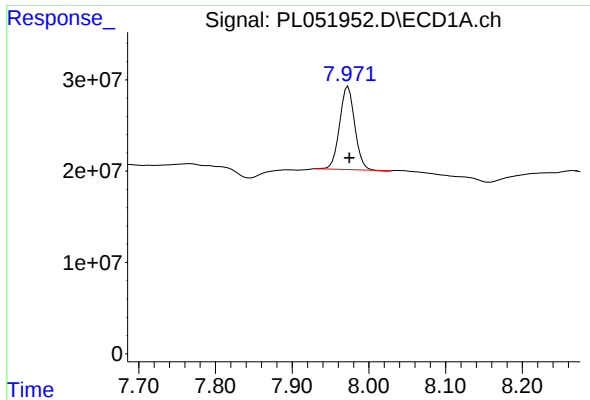


#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 123692261
Conc: 10.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
T3-S-A

Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:01 PM

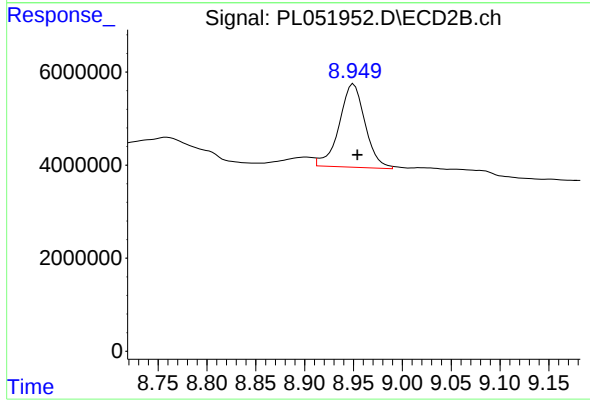

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.005 min
Response: 32316455
Conc: 10.62 ng/ml m