

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 12:05
 Operator : SG\AJ
 Sample : K4567-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-S

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:45:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:44:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.924	170.7E6	41099430	19.941	18.811
28)	SA Decachlor...	7.971	8.950	222.4E6	51288609	18.325	16.850
Target Compounds							
17)	MA 4,4'-DDT	6.162	7.034	12049574	3024264	0.945	1.033m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 12:05
Operator : SG\AJ
Sample : K4567-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-7-S


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:44:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

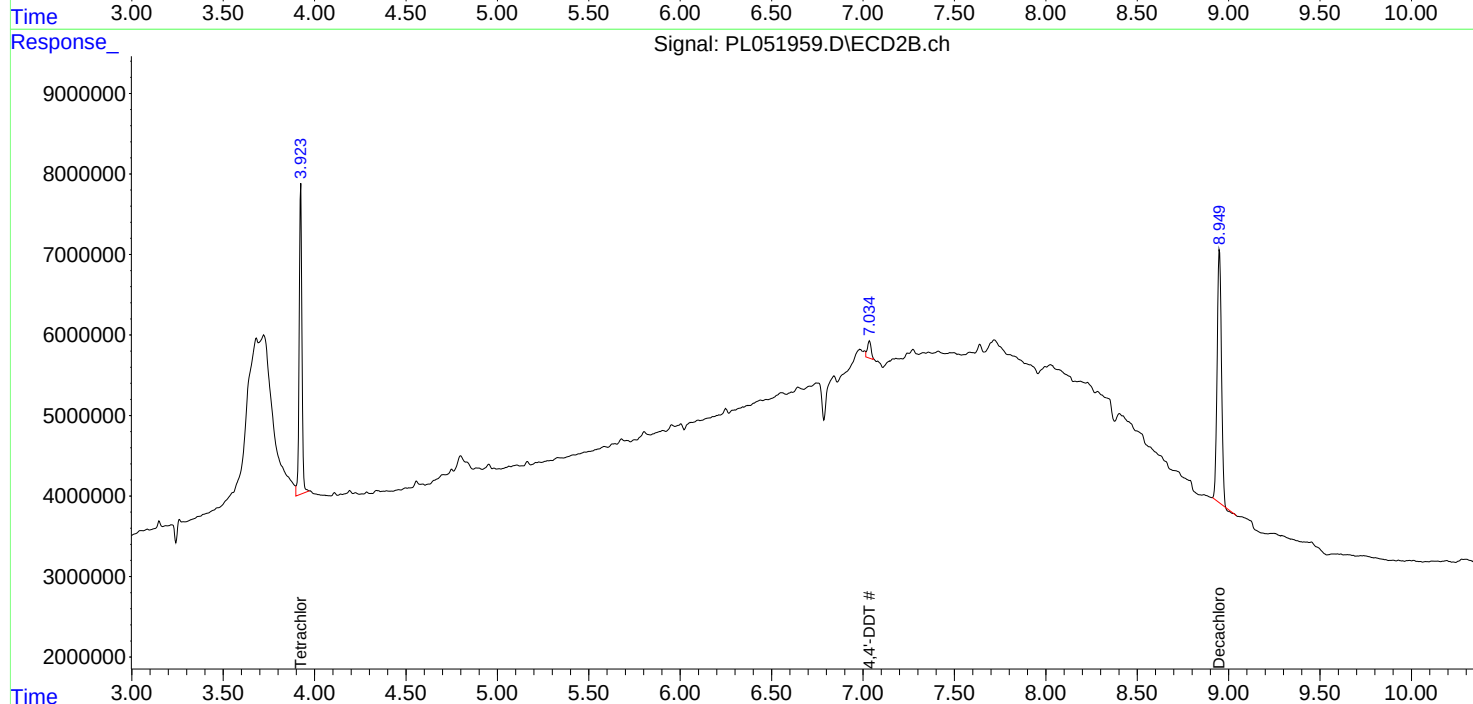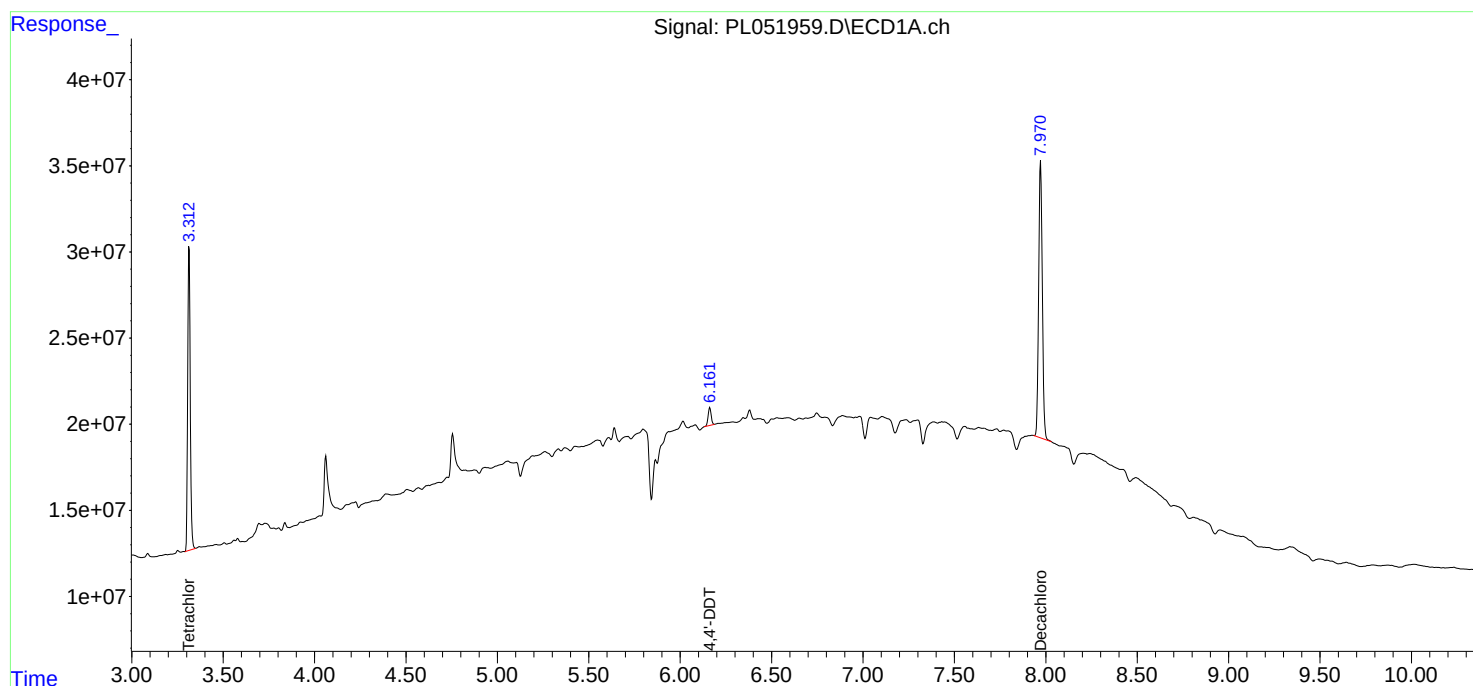

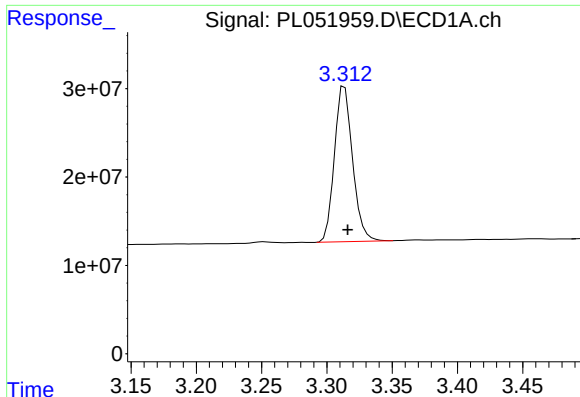


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 170669669
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:20 PM

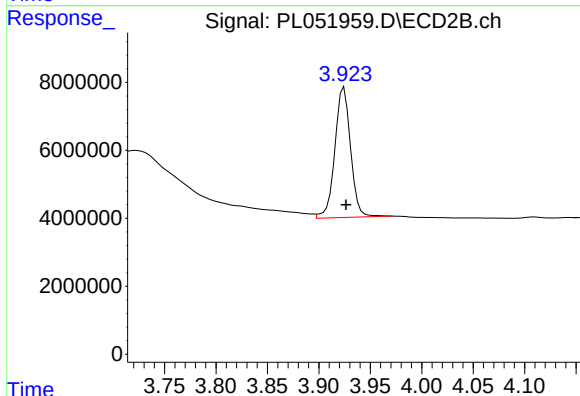


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 41099430
Conc: 18.81 ng/ml

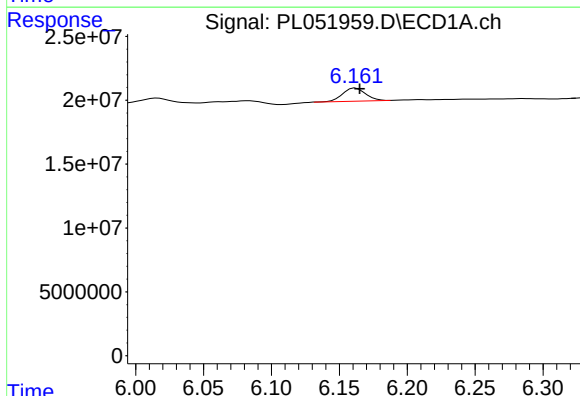


#17 4,4'-DDT

R.T.: 6.162 min
Delta R.T.: -0.003 min
Response: 12049574
Conc: 0.94 ng/ml

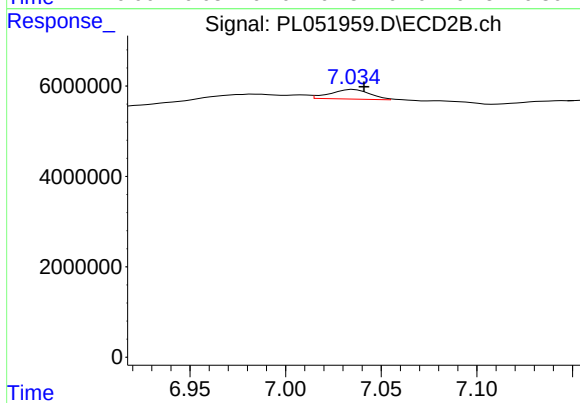

#17 4,4'-DDT

R.T.: 7.034 min
Delta R.T.: -0.007 min
Response: 3024264
Conc: 1.03 ng/ml m

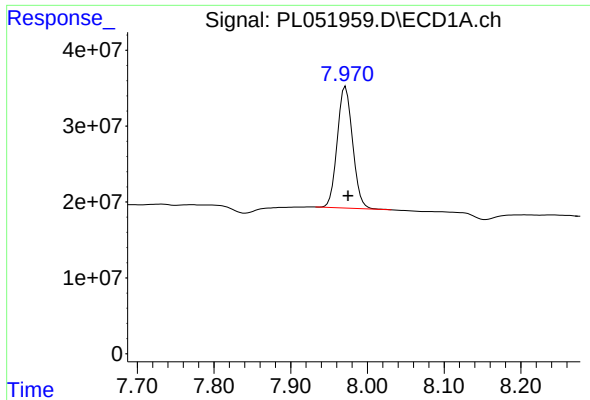


#28 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.003 min
Response: 222430332
Conc: 18.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:20 PM

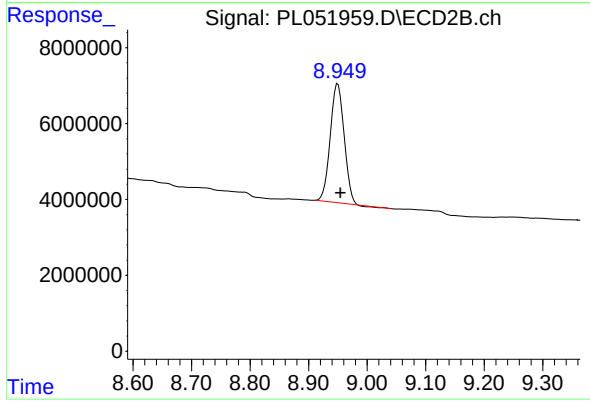

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.004 min
Response: 51288609
Conc: 16.85 ng/ml