

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL051967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 14:34
 Operator : SG\AJ
 Sample : K4439-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2-(1-3)

Manual Integrations
 APPROVED

Ankita
 8/30/2019 5:45:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:45:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	101.6E6	23443657	11.869	10.730
28)	SA Decachlor...	7.972	8.951	123.3E6	33606181	10.159	11.041
Target Compounds							
12)	B 4,4'-DDE	5.418	6.244	13687137	2309229	1.000	0.656m#
17)	MA 4,4'-DDT	6.158	7.036	13212743	1527126	1.036m	0.522m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL051967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 14:34
Operator : SG\AJ
Sample : K4439-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-2-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:45:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

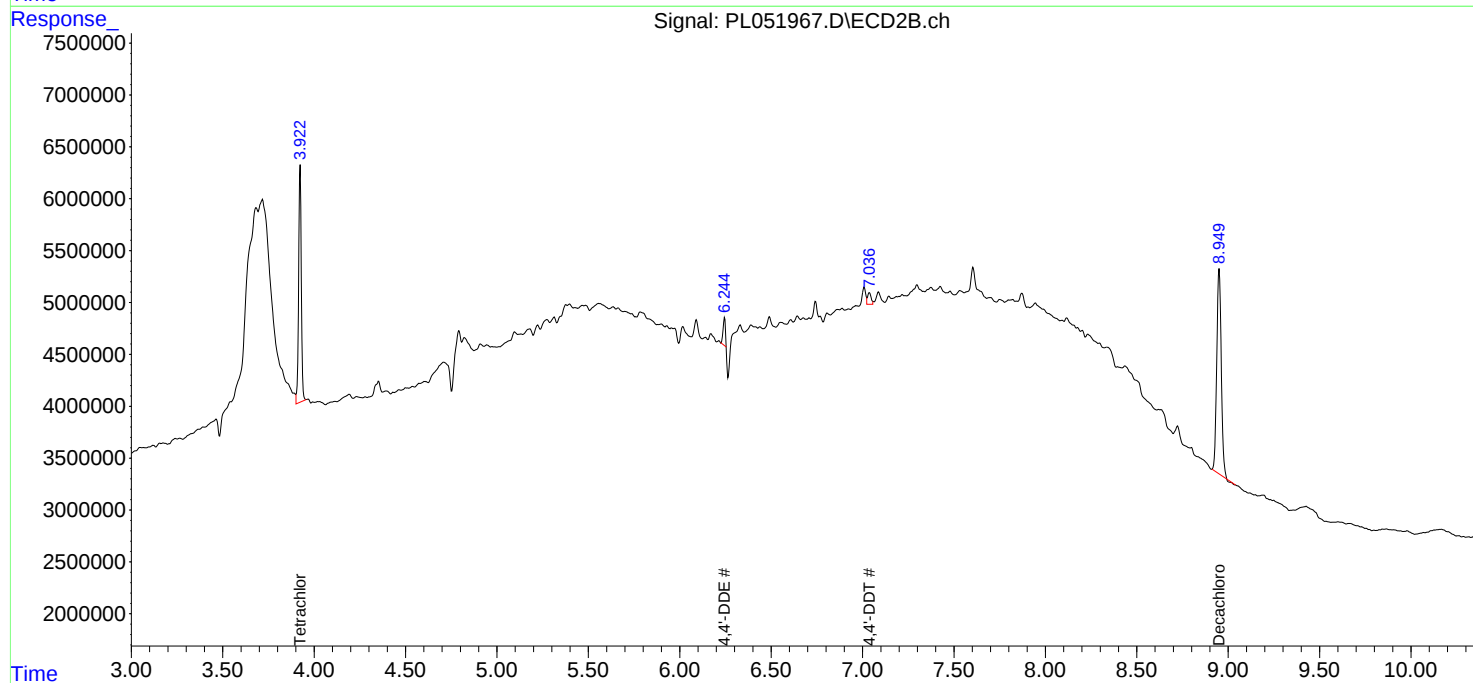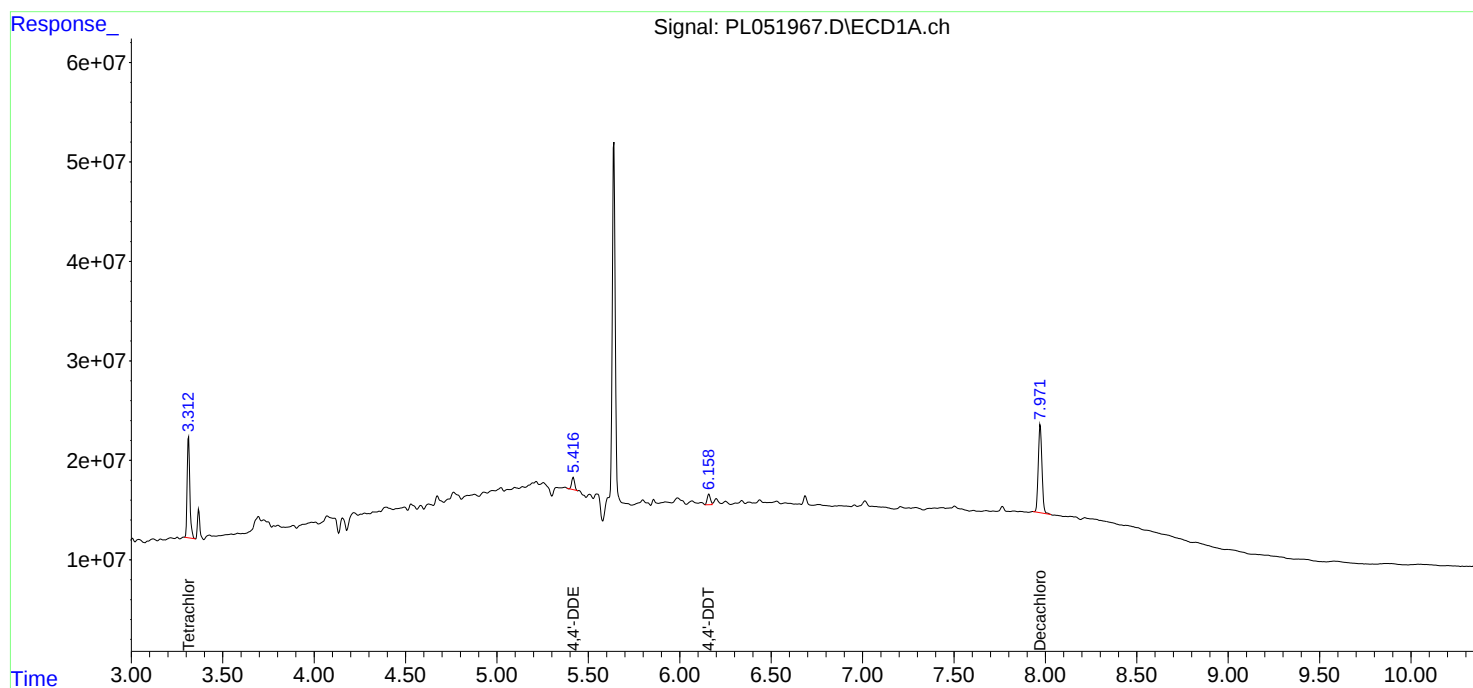

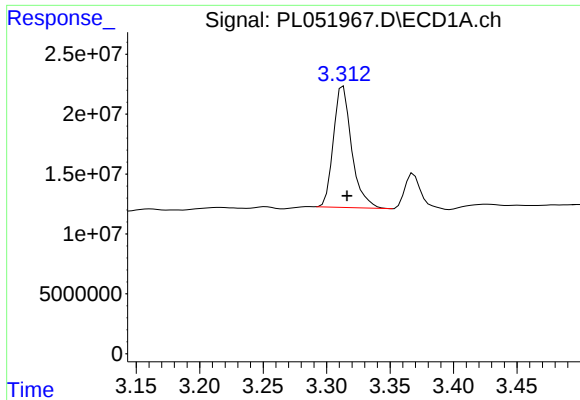


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 101586456
Conc: 11.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:40 PM

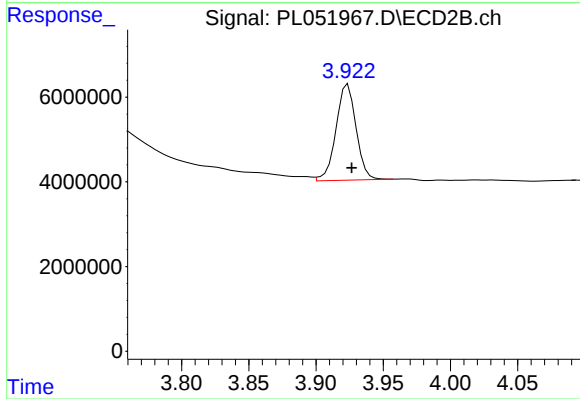


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 23443657
Conc: 10.73 ng/ml

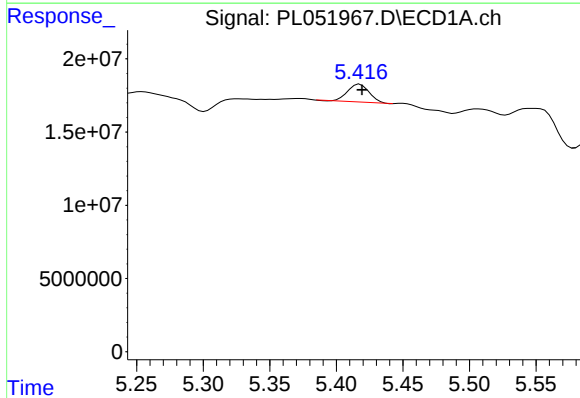


#12 4,4'-DDE

R.T.: 5.418 min
Delta R.T.: -0.002 min
Response: 13687137
Conc: 1.00 ng/ml

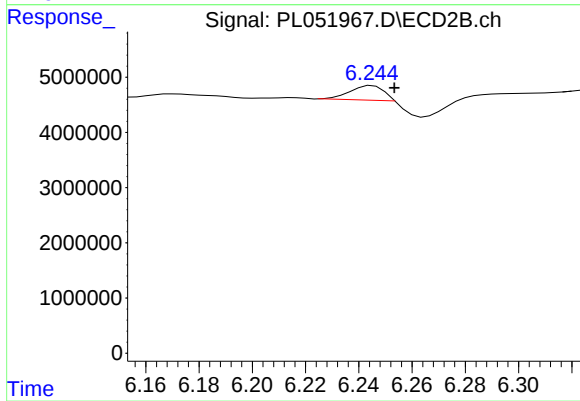

#12 4,4'-DDE

R.T.: 6.244 min
Delta R.T.: -0.010 min
Response: 2309229
Conc: 0.66 ng/ml m

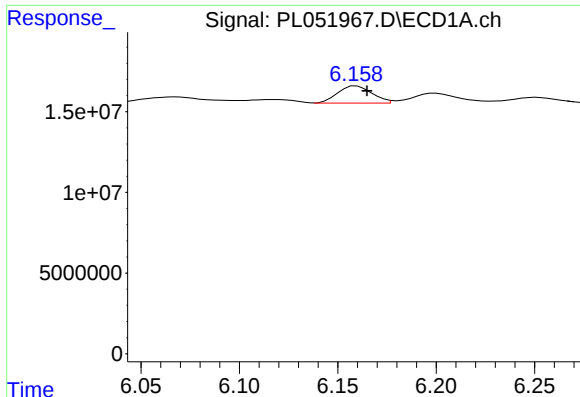


#17 4,4'-DDT

R.T.: 6.158 min
Delta R.T.: -0.007 min
Response: 13212743
Conc: 1.04 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-2-(1-3)


Manual Integrations
APPROVED

Ankita
8/30/2019 5:45:40 PM

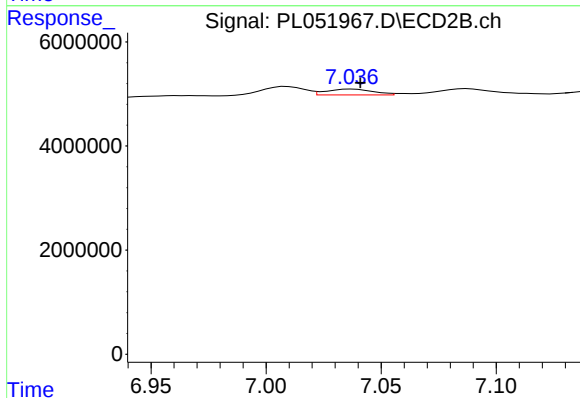


#17 4,4'-DDT

R.T.: 7.036 min
Delta R.T.: -0.005 min
Response: 1527126
Conc: 0.52 ng/ml m

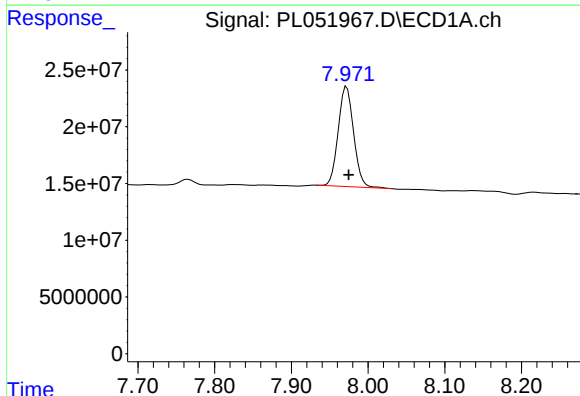

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 123305697
Conc: 10.16 ng/ml

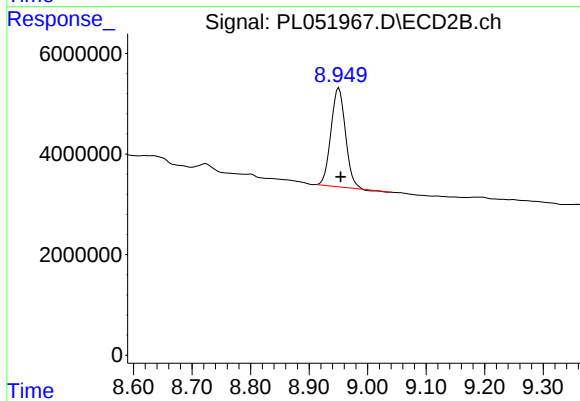

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 33606181
Conc: 11.04 ng/ml