

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
 Data File : PL052000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 22:38
 Operator : SG\AJ
 Sample : K4587-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-057

Manual Integrations
 APPROVED

Ankita
 8/31/2019 2:40:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 00:53:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	83189745	21306963	9.720	9.752
28)	SA Decachlor...	7.970	8.946	89662361	25225749	7.387	8.287m
Target Compounds							
10)	B gamma-Chl...	5.197	6.017	4002865	1510924	0.268m	0.414m#
11)	B alpha-Chl...	5.250	6.090	6911905	3975306	0.478	1.152m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082919\
Data File : PL052000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 22:38
Operator : SG\AJ
Sample : K4587-01
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-057


Manual Integrations
APPROVED

Ankita
8/31/2019 2:40:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 00:53:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

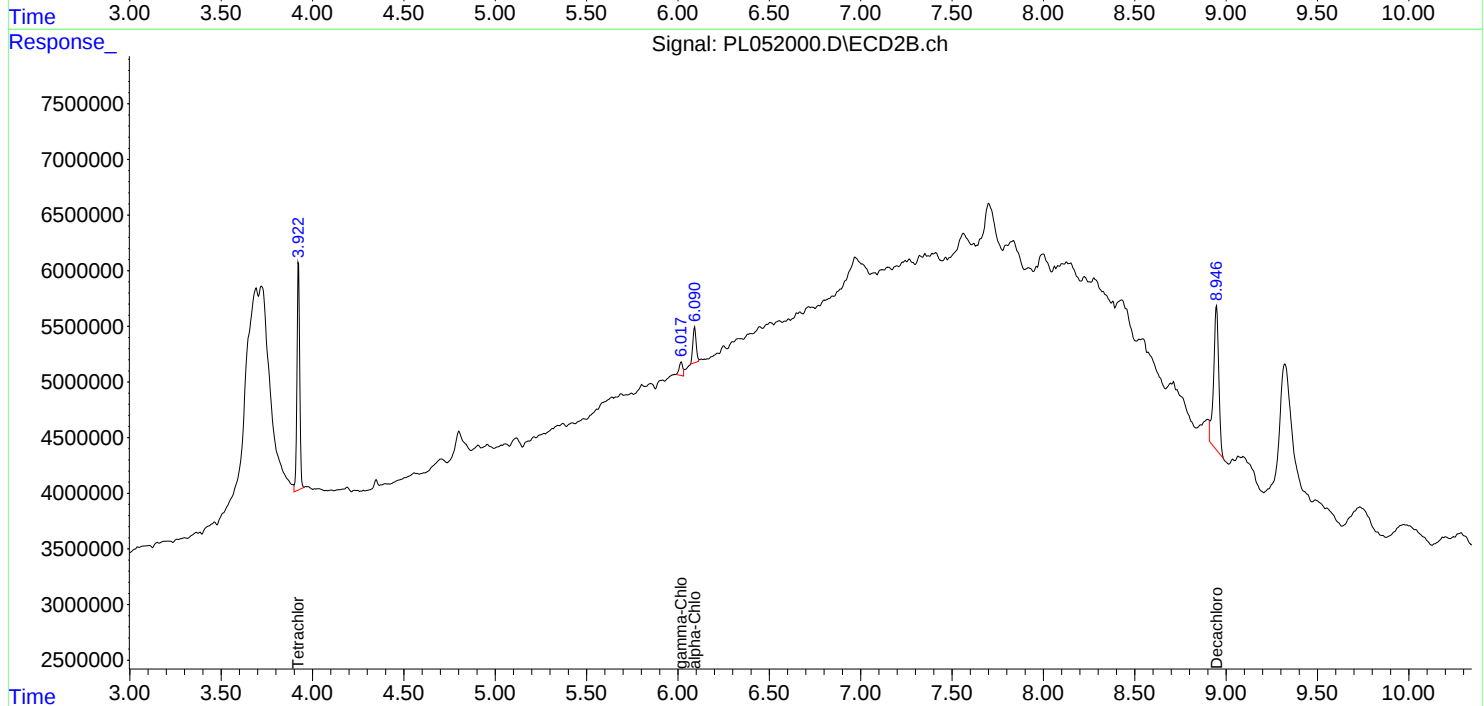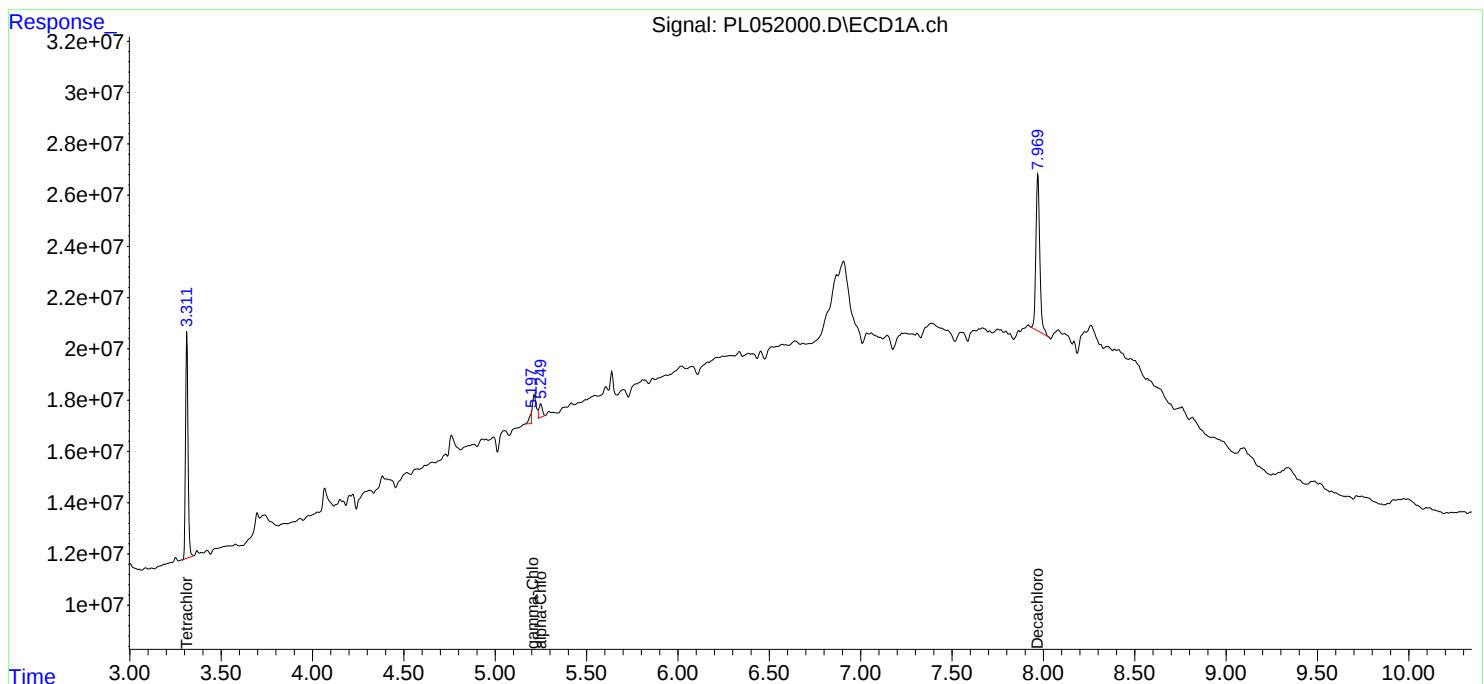

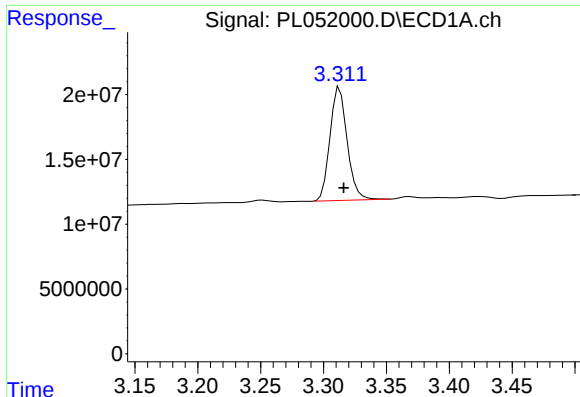


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 83189745
Conc: 9.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-057


Manual Integrations
APPROVED

Ankita
8/31/2019 2:40:18 PM

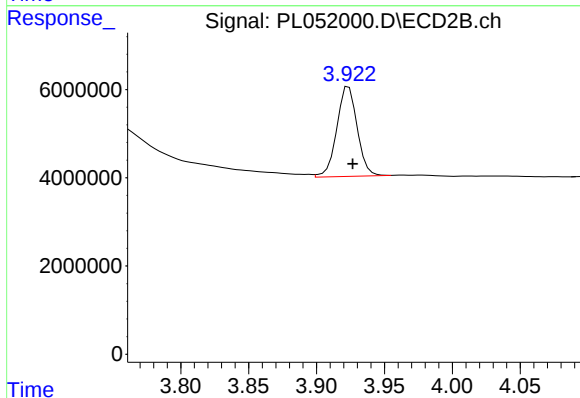


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 21306963
Conc: 9.75 ng/ml

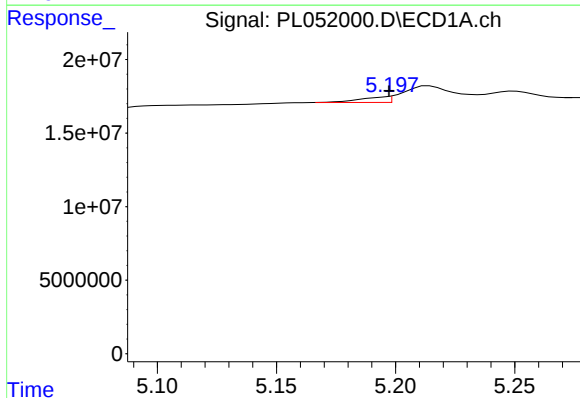


#10 gamma-Chlordane

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 4002865
Conc: 0.27 ng/ml m

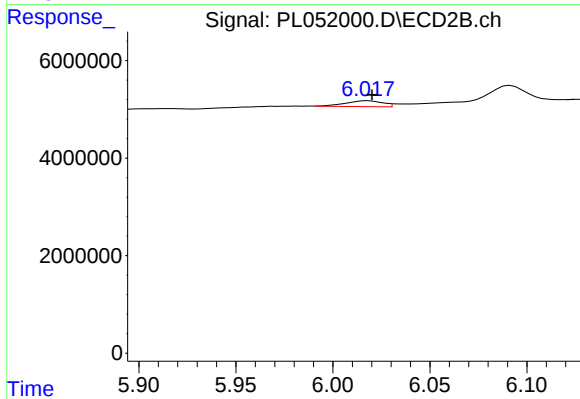

#10 gamma-Chlordane

R.T.: 6.017 min
Delta R.T.: -0.003 min
Response: 1510924
Conc: 0.41 ng/ml m

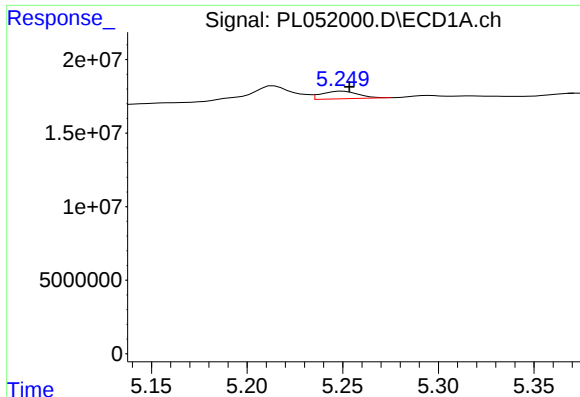


#11 alpha-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.003 min
Response: 6911905
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-057


Manual Integrations
APPROVED

Ankita
8/31/2019 2:40:18 PM

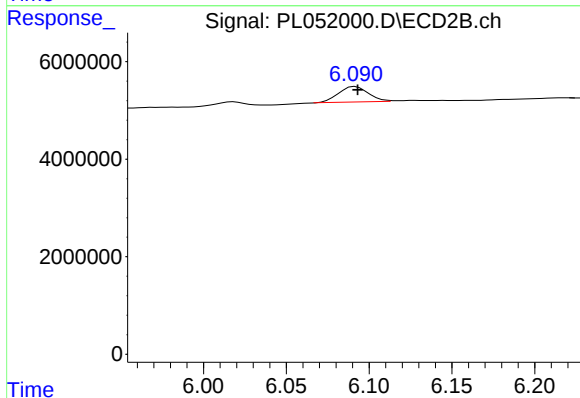


#11 alpha-Chlordane

R.T.: 6.090 min
Delta R.T.: -0.003 min
Response: 3975306
Conc: 1.15 ng/ml m

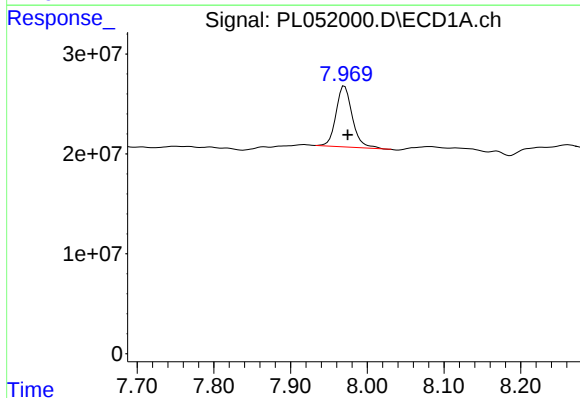

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.004 min
Response: 89662361
Conc: 7.39 ng/ml

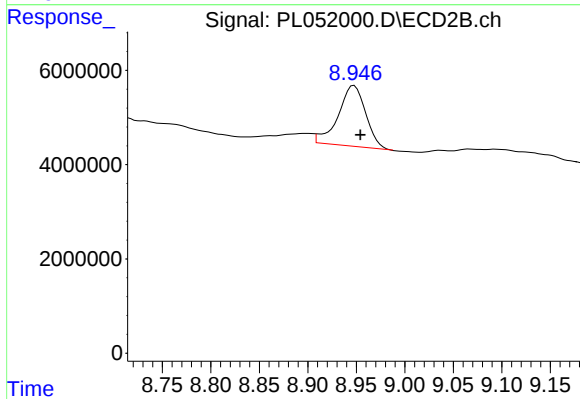

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.008 min
Response: 25225749
Conc: 8.29 ng/ml m