

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082922\
 Data File : PL077349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2022 13:28
 Operator : AR\AJ
 Sample : PB147321BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 15:22:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.630	21416680	46776443	15.740	15.220
28)	SA Decachlor...	8.909	7.733	18700114	41057791	15.957	14.714
Target Compounds							
2)	A alpha-BHC	3.908f	3.109	501768	292670	0.271	0.067 #
4)	MA Heptachlor	0.000	3.760f	0	1440132	N.D.	0.369 #
6)	B beta-BHC	0.000	3.760	0	1440132	N.D.	0.873 #
7)	B delta-BHC	4.647f	0.000	644897	0	0.417	N.D. #
14)	MA Endrin	6.478f	5.481f	526830	223972	0.447	0.082 #
15)	B Endosulfa...	6.688	0.000	922848	0	0.842	N.D. #
21)	B Endrin ke...	7.556	0.000	391507	0	0.321	N.D. #
27)	Chlordane-5	0.000	5.558f	0	4059546	N.D.	46.367 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082922\
Data File : PL077349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2022 13:28
Operator : AR\AJ
Sample : PB147321BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 15:22:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

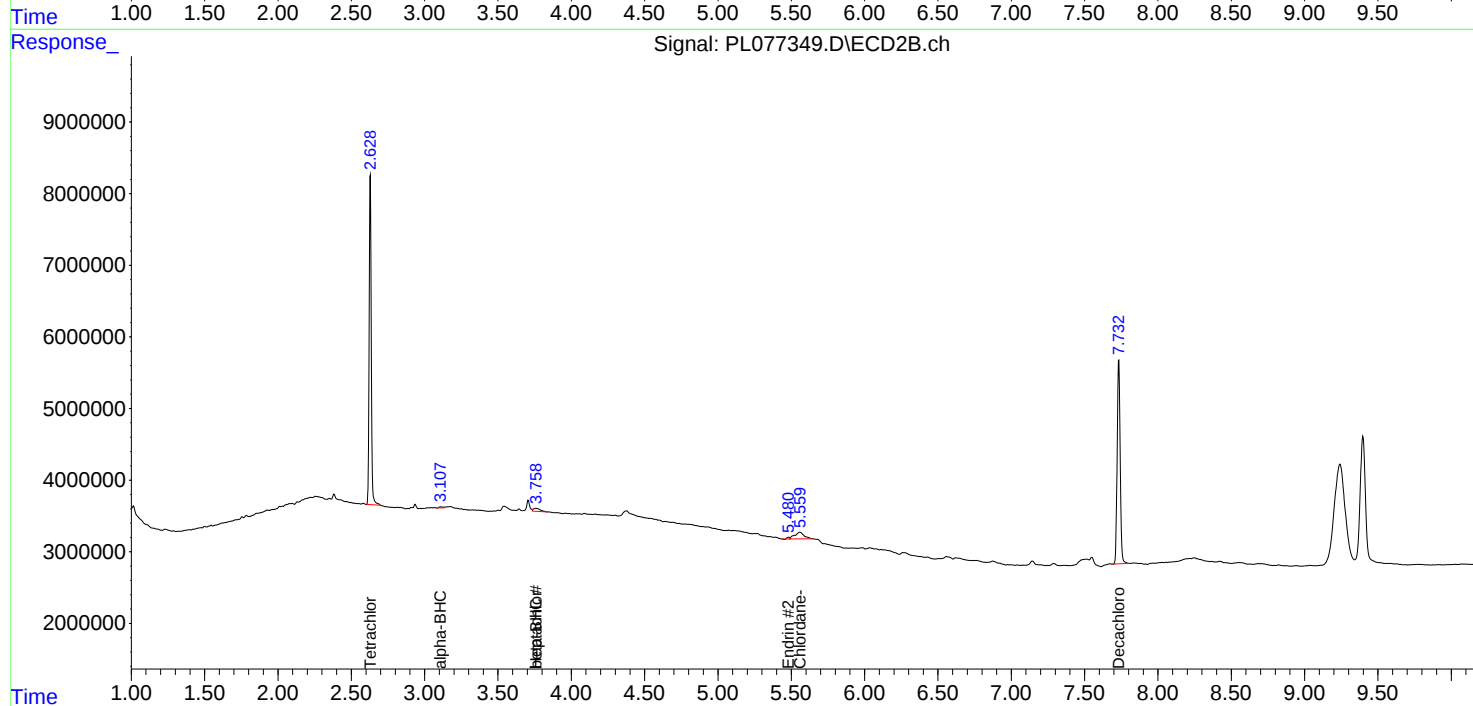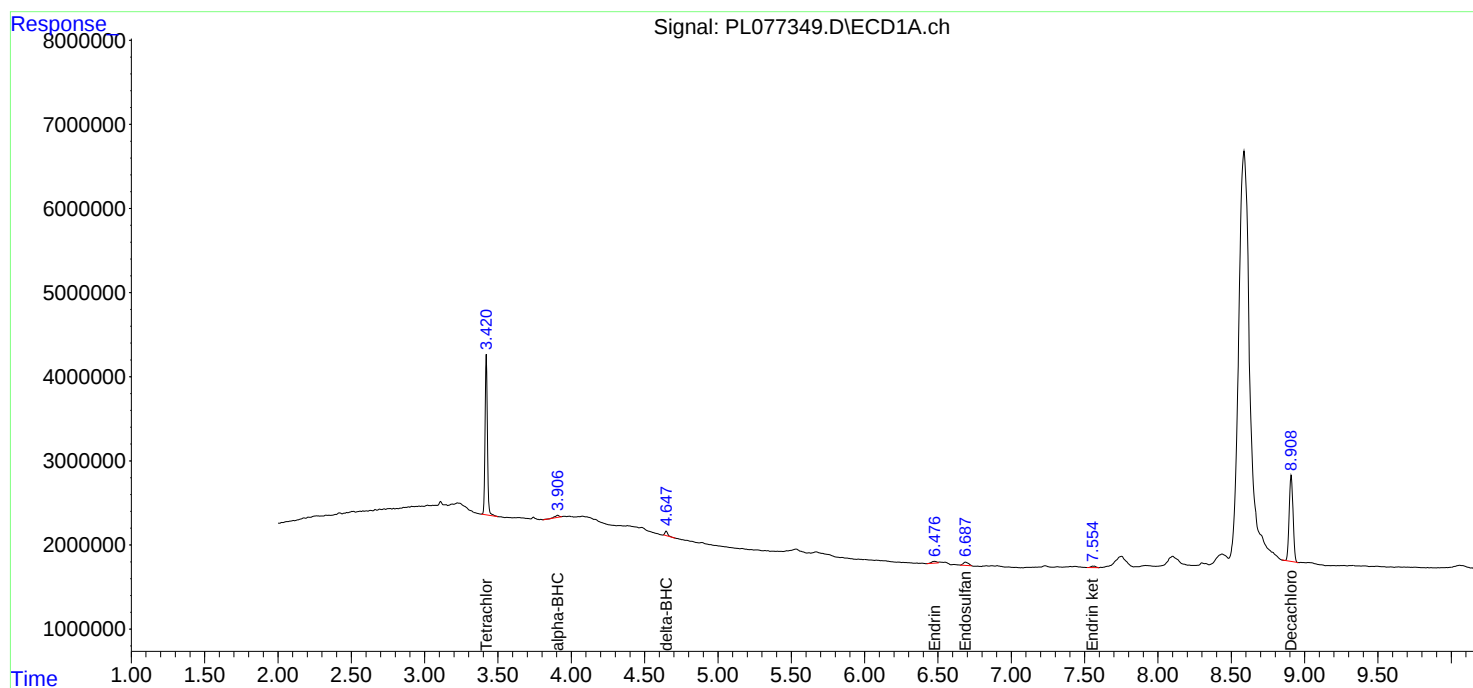


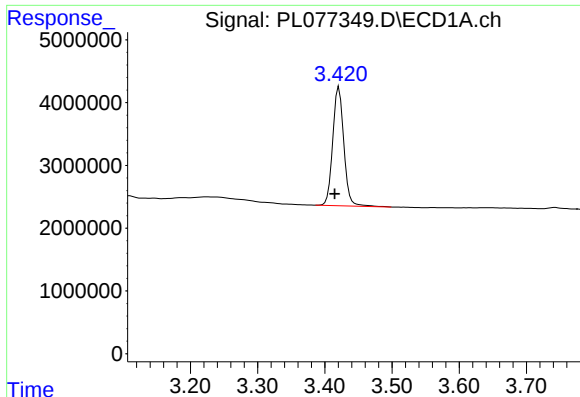

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.006 min
Response: 21416680
Conc: 15.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

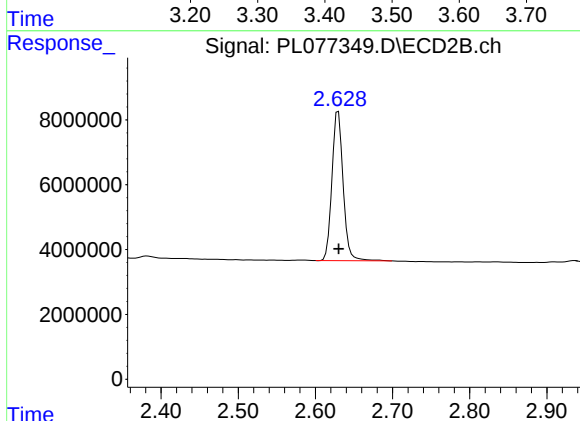


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 46776443
Conc: 15.22 ng/ml

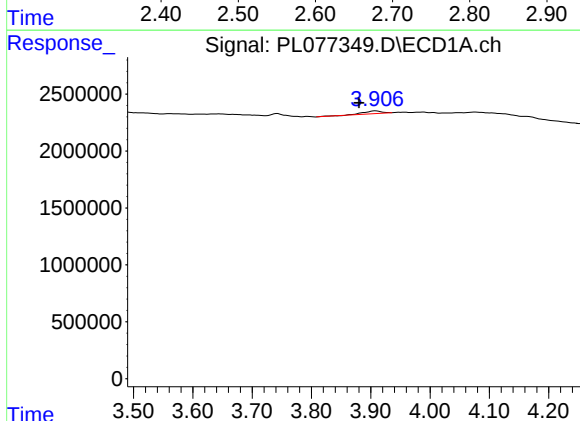


#2 alpha-BHC

R.T.: 3.908 min
Delta R.T.: 0.028 min
Response: 501768
Conc: 0.27 ng/ml

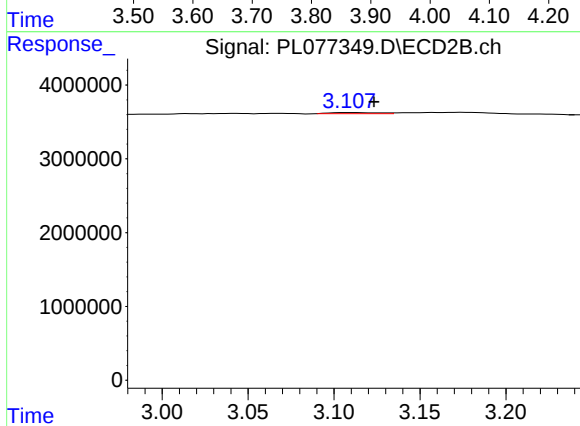

#2 alpha-BHC


R.T.: 3.109 min
Delta R.T.: -0.014 min
Response: 292670
Conc: 0.07 ng/ml

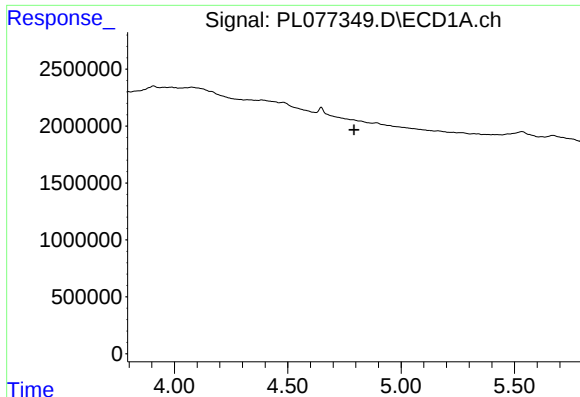

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

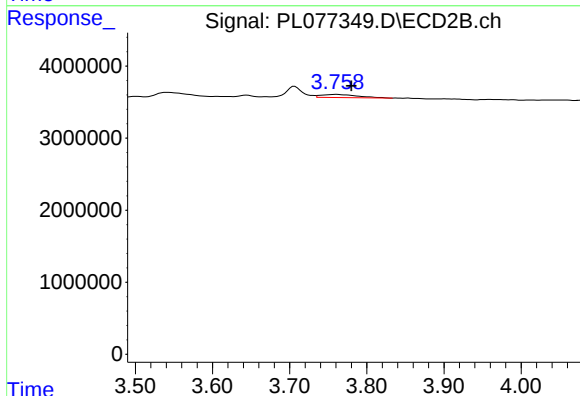


#4 Heptachlor

R.T.: 3.760 min
Delta R.T.: -0.020 min
Response: 1440132
Conc: 0.37 ng/ml

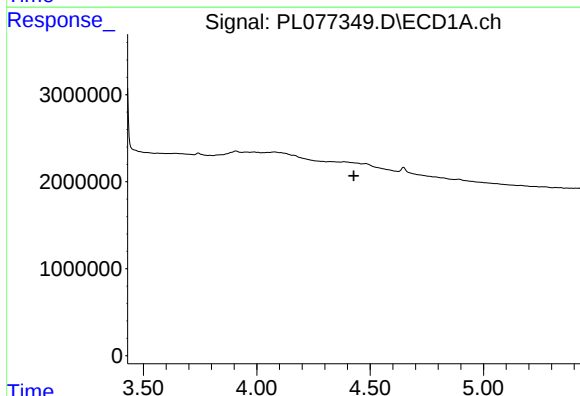


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.427 min
Response: 0
Conc: N.D.

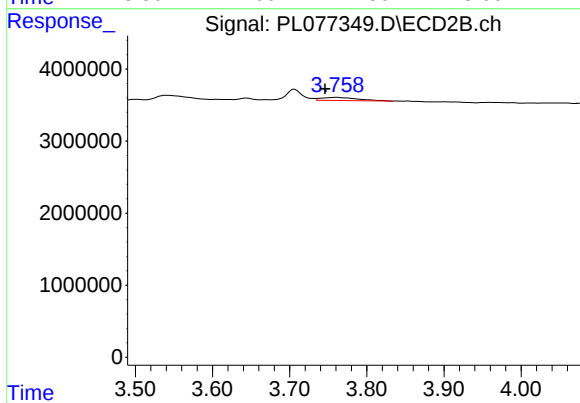

#6 beta-BHC


R.T.: 3.760 min
Delta R.T.: 0.014 min
Response: 1440132
Conc: 0.87 ng/ml

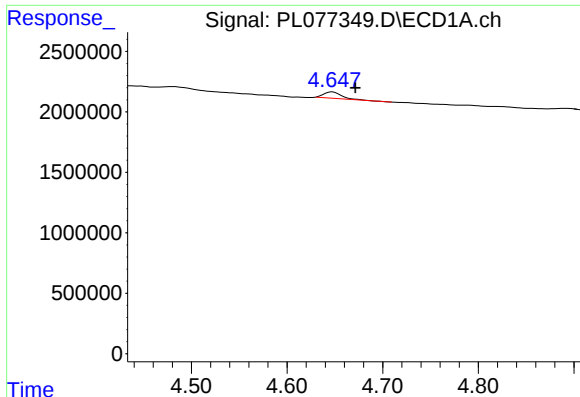

#7 delta-BHC


R.T.: 4.647 min
Delta R.T.: -0.024 min
Response: 644897
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

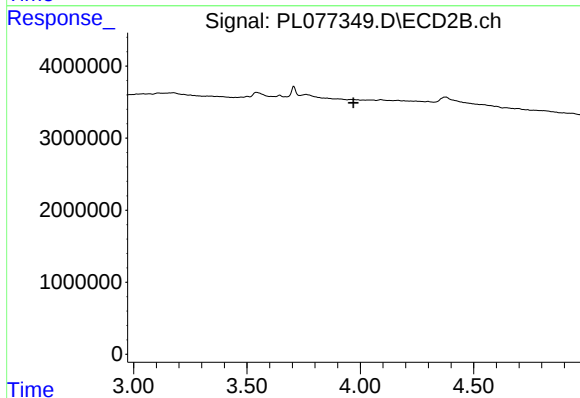


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

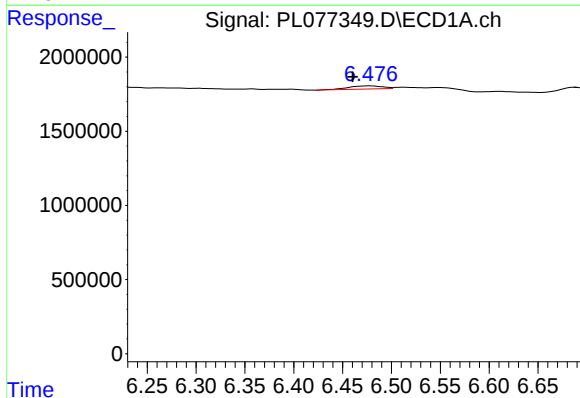


#14 Endrin

R.T.: 6.478 min
Delta R.T.: 0.017 min
Response: 526830
Conc: 0.45 ng/ml

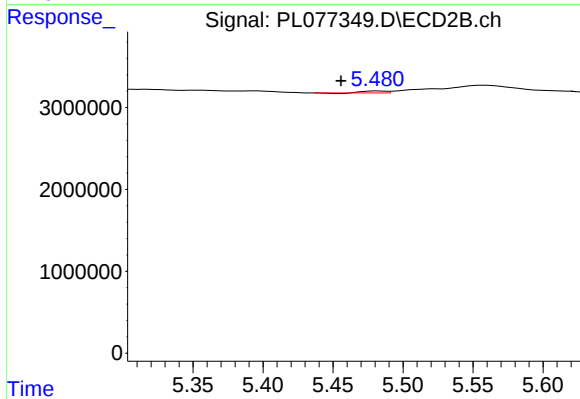

#14 Endrin


R.T.: 5.481 min
Delta R.T.: 0.026 min
Response: 223972
Conc: 0.08 ng/ml

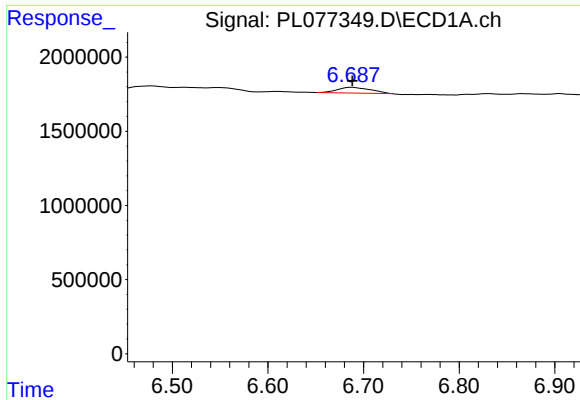

#15 Endosulfan II


R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 922848
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

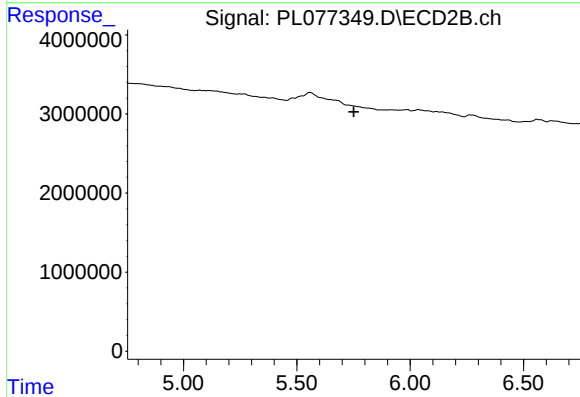


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

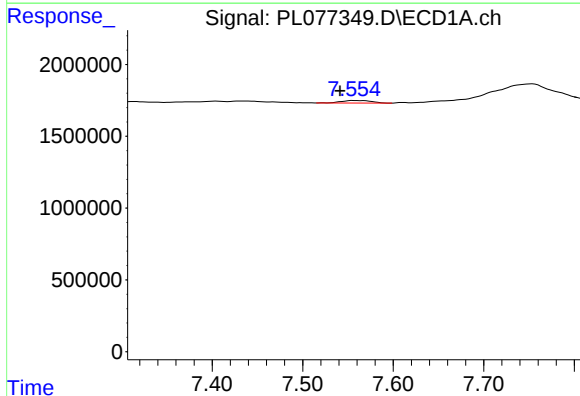


#21 Endrin ketone

R.T.: 7.556 min
Delta R.T.: 0.015 min
Response: 391507
Conc: 0.32 ng/ml

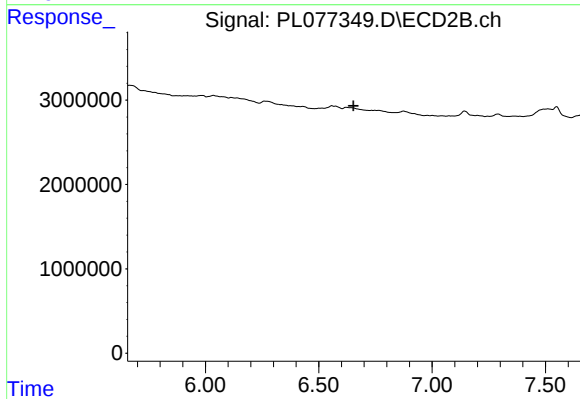

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.654 min
Response: 0
Conc: N.D.

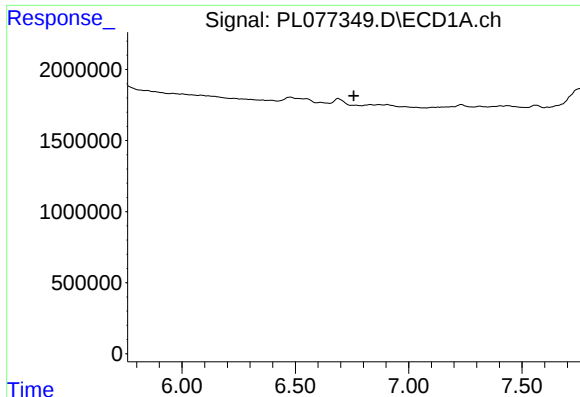

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

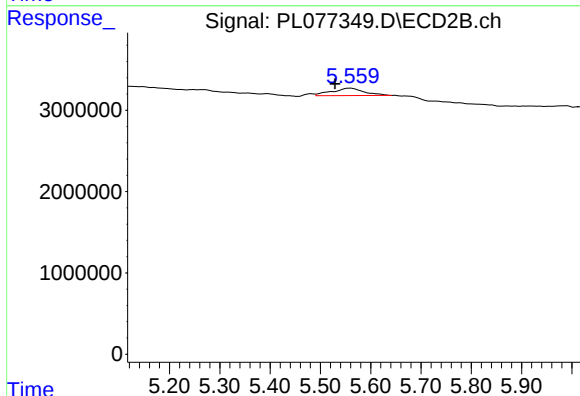


#27 Chlordane-5

R.T.: 5.558 min
Delta R.T.: 0.029 min
Response: 4059546
Conc: 46.37 ng/ml

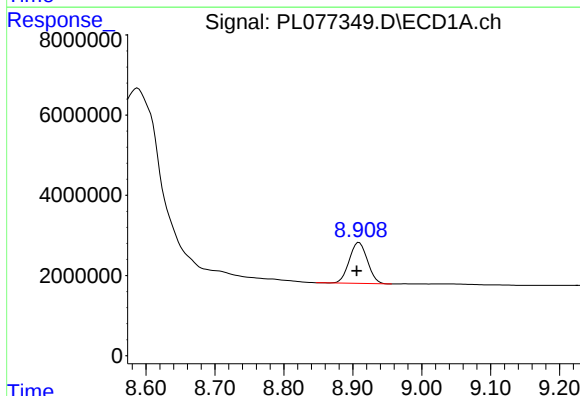

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.004 min
Response: 18700114
Conc: 15.96 ng/ml

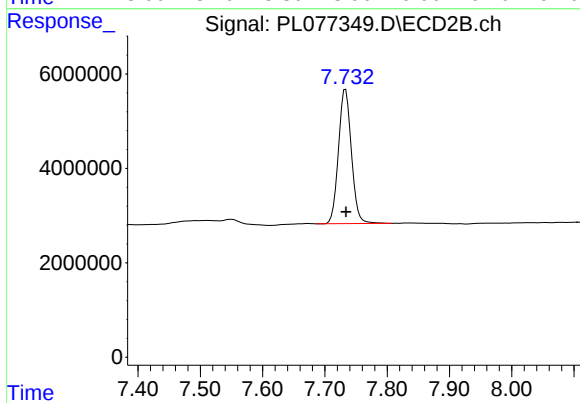

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 41057791
Conc: 14.71 ng/ml