

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082922\
 Data File : PL077348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2022 13:04
 Operator : AR\AJ
 Sample : N4395-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220738-MANASQUAN-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 15:22:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.647f	29475501	60485342	21.663	19.681
28)	SA Decachlor...	8.910	7.751f	19883311	44391575	16.967	15.909

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082922\
Data File : PL077348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2022 13:04
Operator : AR\AJ
Sample : N4395-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20220738-MANASQUAN-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 15:22:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

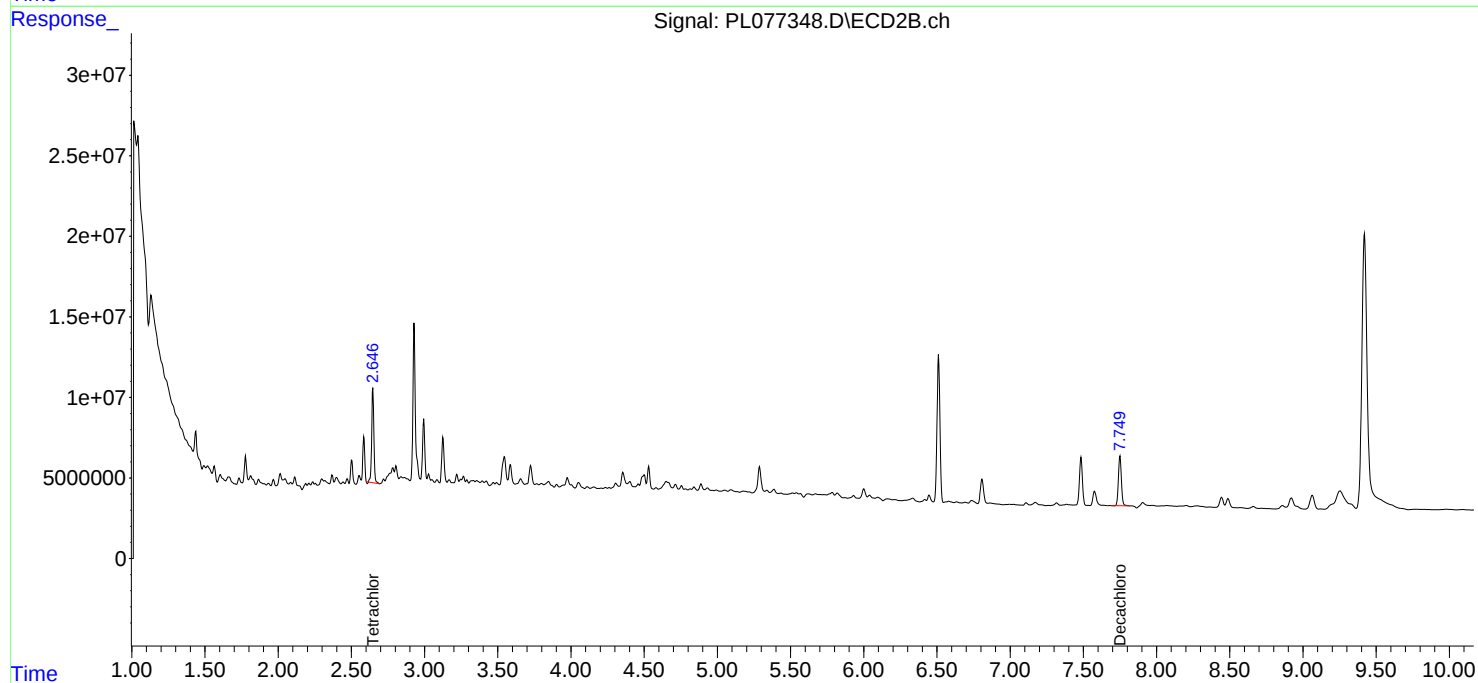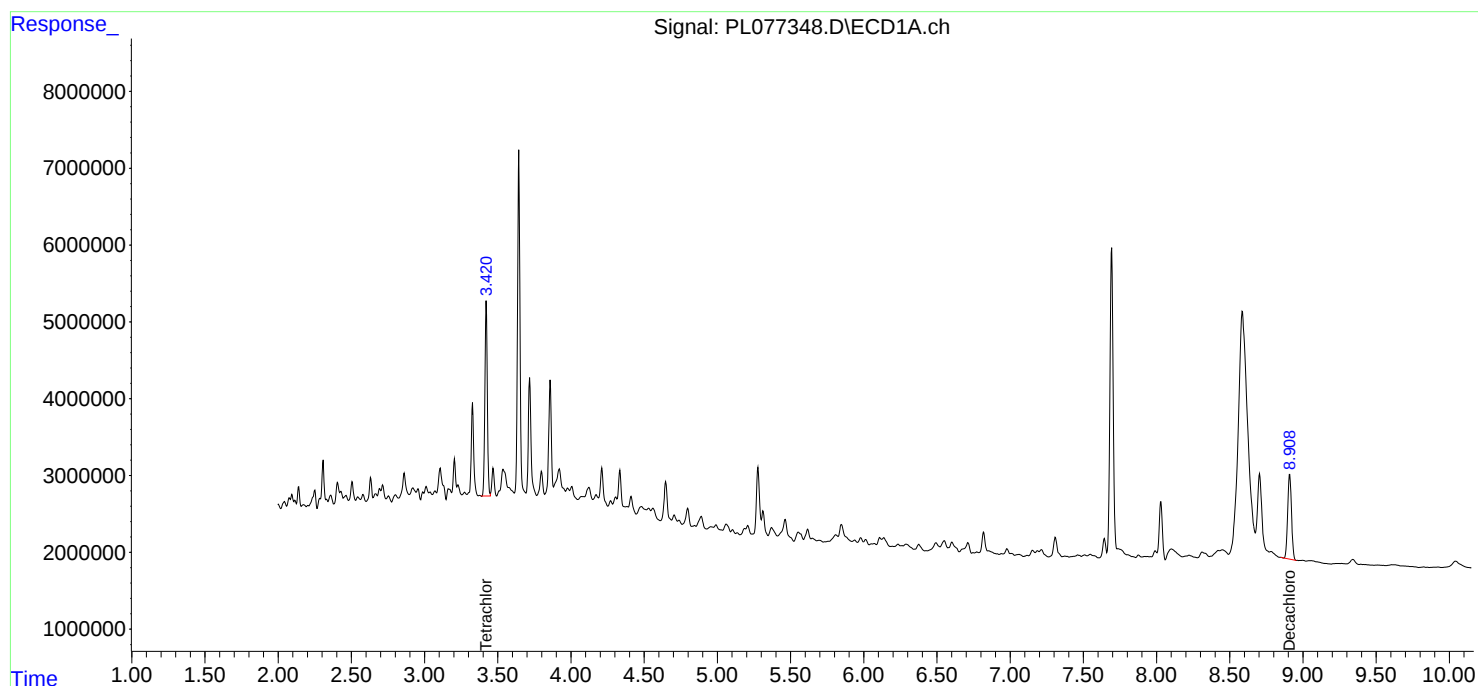


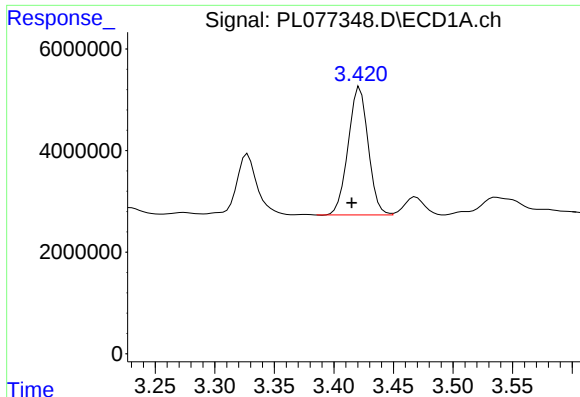

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.007 min
Response: 29475501
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220738-MANASQUAN-WATER

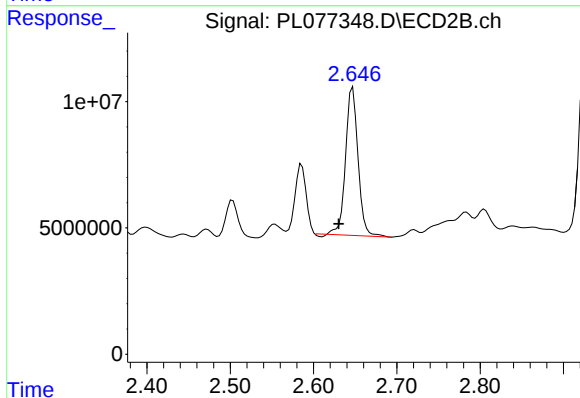


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.017 min
Response: 60485342
Conc: 19.68 ng/ml

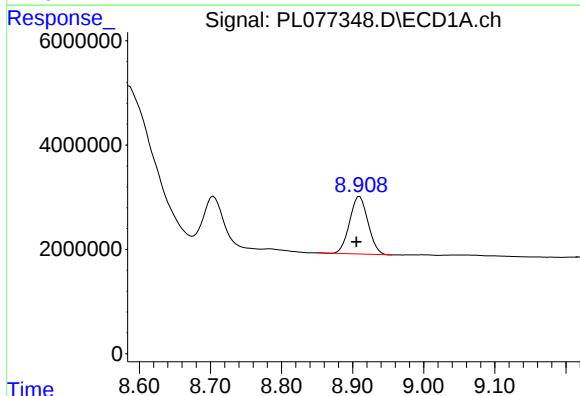

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.004 min
Response: 19883311
Conc: 16.97 ng/ml

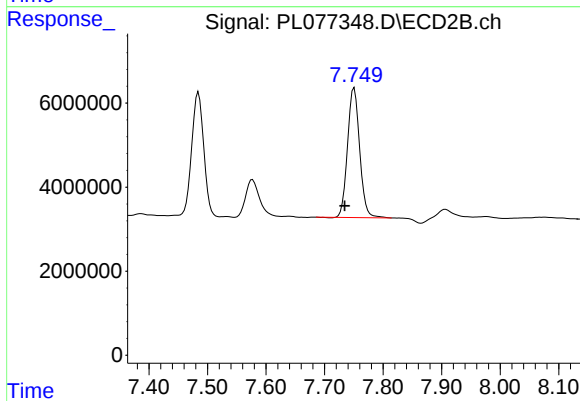

#28 Decachlorobiphenyl

R.T.: 7.751 min
Delta R.T.: 0.016 min
Response: 44391575
Conc: 15.91 ng/ml