
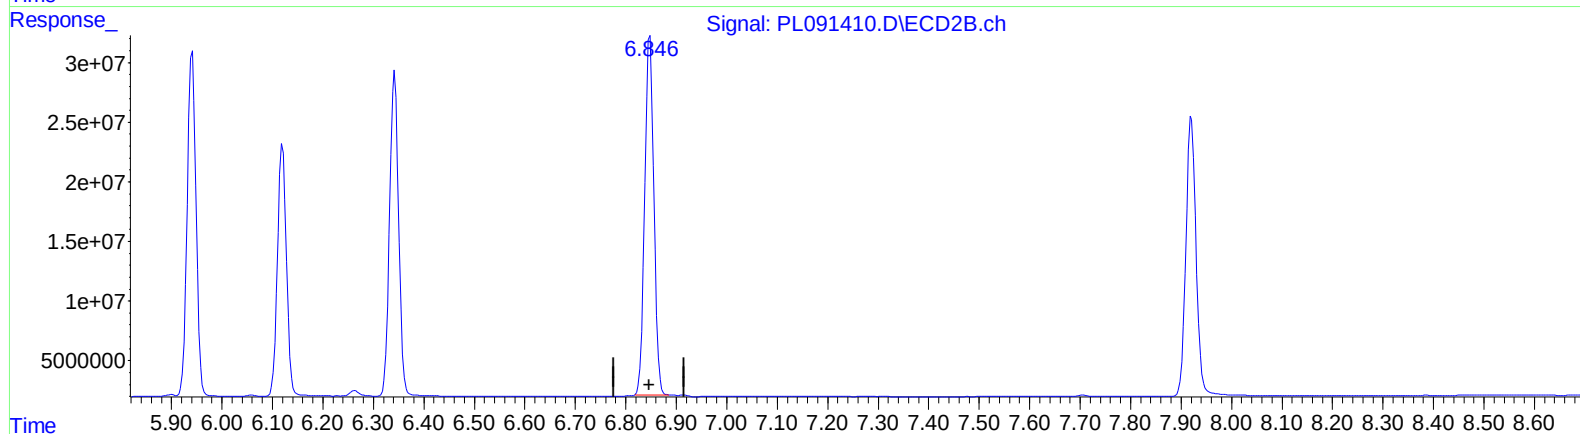


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082924\
Data File : PL091410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 08:33
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 09:22:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082924CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 29 09:22:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

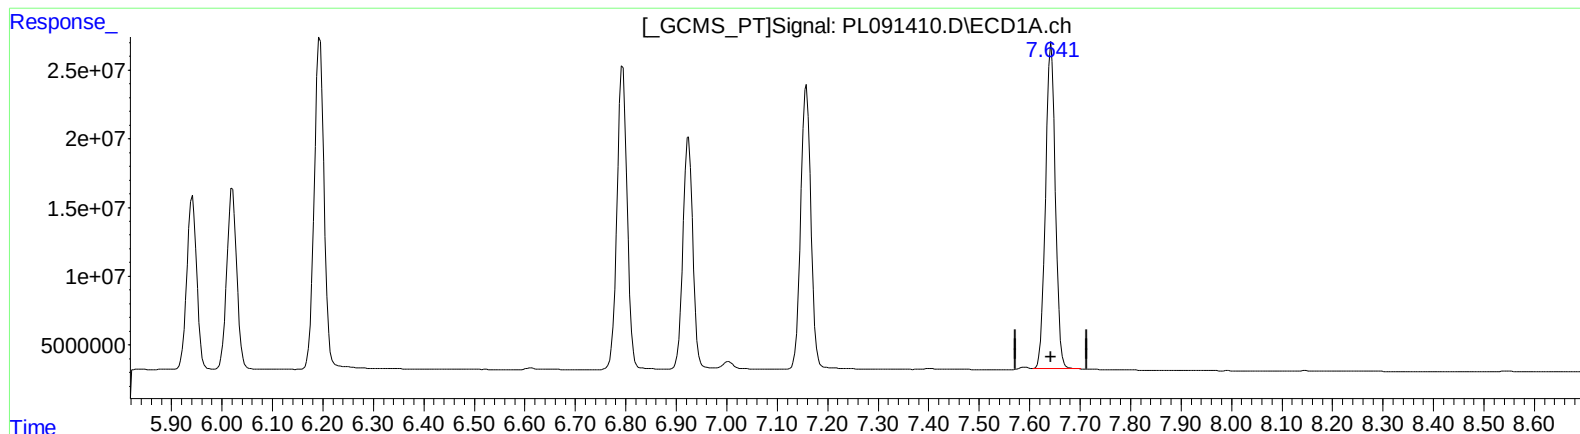

QEdit

(21) Endrin ketone (B)

7.643min 140.650 ng/ml

response 321465576

(21) Endrin ketone #2 (B)

6.848min 158.409 ng/ml



response 382349805

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082924\
Data File : PL091410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 08:33
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 09:22:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082924CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 29 09:22:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

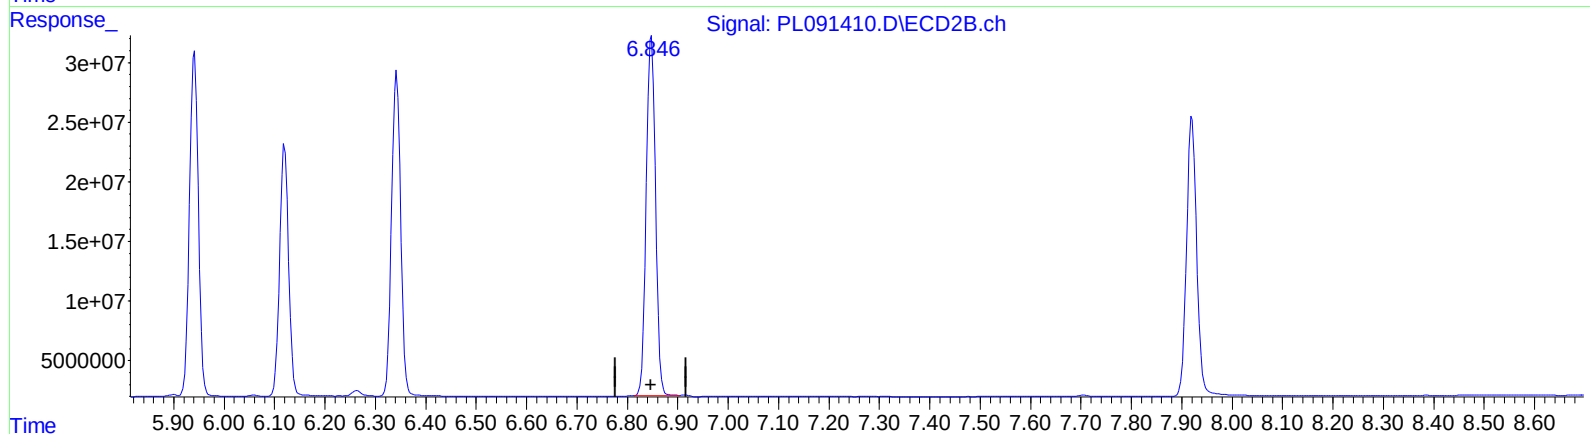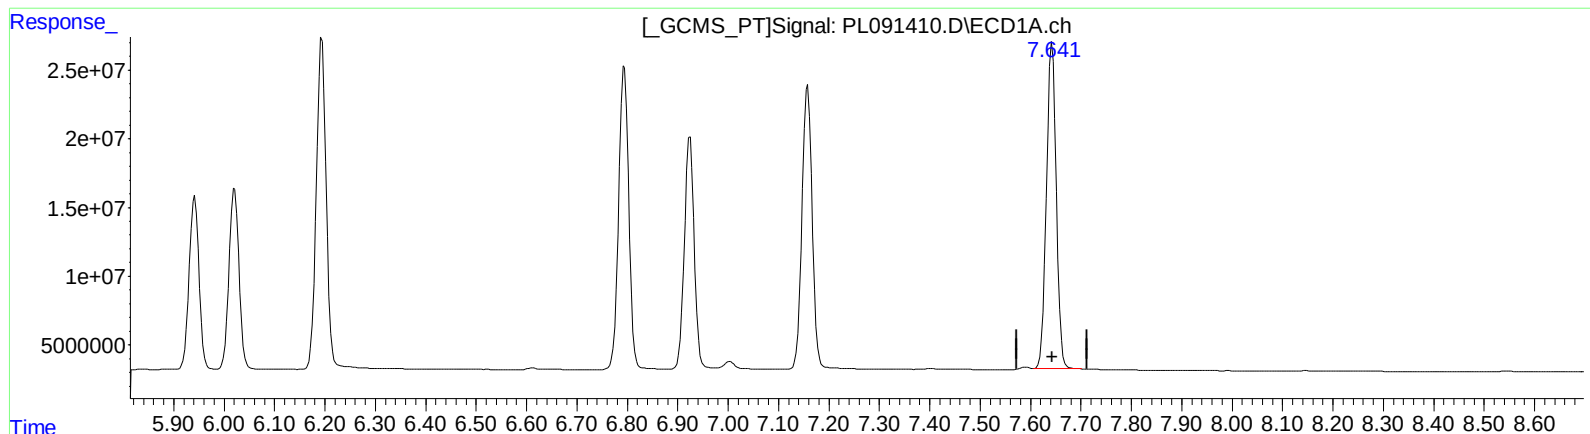

QEdit

(21) Endrin ketone (B)

7.643min 140.650 ng/ml

response 321465576

(21) Endrin ketone #2 (B)

6.846min 159.289 ng/ml m

response 384474567

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082924\
 Data File : PL091410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2024 08:33
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 09:22:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082924CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 29 09:22:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.783	162.3E6	178.1E6	71.387	78.833
27)	SA Decachlor...	9.053	7.921	233.7E6	326.7E6	133.238	146.275
Target Compounds							
5)	MB Aldrin	5.260	4.236	196.1E6	215.0E6	68.914	80.804
6)	B beta-BHC	4.527	3.915	104.8E6	108.0E6	68.418	76.501
7)	B delta-BHC	4.774	4.144	237.5E6	264.6E6	73.115	85.963
8)	B Heptachlo...	5.686	4.738	185.9E6	203.8E6	64.168	79.431
10)	B trans-Chl...	5.942	4.987	171.4E6	199.2E6	66.041	79.129
11)	B cis-Chlor...	6.021	5.051	182.3E6	203.4E6	68.318	78.487
12)	B 4,4'-DDE	6.194	5.240	325.4E6	398.6E6	146.395	167.485
15)	B Endosulfa...	6.794	5.941	307.0E6	350.8E6	137.625	158.513
18)	B Endrin al...	6.924	6.120	228.5E6	261.4E6	135.548	154.035
19)	B Endosulfa...	7.158	6.342	287.8E6	341.6E6	135.803	155.404
21)	B Endrin ke...	7.643	6.846	321.5E6	384.5E6	140.650	159.289m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082924\
Data File : PL091410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 08:33
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 09:22:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082924CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 29 09:22:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

