

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
 Data File : PL039629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 21:10
 Operator : AJ\SJ
 Sample : J4275-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:07:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	138.6E6	58043271	19.834	21.651
28)	SA Decachlor...	7.957	8.893	123.4E6	48252583	17.575	20.793
Target Compounds							
3)	MA gamma-BHC...	4.048f	0.000	9005732	0	0.849	N.D. #
6)	B beta-BHC	4.216f	0.000	3115194	0	0.671	N.D. #
7)	B delta-BHC	0.000	4.930	0	4024854	N.D.	1.011 #
9)	A Endosulfan I	5.318	0.000	7782008	0	0.889	N.D. #
19)	B Endosulfa...	6.453	0.000	19052386	0	2.342	N.D. #
23)	Chlordane-1	0.000	4.930	0	4024854	N.D.	32.216 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
Data File : PL039629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 21:10
Operator : AJ\SJ
Sample : J4275-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:07:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

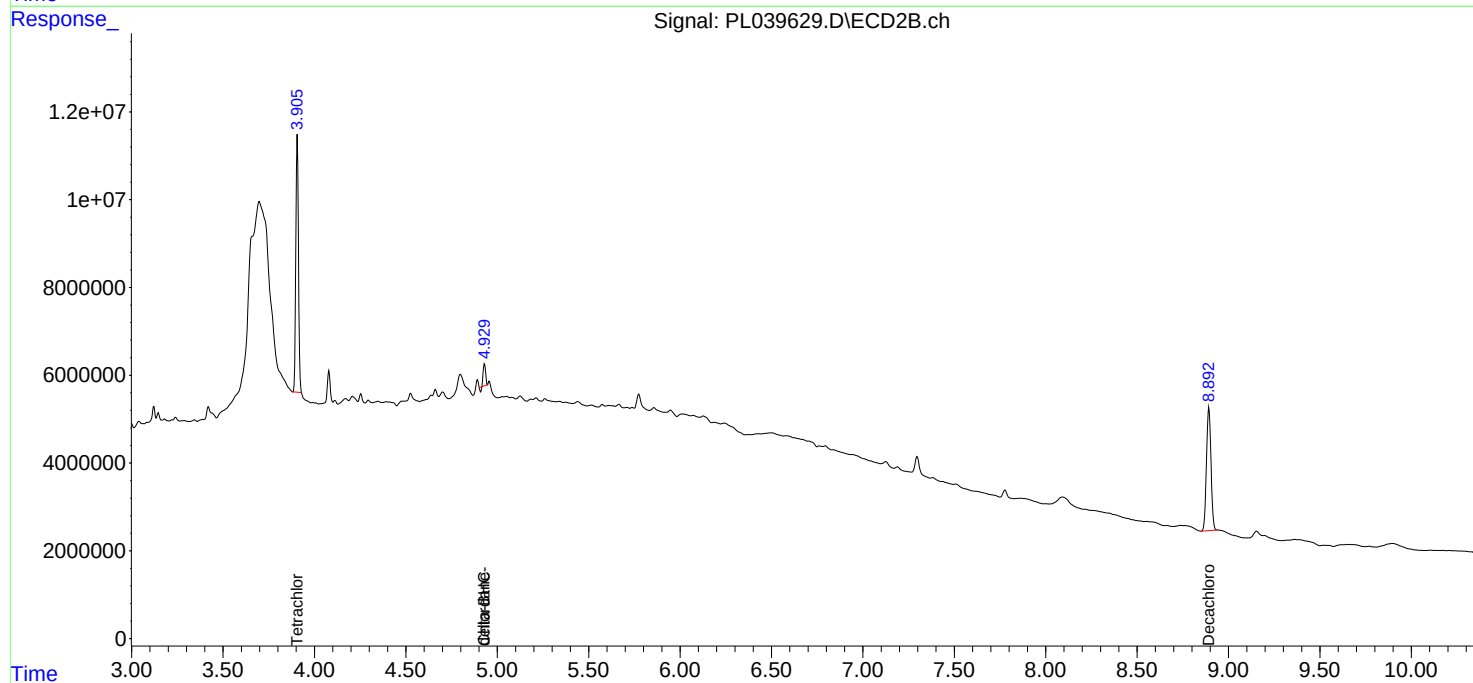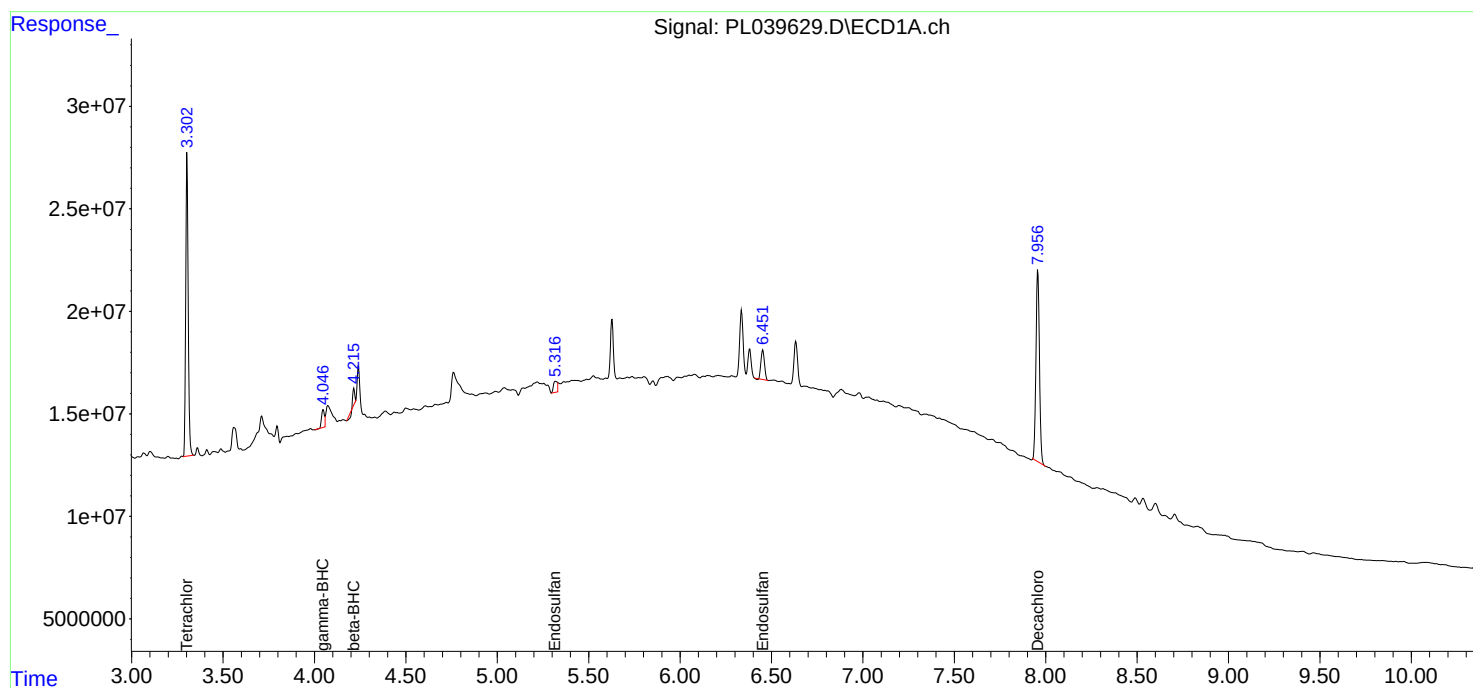


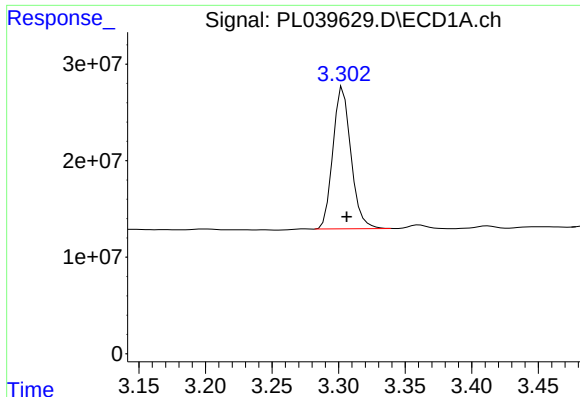

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 138648727
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

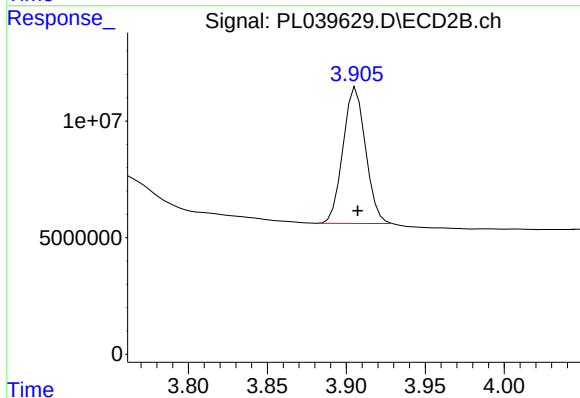


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 58043271
Conc: 21.65 ng/ml

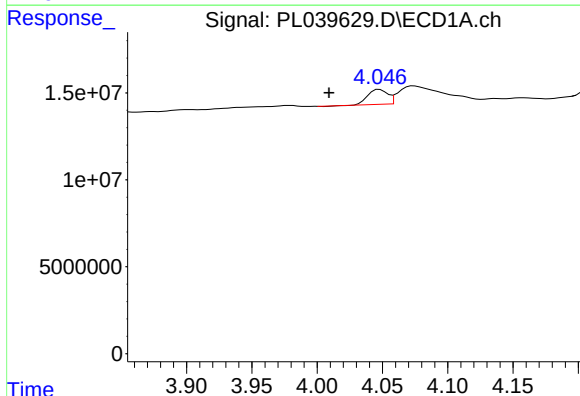


#3 gamma-BHC (Lindane)

R.T.: 4.048 min
Delta R.T.: 0.039 min
Response: 9005732
Conc: 0.85 ng/ml

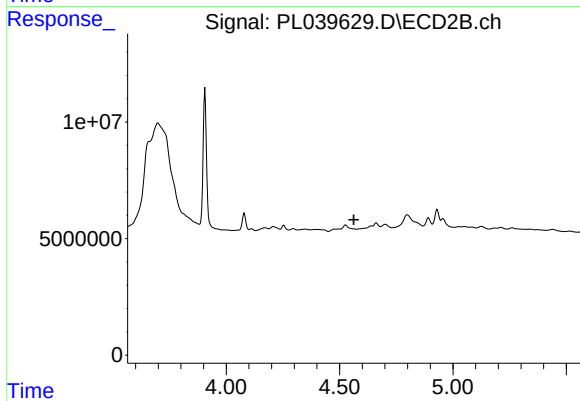

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

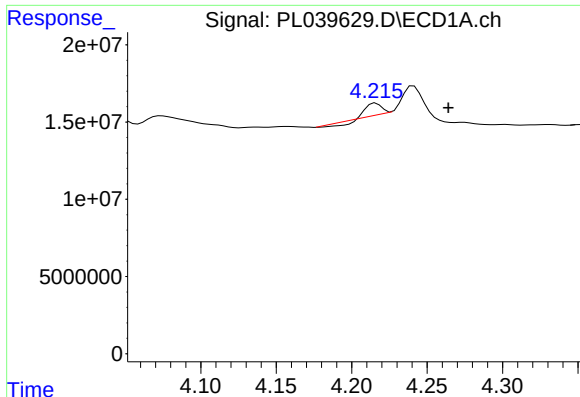

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 3115194
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

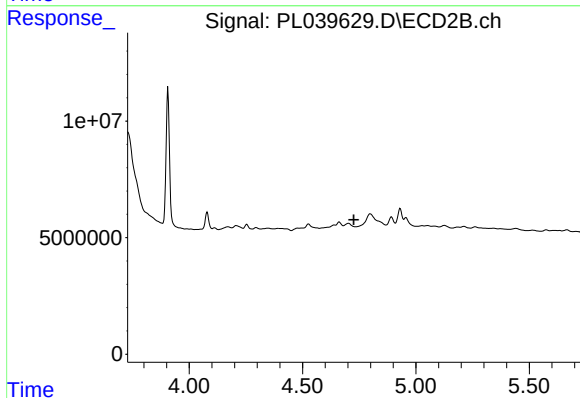


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

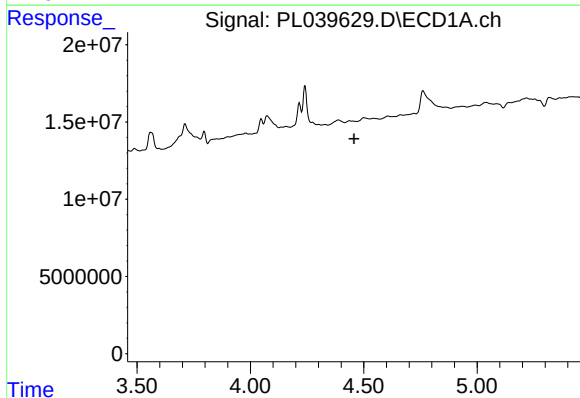


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

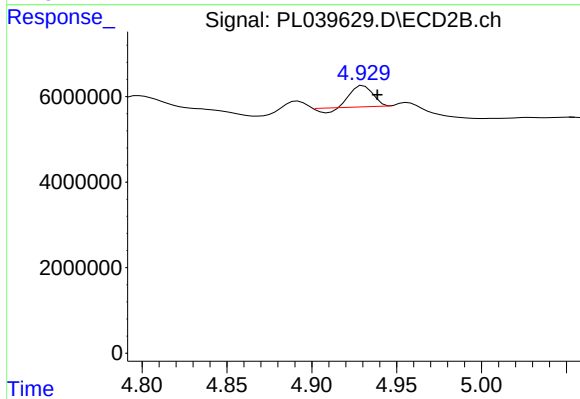

#7 delta-BHC


R.T.: 4.930 min
Delta R.T.: -0.008 min
Response: 4024854
Conc: 1.01 ng/ml

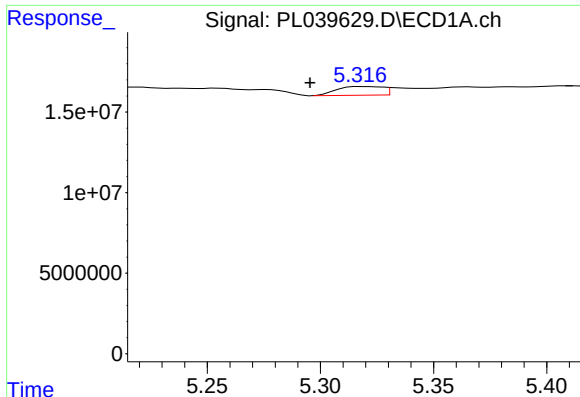

#9 Endosulfan I


R.T.: 5.318 min
Delta R.T.: 0.023 min
Response: 7782008
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

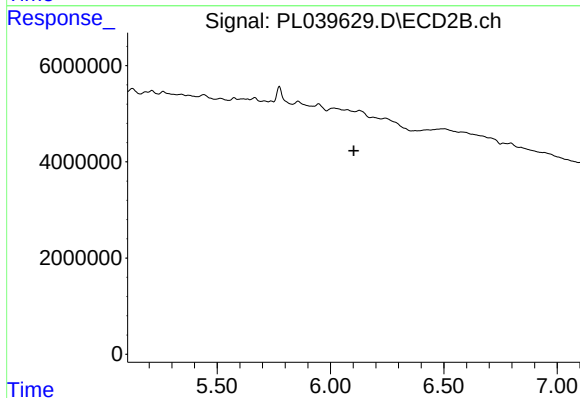


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

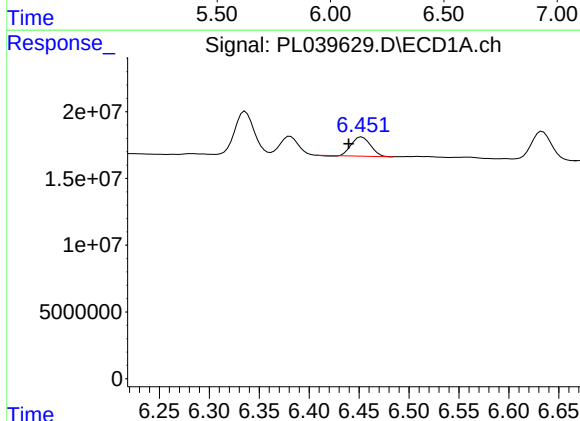


#19 Endosulfan Sulfate

R.T.: 6.453 min
Delta R.T.: 0.013 min
Response: 19052386
Conc: 2.34 ng/ml

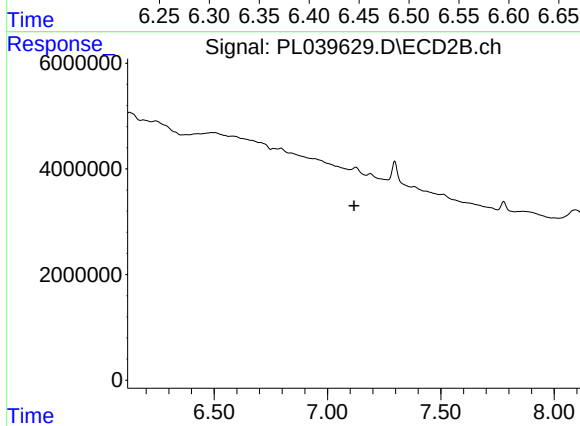

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

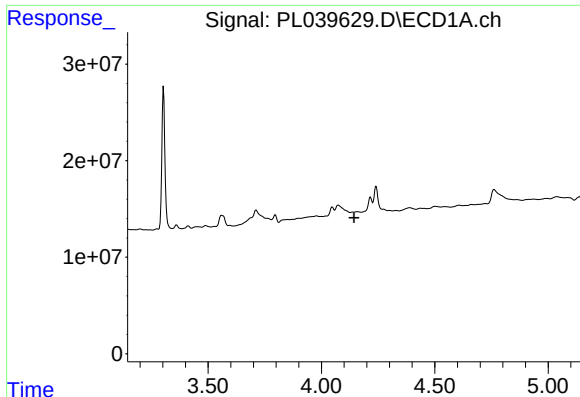

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

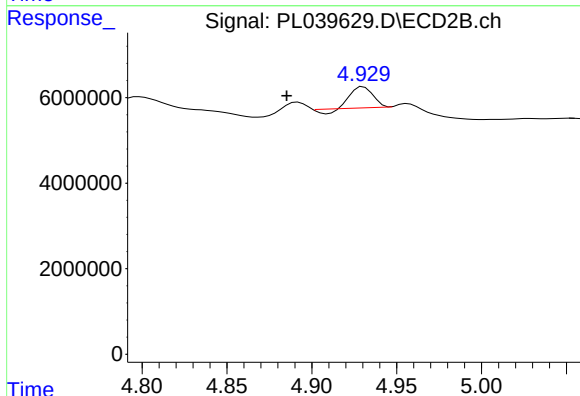


#23 Chlordane-1

R.T.: 4.930 min
Delta R.T.: 0.045 min
Response: 4024854
Conc: 32.22 ng/ml

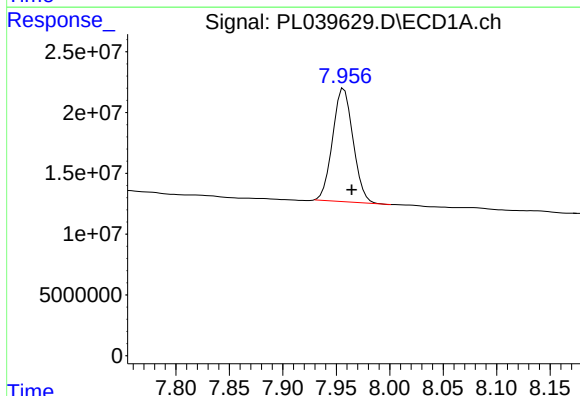

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 123436964
Conc: 17.58 ng/ml

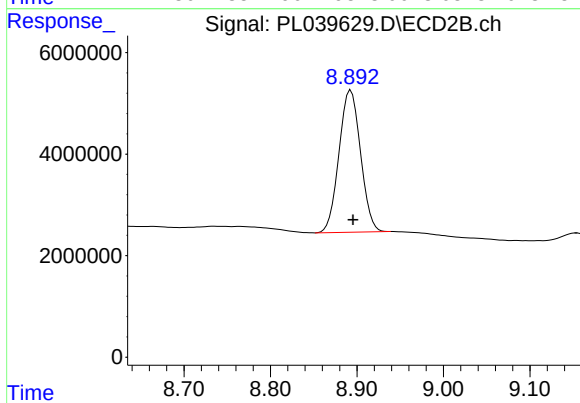

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.003 min
Response: 48252583
Conc: 20.79 ng/ml