

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
 Data File : PL039635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 22:36
 Operator : AJ\SJ
 Sample : J4699-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:09:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	144.5E6	61278044	20.676	22.857
28)	SA Decachlor...	7.957	8.893	135.9E6	53576448	19.354	23.087
Target Compounds							
5)	MB Aldrin	4.529	0.000	5662880	0	0.565	N.D. #
6)	B beta-BHC	4.215f	0.000	22625552	0	4.870	N.D. #
7)	B delta-BHC	0.000	4.930	0	8255539	N.D.	2.073 #
8)	B Heptachlo...	4.928f	0.000	1960793	0	0.205	N.D. #
9)	A Endosulfan I	5.326	0.000	7913829	0	0.904	N.D. #
19)	B Endosulfa...	6.452	0.000	17867748	0	2.196	N.D. #
21)	B Endrin ke...	6.866f	0.000	12586936	0	1.462	N.D. #
23)	Chlordane-1	4.138	4.930	3342143	8255539	10.557	66.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
Data File : PL039635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 22:36
Operator : AJ\SJ
Sample : J4699-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:09:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

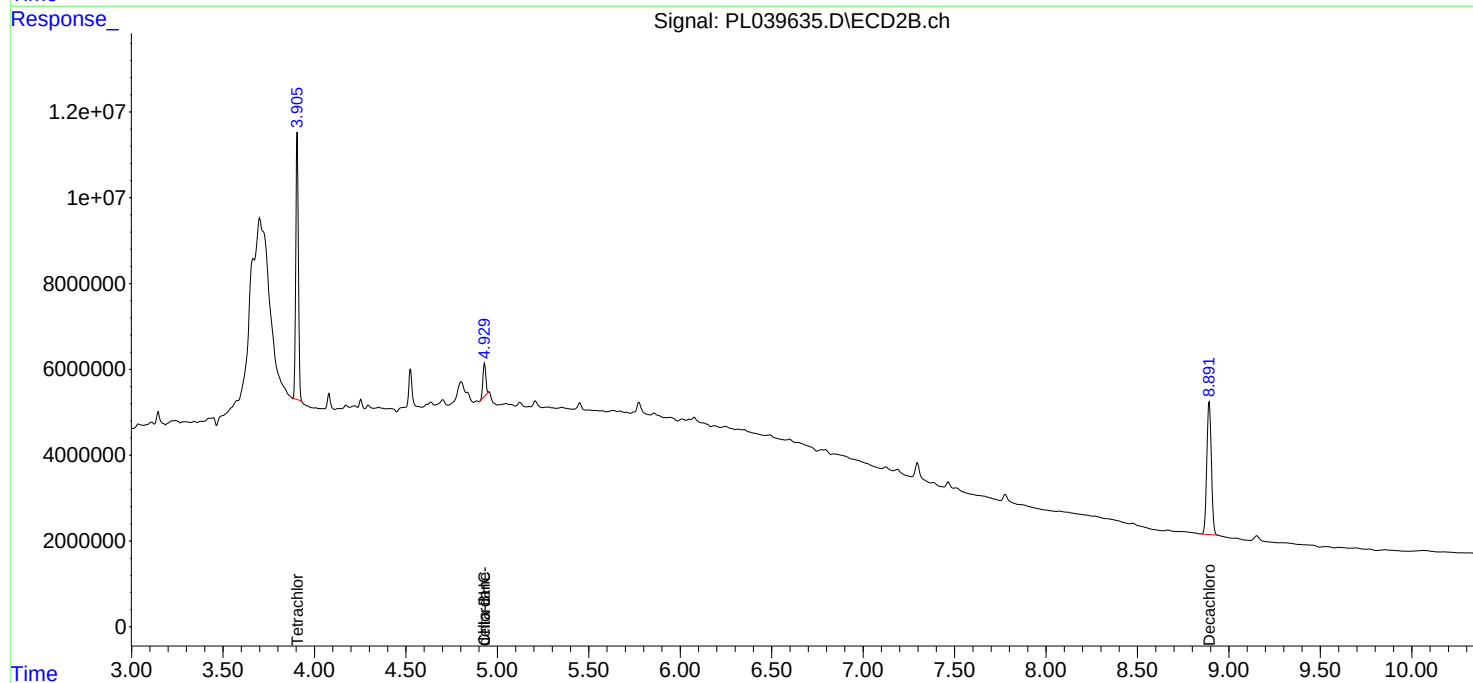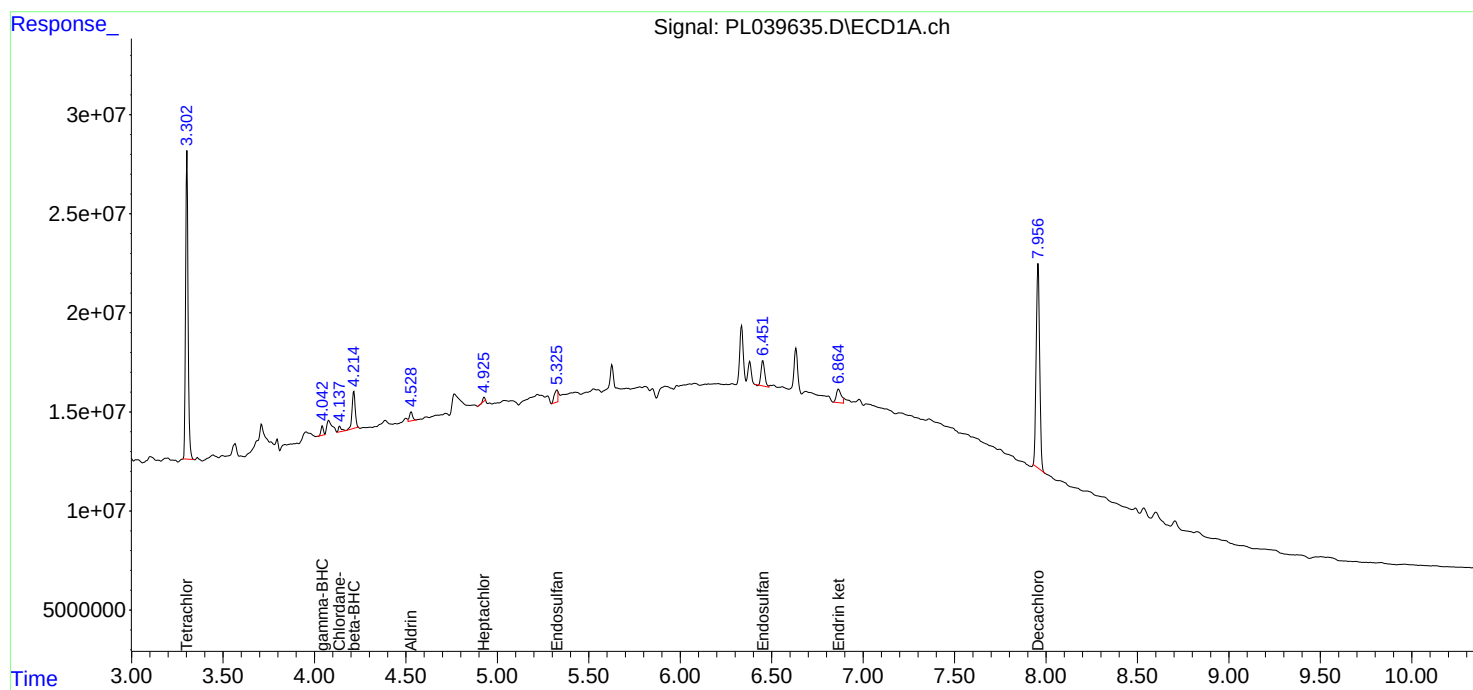


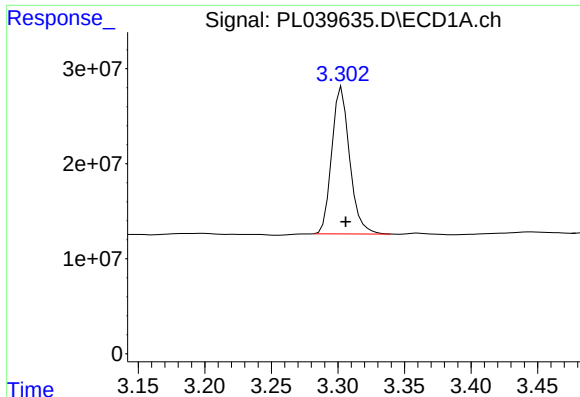

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 144536344
Conc: 20.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

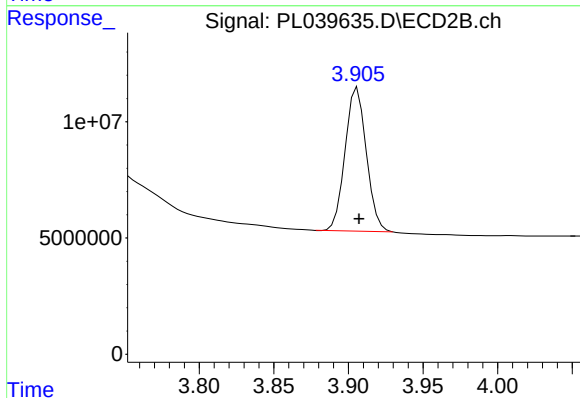


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 61278044
Conc: 22.86 ng/ml

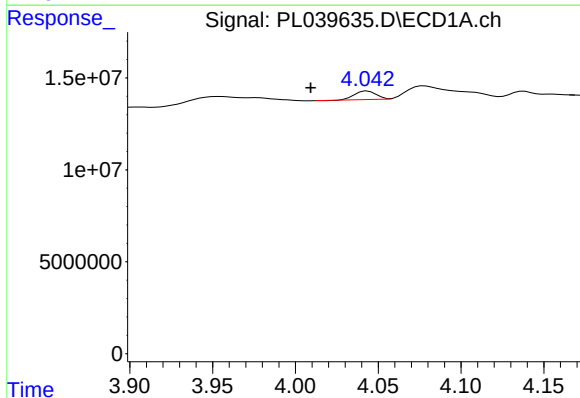


#3 gamma-BHC (Lindane)

R.T.: 4.044 min
Delta R.T.: 0.034 min
Response: 4254473
Conc: 0.40 ng/ml

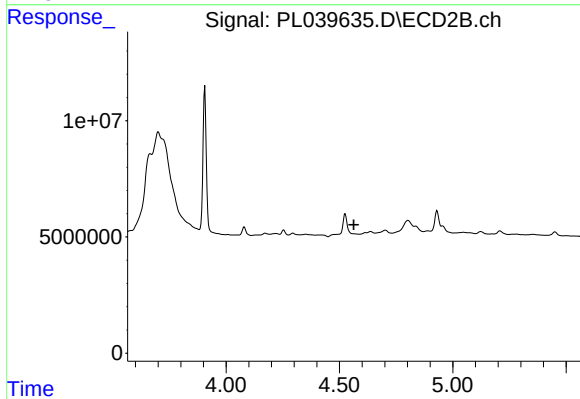

#3 gamma-BHC (Lindane)


R.T.: 4.525 min
Delta R.T.: -0.038 min
Response: -8705094
Conc: N.D.

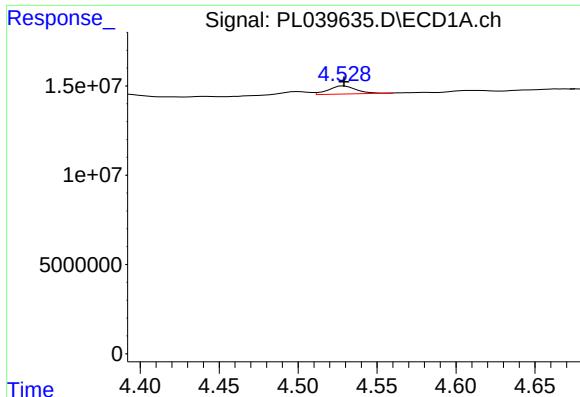

#5 Aldrin


R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 5662880
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

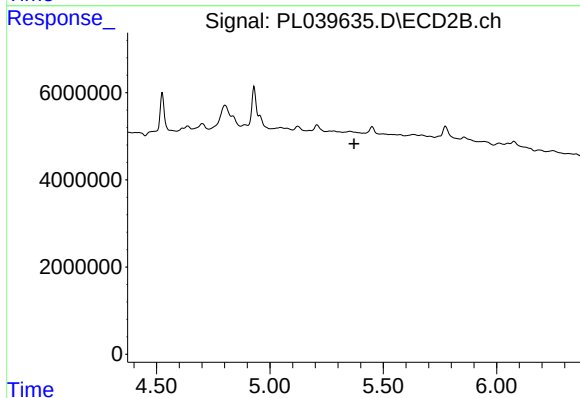


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.372 min
Response: 0
Conc: N.D.

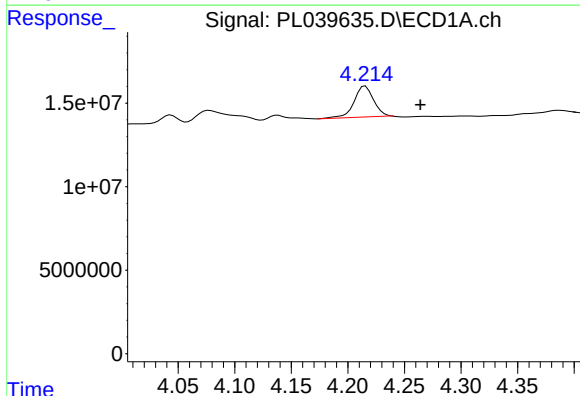


#6 beta-BHC

R.T.: 4.215 min
Delta R.T.: -0.049 min
Response: 22625552
Conc: 4.87 ng/ml

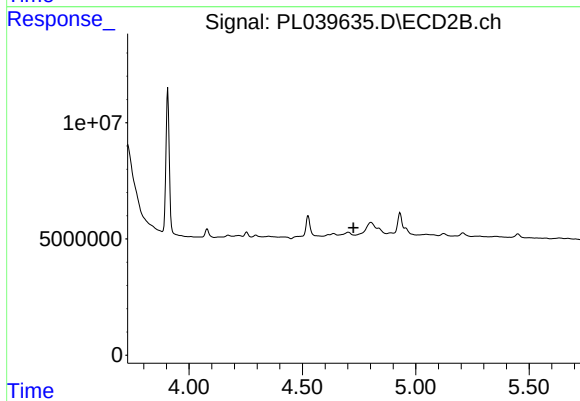

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

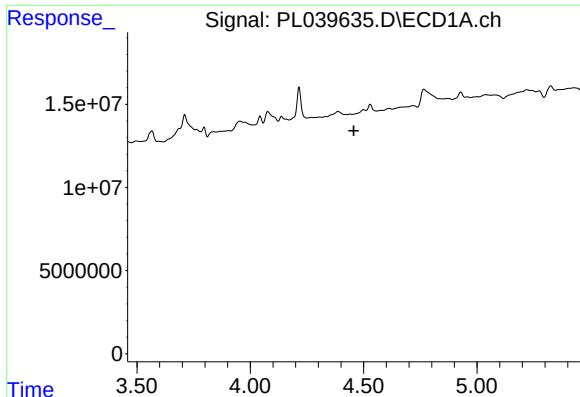

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

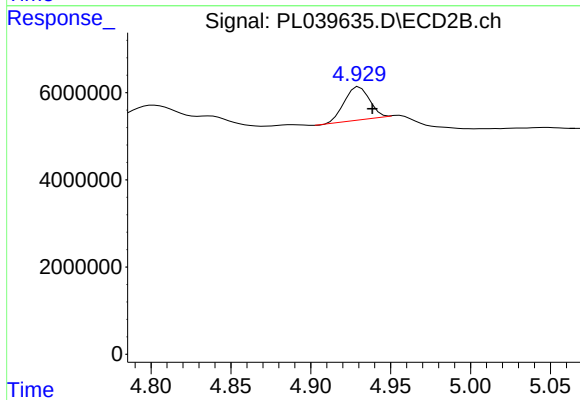


#7 delta-BHC

R.T.: 4.930 min
Delta R.T.: -0.008 min
Response: 8255539
Conc: 2.07 ng/ml

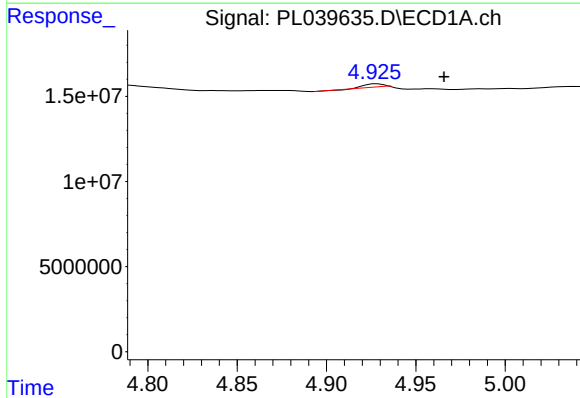


#8 Heptachlor epoxide

R.T.: 4.928 min
Delta R.T.: -0.037 min
Response: 1960793
Conc: 0.21 ng/ml

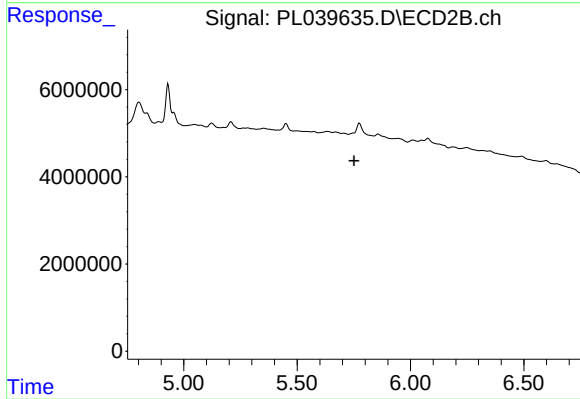

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

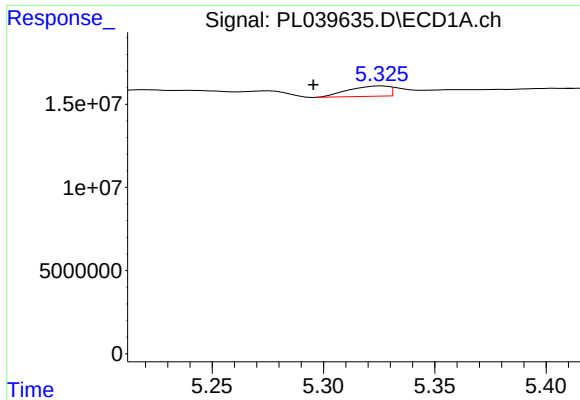

#9 Endosulfan I


R.T.: 5.326 min
Delta R.T.: 0.031 min
Response: 7913829
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

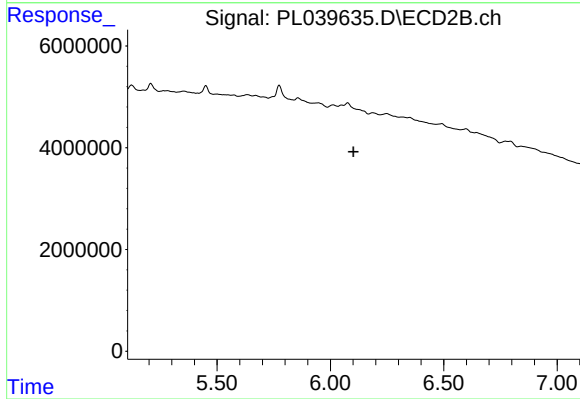


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

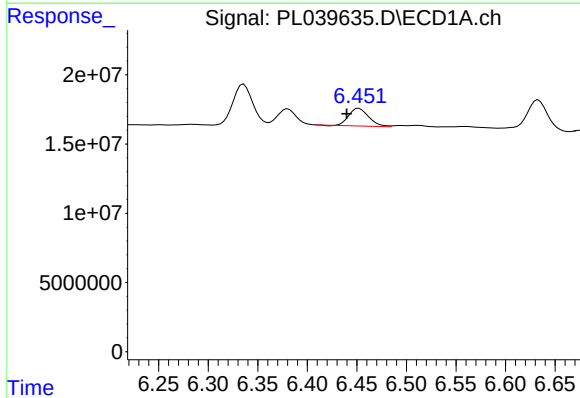


#19 Endosulfan Sulfate

R.T.: 6.452 min
Delta R.T.: 0.012 min
Response: 17867748
Conc: 2.20 ng/ml

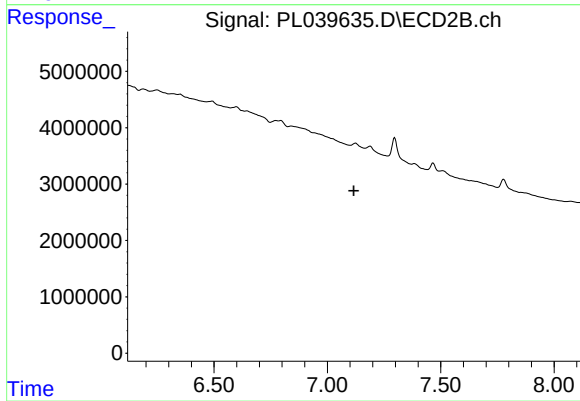

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

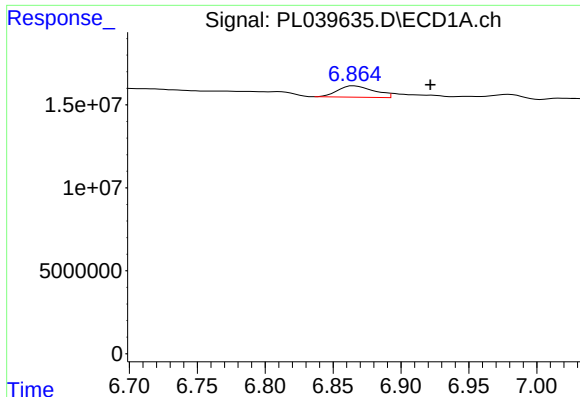

#21 Endrin ketone


R.T.: 6.866 min
Delta R.T.: -0.056 min
Response: 12586936
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

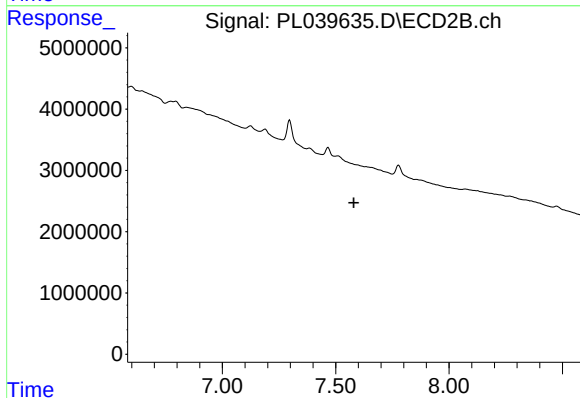


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.580 min
Response: 0
Conc: N.D.

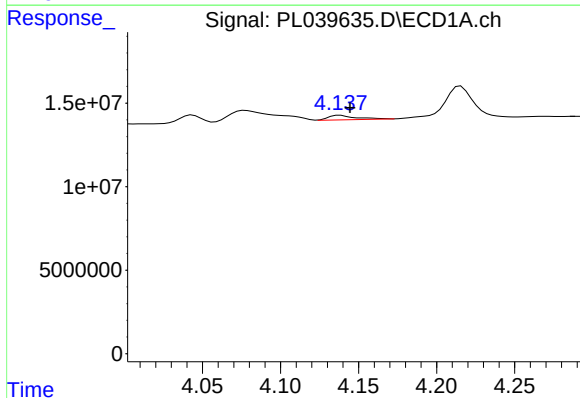


#23 Chlordane-1

R.T.: 4.138 min
Delta R.T.: -0.006 min
Response: 3342143
Conc: 10.56 ng/ml

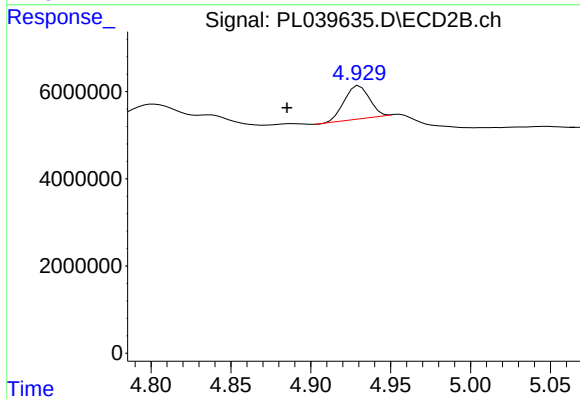

#23 Chlordane-1


R.T.: 4.930 min
Delta R.T.: 0.045 min
Response: 8255539
Conc: 66.08 ng/ml

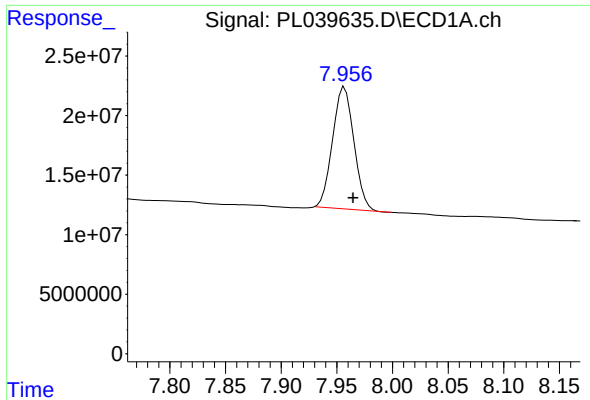

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.008 min
Response: 135933764
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

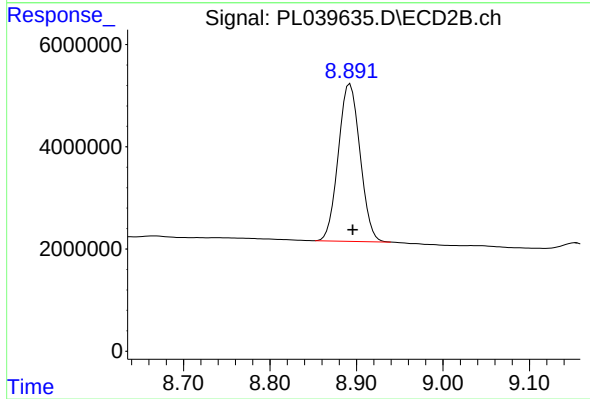

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.003 min
Response: 53576448
Conc: 23.09 ng/ml