

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
 Data File : PL039636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 22:50
 Operator : AJ\SJ
 Sample : J4275-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 03:09:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.906	83788407	34031181	11.986	12.694
28)	SA Decachlor...	7.957	8.893	57740453	26970589	8.221	11.622 #
Target Compounds							
23)	Chlordane-1	4.213	0.000	10970534	0	34.653	N.D. #
24)	Chlordane-2	4.665	0.000	13356126	0	38.205	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083018\
Data File : PL039636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 22:50
Operator : AJ\SJ
Sample : J4275-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 03:09:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

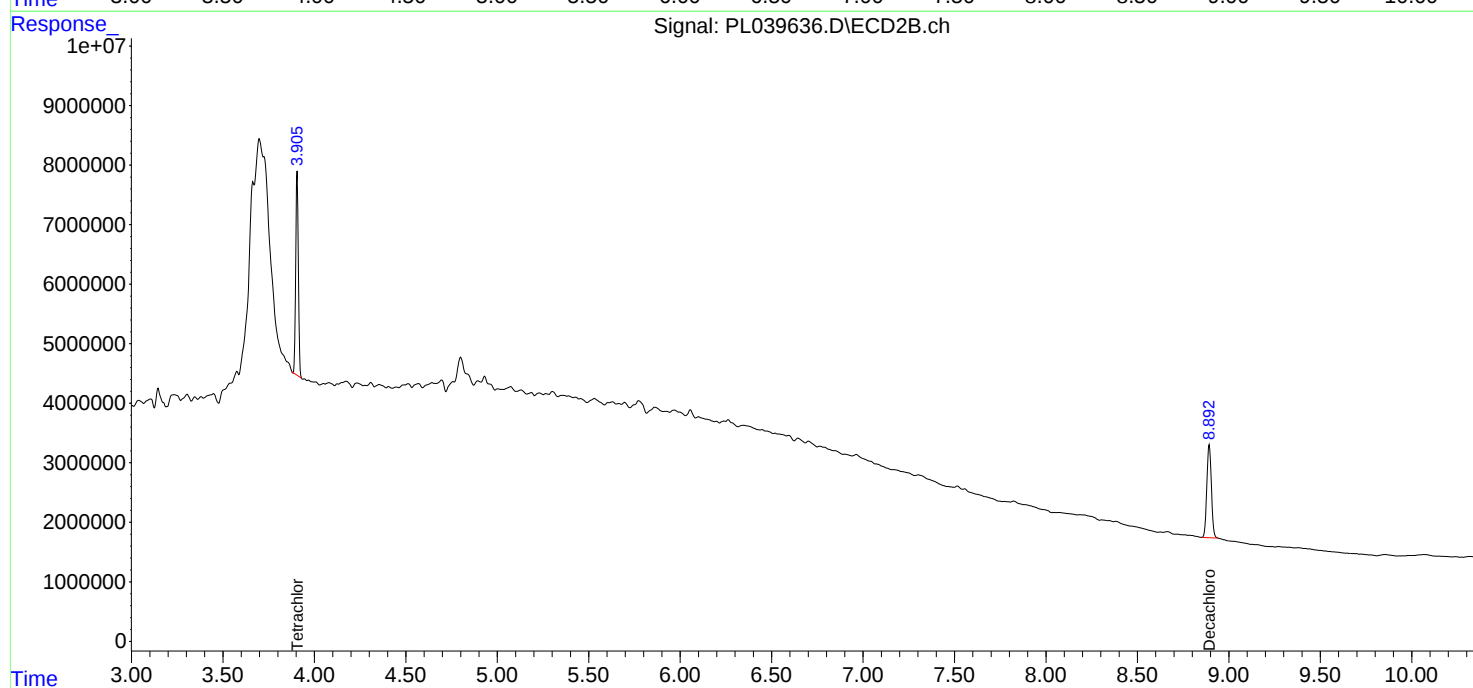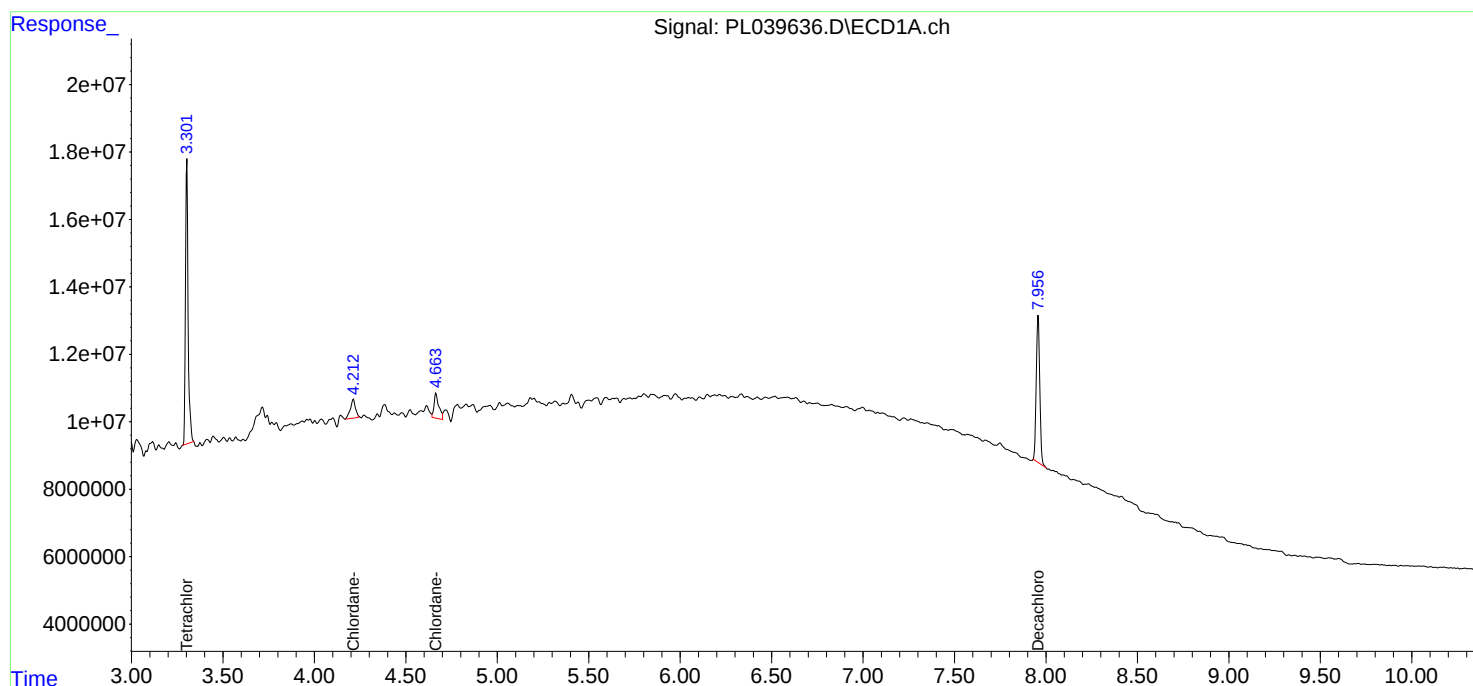


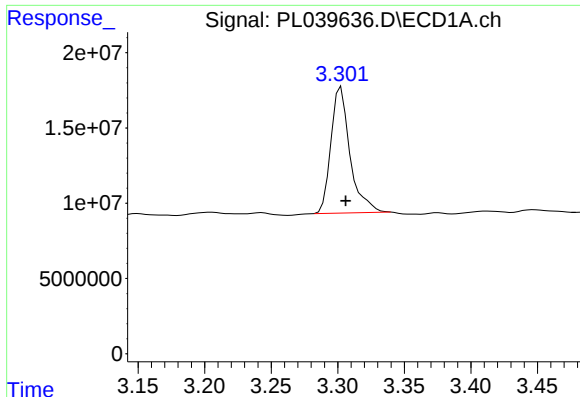

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 83788407
Conc: 11.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

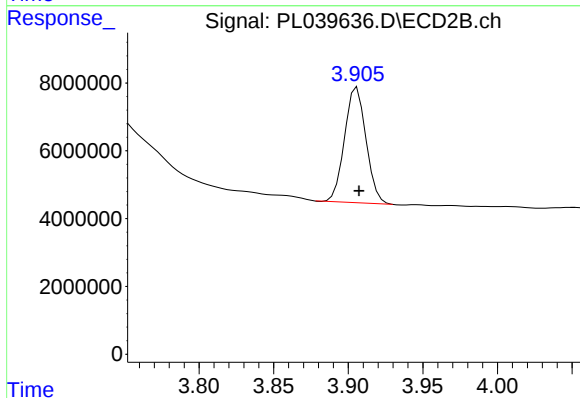


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 34031181
Conc: 12.69 ng/ml

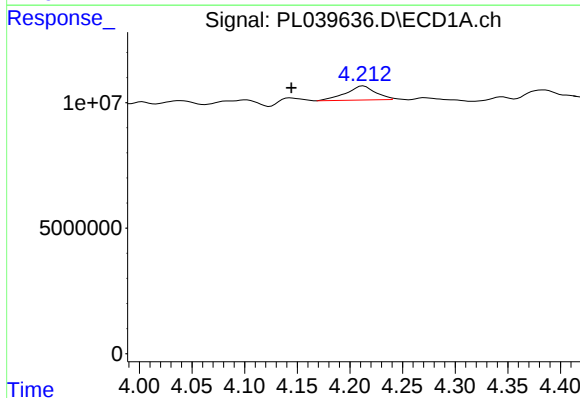


#23 Chlordane-1

R.T.: 4.213 min
Delta R.T.: 0.068 min
Response: 10970534
Conc: 34.65 ng/ml

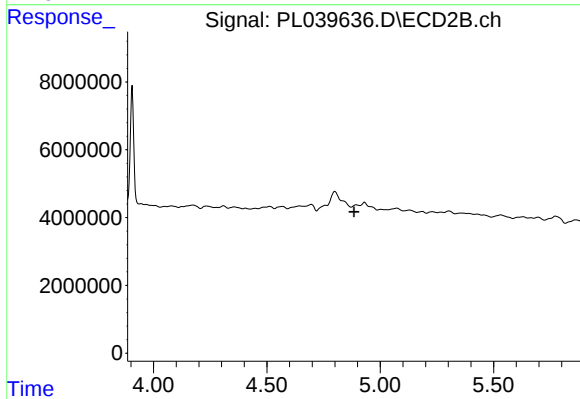

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

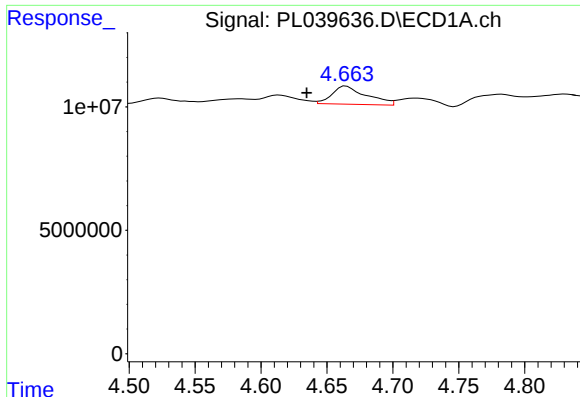

#24 Chlordane-2


R.T.: 4.665 min
Delta R.T.: 0.030 min
Response: 13356126
Conc: 38.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

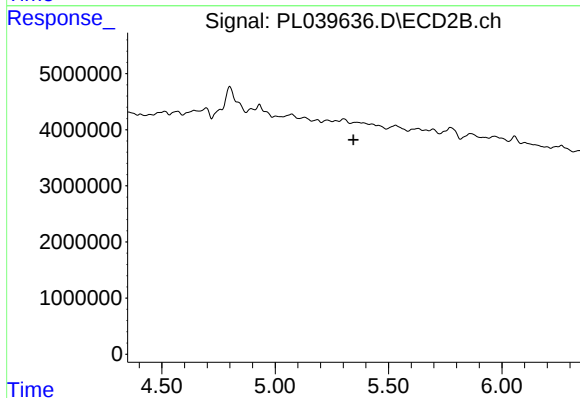


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

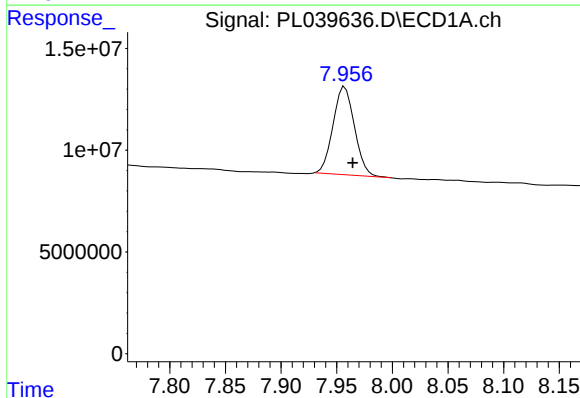

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 57740453
Conc: 8.22 ng/ml

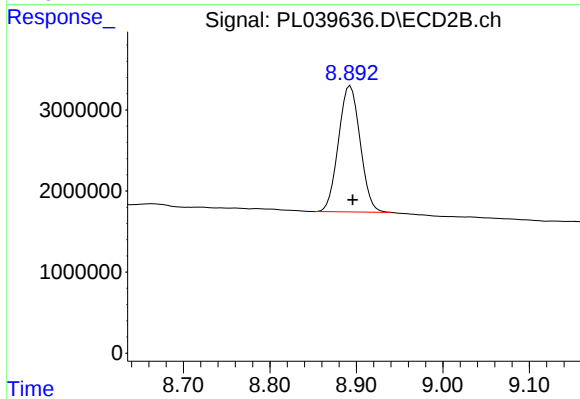

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 26970589
Conc: 11.62 ng/ml