

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 18:30
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 22:50:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	228.4E6	56354112	26.691	25.794
28)	SA Decachlor...	7.970	8.949	298.2E6	73390327	24.570	24.111
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	452435	N.D.	0.310 #
8)	B Heptachlo...	0.000	5.784	0	21545079	N.D.	6.384 #
9)	A Endosulfan I	5.324f	0.000	15029237	0	1.118	N.D. #
11)	B alpha-Chl...	0.000	6.094	0	139133	N.D.	0.040 #
13)	MA Dieldrin	5.540	6.409	9633670	-240488	0.634	N.D. #
14)	MA Endrin	5.808	6.620	4442305	-209420	0.305	N.D. #
15)	B Endosulfa...	0.000	6.842	0	282904	N.D.	0.086 #
18)	B Endrin al...	0.000	6.978f	0	855659	N.D.	0.303 #
26)	Chlordane-4	0.000	6.094	0	139133	N.D.	0.256 #
27)	Chlordane-5	0.000	6.914f	0	545260	N.D.	5.531 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 18:30
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 22:50:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

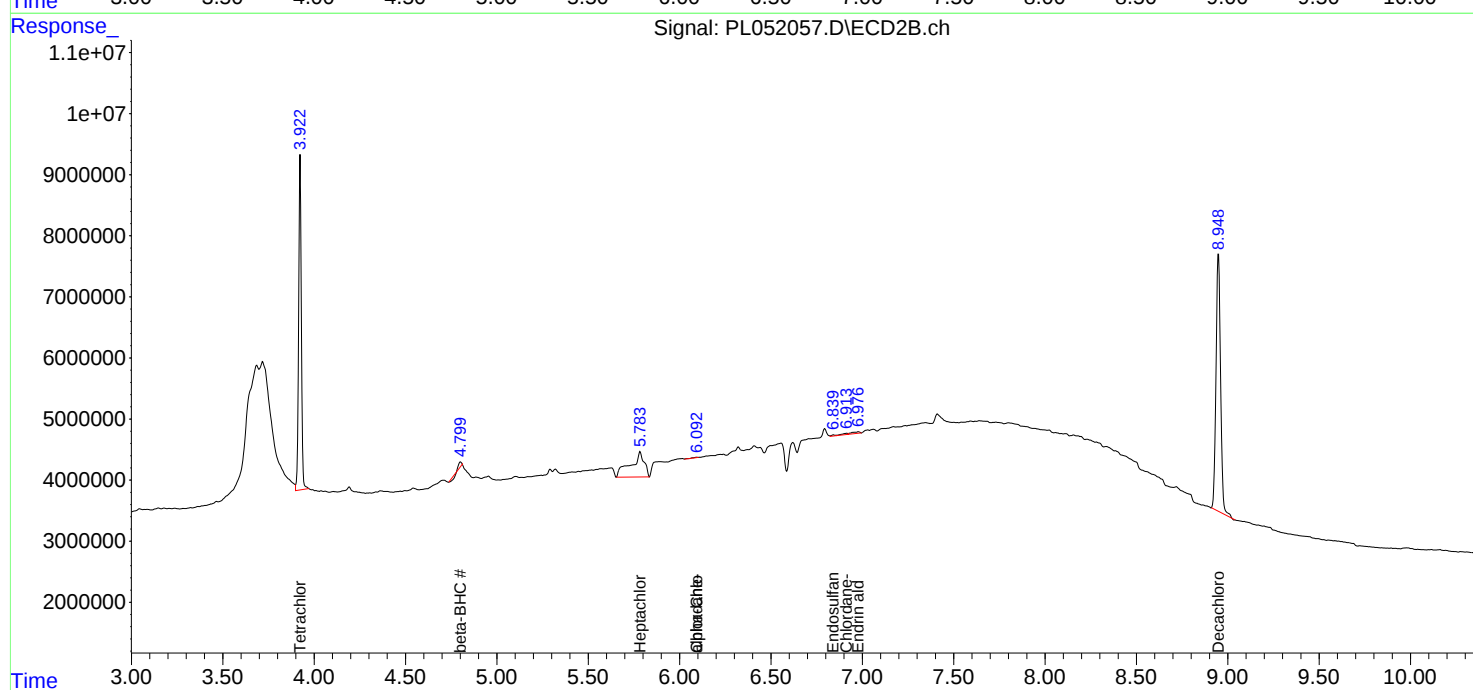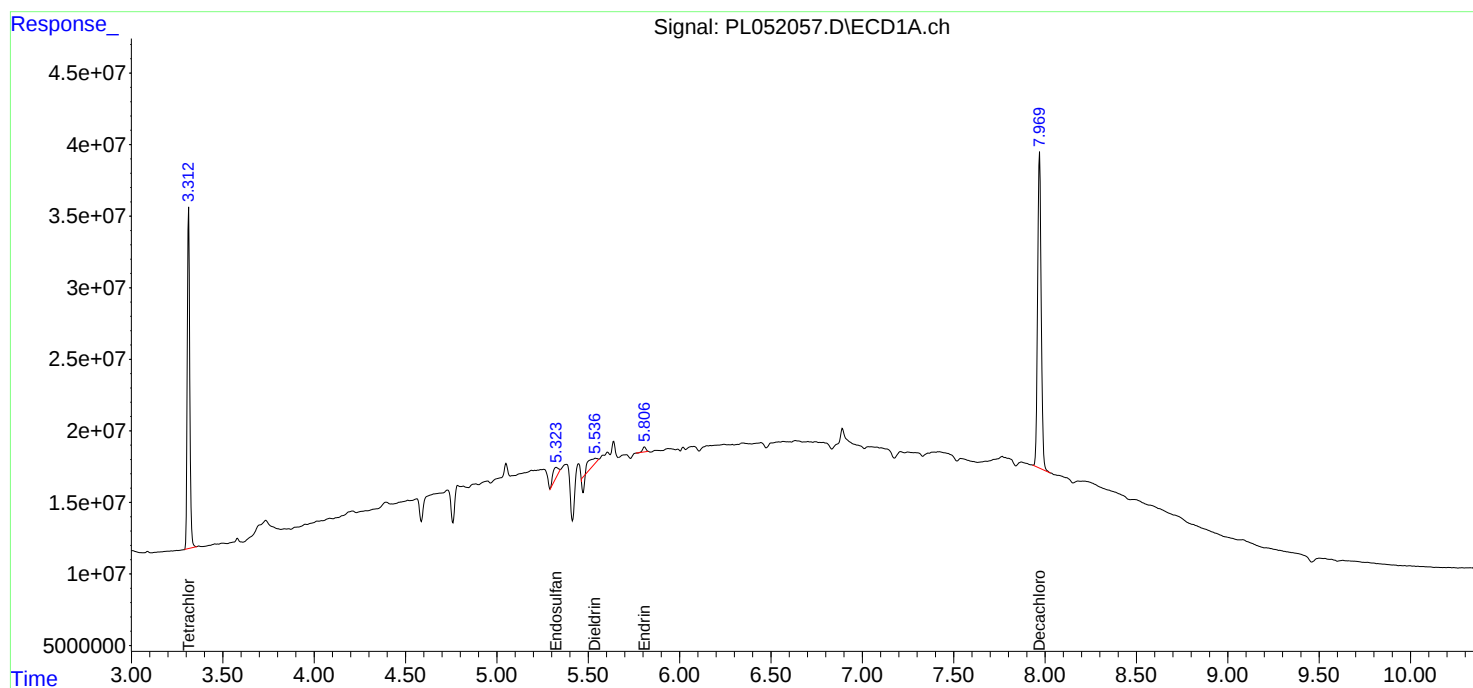


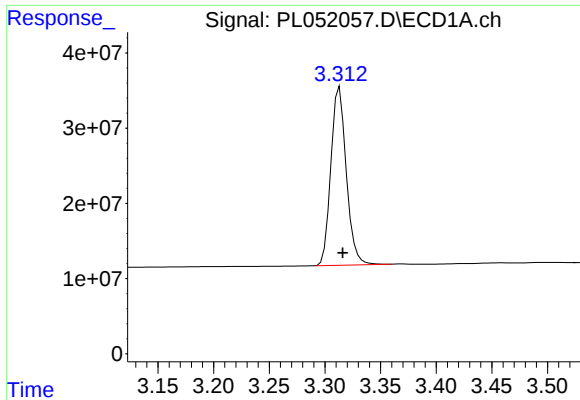

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 228435835
Conc: 26.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

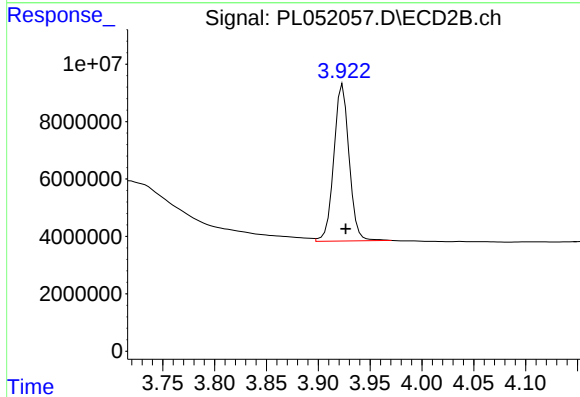


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 56354112
Conc: 25.79 ng/ml

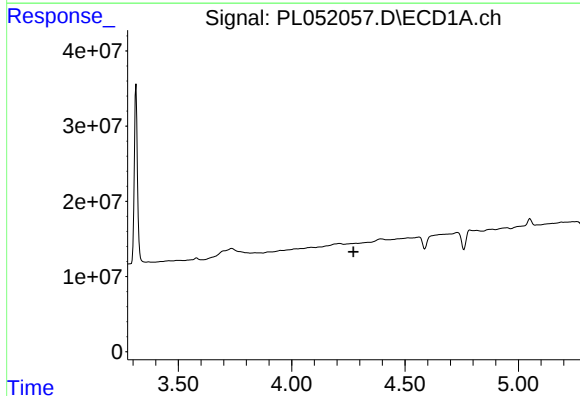


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

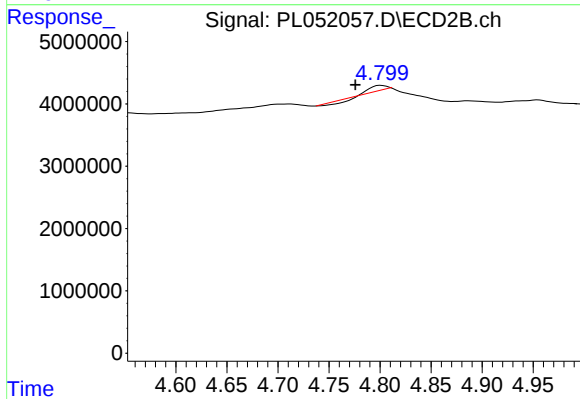

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 452435
Conc: 0.31 ng/ml

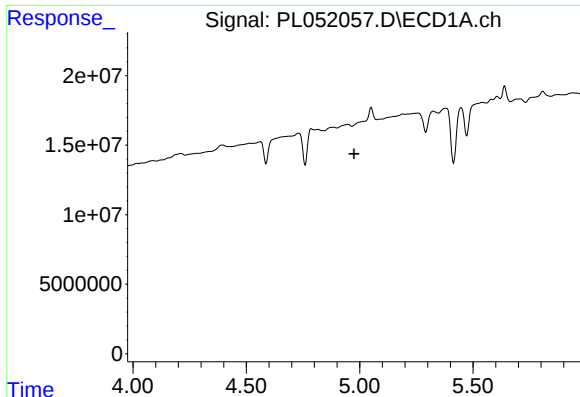

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

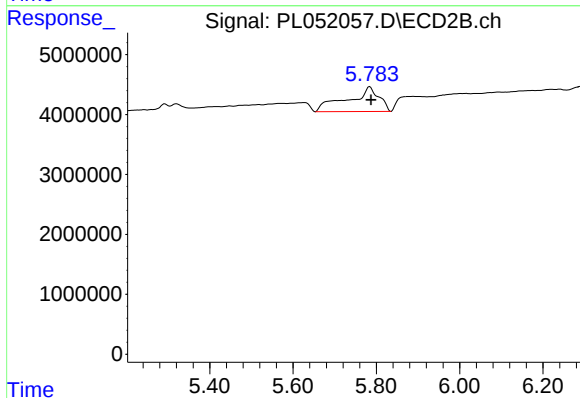


#8 Heptachlor epoxide

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 21545079
Conc: 6.38 ng/ml

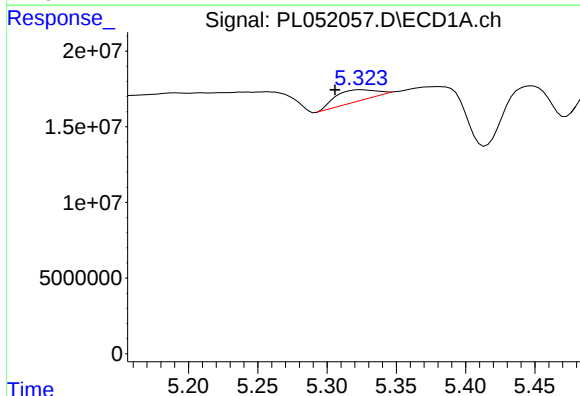


#9 Endosulfan I

R.T.: 5.324 min
Delta R.T.: 0.019 min
Response: 15029237
Conc: 1.12 ng/ml

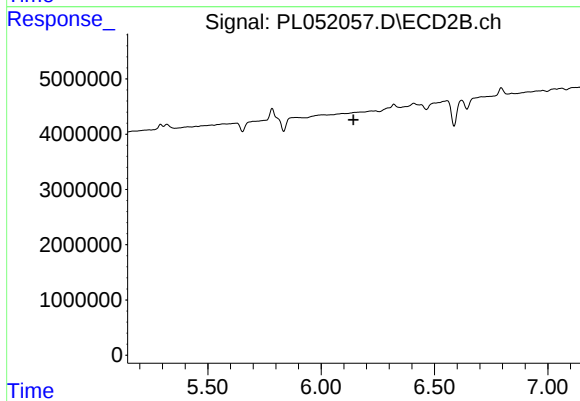

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

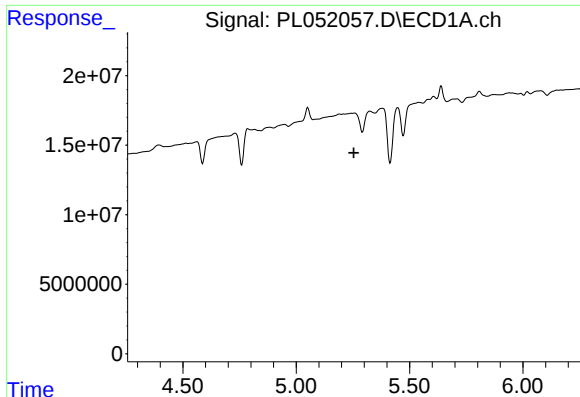

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

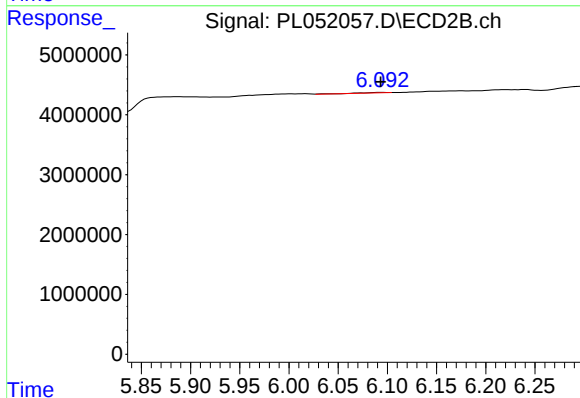


#11 alpha-Chlordane

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 139133
Conc: 0.04 ng/ml

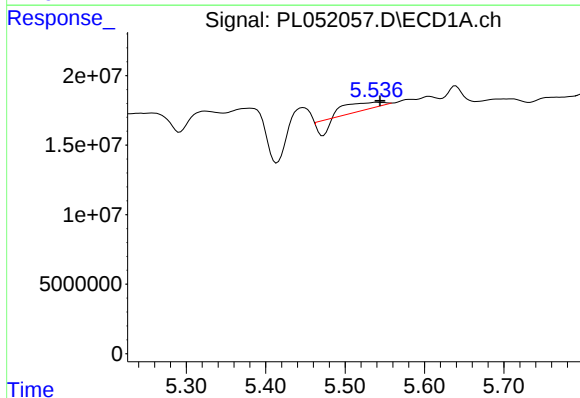


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: -0.004 min
Response: 9633670
Conc: 0.63 ng/ml

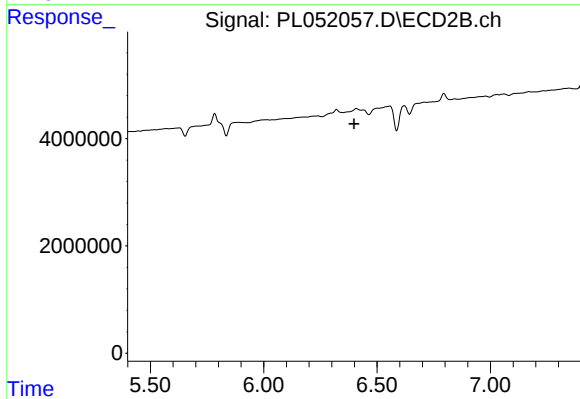

#13 Dieldrin


R.T.: 6.409 min
Delta R.T.: 0.010 min
Response: -240488
Conc: N.D.

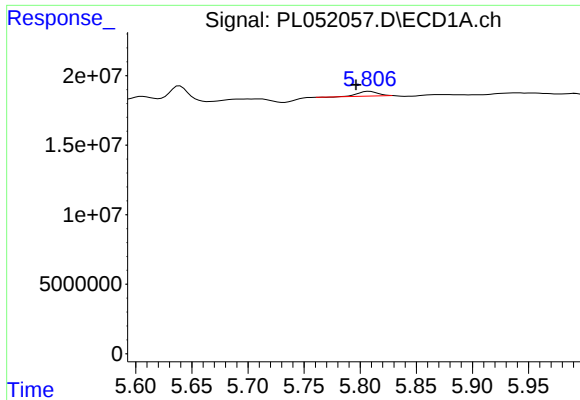

#14 Endrin


R.T.: 5.808 min
Delta R.T.: 0.012 min
Response: 4442305
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

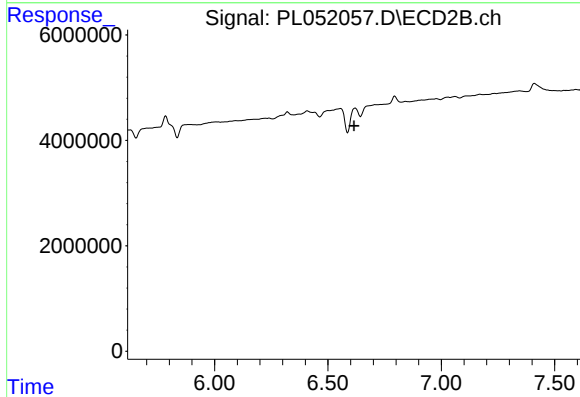


#14 Endrin

R.T.: 6.620 min
Delta R.T.: 0.005 min
Response: -209420
Conc: N.D.

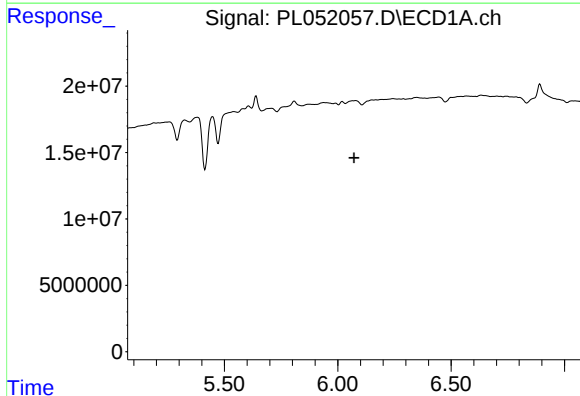


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

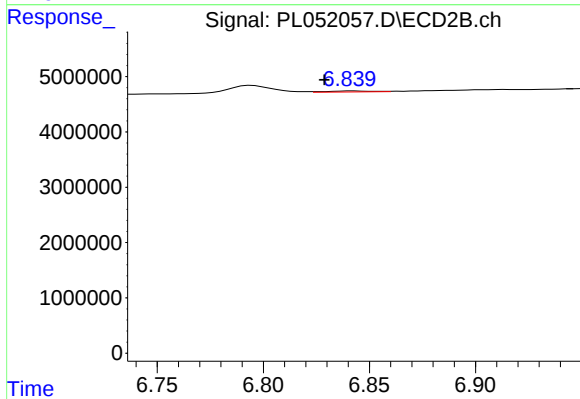

#15 Endosulfan II


R.T.: 6.842 min
Delta R.T.: 0.013 min
Response: 282904
Conc: 0.09 ng/ml

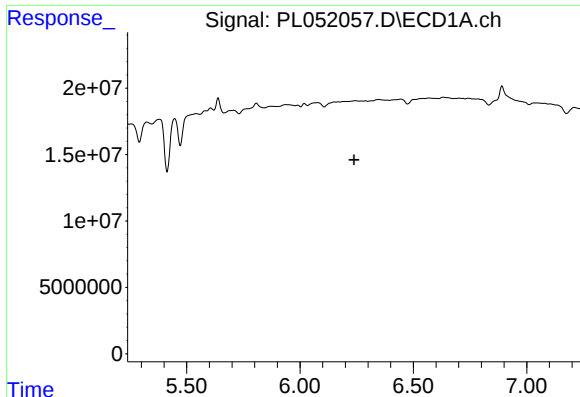

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

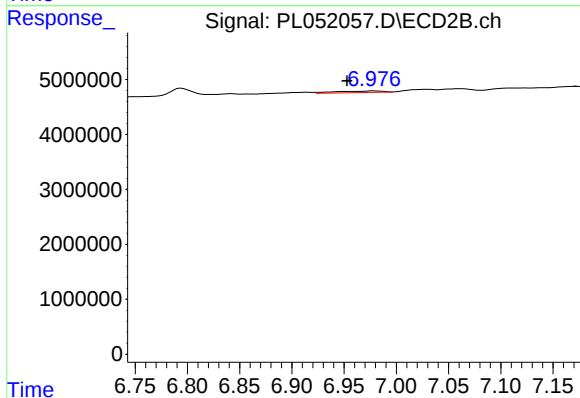


#18 Endrin aldehyde

R.T.: 6.978 min
Delta R.T.: 0.025 min
Response: 855659
Conc: 0.30 ng/ml

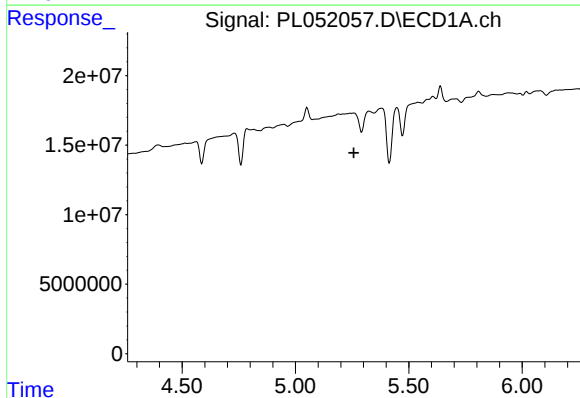


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

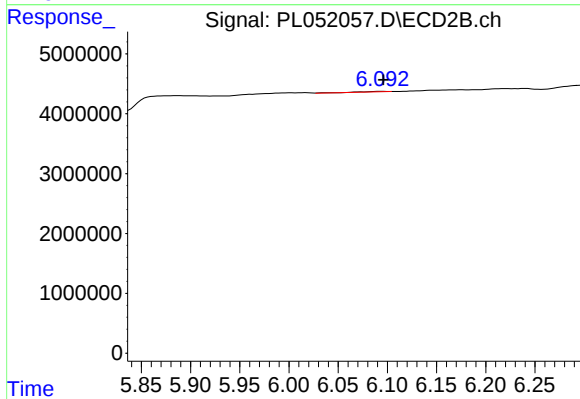

#26 Chlordane-4


R.T.: 6.094 min
Delta R.T.: -0.002 min
Response: 139133
Conc: 0.26 ng/ml

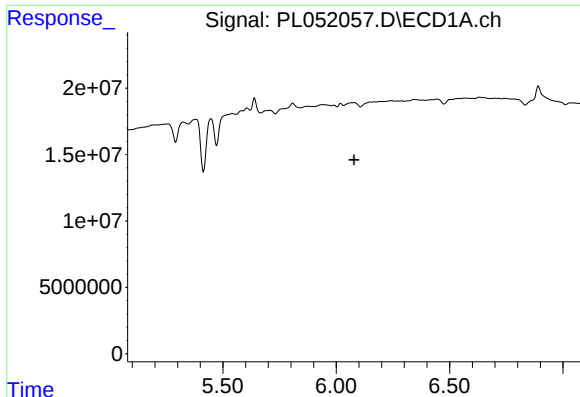

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

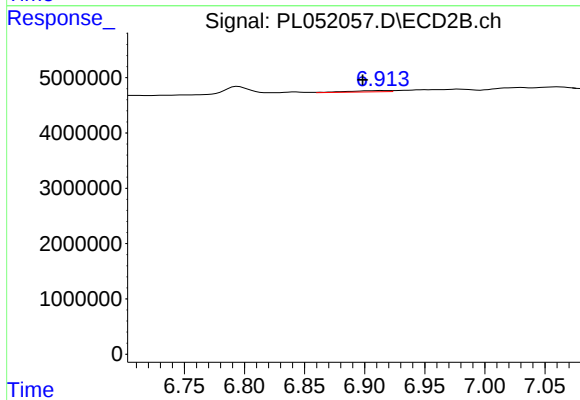


#27 Chlordane-5

R.T.: 6.914 min
Delta R.T.: 0.016 min
Response: 545260
Conc: 5.53 ng/ml

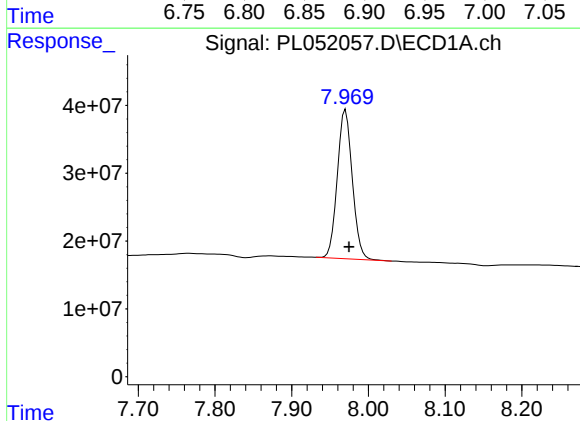

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.004 min
Response: 298229415
Conc: 24.57 ng/ml

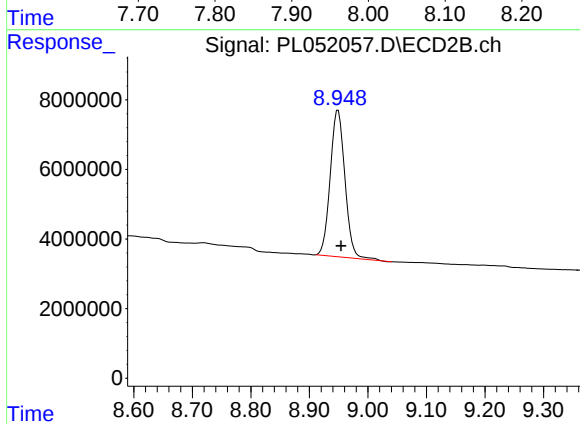

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.005 min
Response: 73390327
Conc: 24.11 ng/ml