

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 23:29
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:22:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	210.0E6	53132296	24.531	24.319
28)	SA Decachlor...	7.970	8.949	272.0E6	67920048	22.408	22.314
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	868456	N.D.	0.596 #
8)	B Heptachlo...	0.000	5.784	0	18906677	N.D.	5.602 #
9)	A Endosulfan I	5.323f	6.151	12511015	652696	0.931	0.202 #
13)	MA Dieldrin	5.541	6.408	7486728	356136	0.492	0.104 #
14)	MA Endrin	5.809	6.619	5563052	-902833	0.381	N.D. #
15)	B Endosulfa...	0.000	6.846f	0	439900	N.D.	0.133 #
18)	B Endrin al...	0.000	6.976f	0	1445104	N.D.	0.511 #
21)	B Endrin ke...	0.000	7.673f	0	857733	N.D.	0.268 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 23:29
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 01:22:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

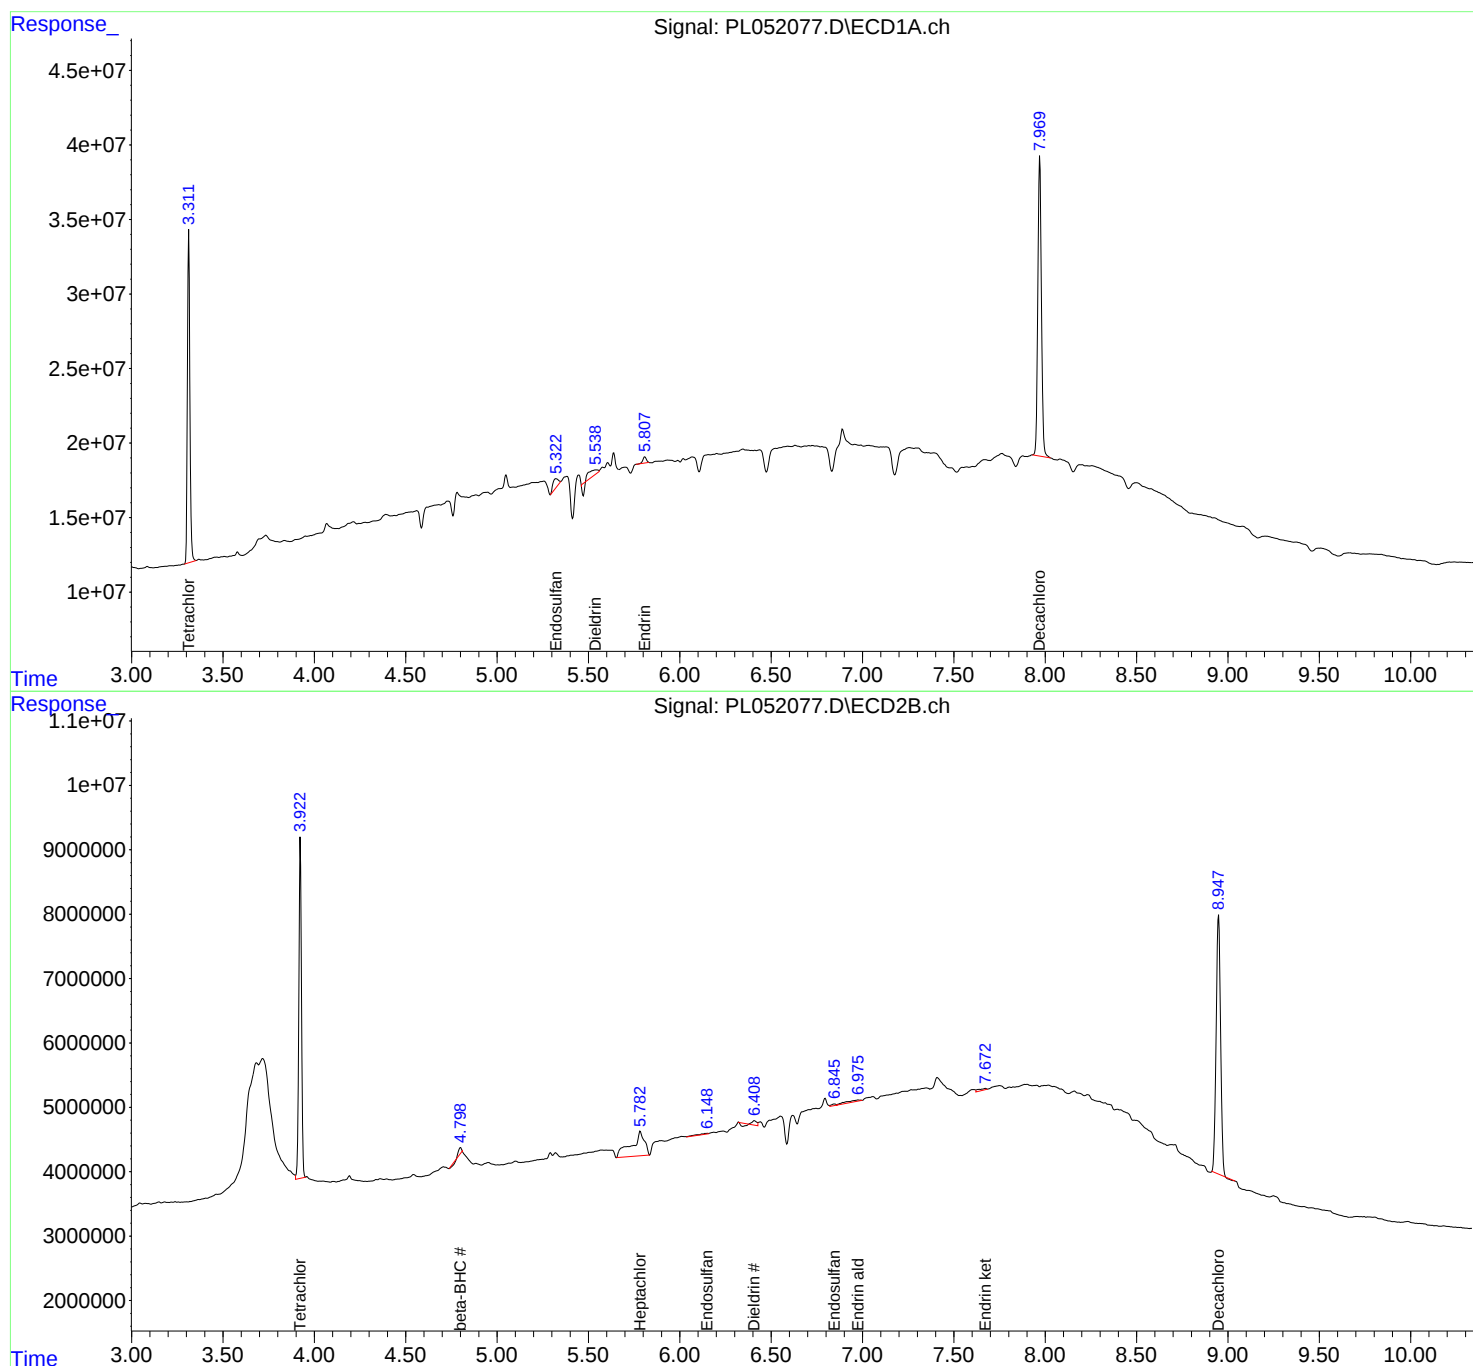


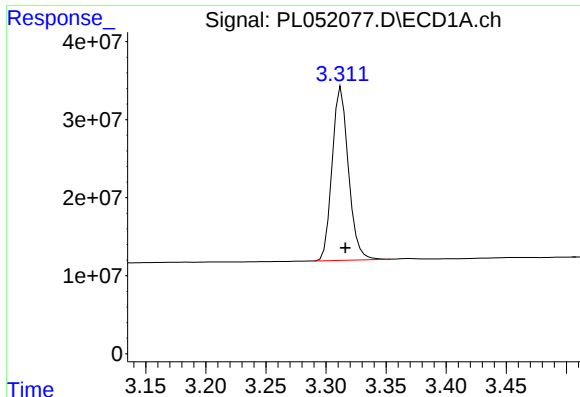

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 209955199
Conc: 24.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

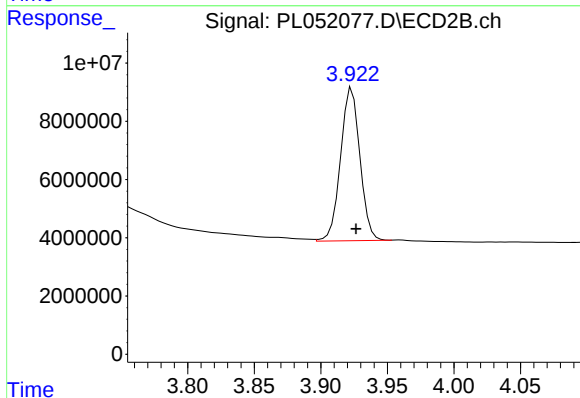


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 53132296
Conc: 24.32 ng/ml

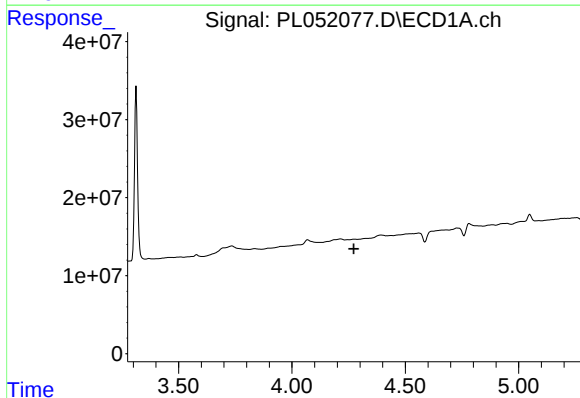


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

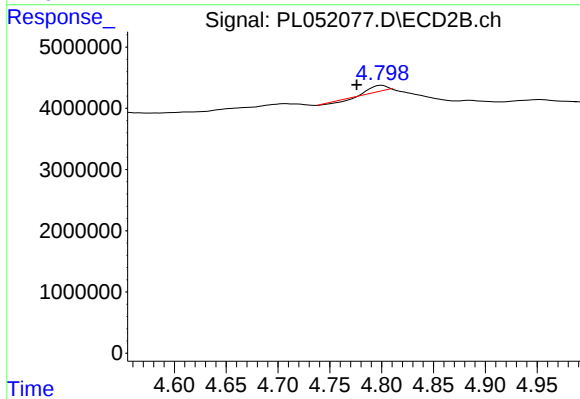

#6 beta-BHC


R.T.: 4.800 min
Delta R.T.: 0.025 min
Response: 868456
Conc: 0.60 ng/ml

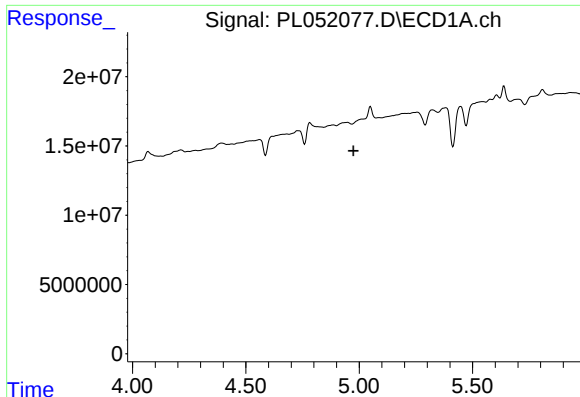

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

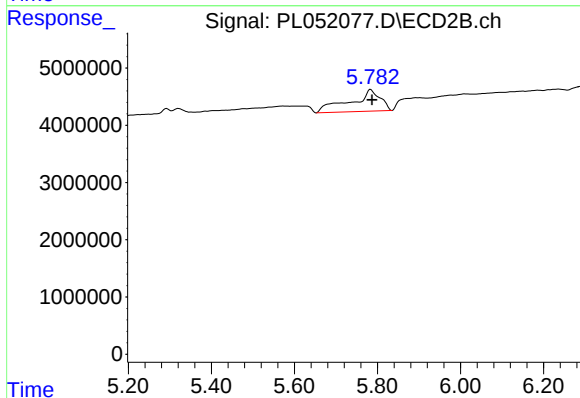


#8 Heptachlor epoxide

R.T.: 5.784 min
Delta R.T.: -0.004 min
Response: 18906677
Conc: 5.60 ng/ml

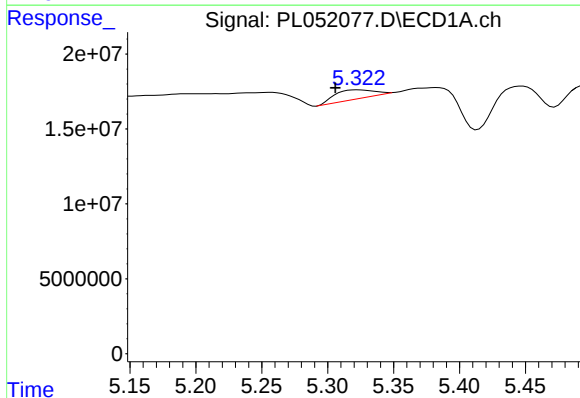


#9 Endosulfan I

R.T.: 5.323 min
Delta R.T.: 0.017 min
Response: 12511015
Conc: 0.93 ng/ml

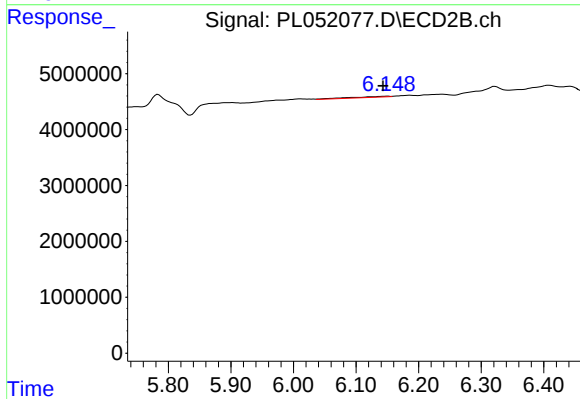

#9 Endosulfan I


R.T.: 6.151 min
Delta R.T.: 0.008 min
Response: 652696
Conc: 0.20 ng/ml

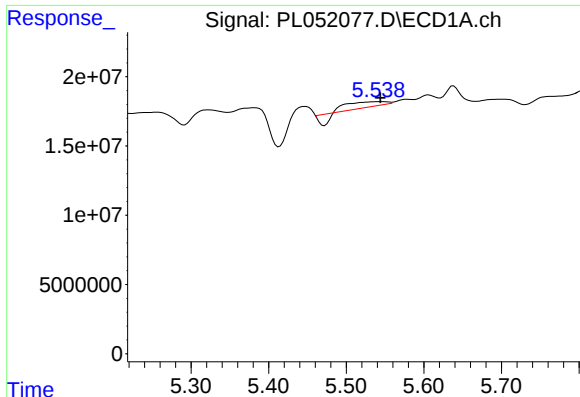

#13 Dieldrin


R.T.: 5.541 min
Delta R.T.: -0.003 min
Response: 7486728
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

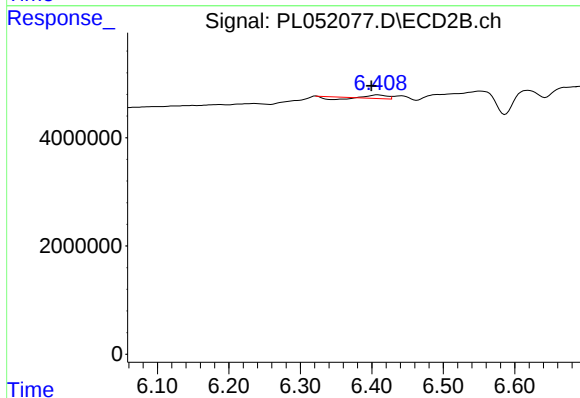


#13 Dieldrin

R.T.: 6.408 min
Delta R.T.: 0.009 min
Response: 356136
Conc: 0.10 ng/ml

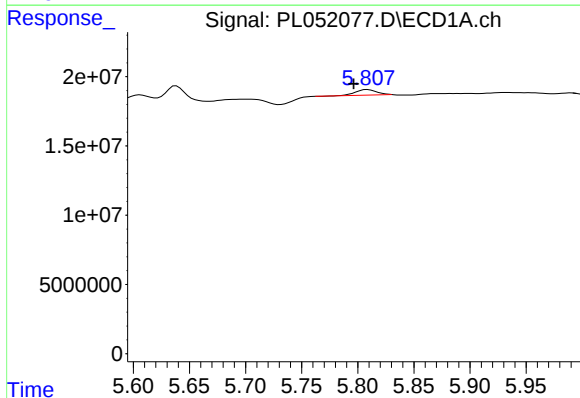


#14 Endrin

R.T.: 5.809 min
Delta R.T.: 0.012 min
Response: 5563052
Conc: 0.38 ng/ml

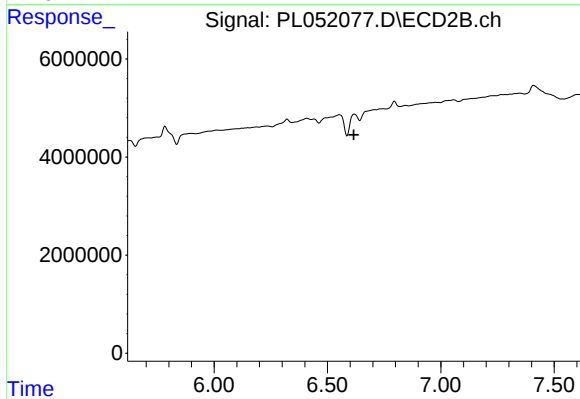

#14 Endrin


R.T.: 6.619 min
Delta R.T.: 0.003 min
Response: -902833
Conc: N.D.

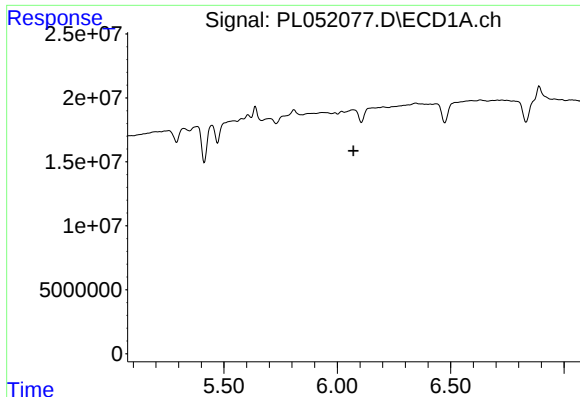

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

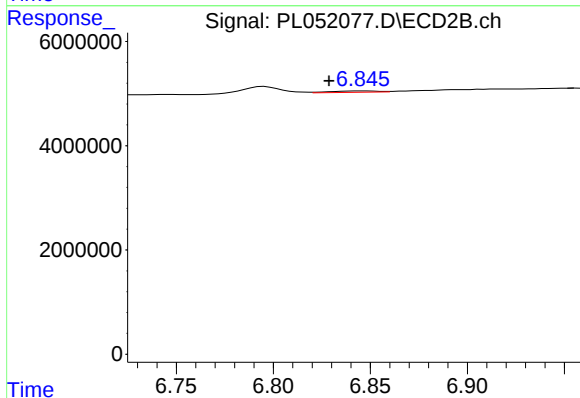


#15 Endosulfan II

R.T.: 6.846 min
Delta R.T.: 0.018 min
Response: 439900
Conc: 0.13 ng/ml

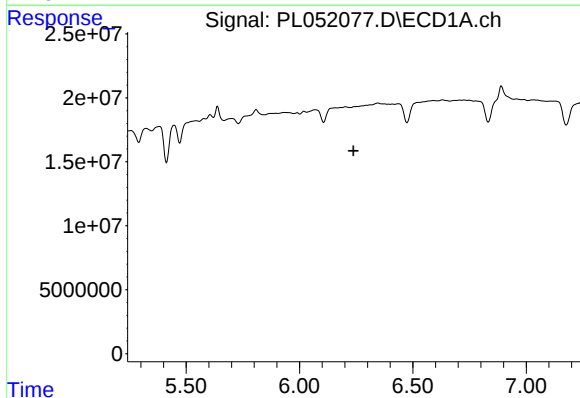


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

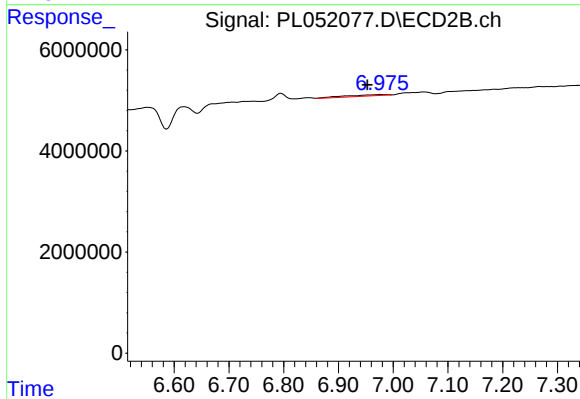

#18 Endrin aldehyde


R.T.: 6.976 min
Delta R.T.: 0.023 min
Response: 1445104
Conc: 0.51 ng/ml

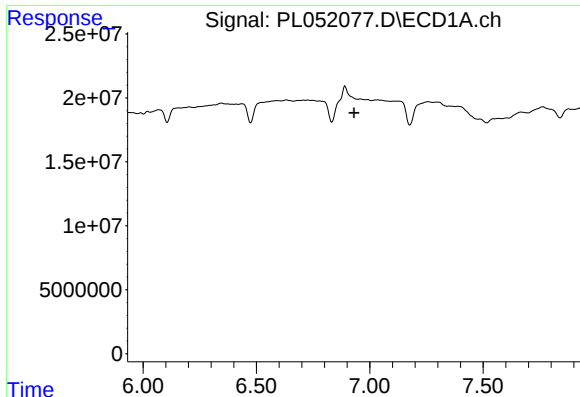

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

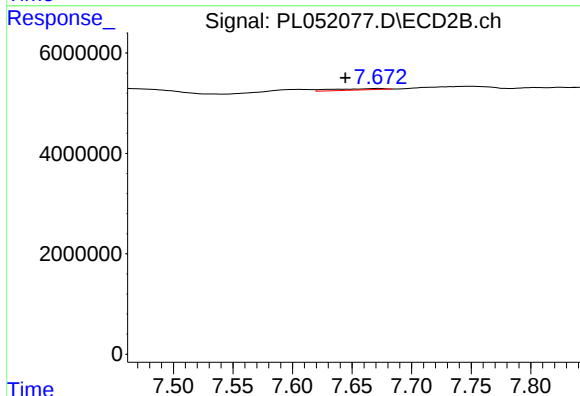


#21 Endrin ketone

R.T.: 7.673 min
Delta R.T.: 0.029 min
Response: 857733
Conc: 0.27 ng/ml

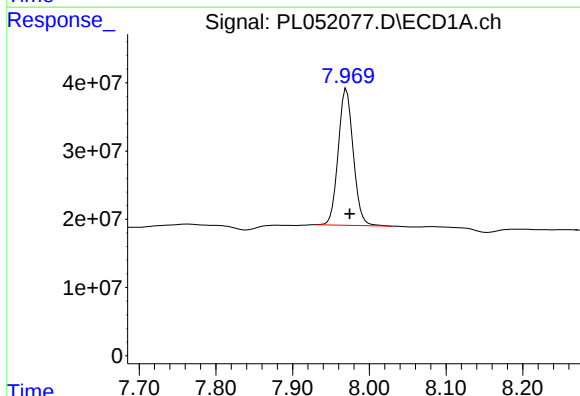

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.005 min
Response: 271982195
Conc: 22.41 ng/ml

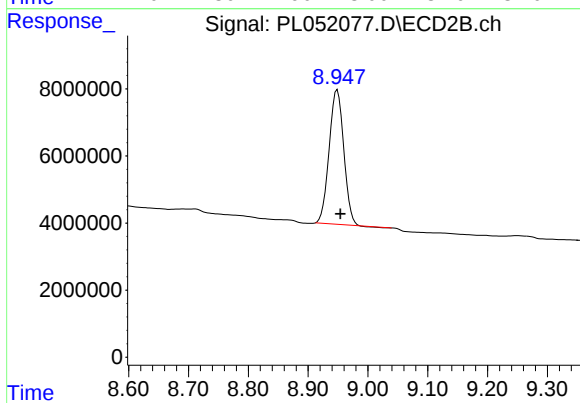

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.005 min
Response: 67920048
Conc: 22.31 ng/ml