

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 06:21
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 06:30:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	230.4E6	55697184	26.920	25.493
28)	SA Decachlor...	7.969	8.947	304.7E6	69171278	25.104	22.725
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	484035	N.D.	0.332 #
8)	B Heptachlo...	0.000	5.783	0	11385453	N.D.	3.374 #
9)	A Endosulfan I	5.324f	0.000	10976394	0	0.816	N.D. #
13)	MA Dieldrin	5.538	6.408	7448092	832241	0.490	0.243 #
14)	MA Endrin	5.807	6.617	4749368	842346	0.326	0.278
15)	B Endosulfa...	0.000	6.847f	0	3232249	N.D.	0.981 #
18)	B Endrin al...	0.000	6.954	0	15103173	N.D.	5.344 #
20)	A Methoxychlor	0.000	7.491	0	136714	N.D.	0.082 #
22)	Mirex	0.000	8.114f	0	1723982	N.D.	0.709 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 06:21
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 06:30:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

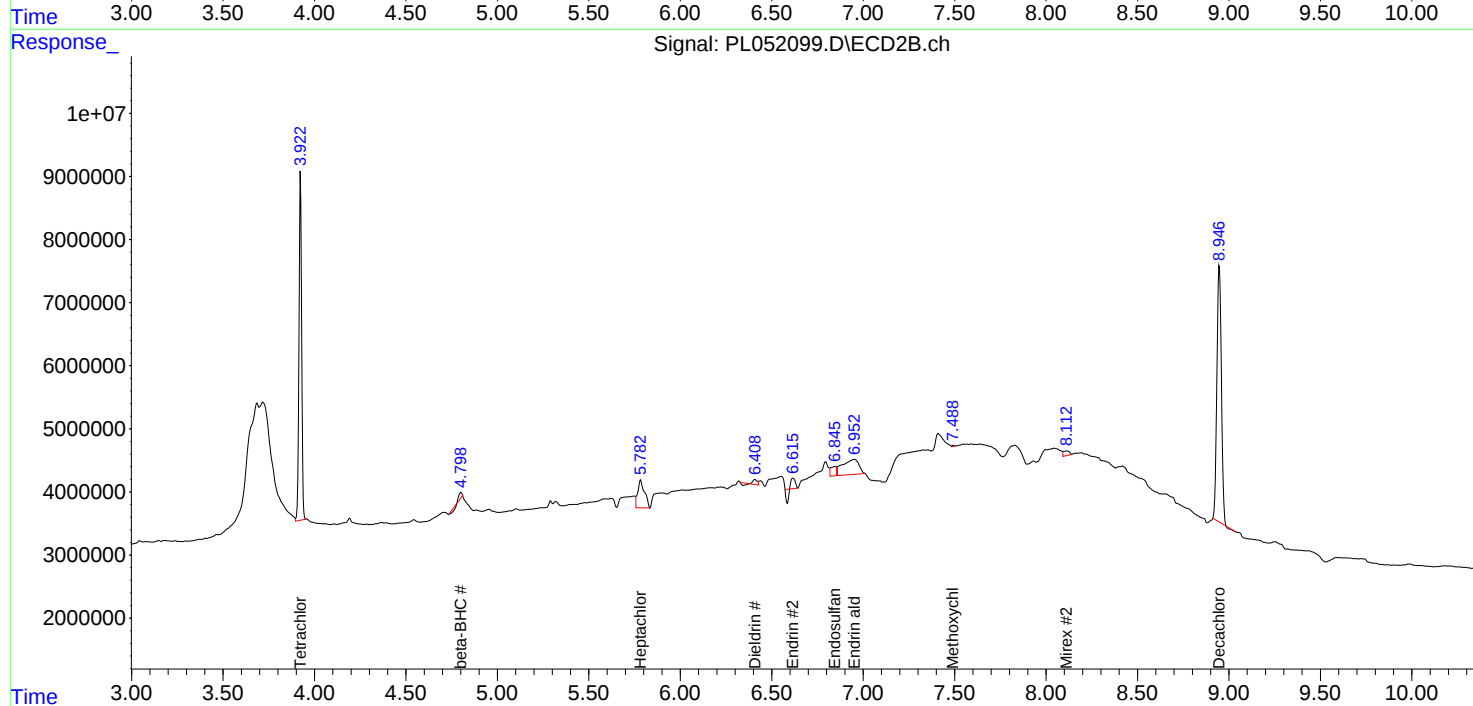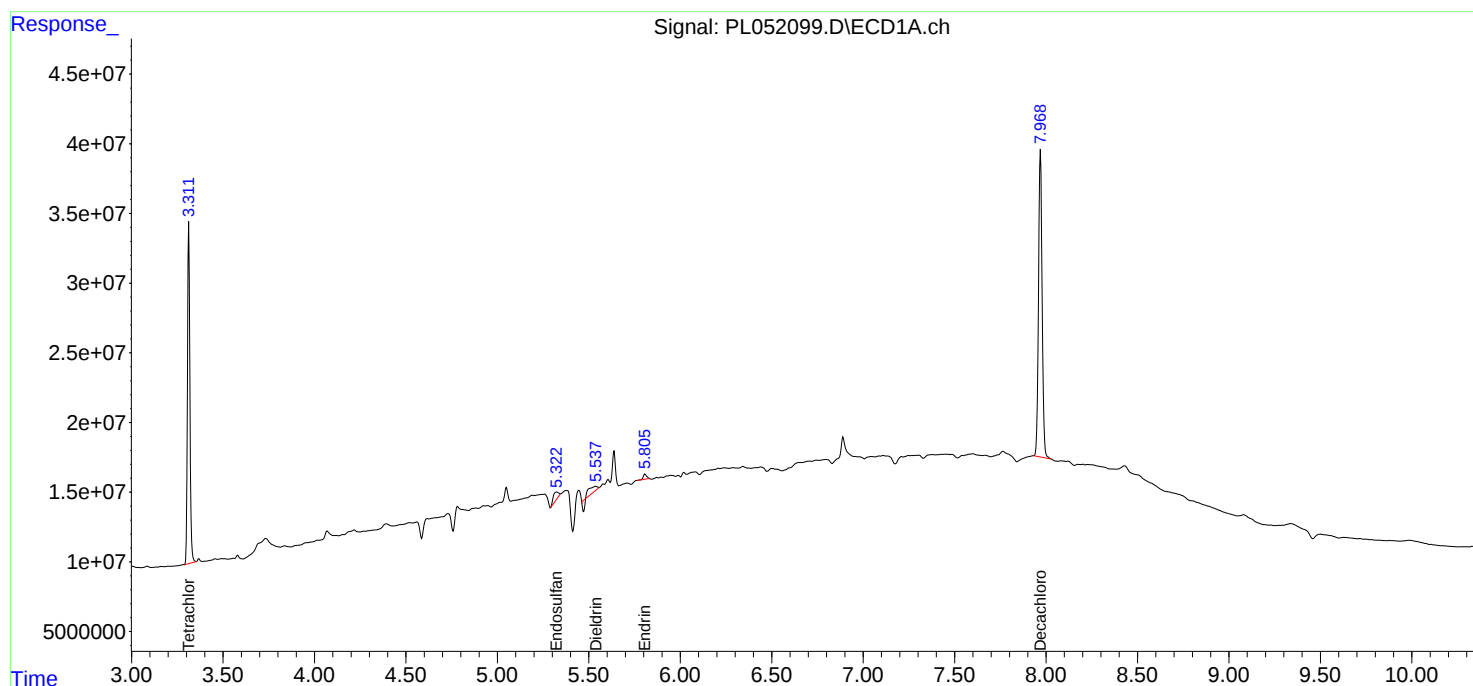


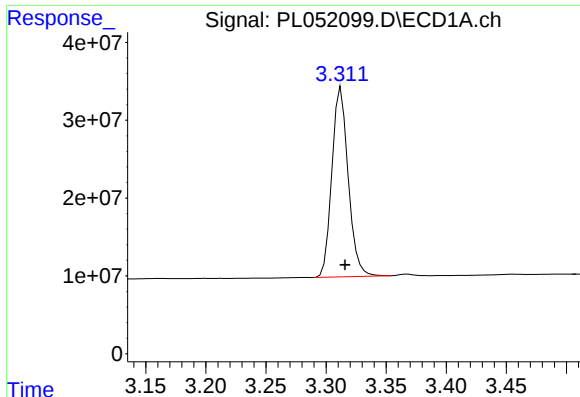

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 230395821
Conc: 26.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

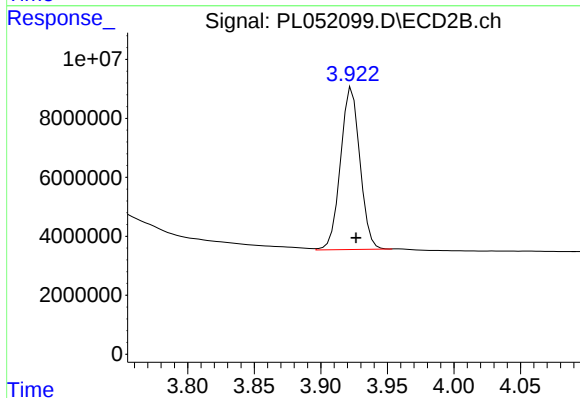


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 55697184
Conc: 25.49 ng/ml

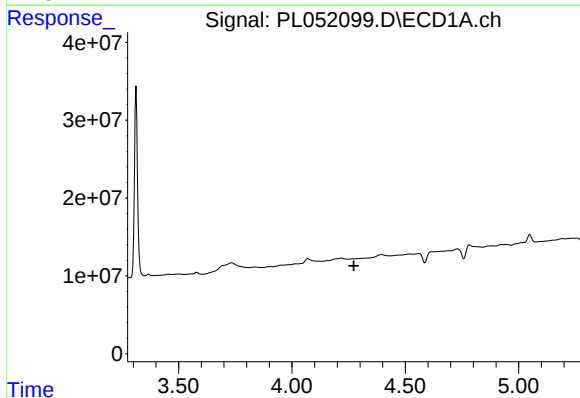


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

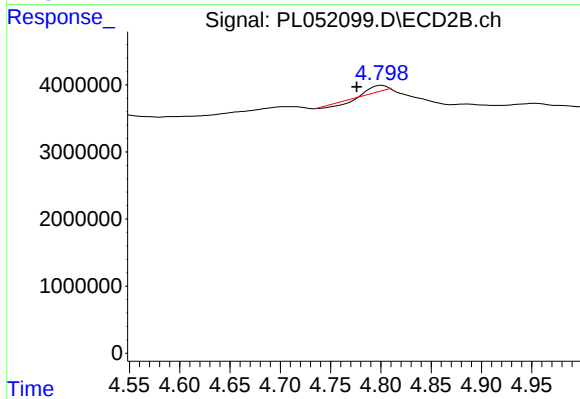

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 484035
Conc: 0.33 ng/ml

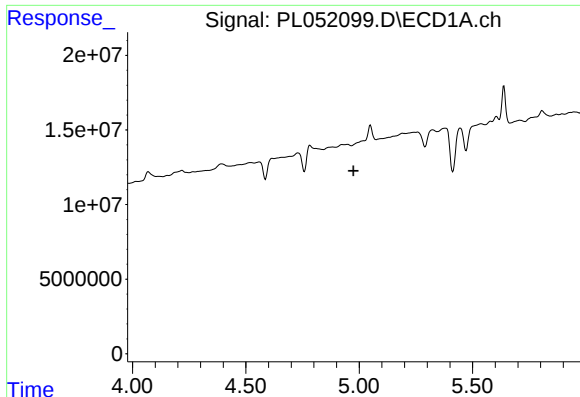

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

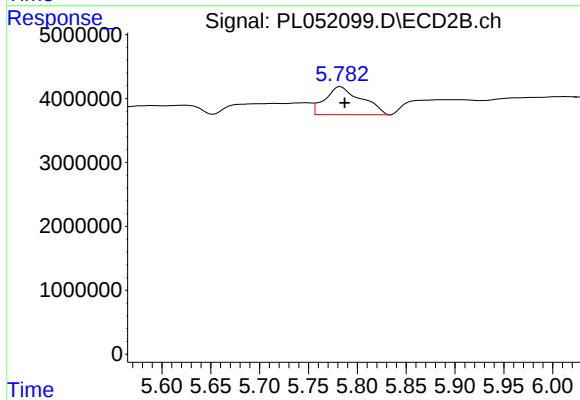


#8 Heptachlor epoxide

R.T.: 5.783 min
Delta R.T.: -0.004 min
Response: 11385453
Conc: 3.37 ng/ml

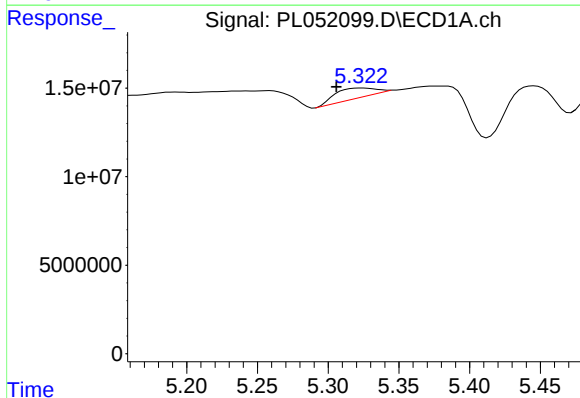


#9 Endosulfan I

R.T.: 5.324 min
Delta R.T.: 0.018 min
Response: 10976394
Conc: 0.82 ng/ml

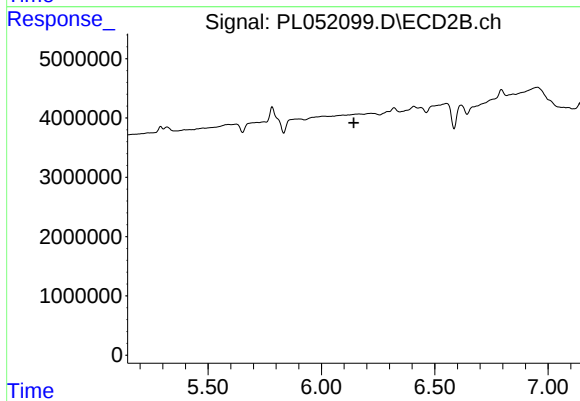

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

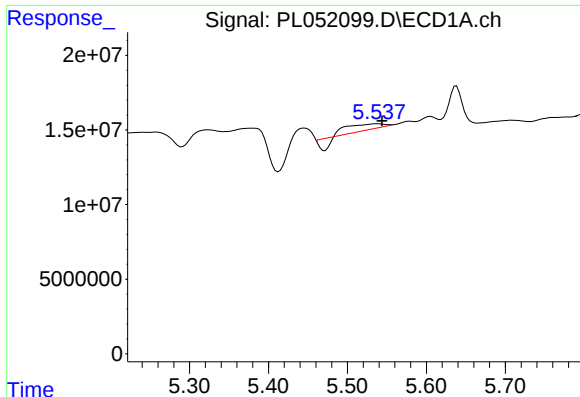

#13 Dieldrin


R.T.: 5.538 min
Delta R.T.: -0.006 min
Response: 7448092
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

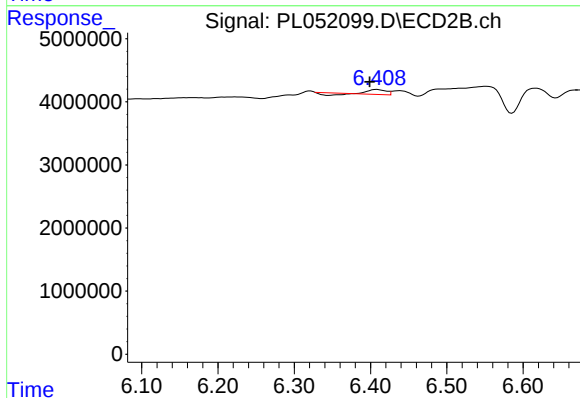


#13 Dieldrin

R.T.: 6.408 min
Delta R.T.: 0.009 min
Response: 832241
Conc: 0.24 ng/ml

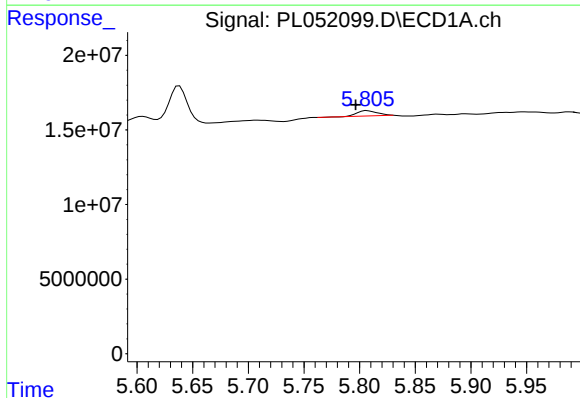


#14 Endrin

R.T.: 5.807 min
Delta R.T.: 0.010 min
Response: 4749368
Conc: 0.33 ng/ml

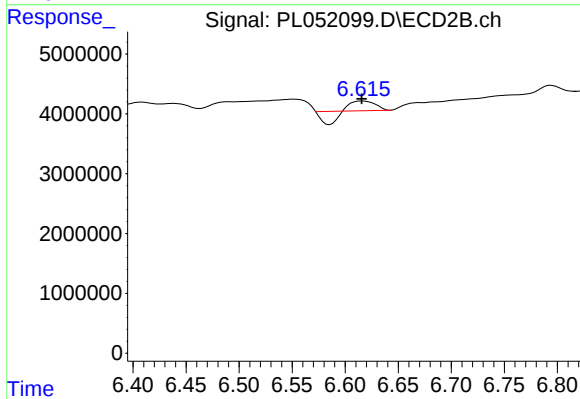

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 842346
Conc: 0.28 ng/ml

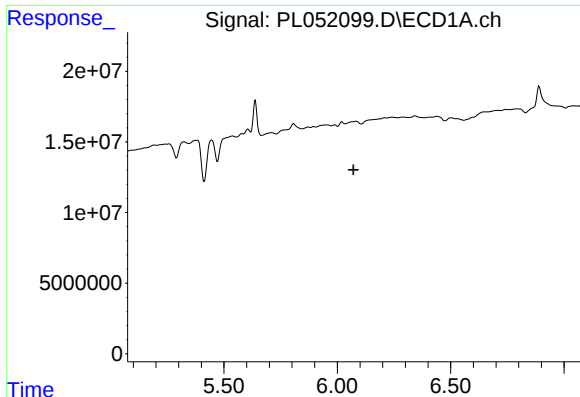

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

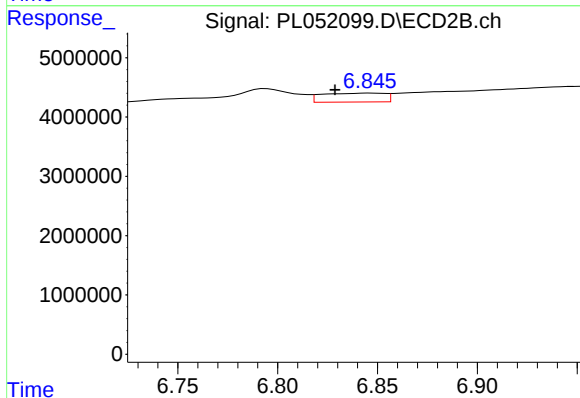


#15 Endosulfan II

R.T.: 6.847 min
Delta R.T.: 0.018 min
Response: 3232249
Conc: 0.98 ng/ml

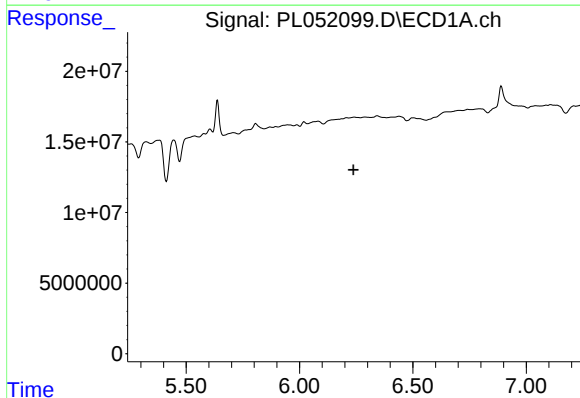


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

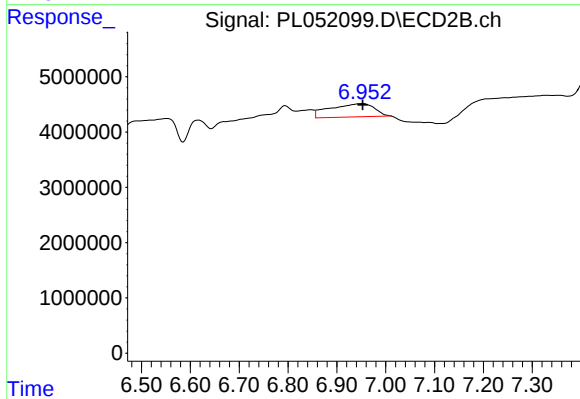

#18 Endrin aldehyde


R.T.: 6.954 min
Delta R.T.: 0.001 min
Response: 15103173
Conc: 5.34 ng/ml

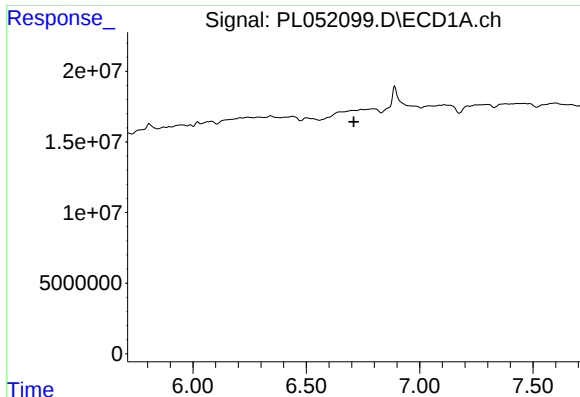

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

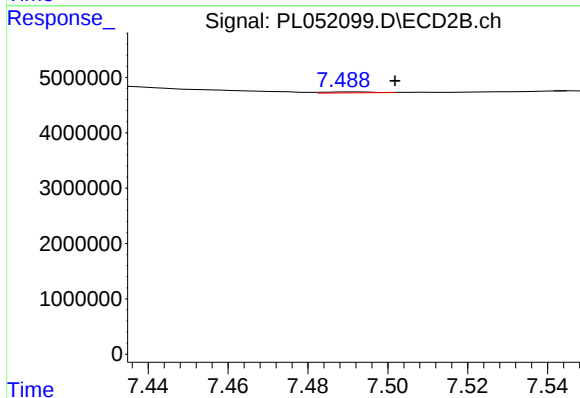


#20 Methoxychlor

R.T.: 7.491 min
Delta R.T.: -0.011 min
Response: 136714
Conc: 0.08 ng/ml

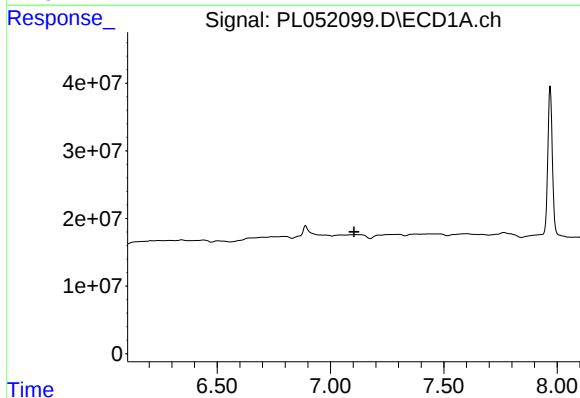


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.104 min
Response: 0
Conc: N.D.

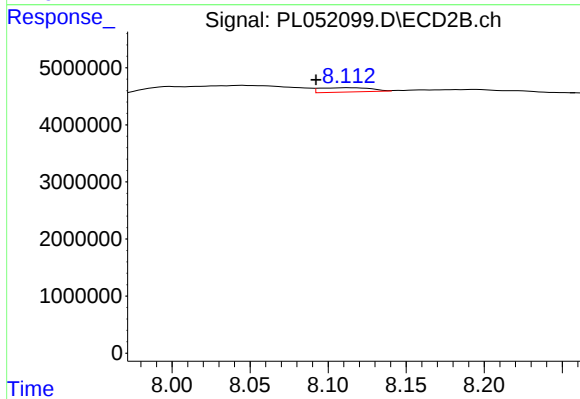

#22 Mirex


R.T.: 8.114 min
Delta R.T.: 0.021 min
Response: 1723982
Conc: 0.71 ng/ml

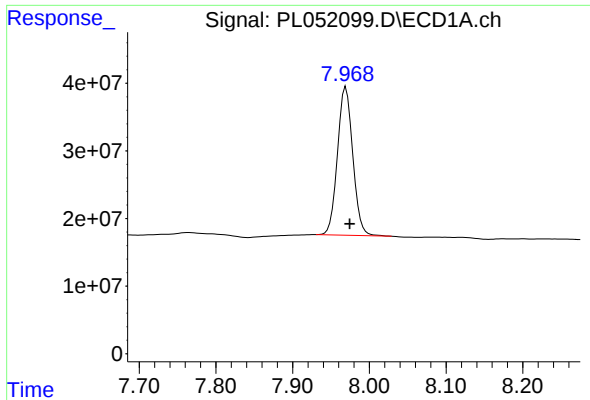

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.005 min
Response: 304712103
Conc: 25.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

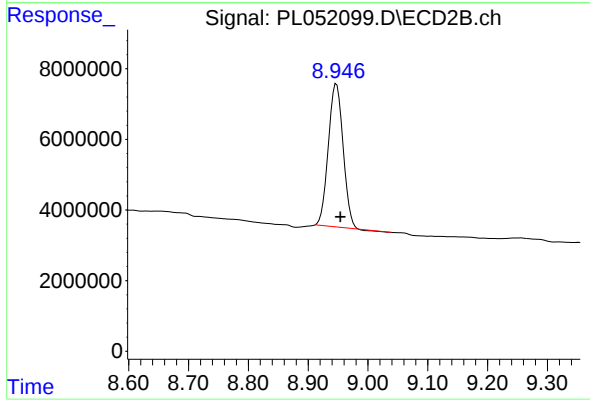

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 69171278
Conc: 22.72 ng/ml