

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 12:34
 Operator : SG\AJ
 Sample : SURR. SPK. TEST 10X
 Misc : 200PPB PEST./PCB SURR. SPIKE
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURR. SPK. TEST 10X

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 22:45:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.925	256.9E6	61297038	30.018	28.056
28)	SA Decachlor...	7.977	8.953	454.5E6	109.3E6	37.447	35.905

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 12:34
Operator : SG\AJ
Sample : SURR. SPK. TEST 10X
Misc : 200PPB PEST./PCB SURR. SPIKE
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SURR. SPK. TEST 10X

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 22:45:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

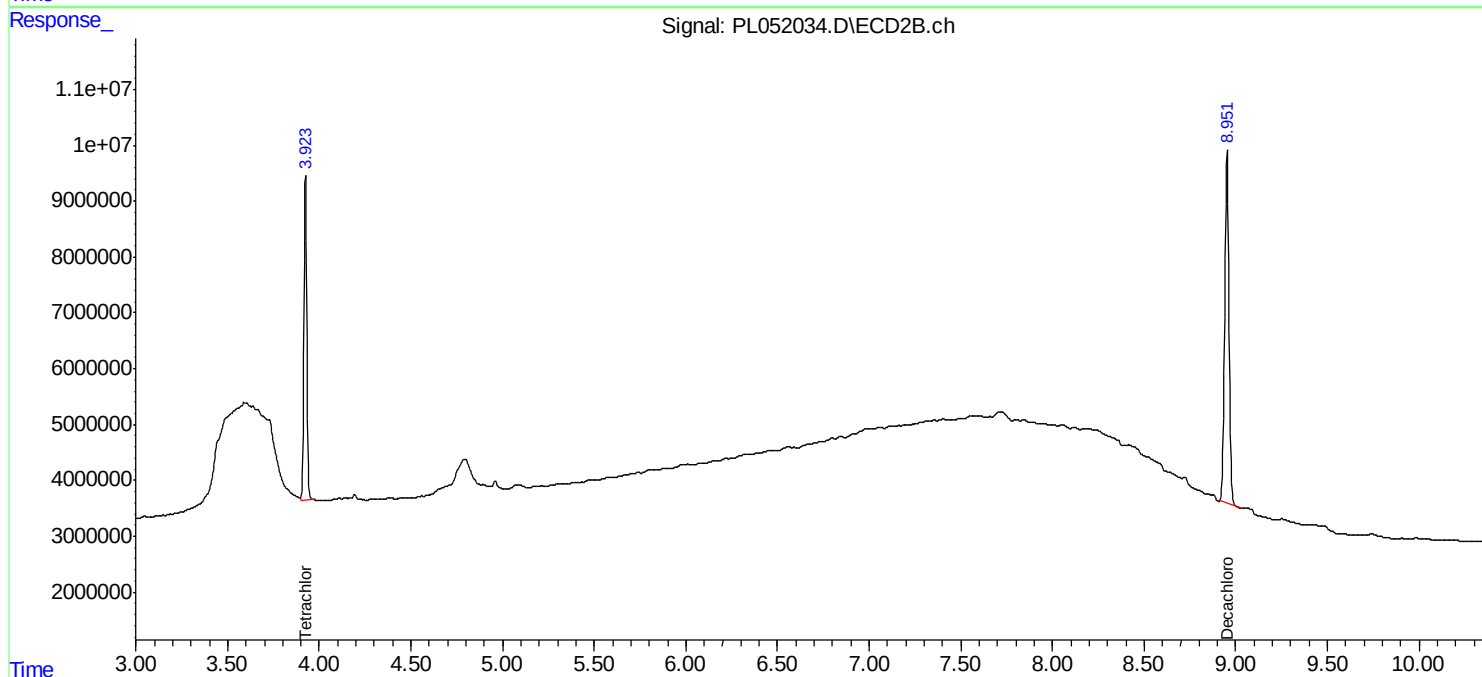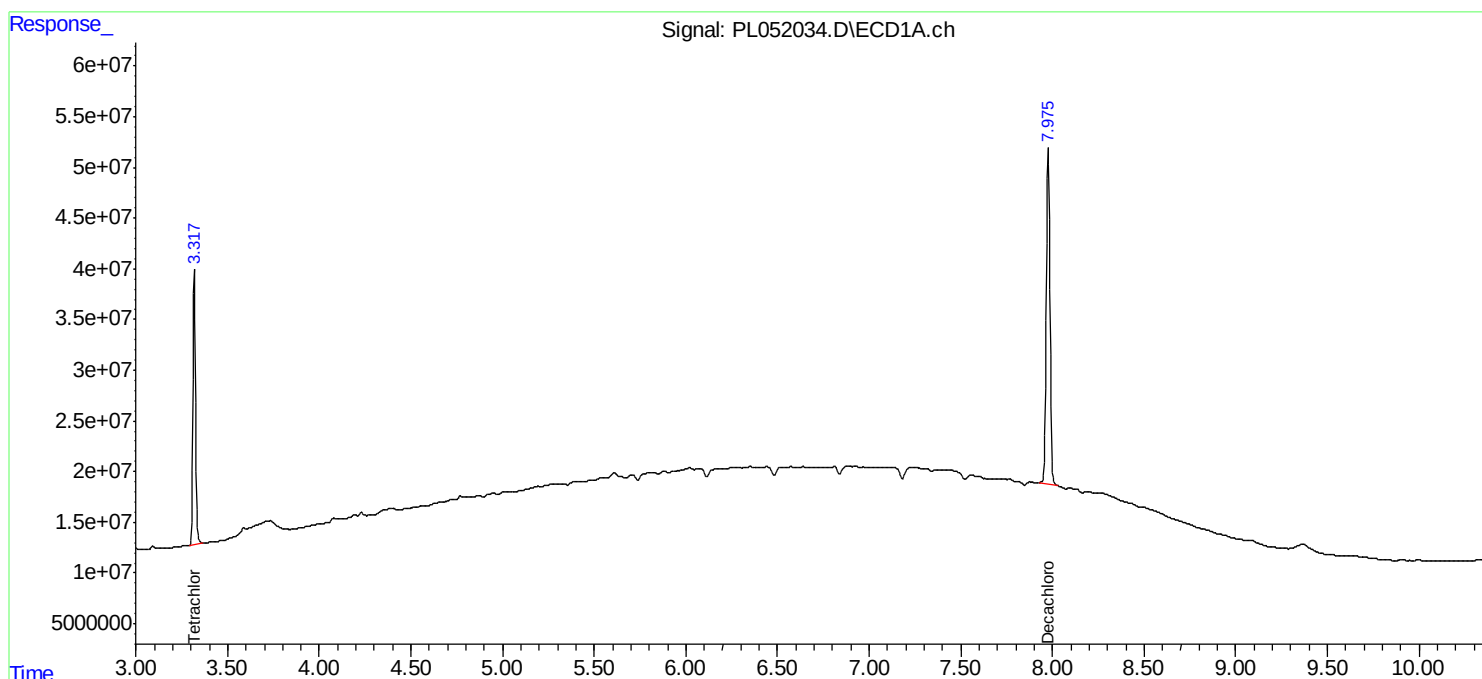


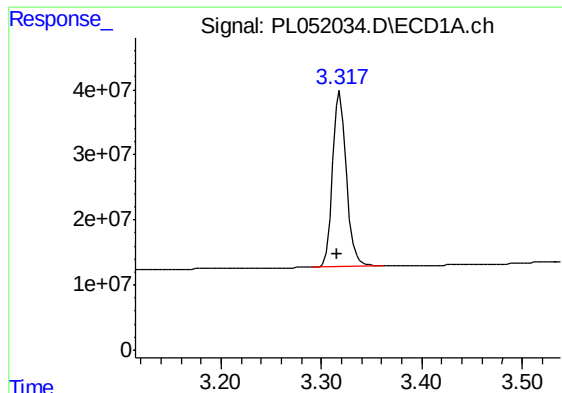

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.003 min
Response: 256912017
Conc: 30.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURR. SPK. TEST 10X

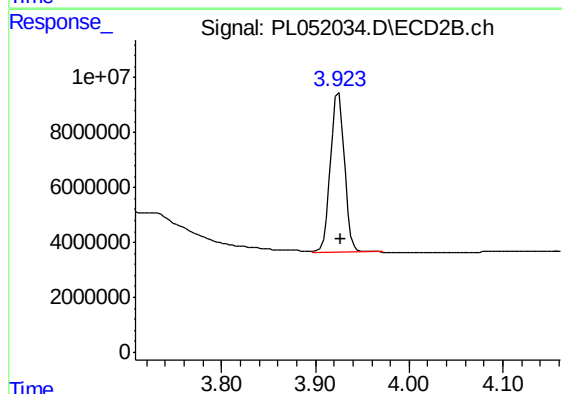


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 61297038
Conc: 28.06 ng/ml

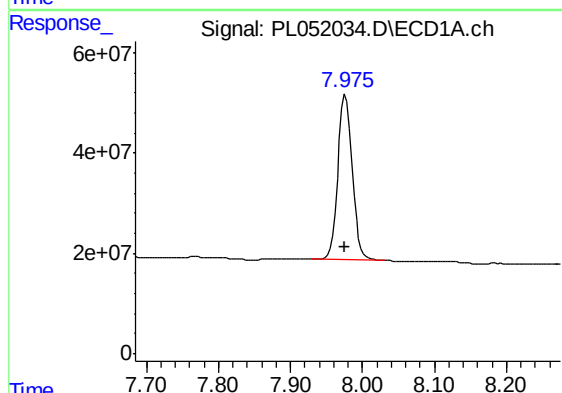

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: 0.002 min
Response: 454524274
Conc: 37.45 ng/ml

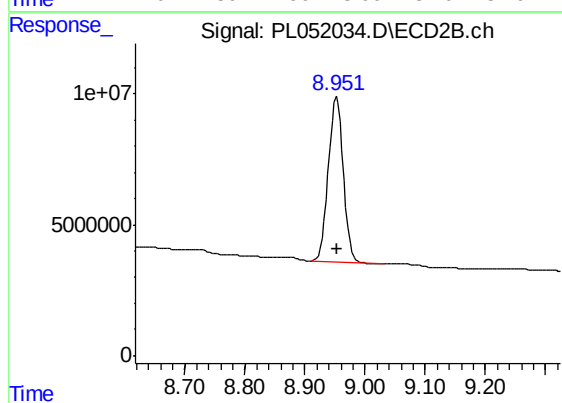

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.001 min
Response: 109289836
Conc: 35.90 ng/ml