

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 17:19
 Operator : SG\AJ
 Sample : K4089-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-082919

Manual Integrations
 APPROVED

Ankita
 9/3/2019 2:12:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 22:49:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	196.6E6	49978486	22.971	22.875
28)	SA Decachlor...	7.970	8.947	181.3E6	45447821	14.937	14.931m

Ankita

9/3/2019 2:12:55 PM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 17:19
Operator : SG\AJ
Sample : K4089-08
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-082919


Manual Integrations
APPROVED

Ankita
9/3/2019 2:12:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 22:49:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

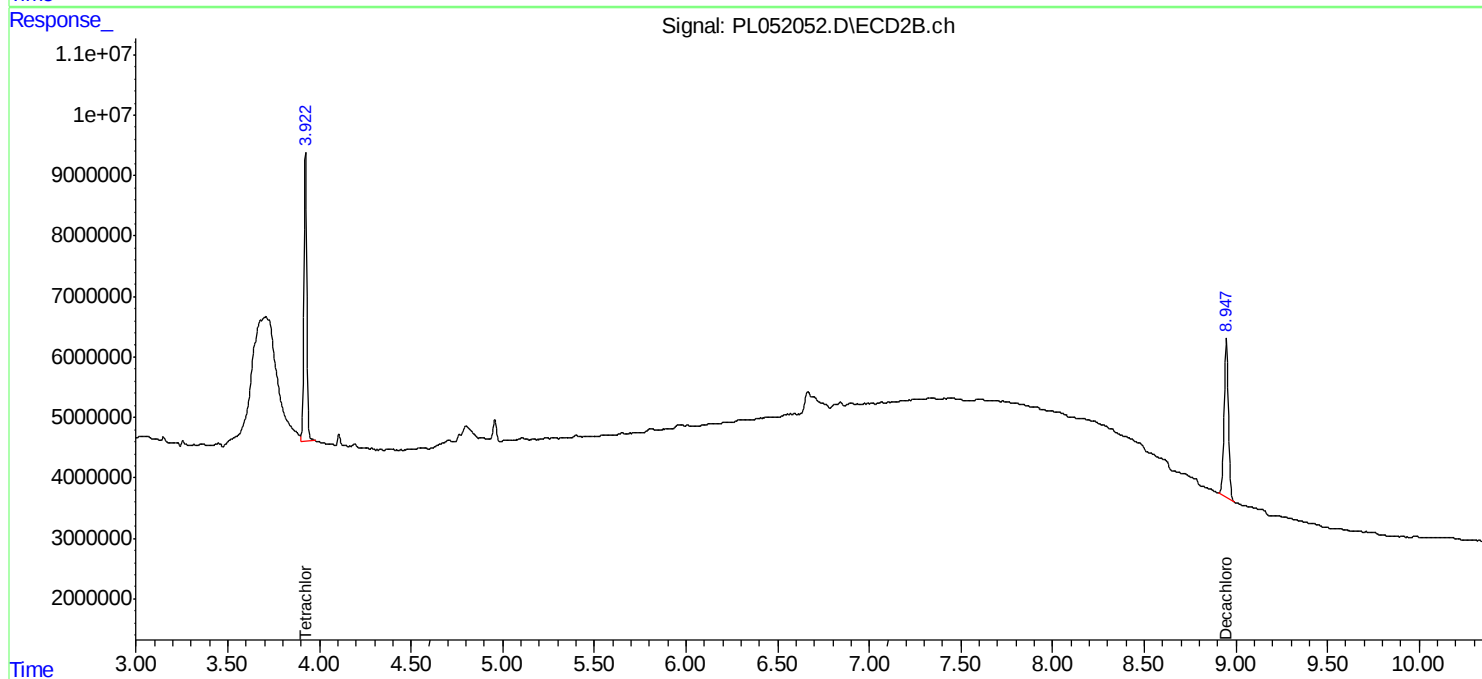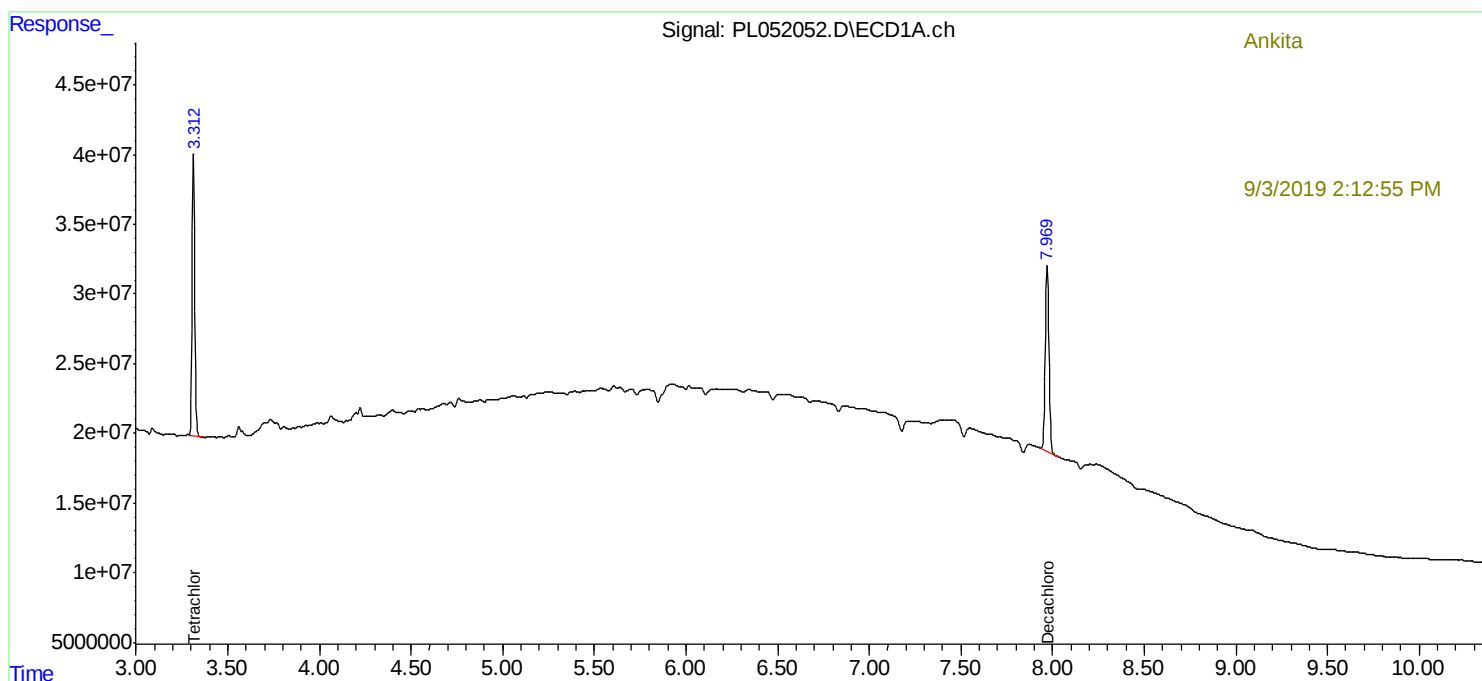

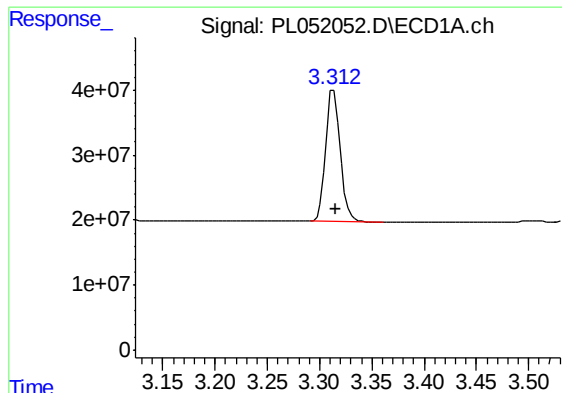


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.002 min
Response: 196598354
Conc: 22.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-082919

Manual Integrations
APPROVED


Ankita
9/3/2019 2:12:55 PM

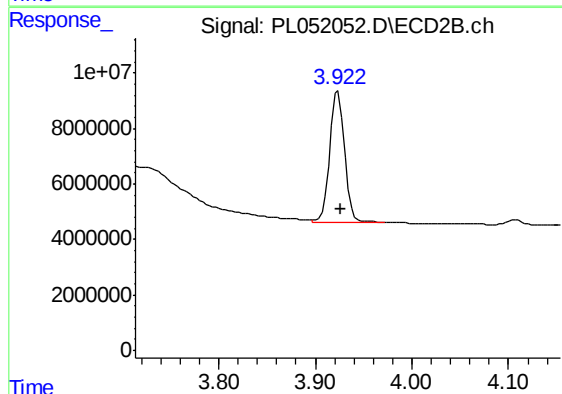

#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 49978486
Conc: 22.88 ng/ml


Ankita

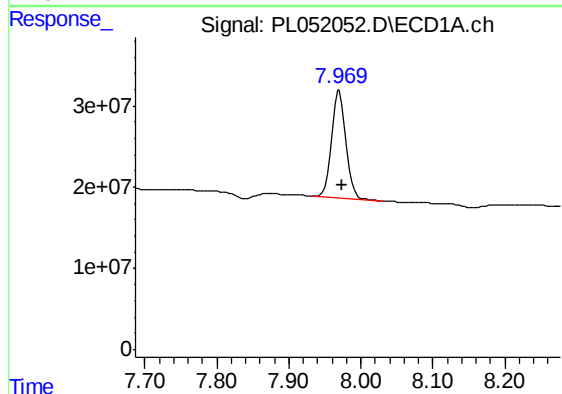

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.004 min
Response: 181296783
Conc: 14.94 ng/ml

9/3/2019 2:12:55 PM

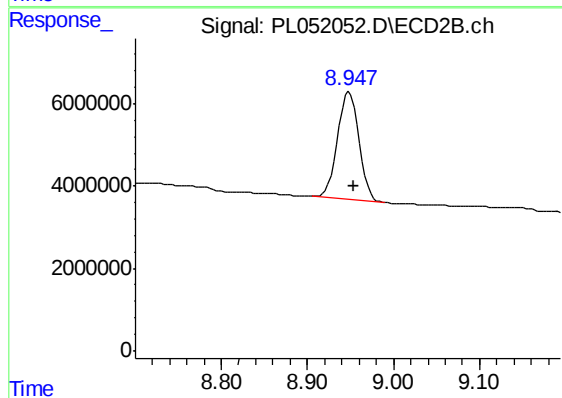

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 45447821
Conc: 14.93 ng/ml m