

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
 Data File : PL052097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2019 05:53
 Operator : SG\AJ
 Sample : K4619-27
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP9-COMP

Manual Integrations
 APPROVED

Ankita
 9/3/2019 2:14:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 06:29:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.923	188.3E6	48623820	21.999	22.255
28)	SA Decachlor...	7.969	8.946	221.5E6	53491450	18.245	17.573m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083019\
Data File : PL052097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2019 05:53
Operator : SG\AJ
Sample : K4619-27
Misc :
ALS Vial : 69 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP9-COMP


Manual Integrations
APPROVED

Ankita
9/3/2019 2:14:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 06:29:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

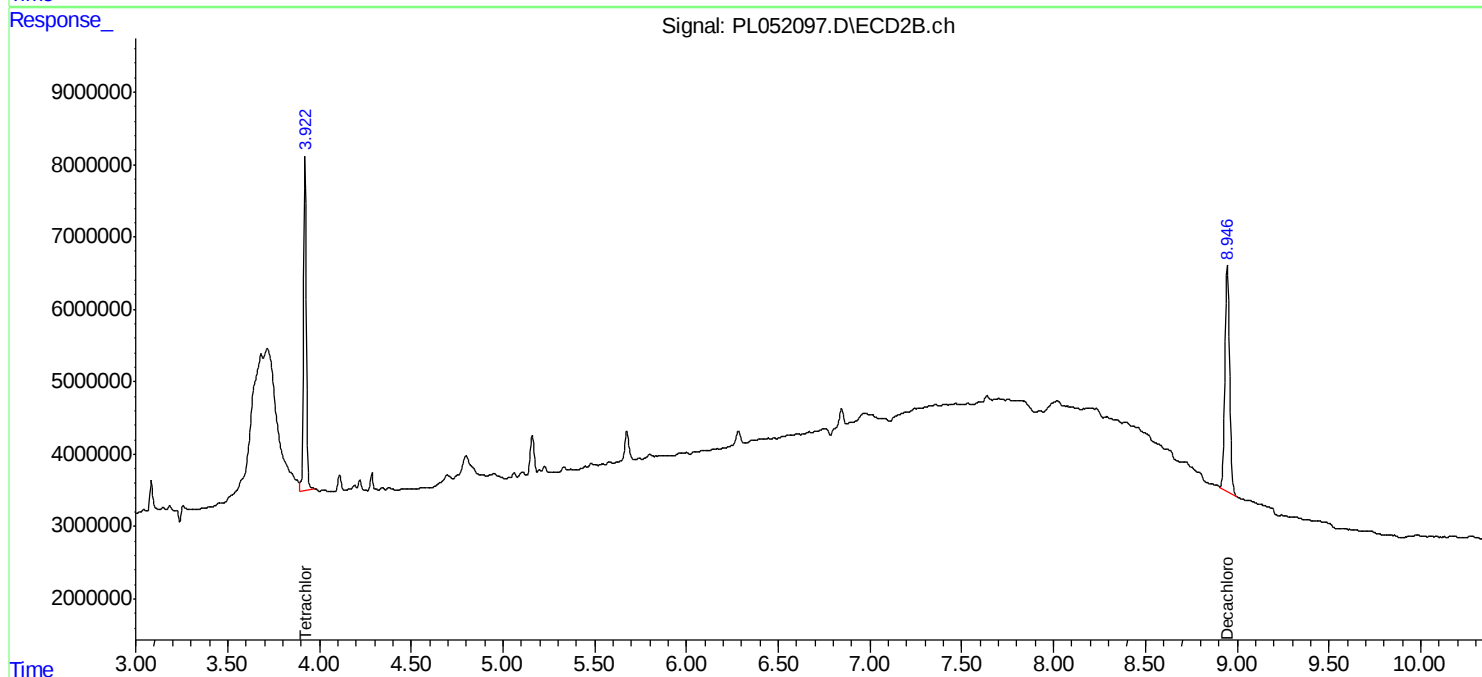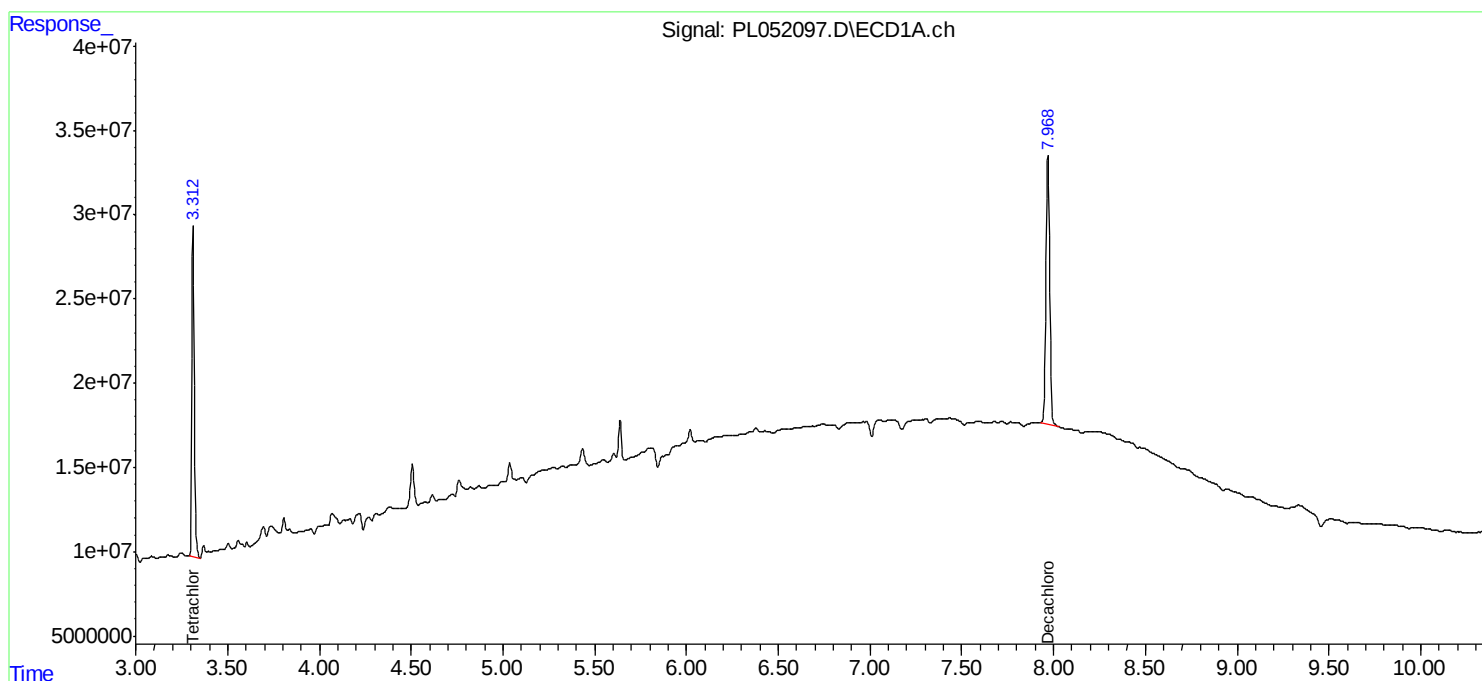

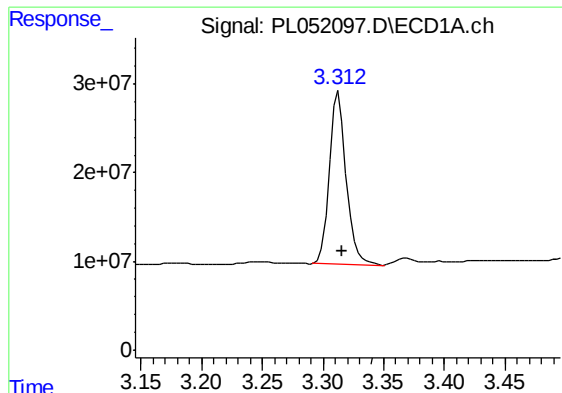


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 188281141
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP9-COMP


Manual Integrations
APPROVED

Ankita
9/3/2019 2:14:27 PM

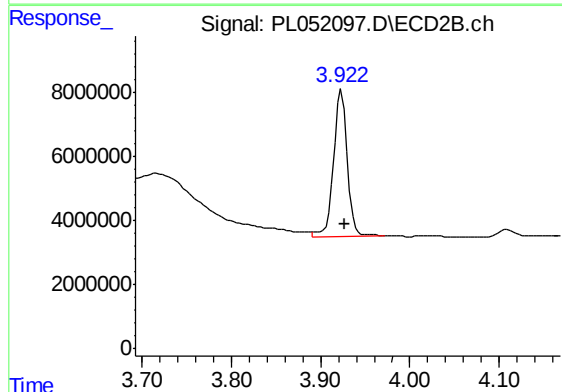


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 48623820
Conc: 22.26 ng/ml

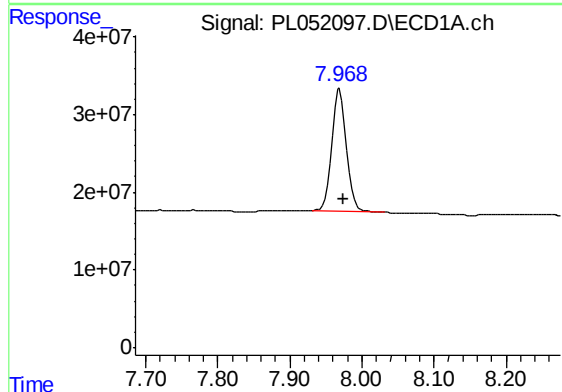

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: -0.006 min
Response: 221453615
Conc: 18.24 ng/ml

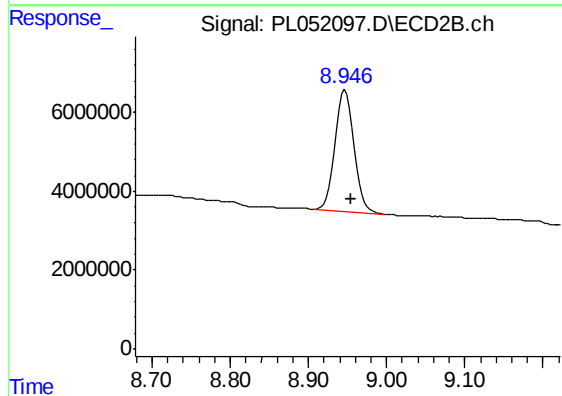

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.009 min
Response: 53491450
Conc: 17.57 ng/ml m