

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
 Data File : PL069566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2021 11:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:51:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.633	5.570	6874194	27079305	22.081	21.524
28) SA Decachlor...	10.401	11.493	13194127	24775273	22.373	21.955
Target Compounds						
4) MA Heptachlor	6.150f	0.000	563844	0	1.154	N.D. #
6) B beta-BHC	6.150	0.000	563844	0	2.349	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
Data File : PL069566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2021 11:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 01:51:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

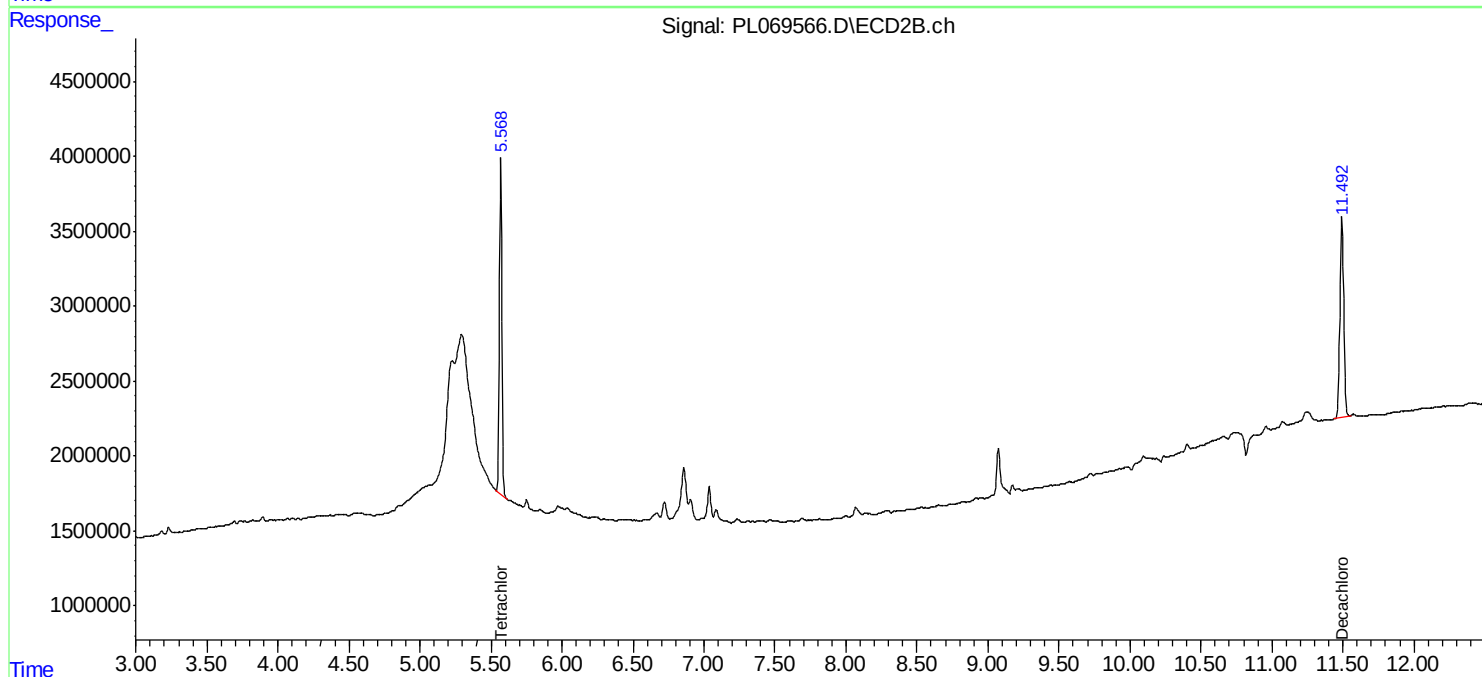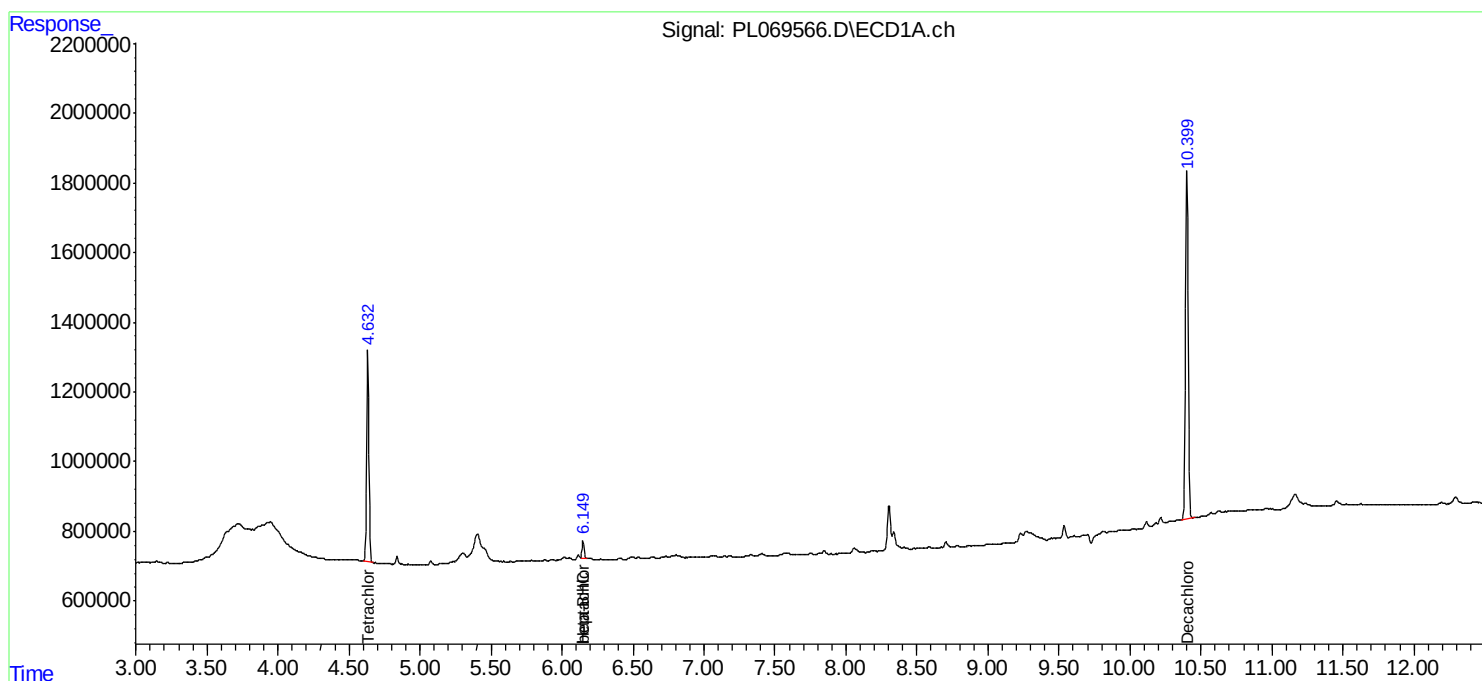


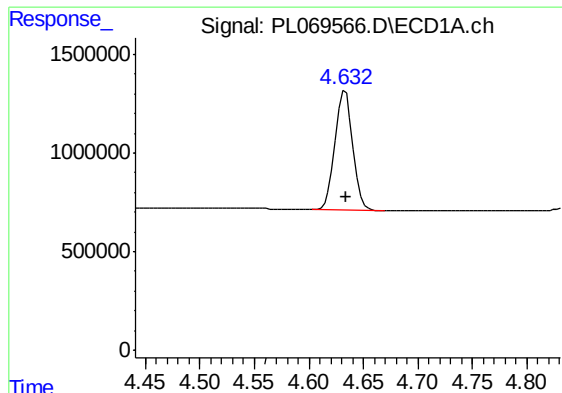

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 6874194
Conc: 22.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

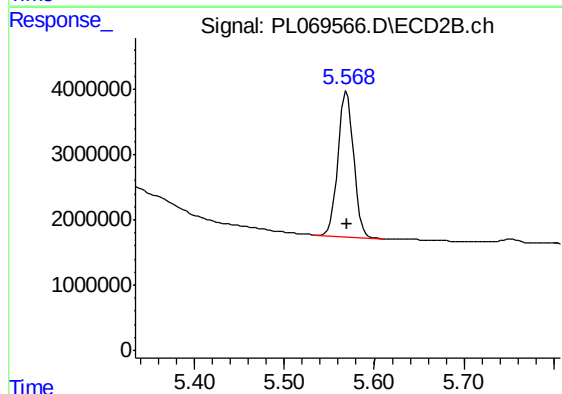


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 27079305
Conc: 21.52 ng/ml

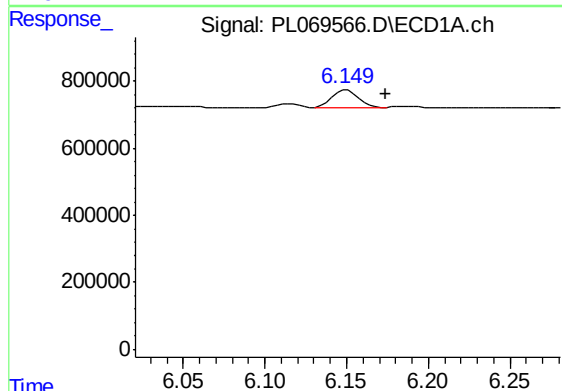


#4 Heptachlor

R.T.: 6.150 min
Delta R.T.: -0.024 min
Response: 563844
Conc: 1.15 ng/ml

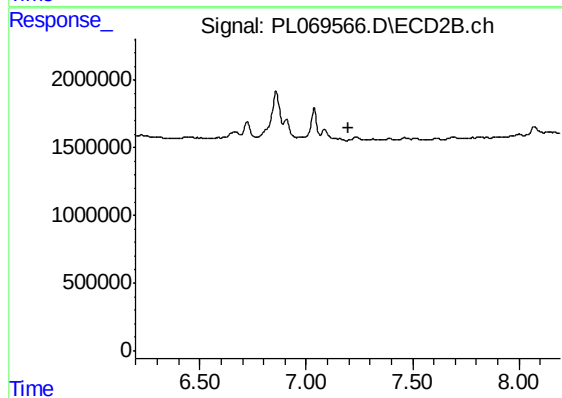

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.196 min
Response: 0
Conc: N.D.

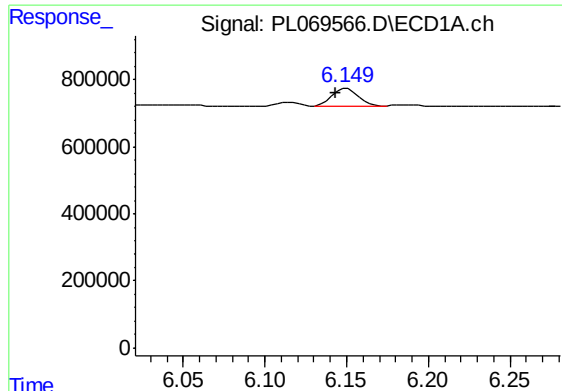

#6 beta-BHC


R.T.: 6.150 min
Delta R.T.: 0.007 min
Response: 563844
Conc: 2.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

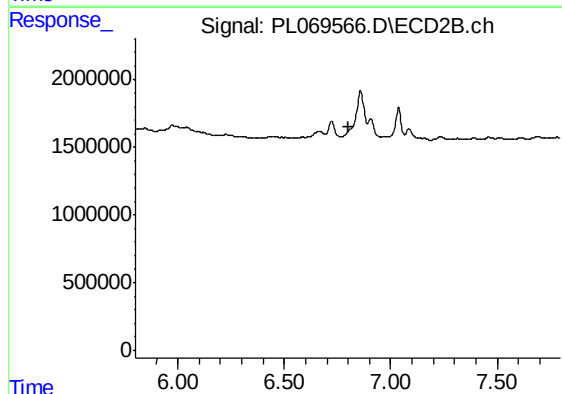


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

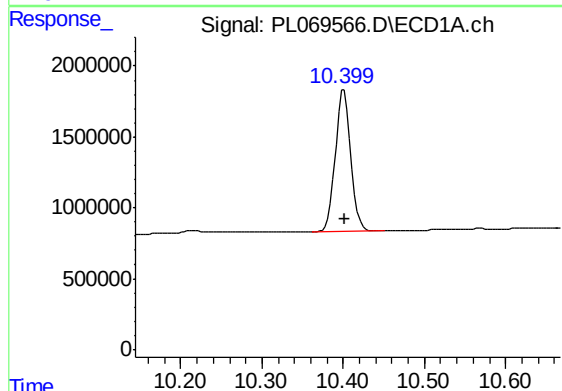

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.001 min
Response: 13194127
Conc: 22.37 ng/ml

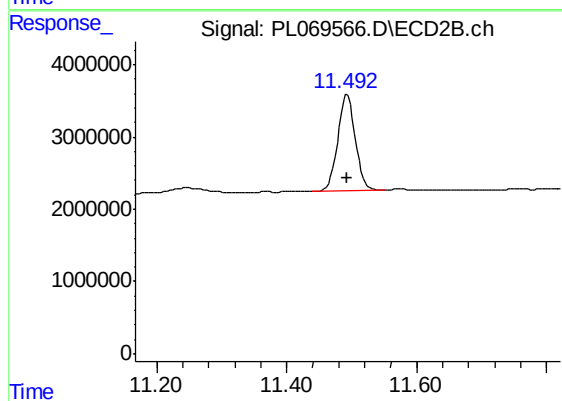

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 24775273
Conc: 21.96 ng/ml