

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
 Data File : PL069592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 00:48
 Operator : AR\AJ
 Sample : M3564-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-237

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 04:49:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.570	6550678	23837645	21.042	18.948
28)	SA Decachlor...	10.402	11.493	8929687	16318725	15.142	14.461
Target Compounds							
9)	A Endosulfan I	7.504f	0.000	1679708	0	3.553	N.D. #
16)	A 4,4'-DDD	0.000	9.108	0	2532775	N.D.	2.329 #
17)	MA 4,4'-DDT	8.480	0.000	701960	0	1.510	N.D. #
18)	B Endrin al...	8.525f	0.000	694555	0	1.623	N.D. #
19)	B Endosulfa...	8.787	0.000	704429	0	1.331	N.D. #
20)	A Methoxychlor	9.050f	0.000	1087301	0	3.528	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
Data File : PL069592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 00:48
Operator : AR\AJ
Sample : M3564-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-237

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 04:49:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

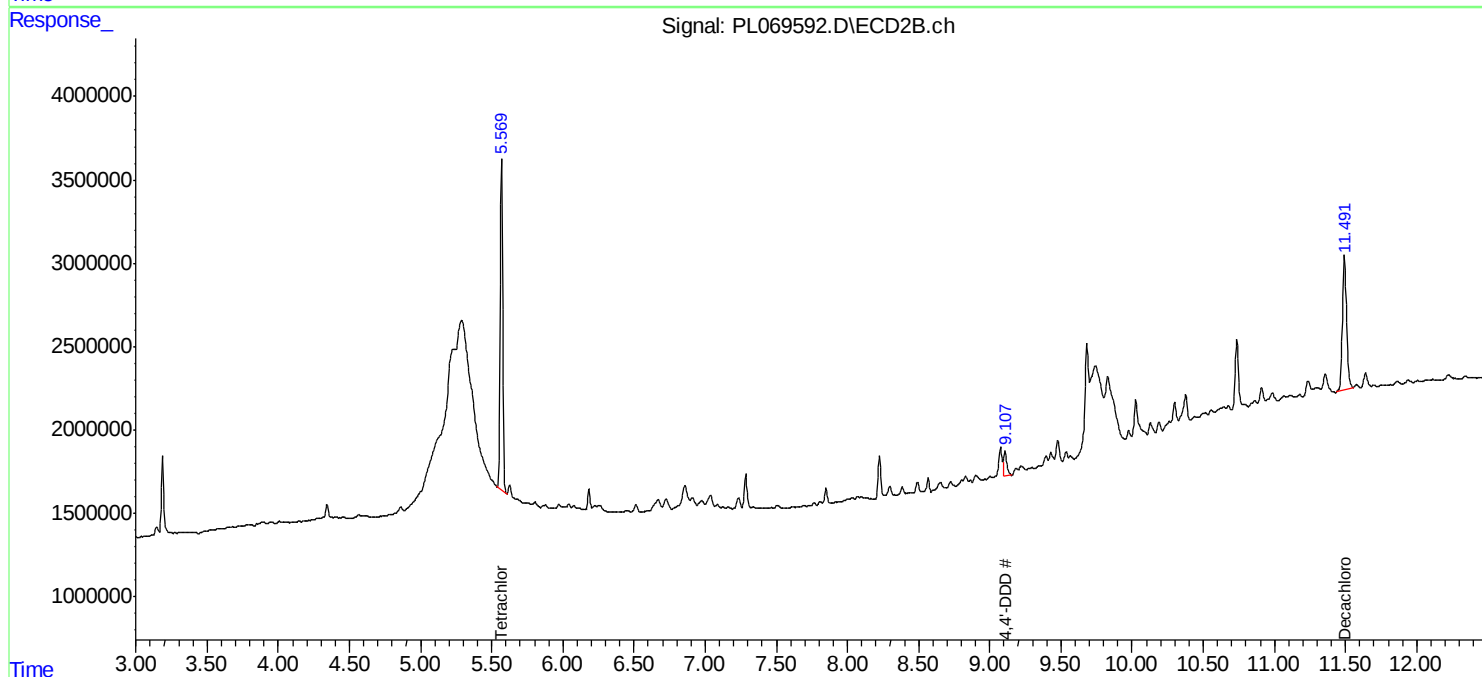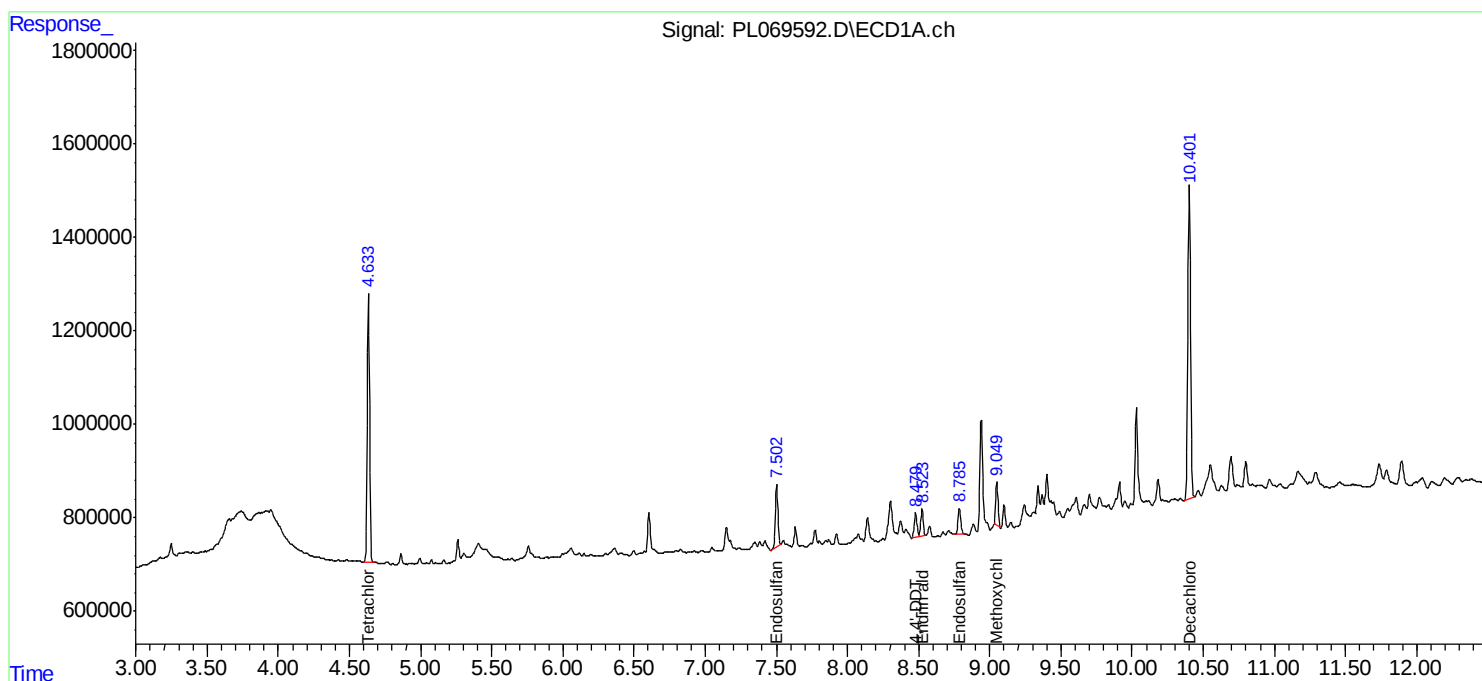


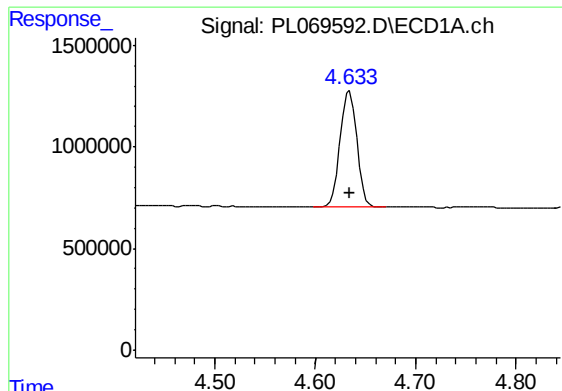

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 6550678
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-237

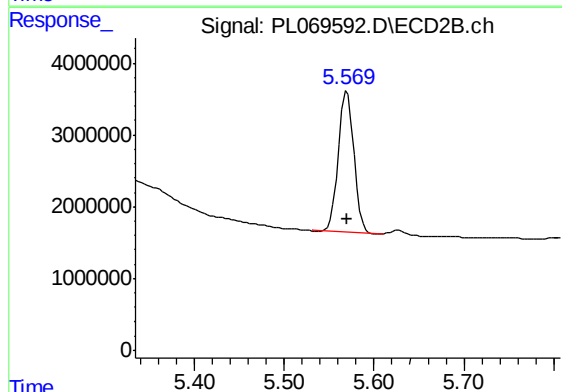


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 23837645
Conc: 18.95 ng/ml

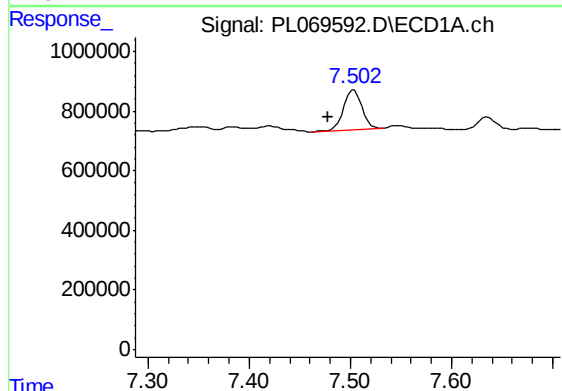


#9 Endosulfan I

R.T.: 7.504 min
Delta R.T.: 0.026 min
Response: 1679708
Conc: 3.55 ng/ml

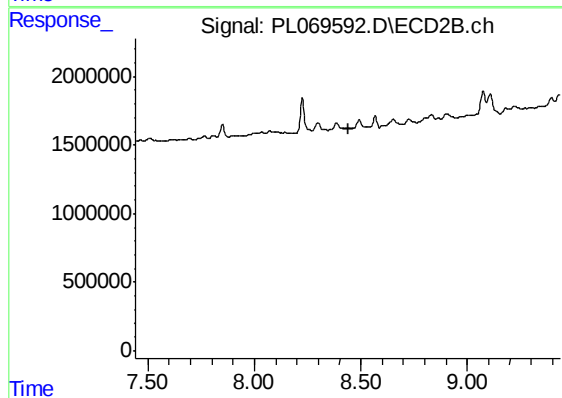

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 8.439 min
Response: 0
Conc: N.D.

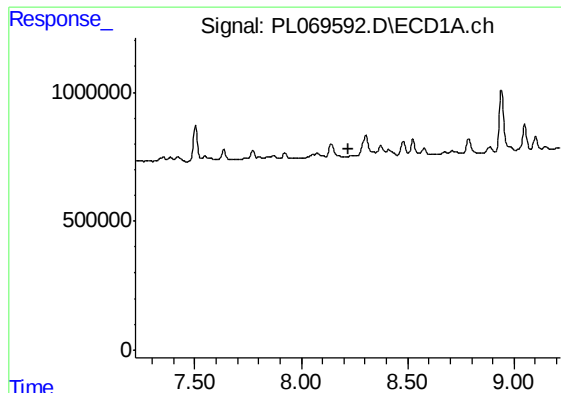

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-237

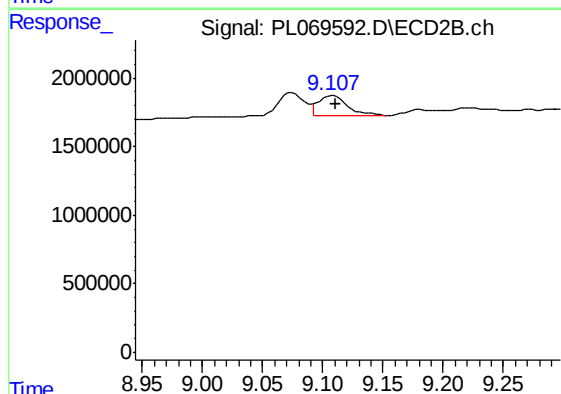


#16 4,4'-DDD

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 2532775
Conc: 2.33 ng/ml

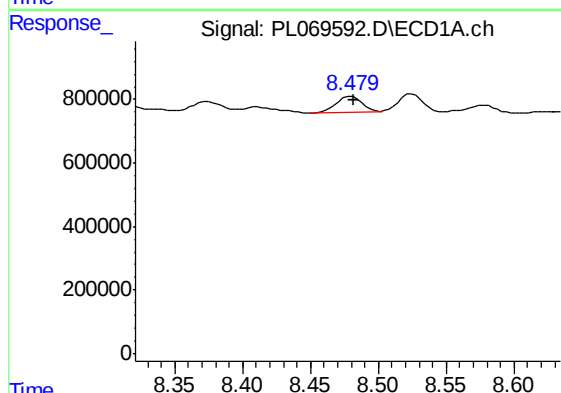


#17 4,4'-DDT

R.T.: 8.480 min
Delta R.T.: -0.002 min
Response: 701960
Conc: 1.51 ng/ml

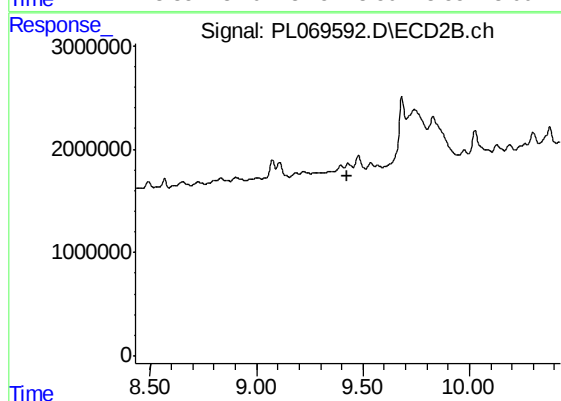

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 9.428 min
Response: 0
Conc: N.D.

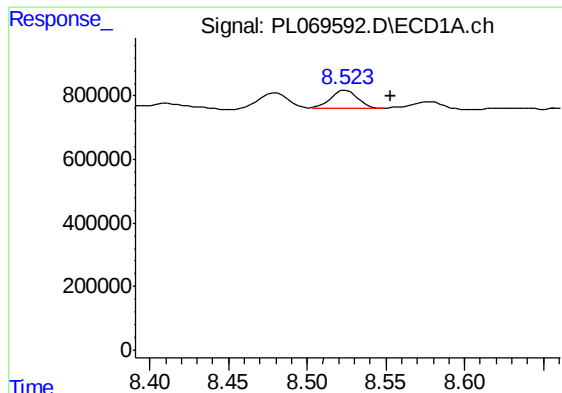

#18 Endrin aldehyde


R.T.: 8.525 min
Delta R.T.: -0.029 min
Response: 694555
Conc: 1.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-237

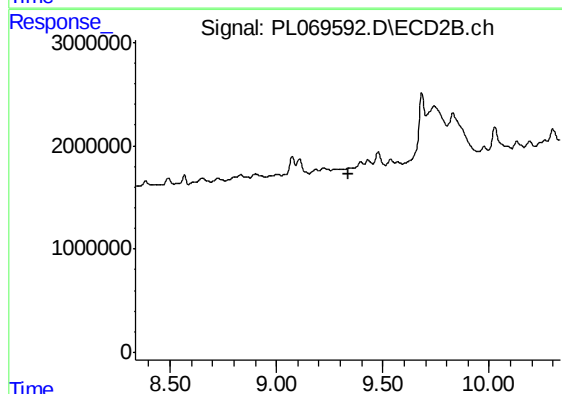


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

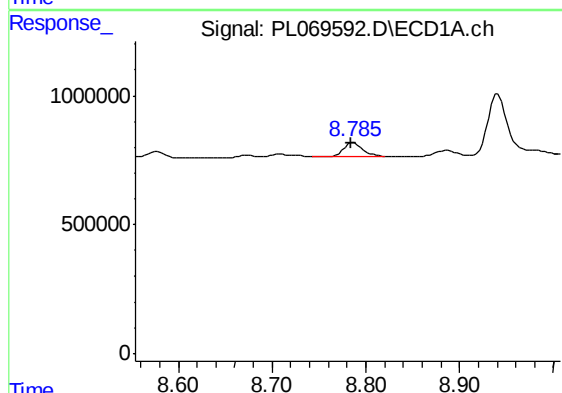


#19 Endosulfan Sulfate

R.T.: 8.787 min
Delta R.T.: 0.002 min
Response: 704429
Conc: 1.33 ng/ml

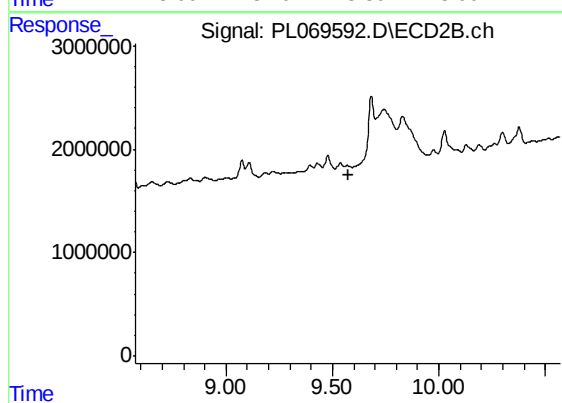

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.574 min
Response: 0
Conc: N.D.

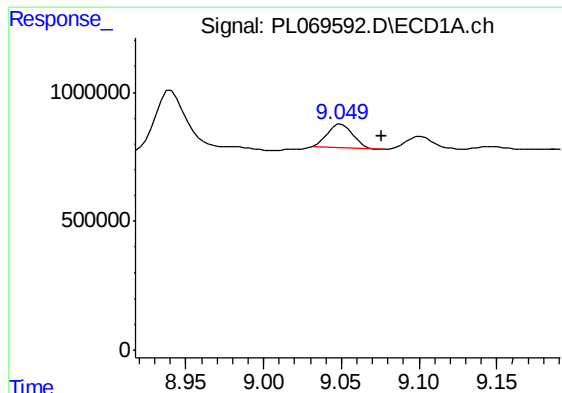

#20 Methoxychlor


R.T.: 9.050 min
Delta R.T.: -0.026 min
Response: 1087301
Conc: 3.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-237

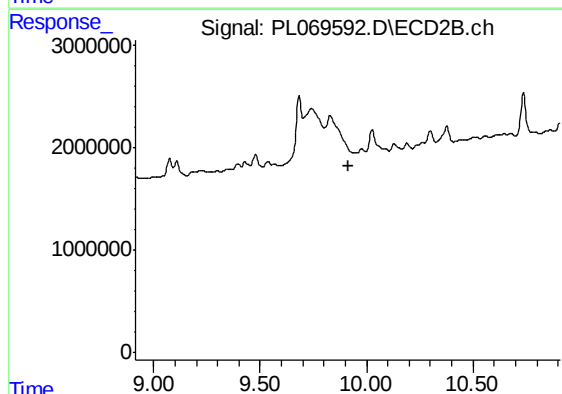


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

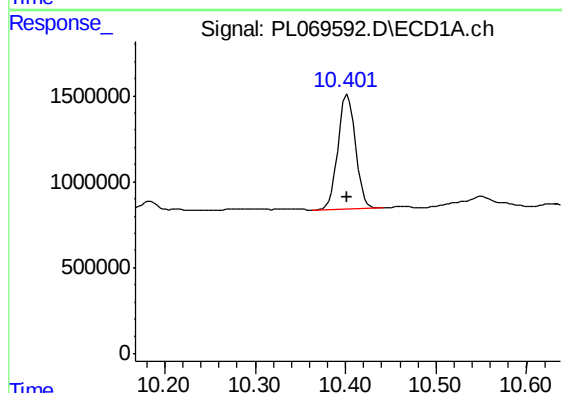

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 8929687
Conc: 15.14 ng/ml

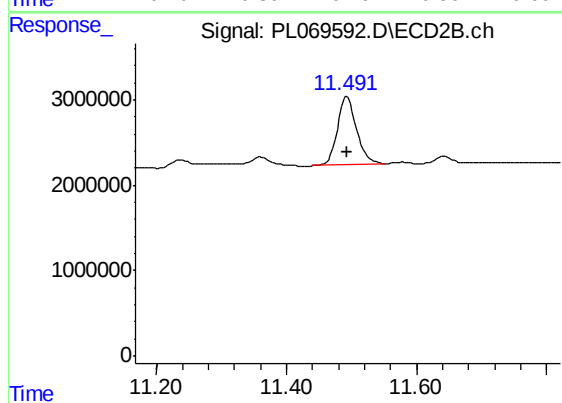

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 16318725
Conc: 14.46 ng/ml