

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
 Data File : PL069600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 03:18
 Operator : AR\AJ
 Sample : M3569-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 04:52:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.569	5331186	20390663	17.125	16.208
28)	SA Decachlor...	10.401	11.491	8730347	16042027	14.804	14.216
Target Compounds							
8)	B Heptachlo...	0.000	8.029	0	1993625	N.D.	1.476 #
10)	B gamma-Chl...	7.351	8.303	4894377	45443483	9.541	32.719 #
11)	B alpha-Chl...	7.421	8.384	5674951	15789779	10.921	11.538
12)	B 4,4'-DDE	7.634	8.565	1065267	2934200	2.363	2.215
13)	MA Dieldrin	7.772	0.000	892081	0	1.804	N.D. #
14)	MA Endrin	8.066	8.964	22516648	1424274	47.185	1.278 #
15)	B Endosulfa...	8.364	0.000	904685	0	1.840	N.D. #
16)	A 4,4'-DDD	8.220	9.110	1168436	6051852	2.894	5.564 #
17)	MA 4,4'-DDT	8.476	9.427	2123432	1532806	4.569	1.406 #
20)	A Methoxychlor	9.049f	0.000	865058	0	2.807	N.D. #
25)	Chlordane-3	7.351	8.303	4894377	45443483	91.752	219.978 #
26)	Chlordane-4	7.421	8.384	5674951	15789779	98.837	63.662 #
27)	Chlordane-5	8.364	0.000	904685	0	40.671	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
Data File : PL069600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 03:18
Operator : AR\AJ
Sample : M3569-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 04:52:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

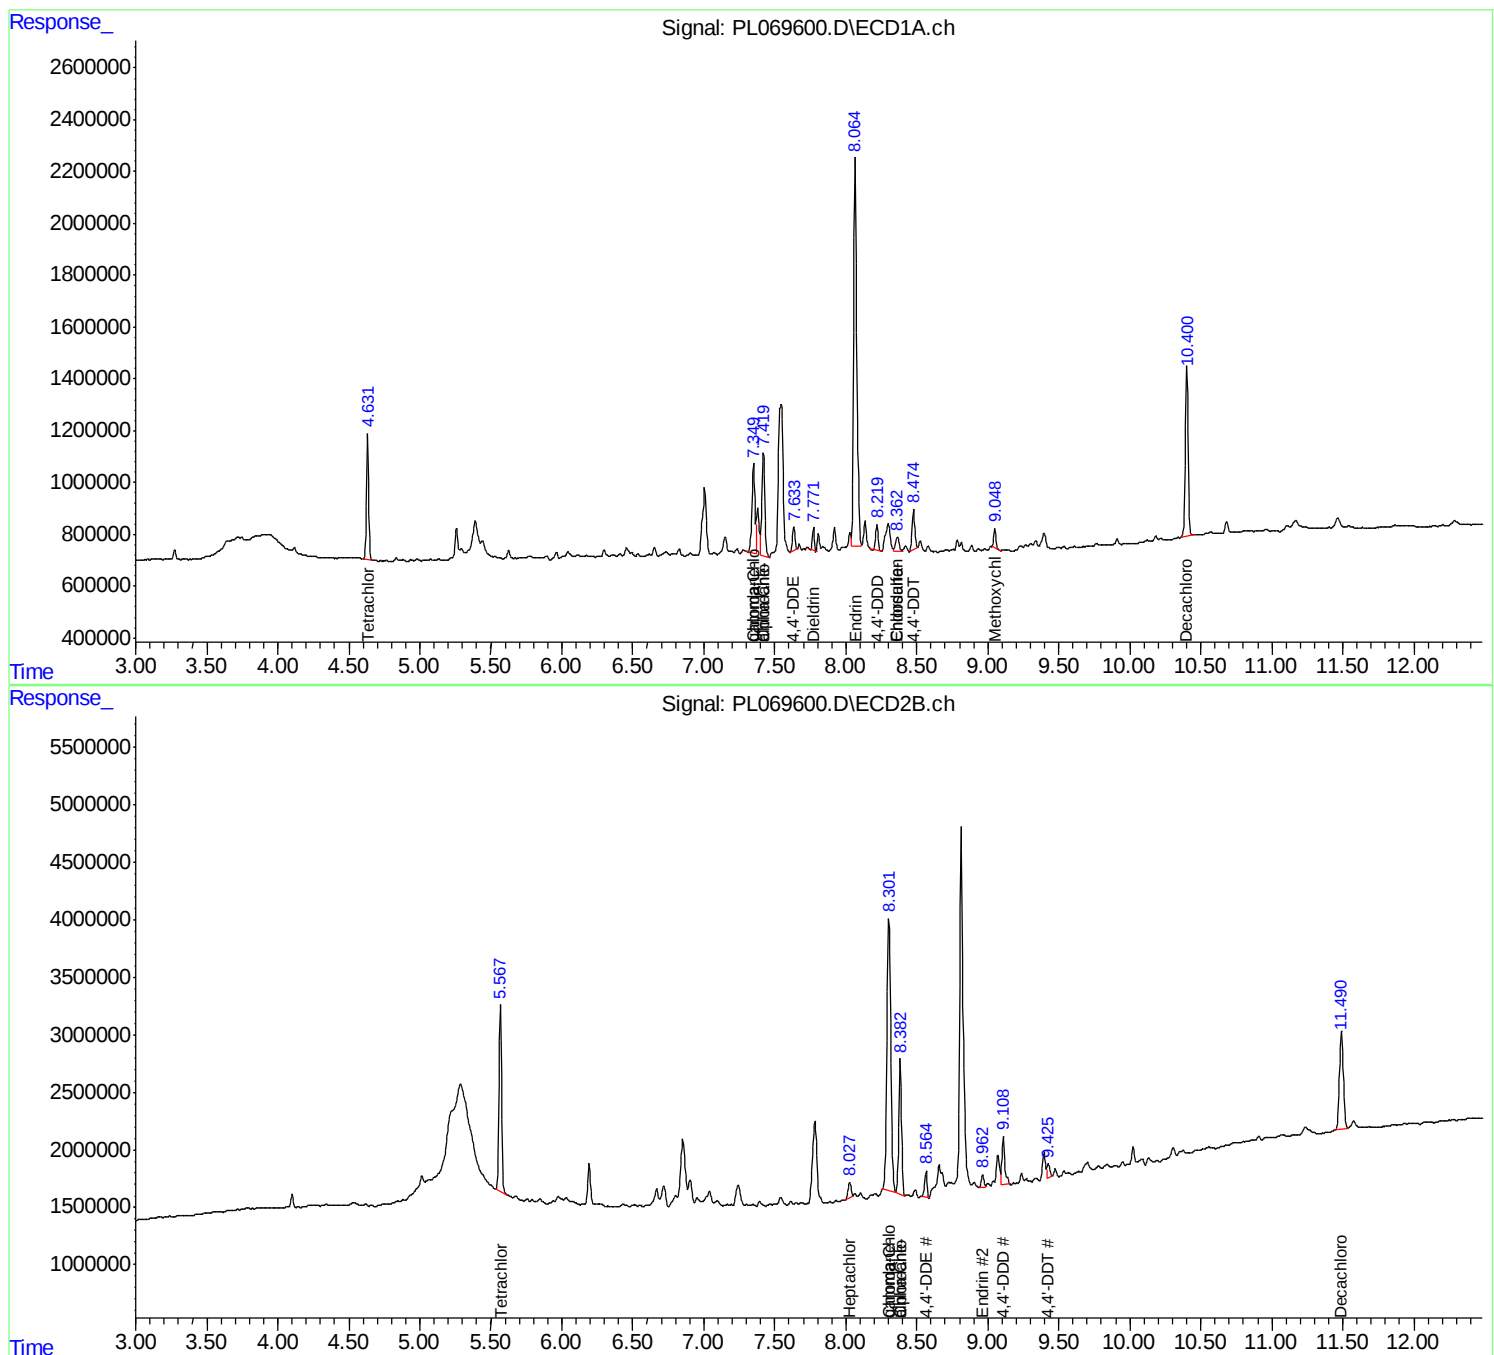


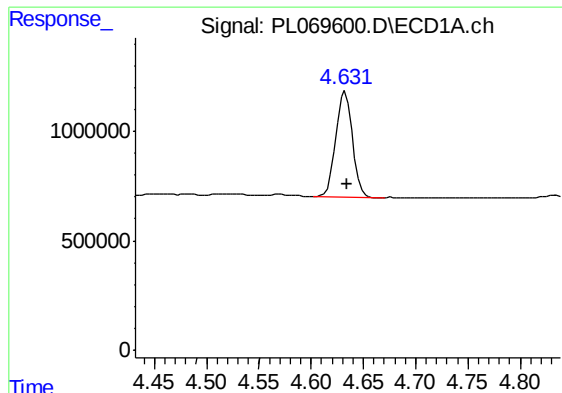

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: -0.001 min
Response: 5331186
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

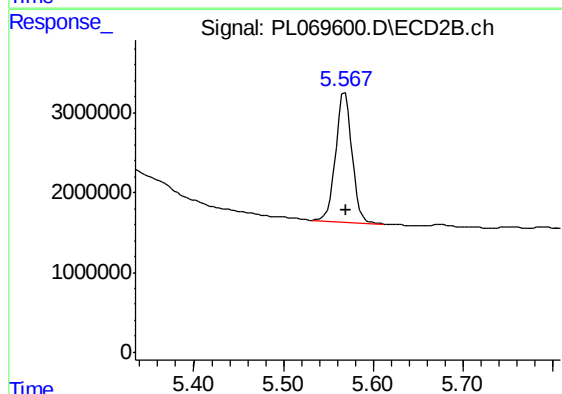


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 20390663
Conc: 16.21 ng/ml

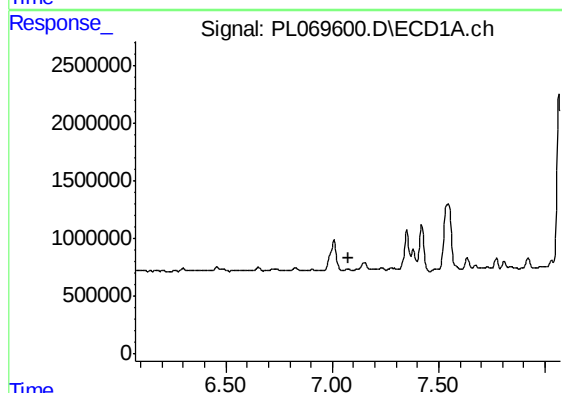


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.075 min
Response: 0
Conc: N.D.

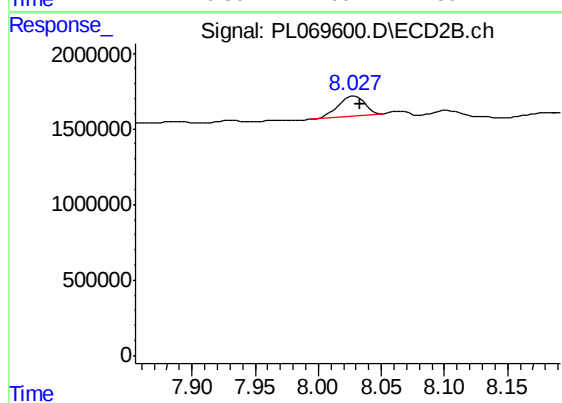

#8 Heptachlor epoxide


R.T.: 8.029 min
Delta R.T.: -0.005 min
Response: 1993625
Conc: 1.48 ng/ml

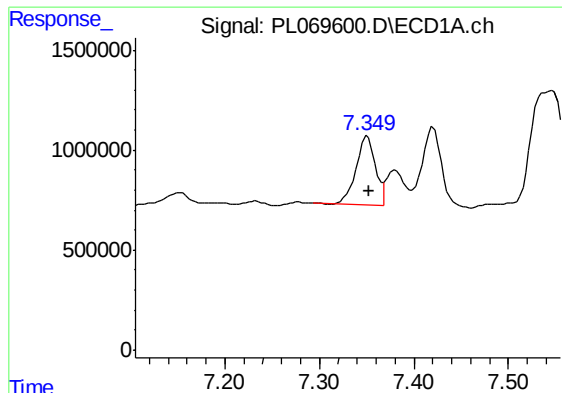

#10 gamma-Chlordane


R.T.: 7.351 min
Delta R.T.: -0.001 min
Response: 4894377
Conc: 9.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

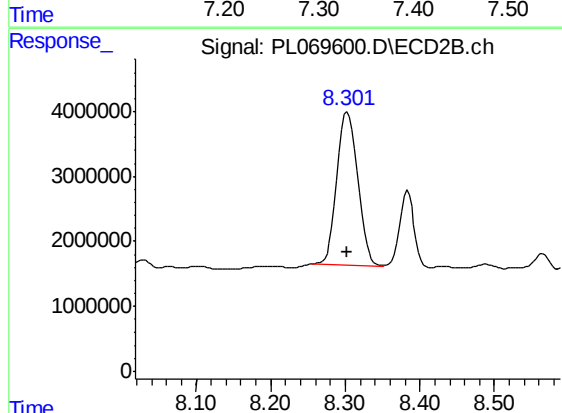


#10 gamma-Chlordane

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 45443483
Conc: 32.72 ng/ml

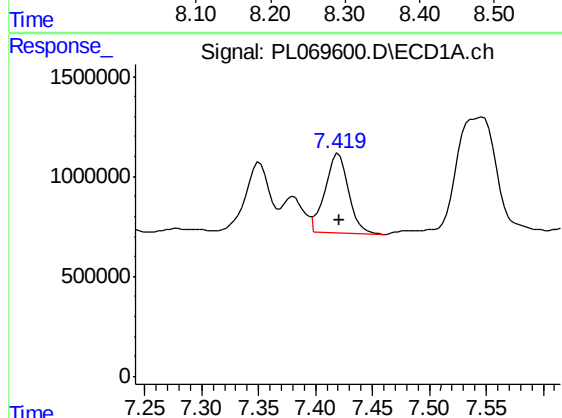


#11 alpha-Chlordane

R.T.: 7.421 min
Delta R.T.: -0.001 min
Response: 5674951
Conc: 10.92 ng/ml

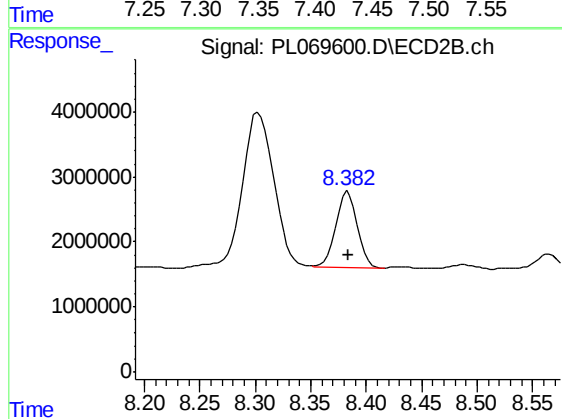

#11 alpha-Chlordane


R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 15789779
Conc: 11.54 ng/ml

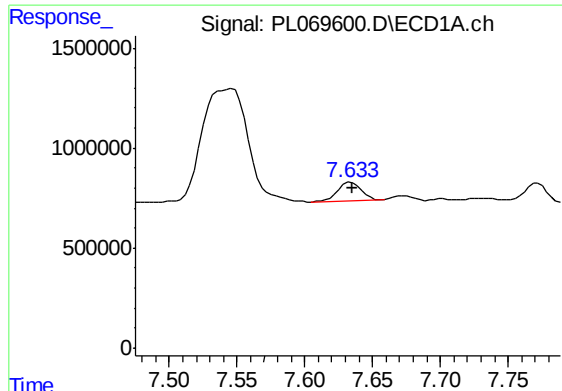

#12 4,4'-DDE


R.T.: 7.634 min
Delta R.T.: -0.001 min
Response: 1065267
Conc: 2.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

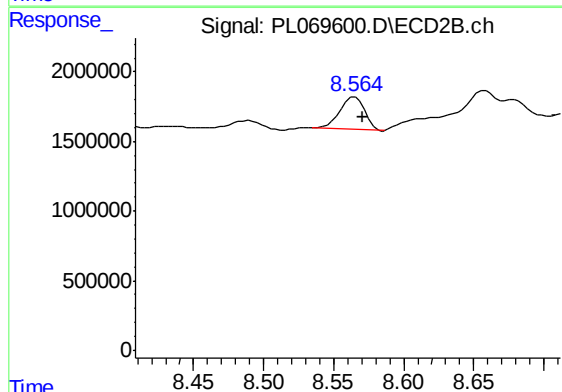


#12 4,4'-DDE

R.T.: 8.565 min
Delta R.T.: -0.006 min
Response: 2934200
Conc: 2.22 ng/ml

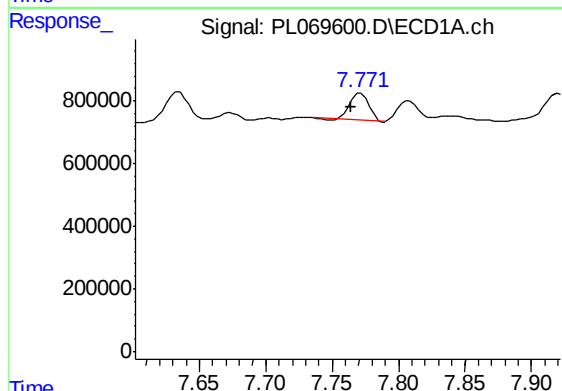


#13 Dieldrin

R.T.: 7.772 min
Delta R.T.: 0.008 min
Response: 892081
Conc: 1.80 ng/ml

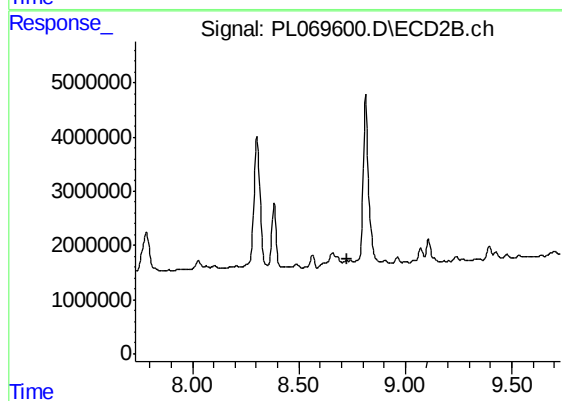

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.729 min
Response: 0
Conc: N.D.

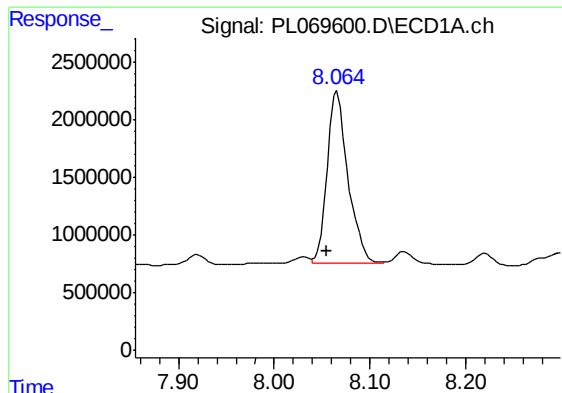

#14 Endrin


R.T.: 8.066 min
Delta R.T.: 0.011 min
Response: 22516648
Conc: 47.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

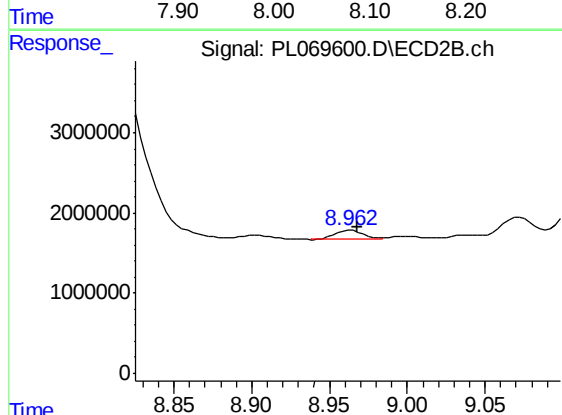


#14 Endrin

R.T.: 8.964 min
Delta R.T.: -0.005 min
Response: 1424274
Conc: 1.28 ng/ml

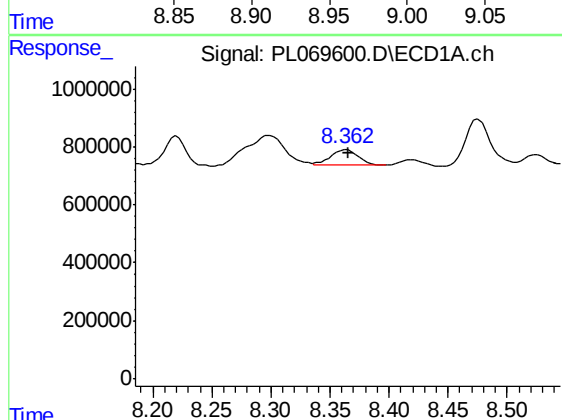


#15 Endosulfan II

R.T.: 8.364 min
Delta R.T.: -0.002 min
Response: 904685
Conc: 1.84 ng/ml

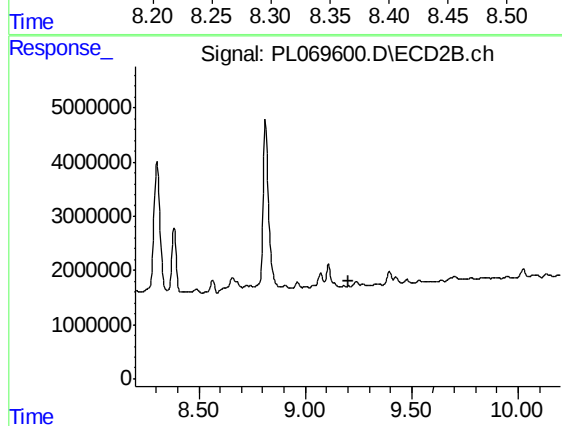

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.202 min
Response: 0
Conc: N.D.

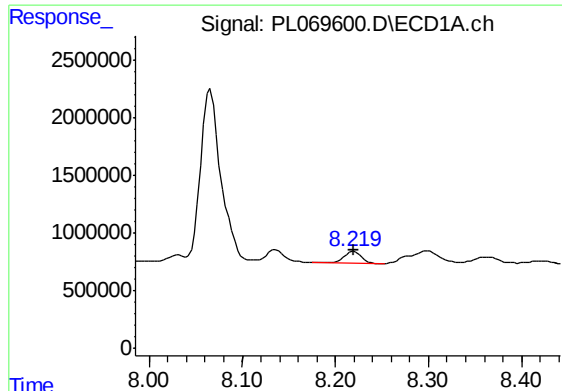

#16 4,4'-DDD


R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 1168436
Conc: 2.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

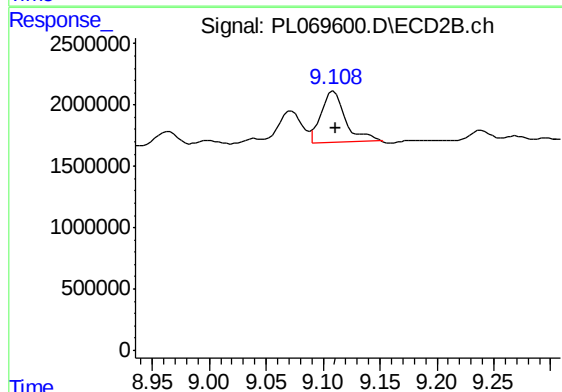


#16 4,4'-DDD

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 6051852
Conc: 5.56 ng/ml

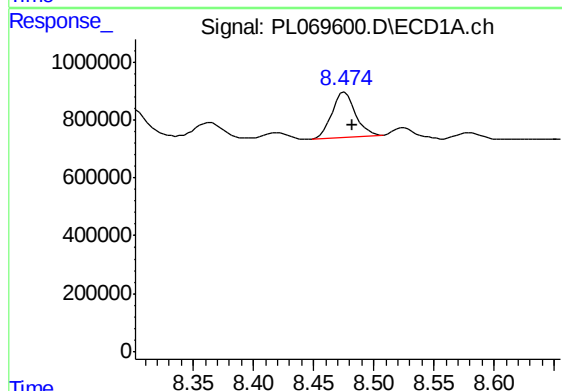


#17 4,4'-DDT

R.T.: 8.476 min
Delta R.T.: -0.006 min
Response: 2123432
Conc: 4.57 ng/ml

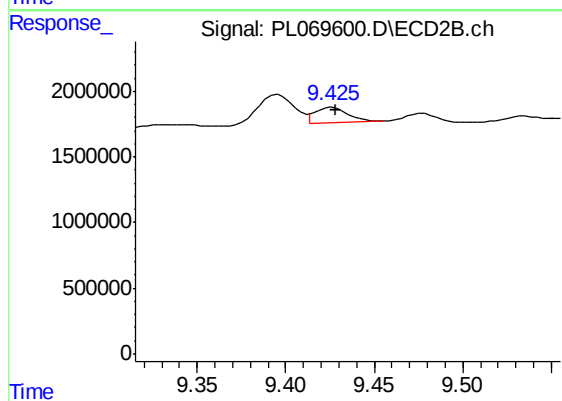

#17 4,4'-DDT


R.T.: 9.427 min
Delta R.T.: -0.002 min
Response: 1532806
Conc: 1.41 ng/ml

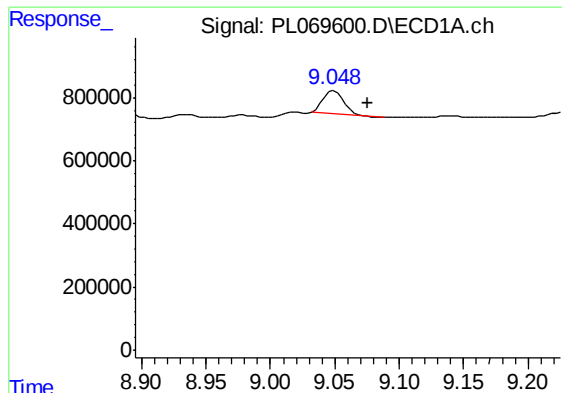

#20 Methoxychlor


R.T.: 9.049 min
Delta R.T.: -0.027 min
Response: 865058
Conc: 2.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

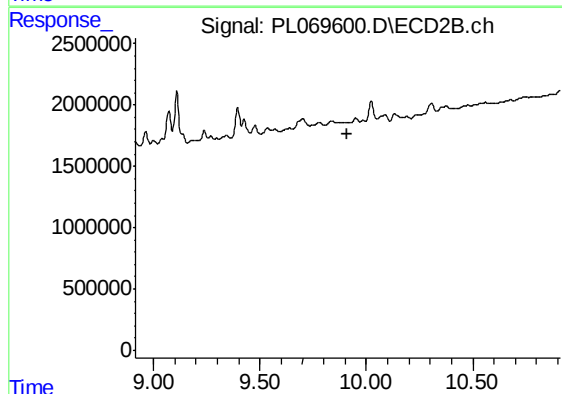


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

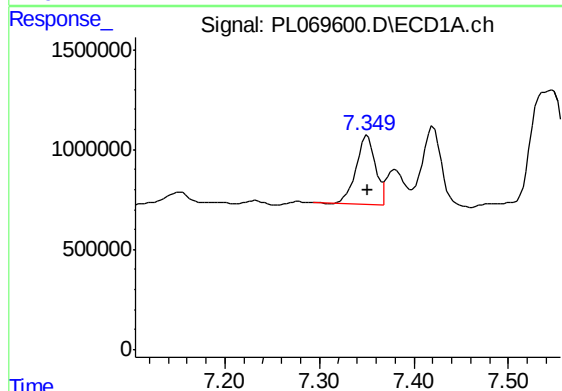


#25 Chlordane-3

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 4894377
Conc: 91.75 ng/ml

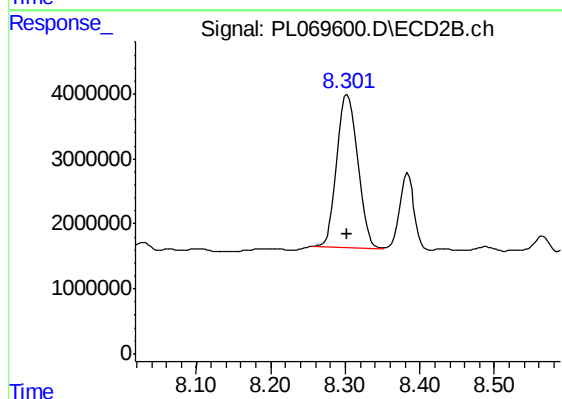

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 45443483
Conc: 219.98 ng/ml

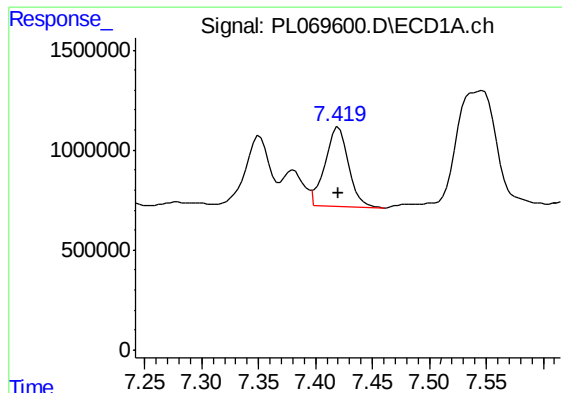

#26 Chlordane-4


R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 5674951
Conc: 98.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

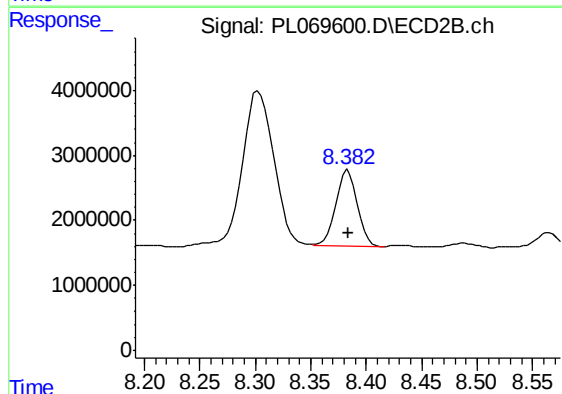


#26 Chlordane-4

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 15789779
Conc: 63.66 ng/ml

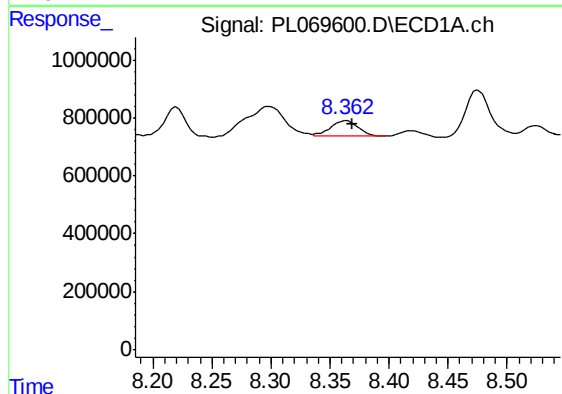


#27 Chlordane-5

R.T.: 8.364 min
Delta R.T.: -0.006 min
Response: 904685
Conc: 40.67 ng/ml

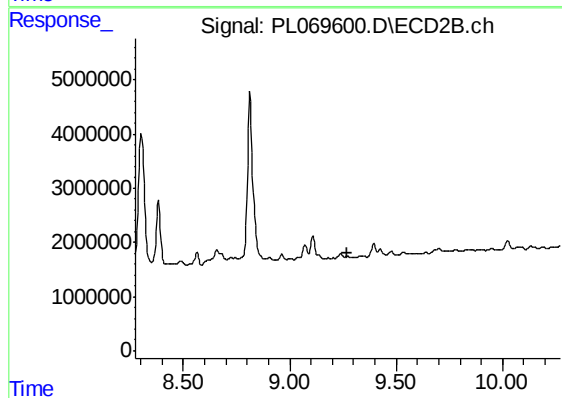

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.272 min
Response: 0
Conc: N.D.

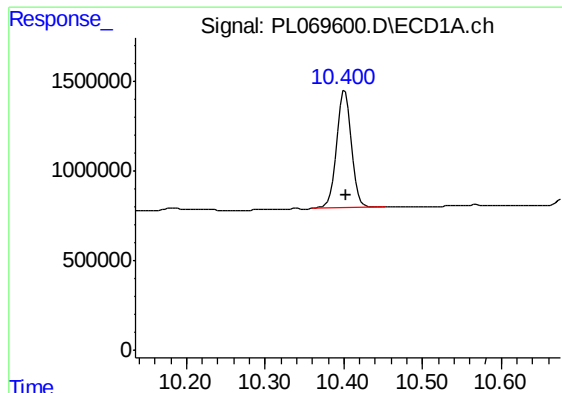

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: 0.000 min
Response: 8730347
Conc: 14.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1

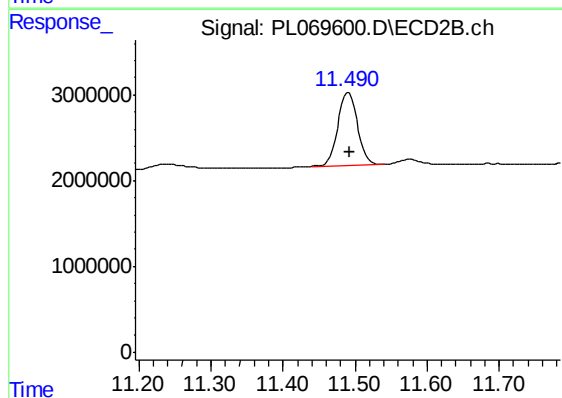

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.002 min
Response: 16042027
Conc: 14.22 ng/ml