

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
 Data File : PL069576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2021 14:35
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Manual Integrations
 APPROVED

Ankita
 8/31/2021 10:39:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:53:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 00:52:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.569	18046555	69432754	50.017m	50.000
28)	SA Decachlor...	10.403	11.494	30266685	58080040	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.965	6.954	6852373	25889652	500.000	500.000
24)	Chlordane-2	6.653	7.545	9695366	26199117	500.000	500.000
25)	Chlordane-3	7.354	8.303	25659382	99997283	500.000	500.000
26)	Chlordane-4	7.422	8.385	27596816	120.4E6	500.000	500.000
27)	Chlordane-5	8.372	9.273	10378845	21162558	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
Data File : PL069576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2021 14:35
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleID :
PCHLORICC500


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:53:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 00:52:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

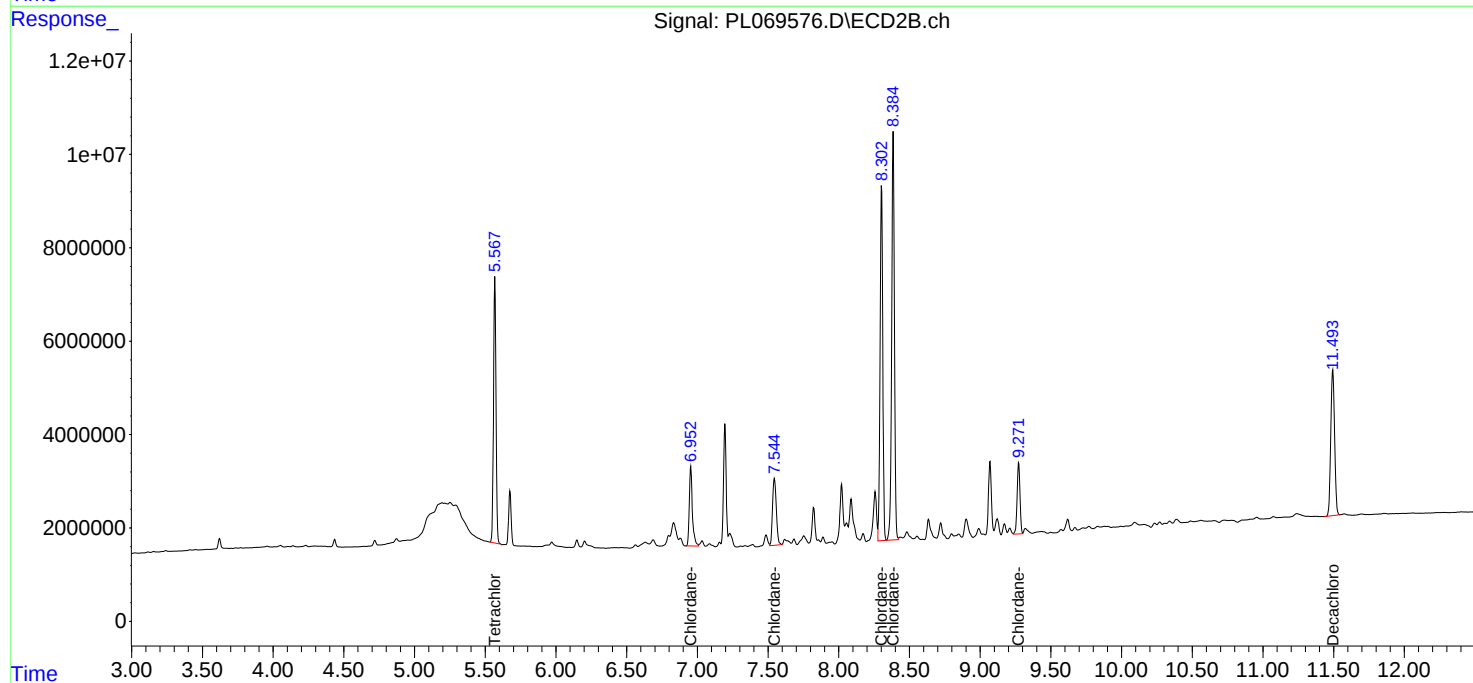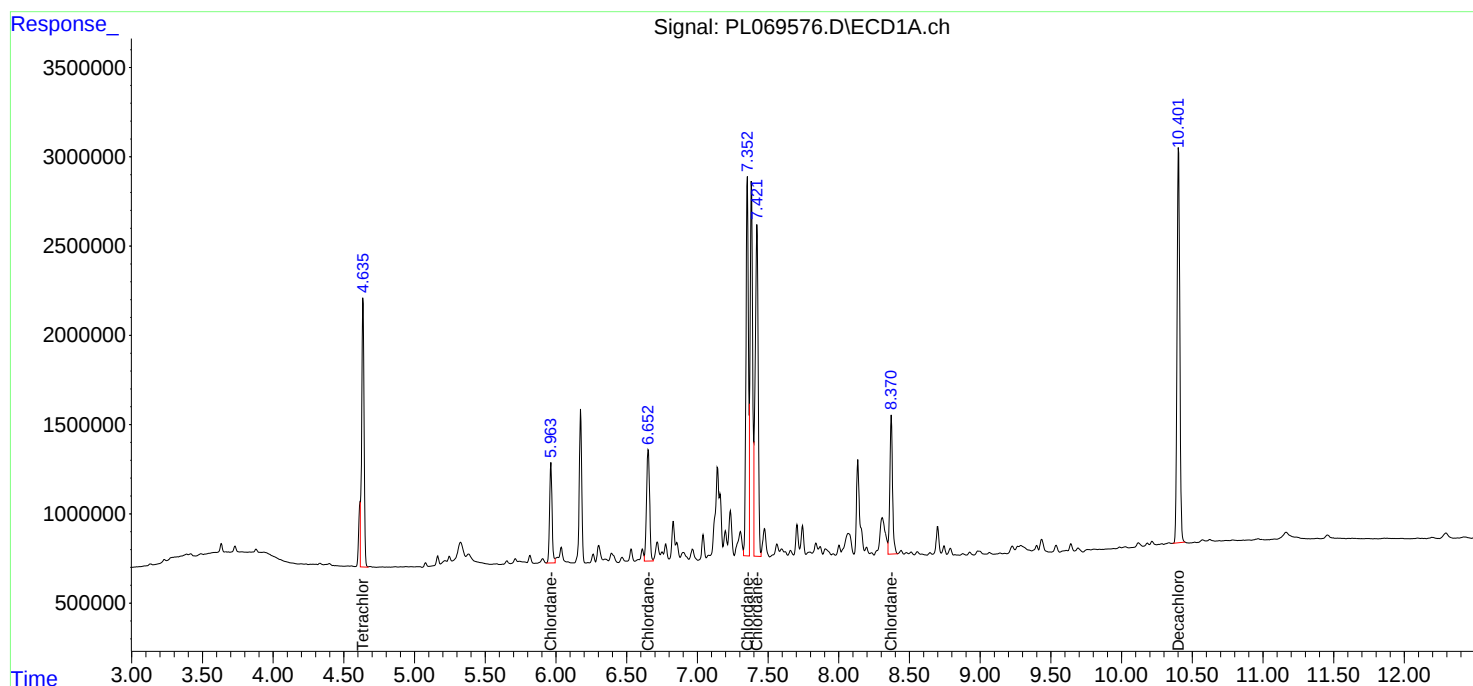

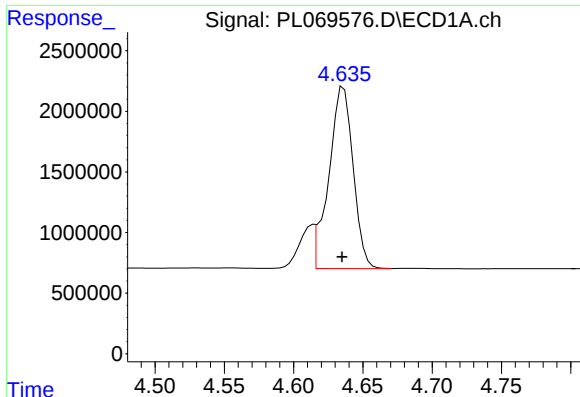


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: 0.000 min
Response: 18046555
Conc: 50.02 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:03 AM

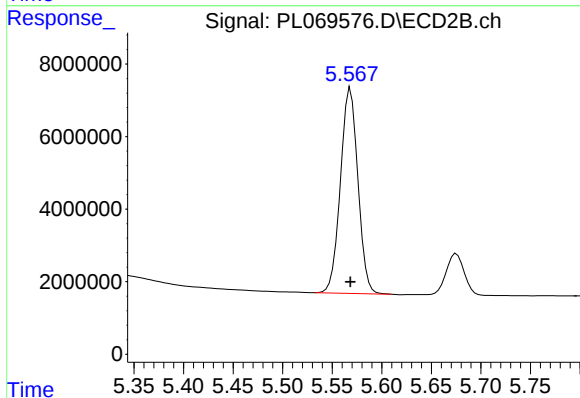


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 69432754
Conc: 50.00 ng/ml

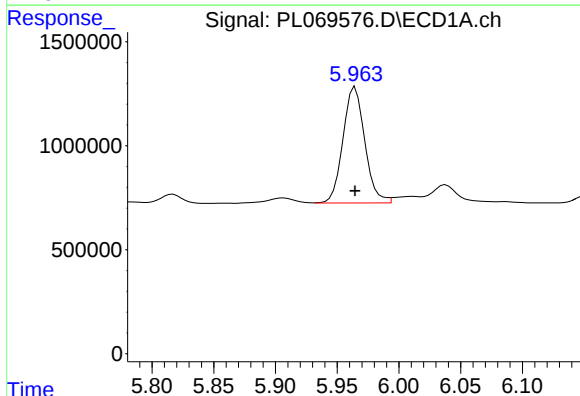


#23 Chlordane-1

R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 6852373
Conc: 500.00 ng/ml

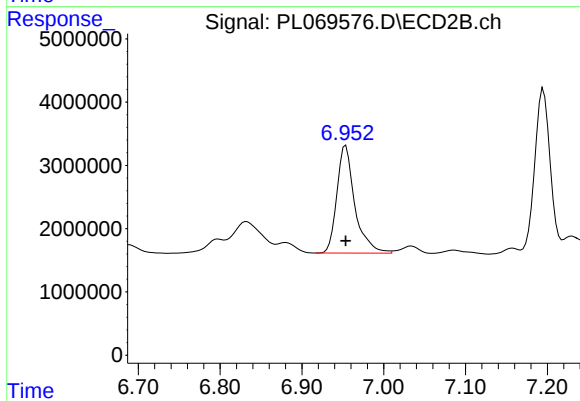

#23 Chlordane-1

R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 25889652
Conc: 500.00 ng/ml

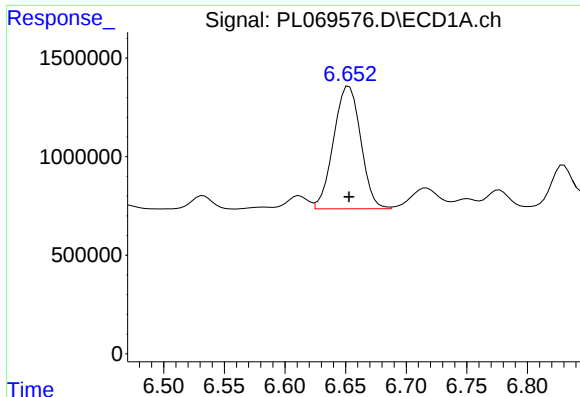


#24 Chlordane-2

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 9695366
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:03 AM

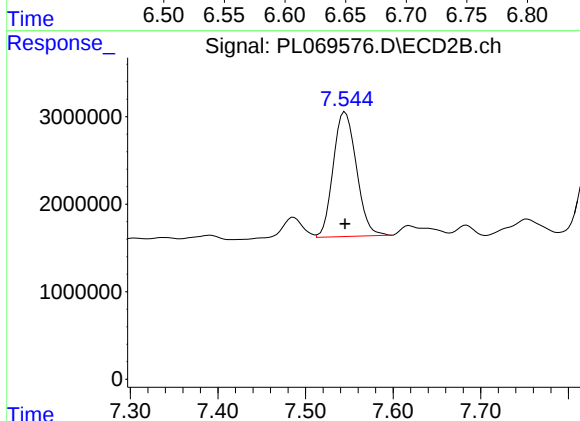


#24 Chlordane-2

R.T.: 7.545 min
Delta R.T.: 0.000 min
Response: 26199117
Conc: 500.00 ng/ml

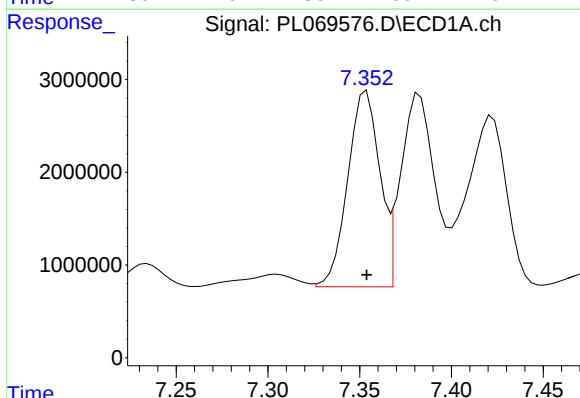


#25 Chlordane-3

R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 25659382
Conc: 500.00 ng/ml

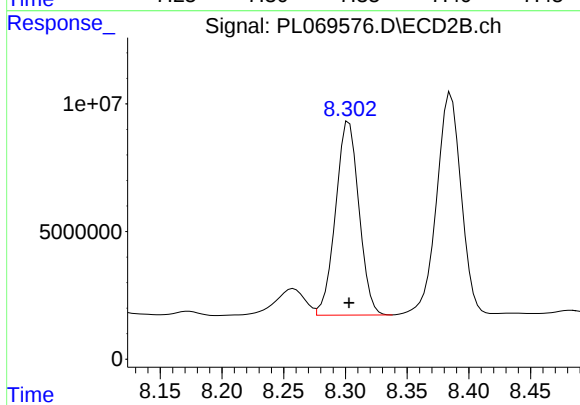

#25 Chlordane-3

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 99997283
Conc: 500.00 ng/ml

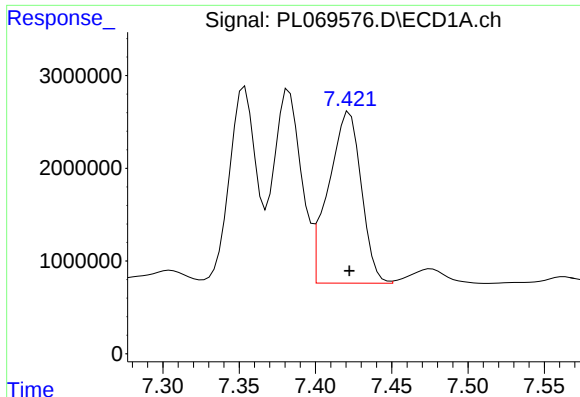


#26 Chlordane-4

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 27596816
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:03 AM

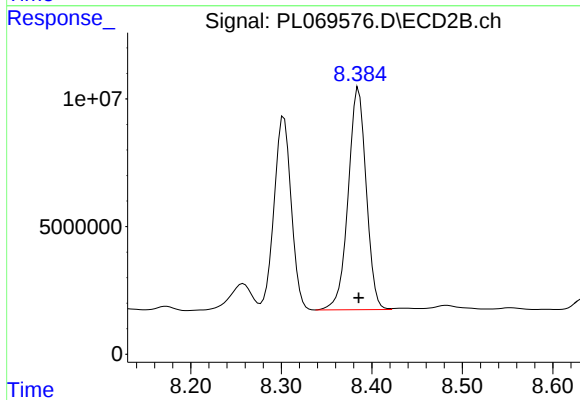


#26 Chlordane-4

R.T.: 8.385 min
Delta R.T.: 0.000 min
Response: 120399794
Conc: 500.00 ng/ml

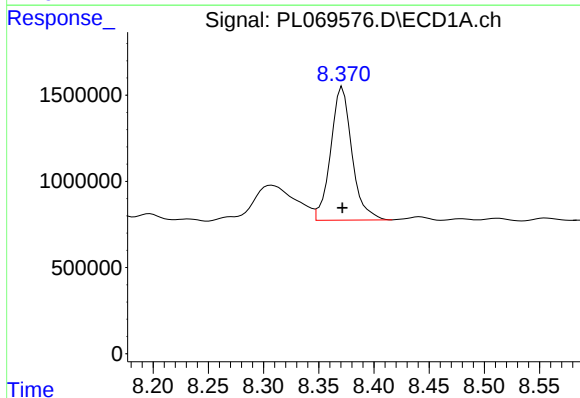


#27 Chlordane-5

R.T.: 8.372 min
Delta R.T.: 0.000 min
Response: 10378845
Conc: 500.00 ng/ml

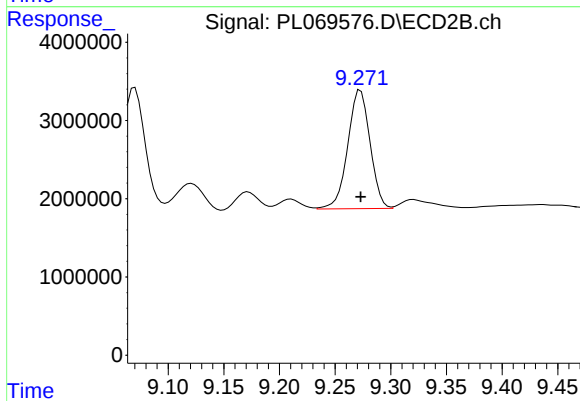

#27 Chlordane-5

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 21162558
Conc: 500.00 ng/ml

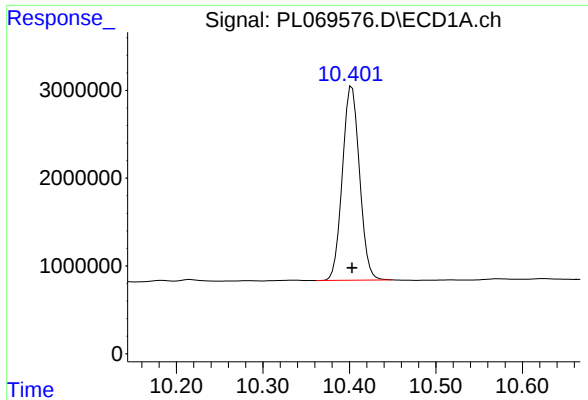


#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: 0.000 min
Response: 30266685
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:03 AM

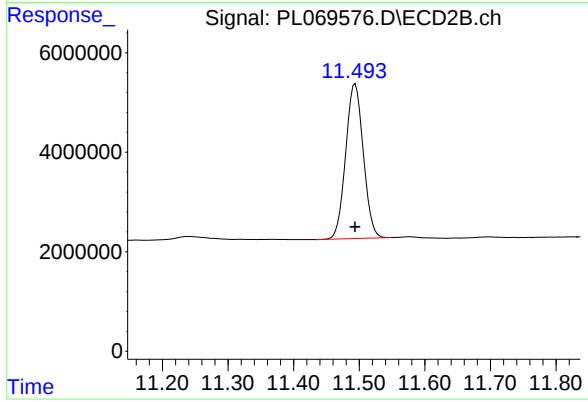

#28 Decachlorobiphenyl

R.T.: 11.494 min
Delta R.T.: 0.000 min
Response: 58080040
Conc: 50.00 ng/ml