

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
 Data File : PL069590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 00:14
 Operator : AR\AJ
 Sample : PB138784BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138784BL

Manual Integrations
 APPROVED

Ankita
 8/31/2021 10:39:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 04:48:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 31 01:49:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.569	7071236	24356029	22.714	19.360
28)	SA Decachlor...	10.411	11.498	13089427	22439580	22.195	19.886m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083021\
Data File : PL069590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 00:14
Operator : AR\AJ
Sample : PB138784BL
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PB138784BL


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 04:48:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL083021.M
Quant Title : GC Extractables
QLast Update : Tue Aug 31 01:49:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

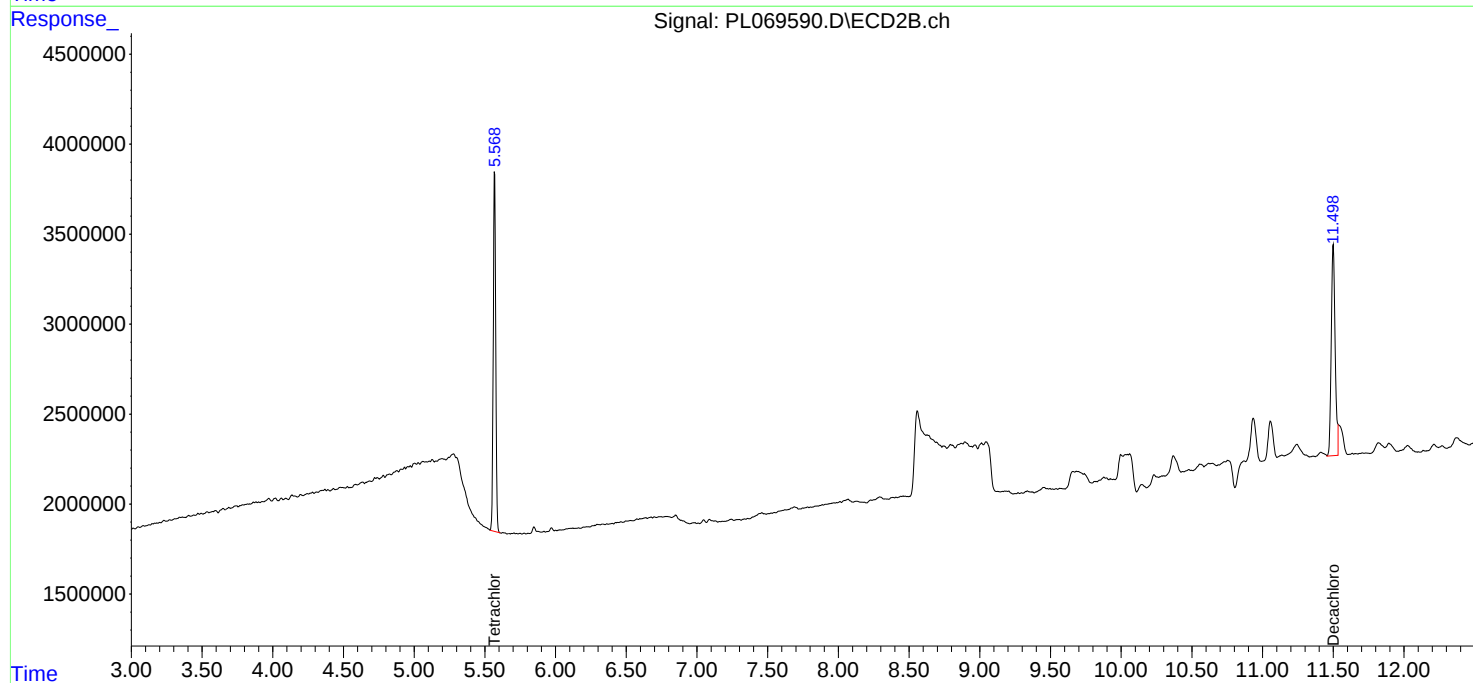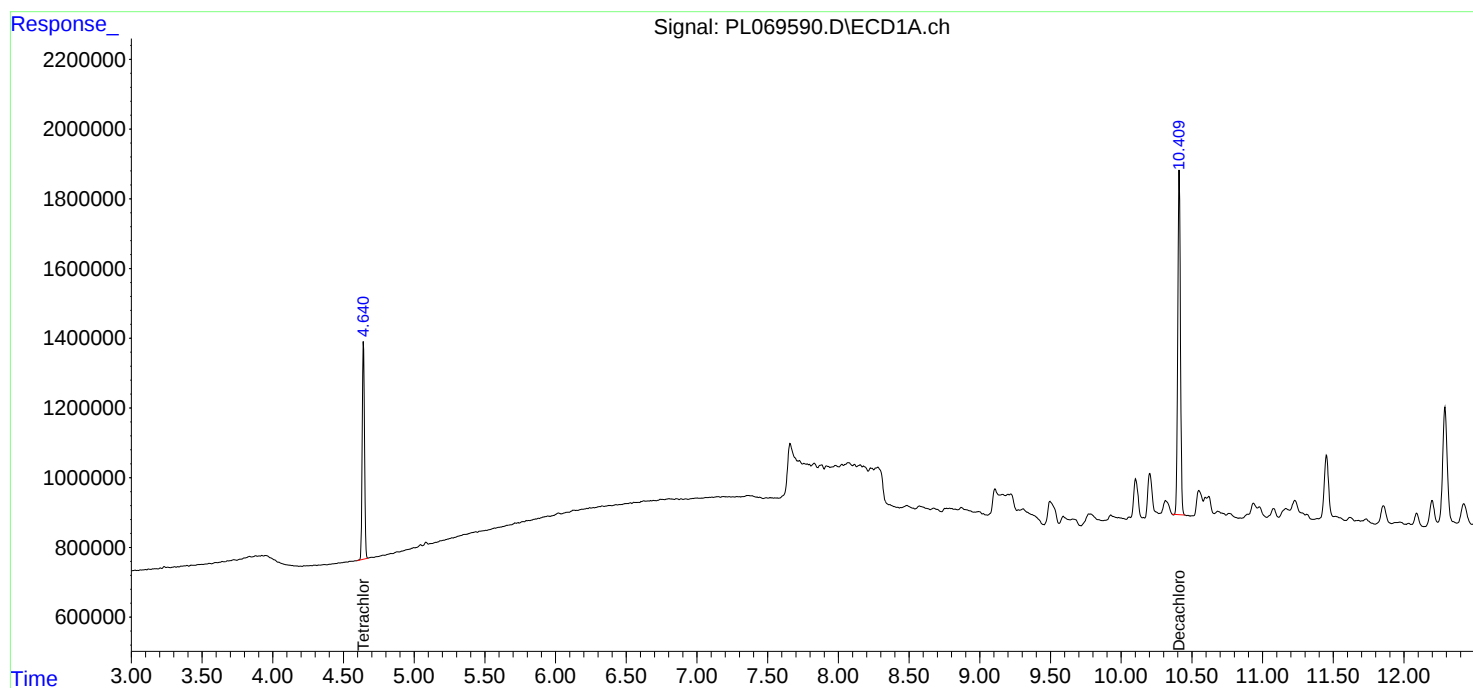

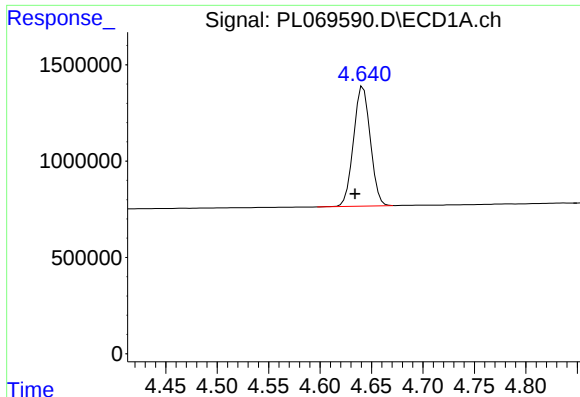


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.008 min
Response: 7071236
Conc: 22.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138784BL


Manual Integrations
APPROVED

Ankita
8/31/2021 10:39:09 AM

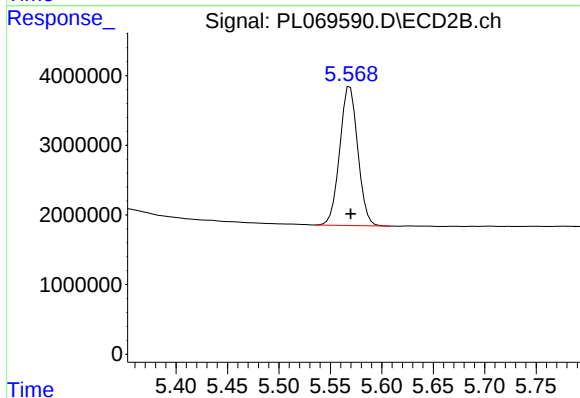


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 24356029
Conc: 19.36 ng/ml

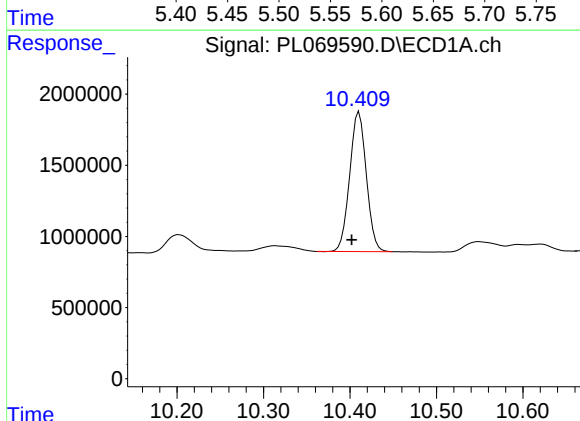

#28 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: 0.009 min
Response: 13089427
Conc: 22.20 ng/ml

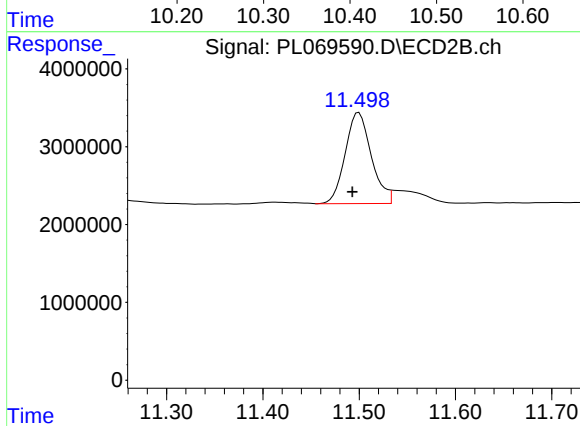

#28 Decachlorobiphenyl

R.T.: 11.498 min
Delta R.T.: 0.005 min
Response: 22439580
Conc: 19.89 ng/ml m