

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
 Data File : PL077372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2022 10:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 16:44:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439f	2.632	23312684	50973062	17.133	16.586
28)	SA Decachlor...	8.933f	7.737	19515811	43126974	16.653	15.456
Target Compounds							
4)	MA Heptachlor	0.000	3.753f	0	263688	N.D.	0.068 #
5)	MB Aldrin	0.000	4.072f	0	919896	N.D.	0.249 #
6)	B beta-BHC	0.000	3.753	0	263688	N.D.	0.160 #
7)	B delta-BHC	4.665	0.000	1322373	0	0.856	N.D. #
8)	B Heptachlo...	0.000	4.572f	0	1089223	N.D.	0.328 #
13)	MA Dieldrin	0.000	5.173	0	401654	N.D.	0.122 #
14)	MA Endrin	0.000	5.481f	0	1357559	N.D.	0.497 #
16)	A 4,4'-DDD	6.579f	0.000	972890	0	0.952	N.D. #
23)	Chlordane-1	0.000	3.612	0	332483	N.D.	3.984 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
Data File : PL077372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2022 10:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 16:44:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

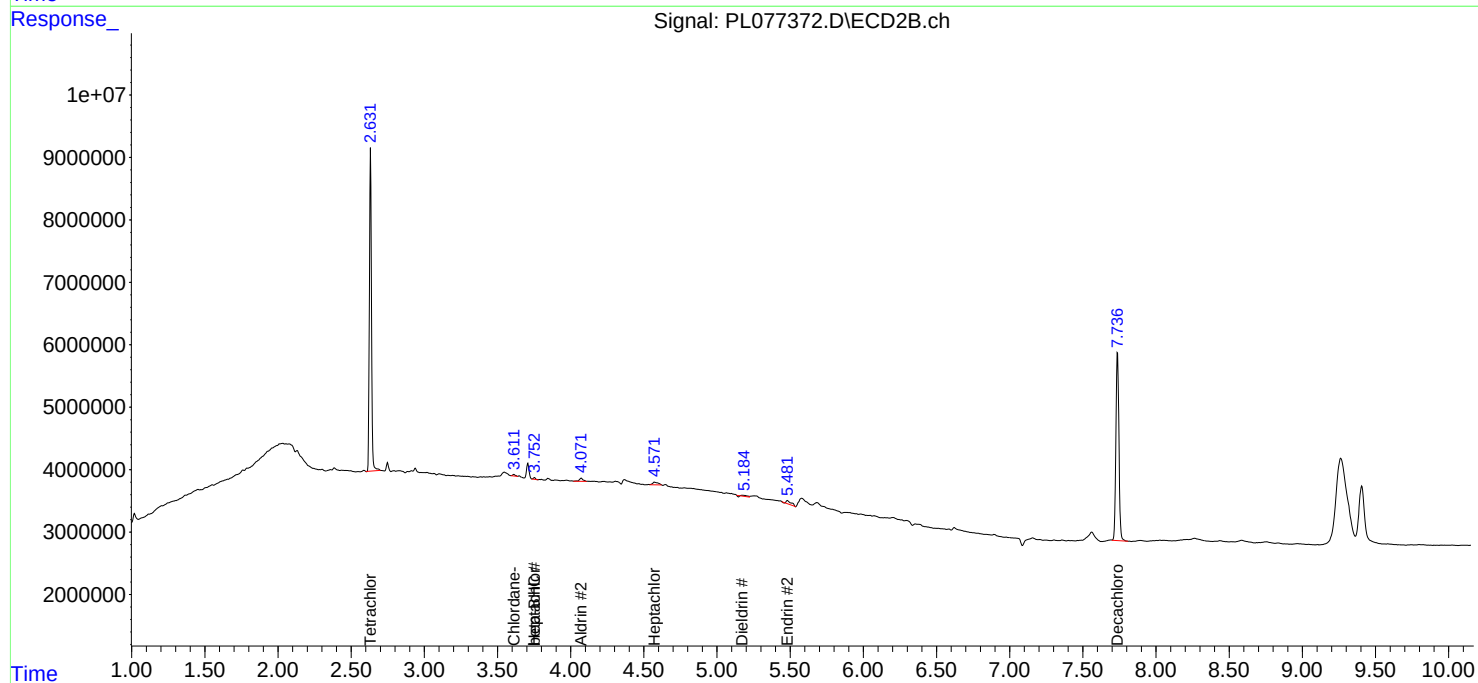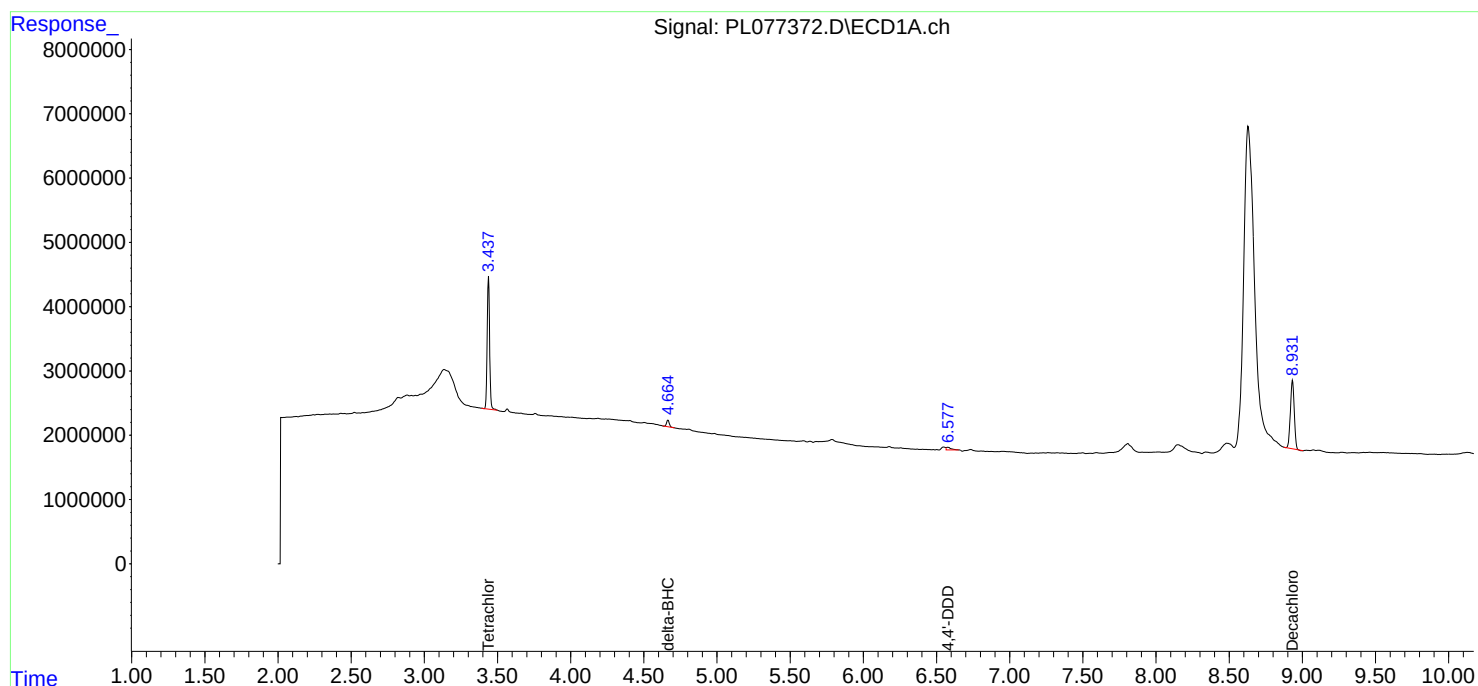


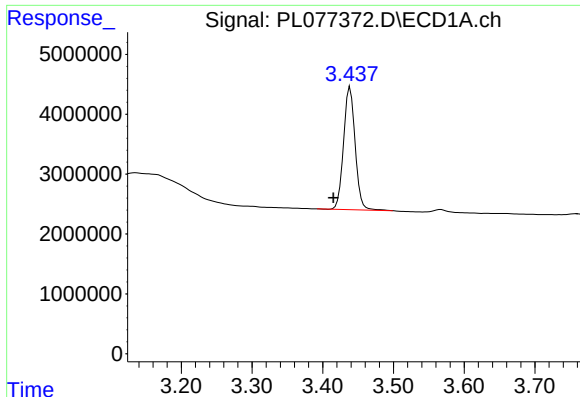

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.024 min
Response: 23312684
Conc: 17.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

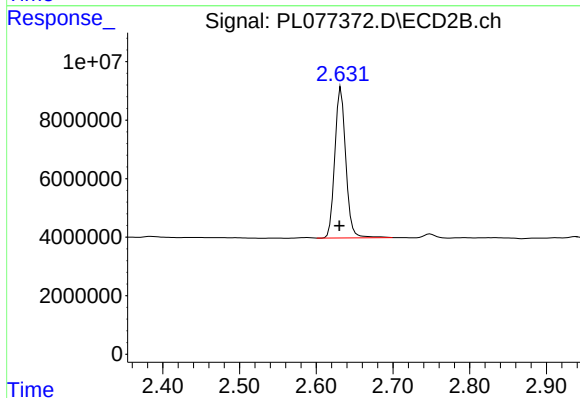


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: 0.002 min
Response: 50973062
Conc: 16.59 ng/ml

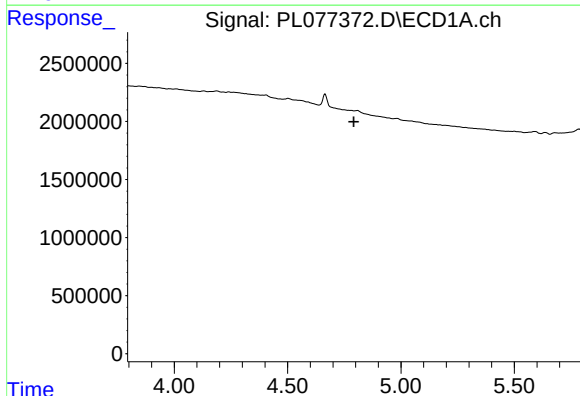


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.792 min
Response: 0
Conc: N.D.

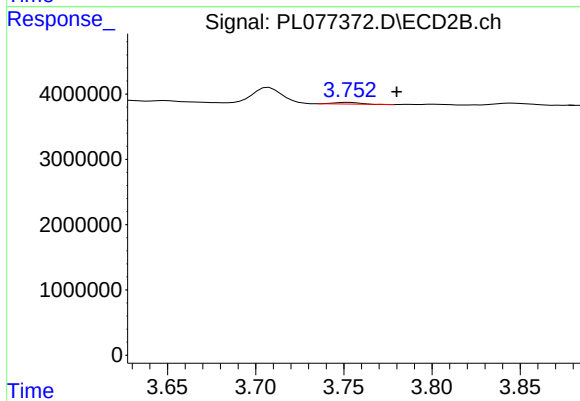

#4 Heptachlor


R.T.: 3.753 min
Delta R.T.: -0.027 min
Response: 263688
Conc: 0.07 ng/ml

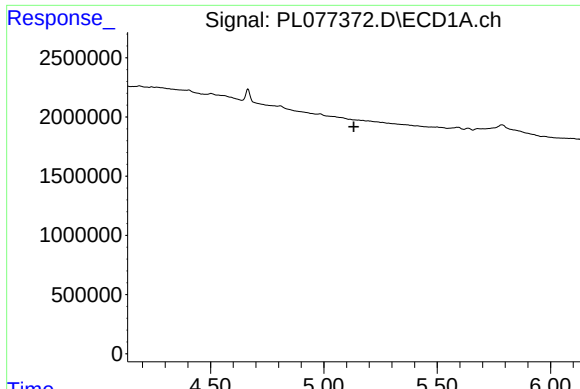

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

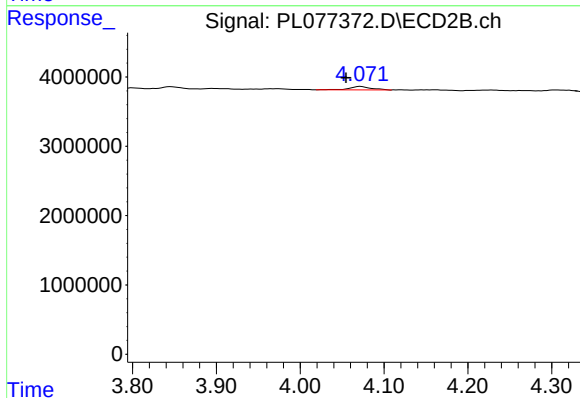


#5 Aldrin

R.T.: 4.072 min
Delta R.T.: 0.017 min
Response: 919896
Conc: 0.25 ng/ml

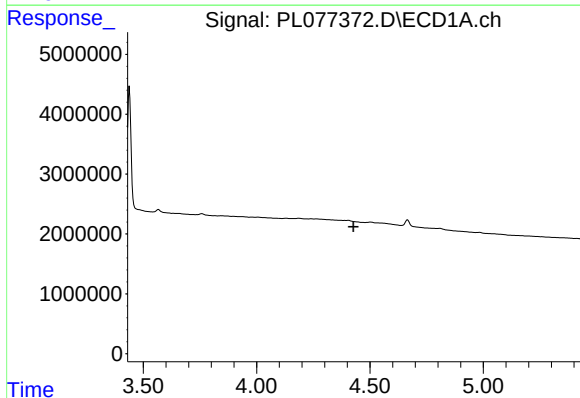


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.427 min
Response: 0
Conc: N.D.

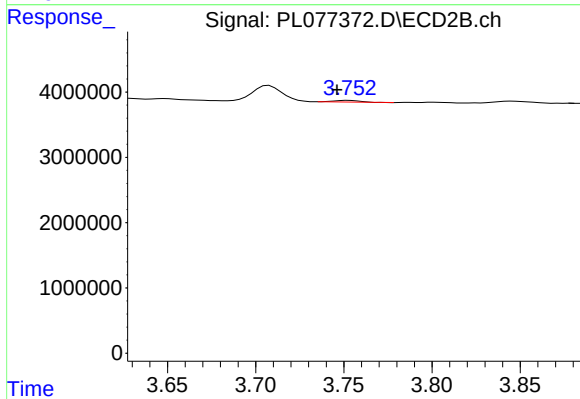

#6 beta-BHC


R.T.: 3.753 min
Delta R.T.: 0.007 min
Response: 263688
Conc: 0.16 ng/ml

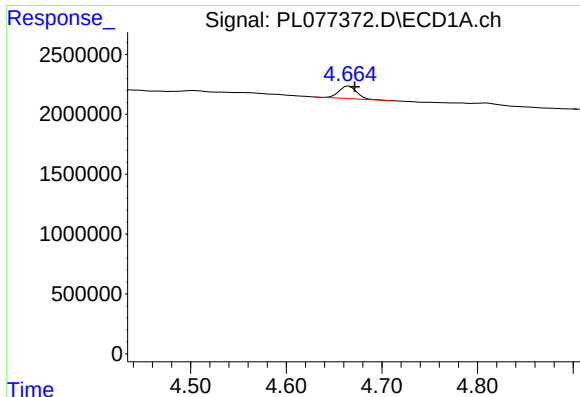

#7 delta-BHC


R.T.: 4.665 min
Delta R.T.: -0.006 min
Response: 1322373
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

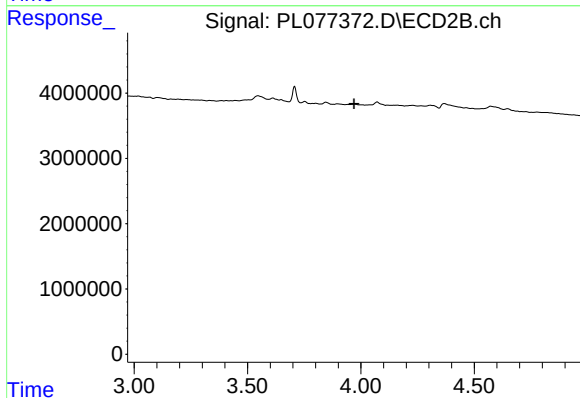


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

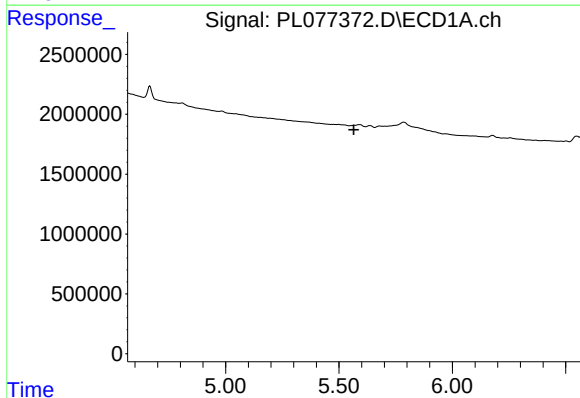


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.565 min
Response: 0
Conc: N.D.

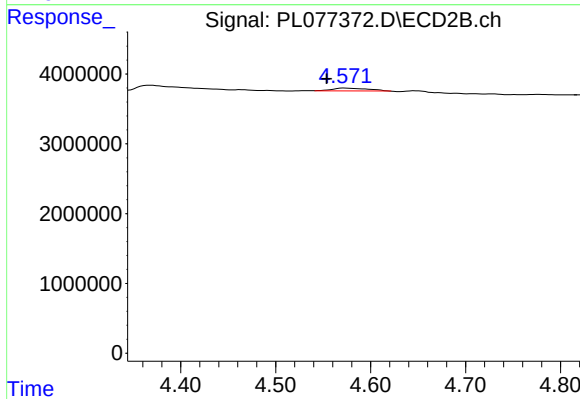

#8 Heptachlor epoxide


R.T.: 4.572 min
Delta R.T.: 0.018 min
Response: 1089223
Conc: 0.33 ng/ml

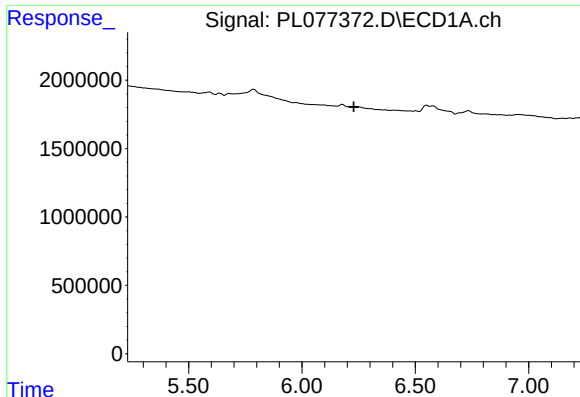

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

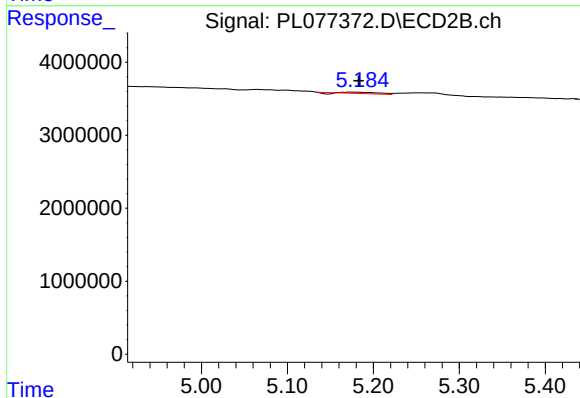


#13 Dieldrin

R.T.: 5.173 min
Delta R.T.: -0.010 min
Response: 401654
Conc: 0.12 ng/ml

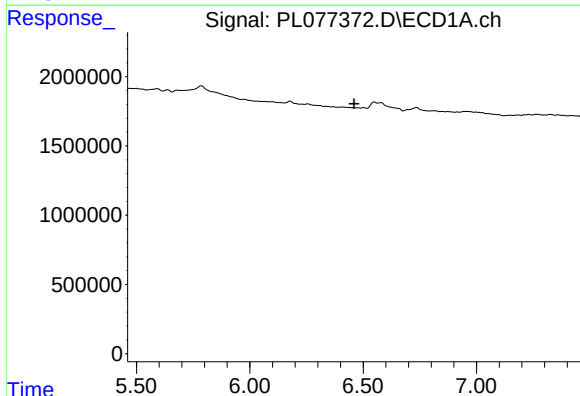


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.460 min
Response: 0
Conc: N.D.

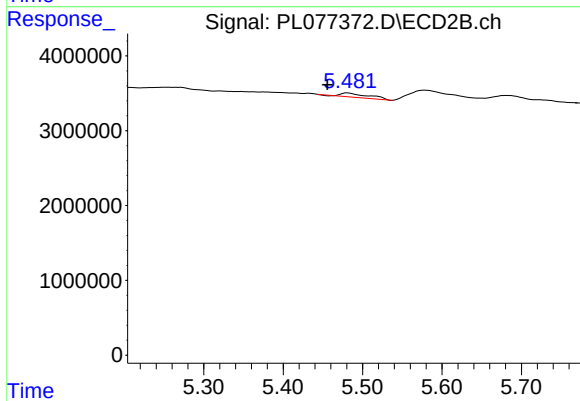

#14 Endrin


R.T.: 5.481 min
Delta R.T.: 0.026 min
Response: 1357559
Conc: 0.50 ng/ml

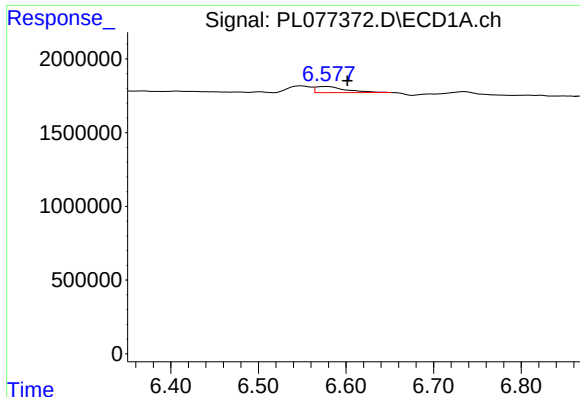

#16 4,4'-DDD


R.T.: 6.579 min
Delta R.T.: -0.023 min
Response: 972890
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

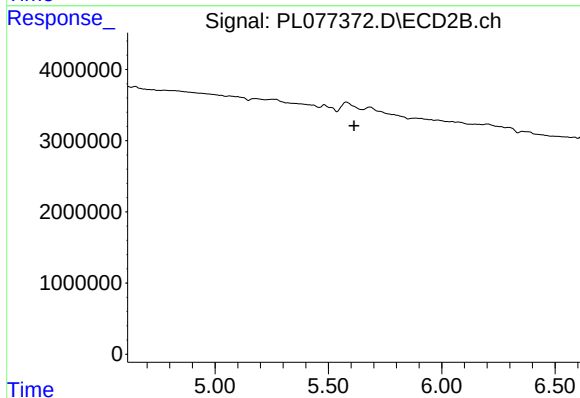


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.613 min
Response: 0
Conc: N.D.

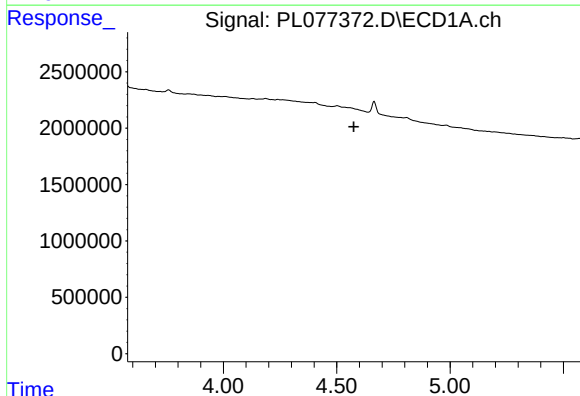


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.576 min
Response: 0
Conc: N.D.

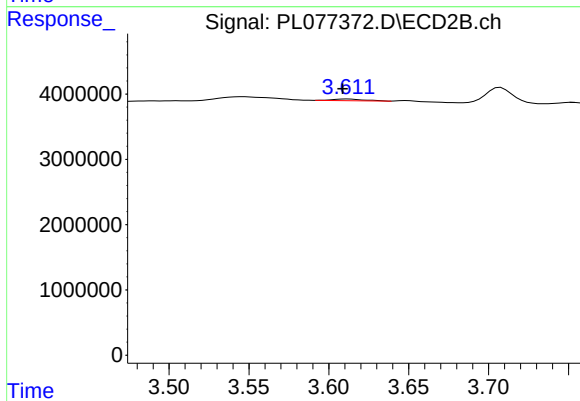

#23 Chlordane-1


R.T.: 3.612 min
Delta R.T.: 0.003 min
Response: 332483
Conc: 3.98 ng/ml

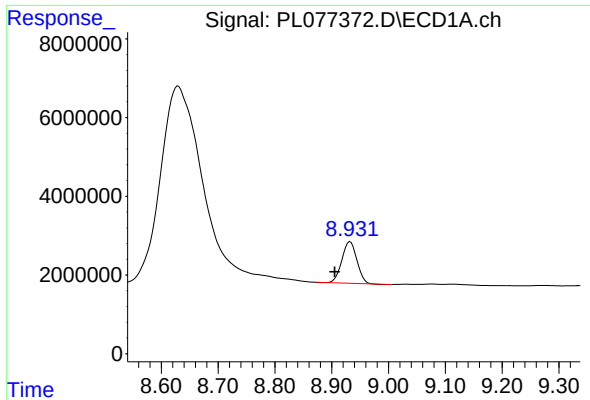

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: 0.027 min
Response: 19515811
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

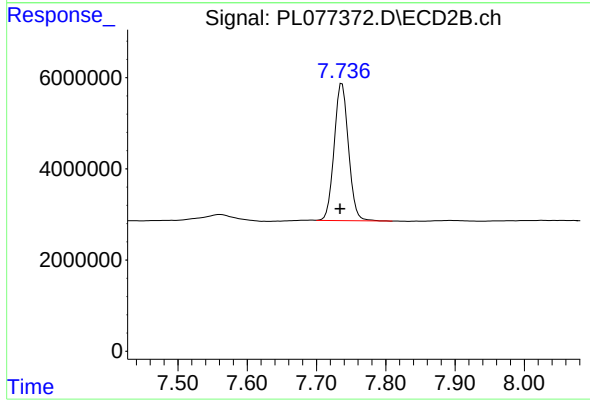

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: 0.003 min
Response: 43126974
Conc: 15.46 ng/ml