

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
 Data File : PL077390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2022 17:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 18:00:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.630	22761343	51810192	16.728	16.858
28)	SA Decachlor...	8.910	7.734	19880609	41507966	16.965	14.876
Target Compounds							
2)	A alpha-BHC	0.000	3.107f	0	125415	N.D.	0.029 #
5)	MB Aldrin	0.000	4.069	0	833935	N.D.	0.225 #
7)	B delta-BHC	4.642f	0.000	342166	0	0.221	N.D. #
8)	B Heptachlo...	5.571	0.000	239701	0	0.178	N.D. #
13)	MA Dieldrin	0.000	5.184	0	3110642	N.D.	0.947 #
14)	MA Endrin	0.000	5.478f	0	2416484	N.D.	0.884 #
15)	B Endosulfa...	6.711f	0.000	406907	0	0.371	N.D. #
16)	A 4,4'-DDD	0.000	5.612	0	1033874	N.D.	0.387 #
23)	Chlordane-1	0.000	3.613	0	250137	N.D.	2.997 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
Data File : PL077390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2022 17:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 18:00:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

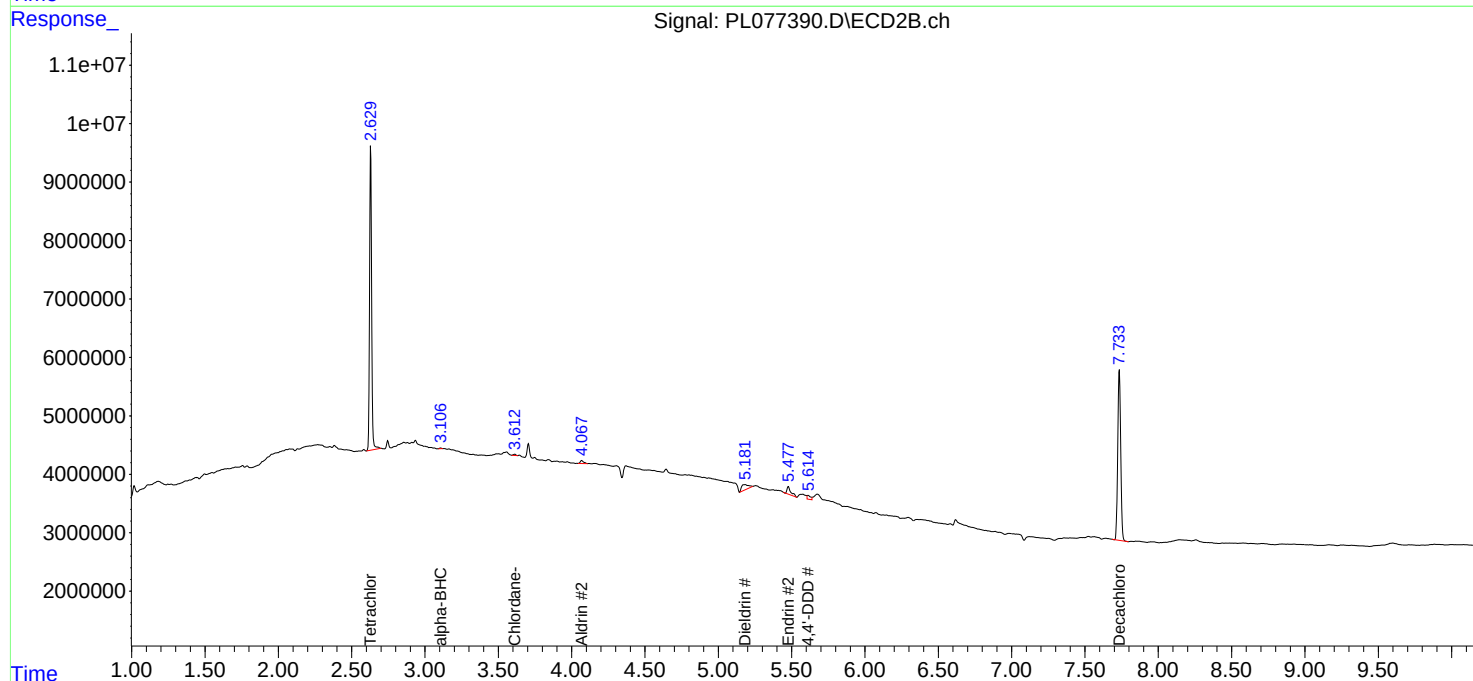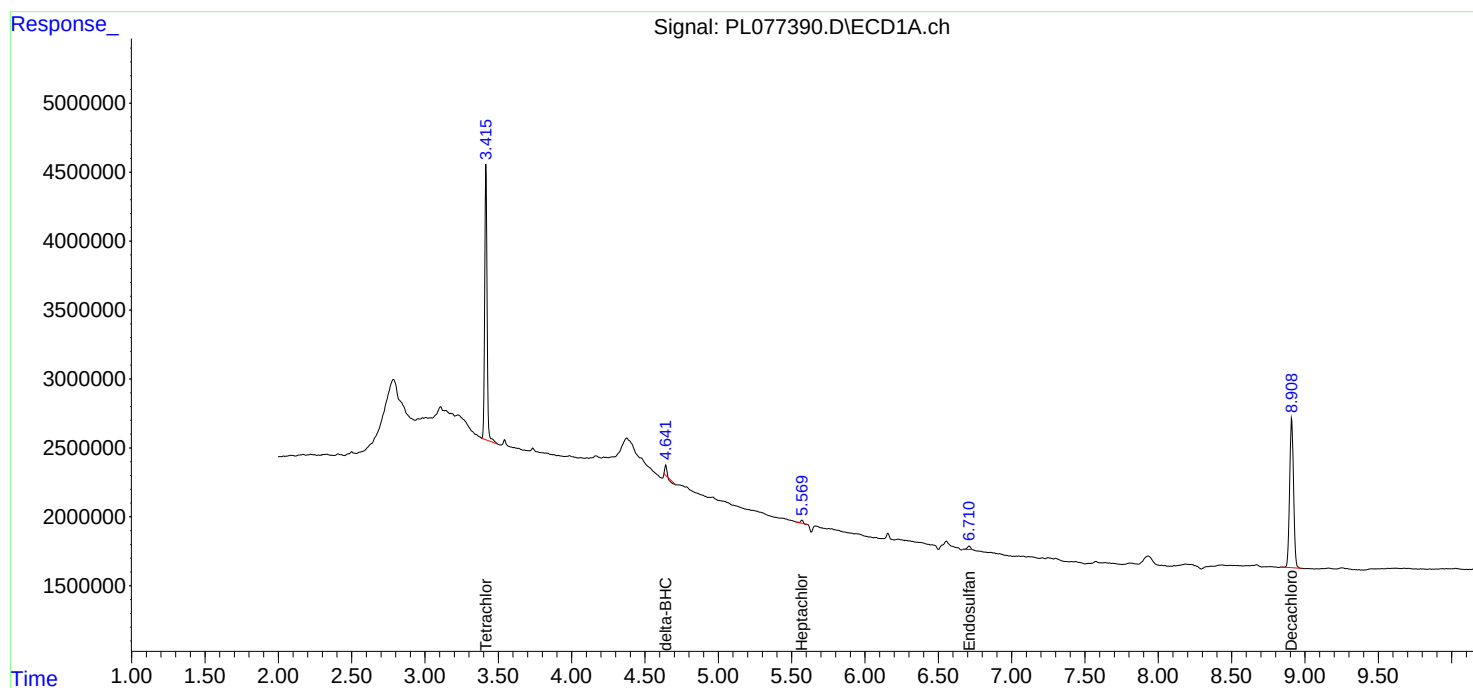


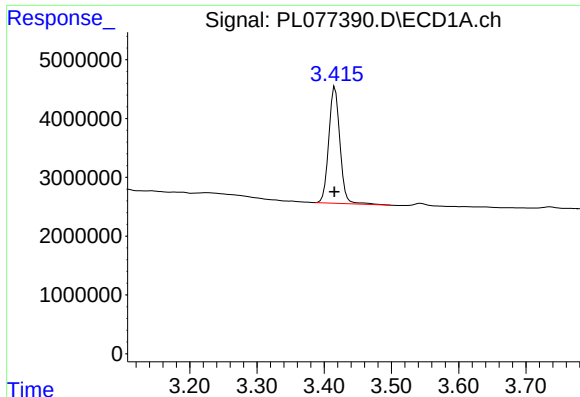

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.001 min
Response: 22761343
Conc: 16.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

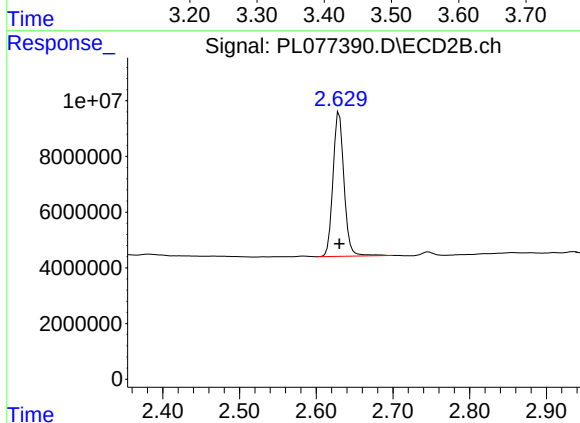


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 51810192
Conc: 16.86 ng/ml

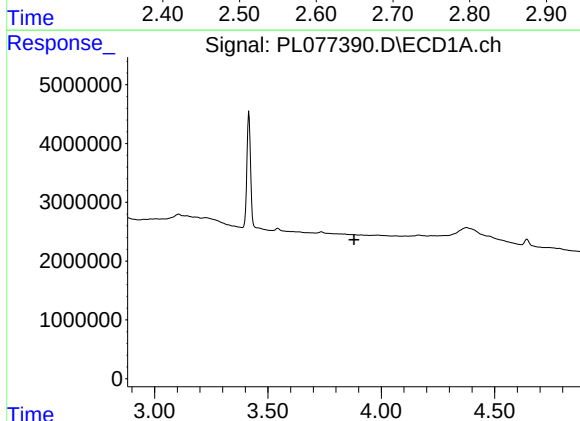


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.880 min
Response: 0
Conc: N.D.

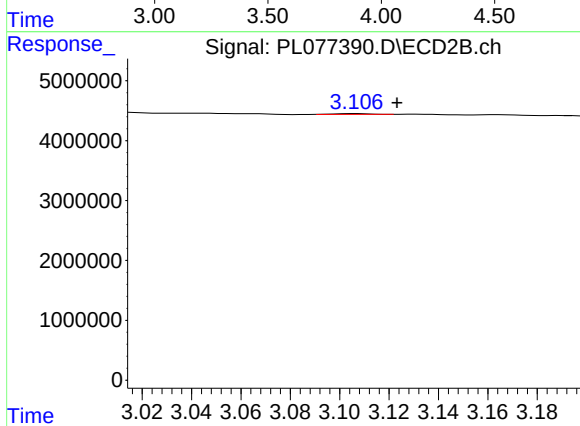

#2 alpha-BHC


R.T.: 3.107 min
Delta R.T.: -0.016 min
Response: 125415
Conc: 0.03 ng/ml

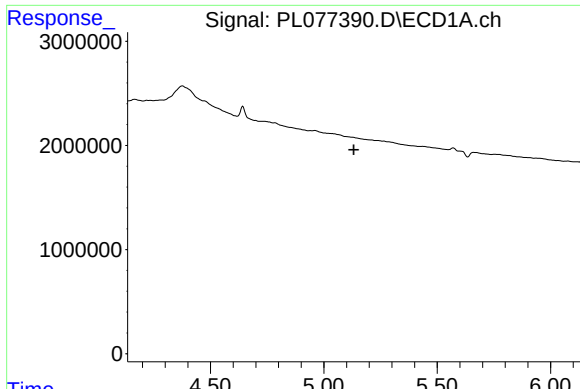

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

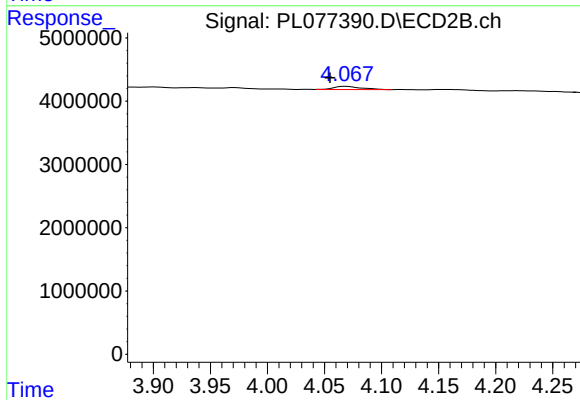


#5 Aldrin

R.T.: 4.069 min
Delta R.T.: 0.014 min
Response: 833935
Conc: 0.23 ng/ml

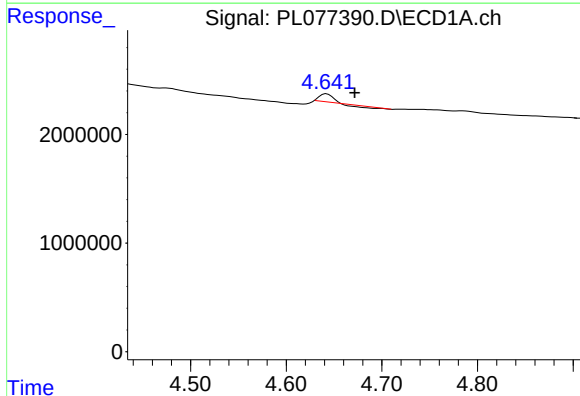


#7 delta-BHC

R.T.: 4.642 min
Delta R.T.: -0.029 min
Response: 342166
Conc: 0.22 ng/ml

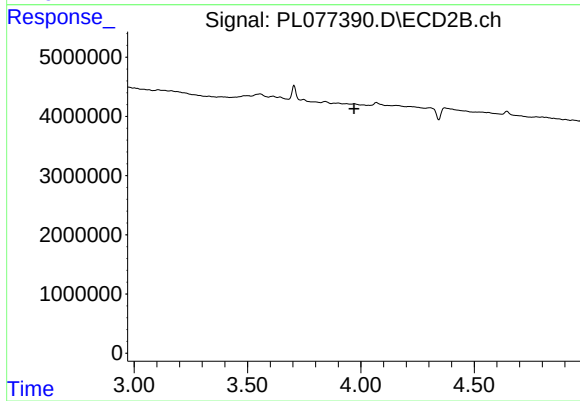

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 3.970 min
Response: 0
Conc: N.D.

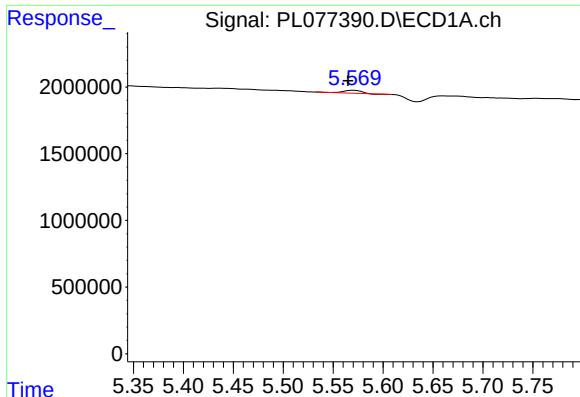

#8 Heptachlor epoxide


R.T.: 5.571 min
Delta R.T.: 0.006 min
Response: 239701
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

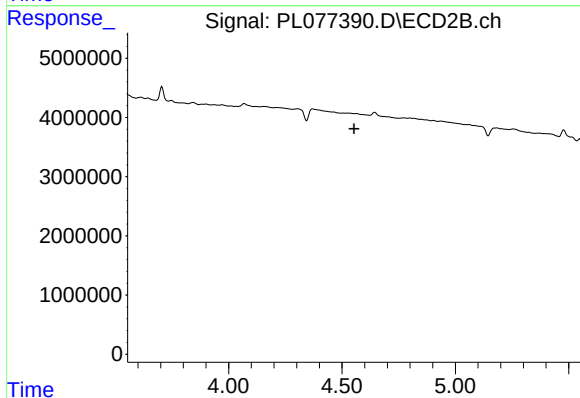


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

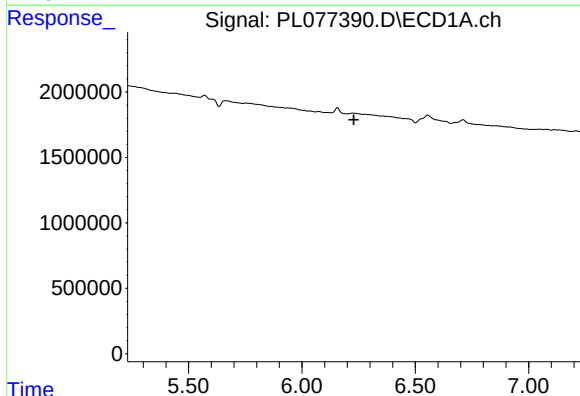


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.229 min
Response: 0
Conc: N.D.

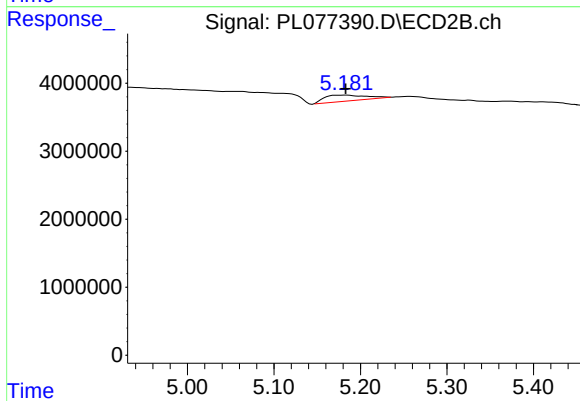

#13 Dieldrin


R.T.: 5.184 min
Delta R.T.: 0.001 min
Response: 3110642
Conc: 0.95 ng/ml

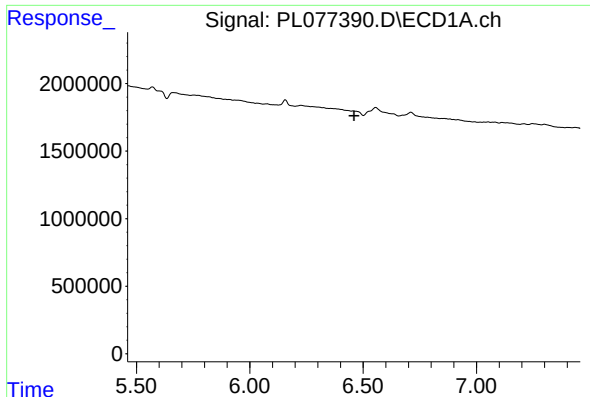

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

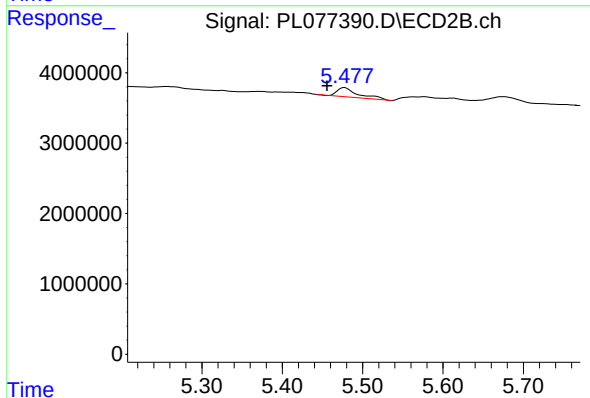


#14 Endrin

R.T.: 5.478 min
Delta R.T.: 0.022 min
Response: 2416484
Conc: 0.88 ng/ml

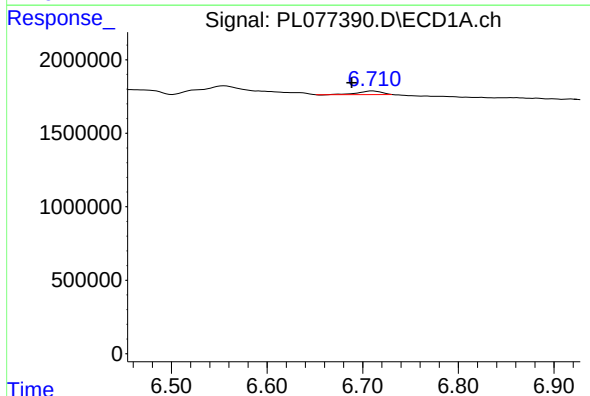


#15 Endosulfan II

R.T.: 6.711 min
Delta R.T.: 0.022 min
Response: 406907
Conc: 0.37 ng/ml

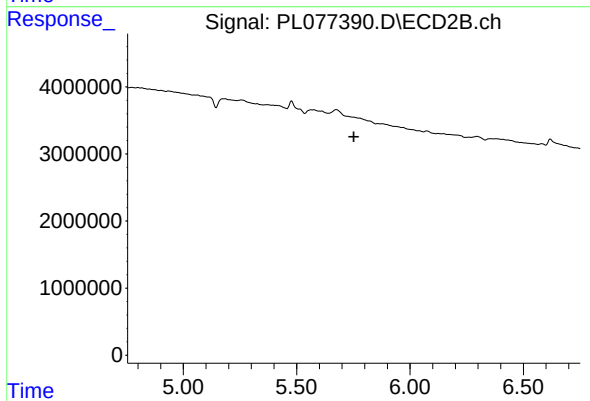

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.752 min
Response: 0
Conc: N.D.

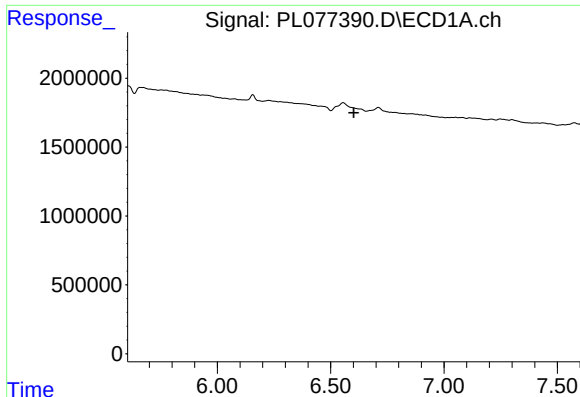

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

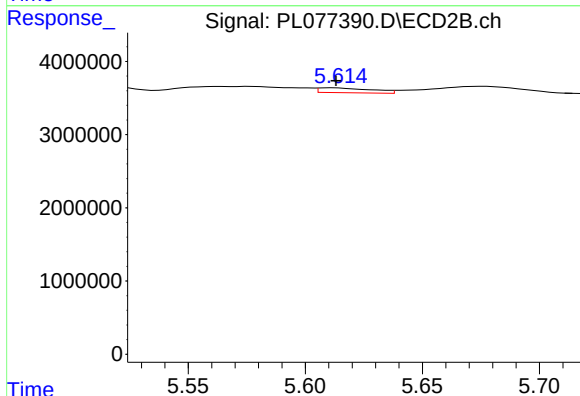


#16 4,4'-DDD

R.T.: 5.612 min
Delta R.T.: -0.001 min
Response: 1033874
Conc: 0.39 ng/ml

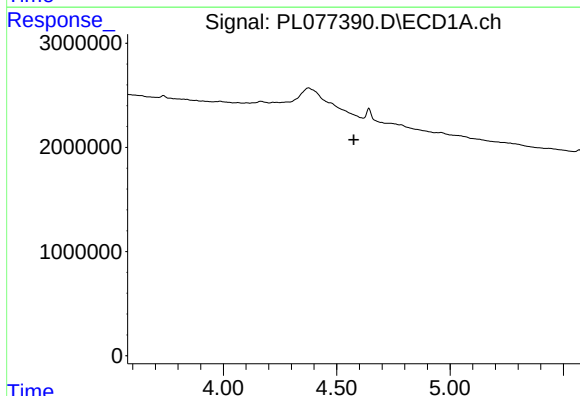


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.576 min
Response: 0
Conc: N.D.

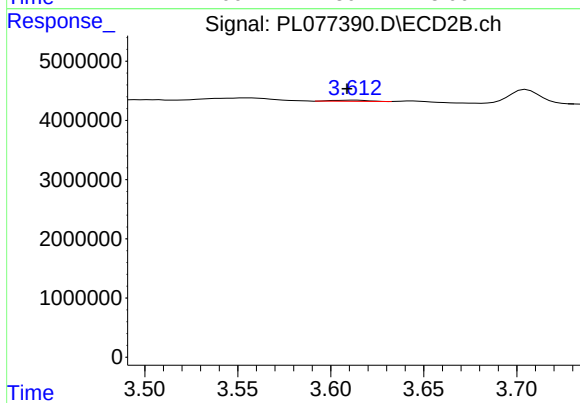

#23 Chlordane-1


R.T.: 3.613 min
Delta R.T.: 0.004 min
Response: 250137
Conc: 3.00 ng/ml

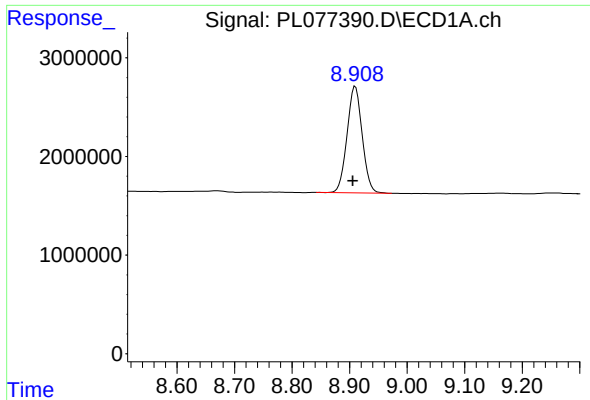

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.004 min
Response: 19880609
Conc: 16.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

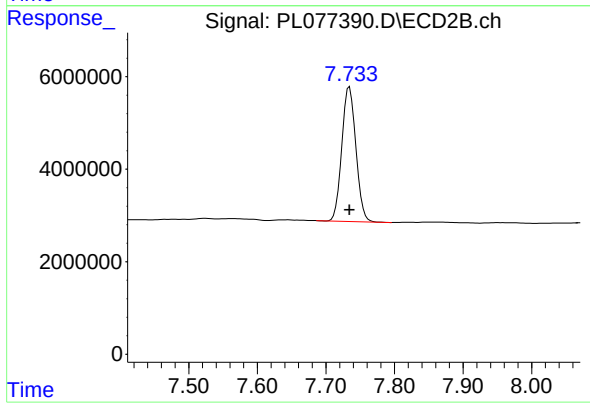

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 41507966
Conc: 14.88 ng/ml