

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
 Data File : PL077371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2022 10:13
 Operator : AR\AJ
 Sample : N4395-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220738-MANASQUAN-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 16:44:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.425	2.633	29512094	61281014	21.689	19.940
28) SA Decachlor...	8.918	7.740	20991663	45955349	17.913	16.470

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL083022\
Data File : PL077371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2022 10:13
Operator : AR\AJ
Sample : N4395-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20220738-MANASQUAN-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 16:44:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

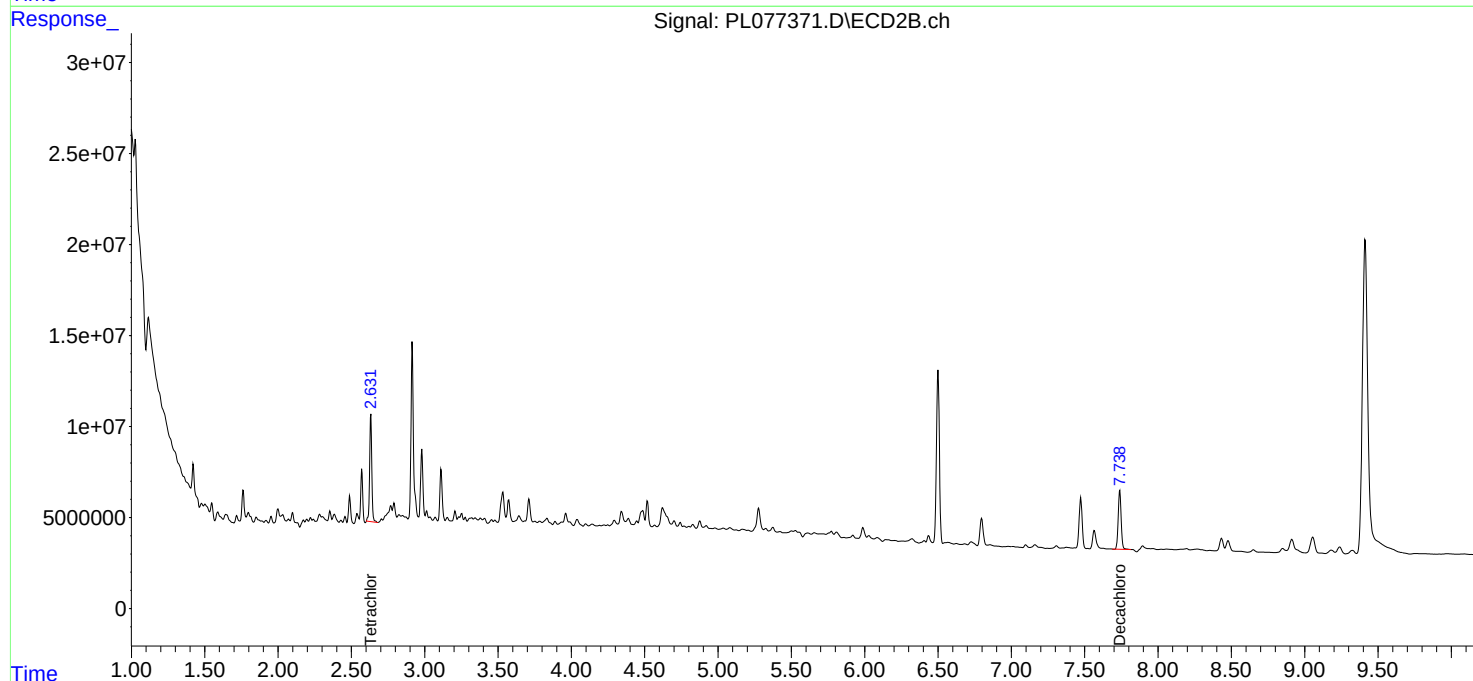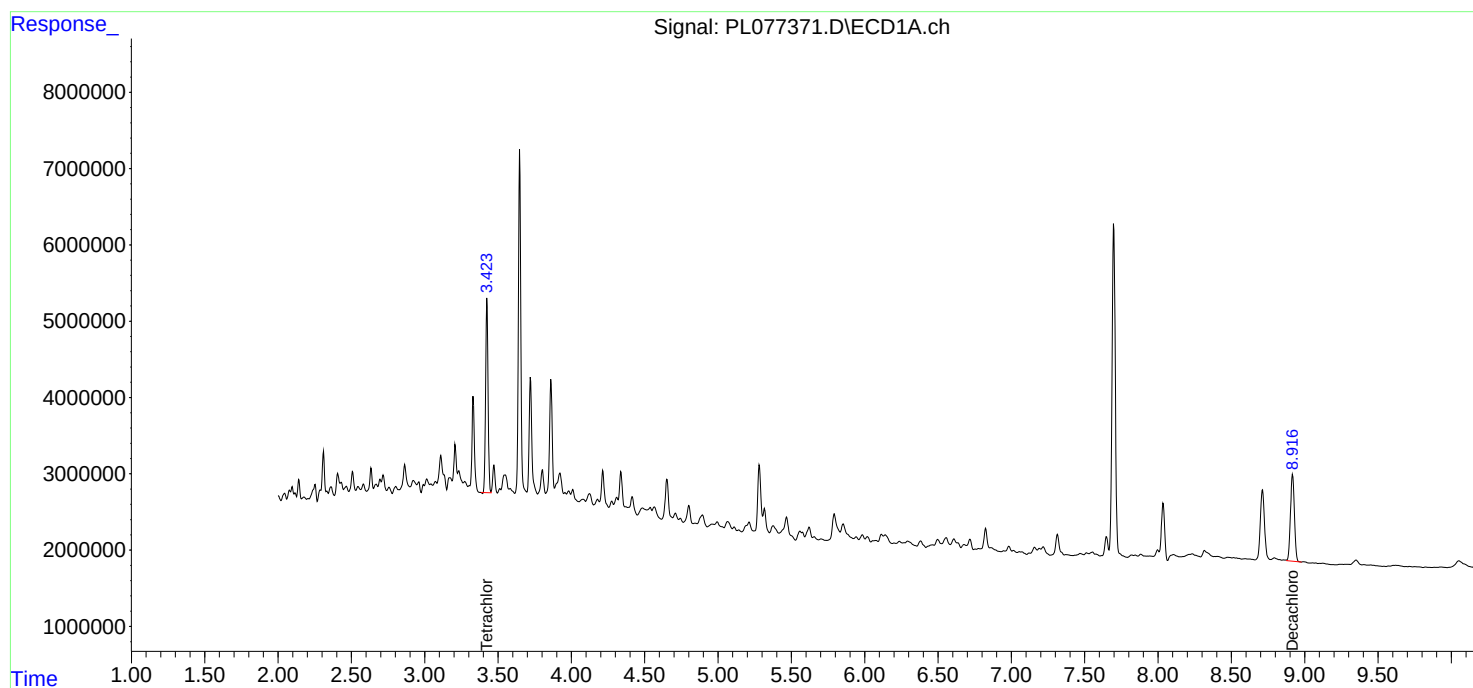


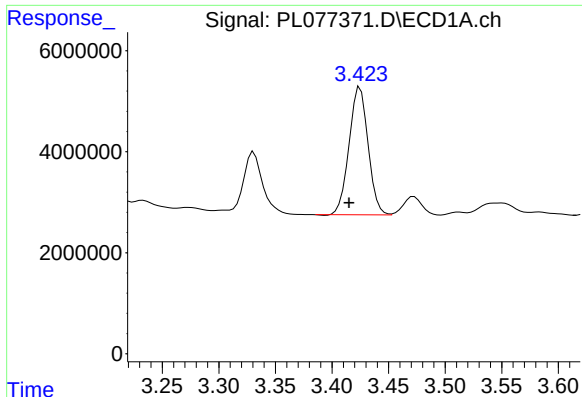

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: 0.010 min
Response: 29512094
Conc: 21.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220738-MANASQUAN-WATER

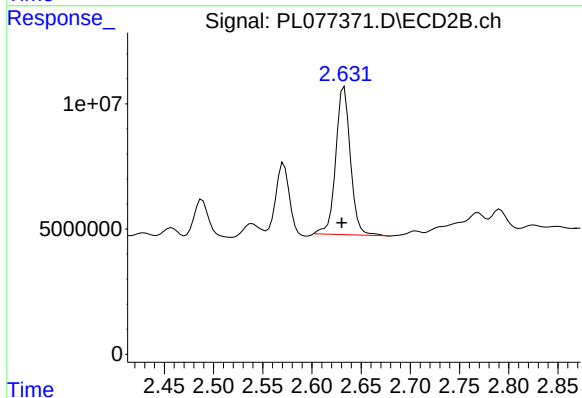


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: 0.003 min
Response: 61281014
Conc: 19.94 ng/ml

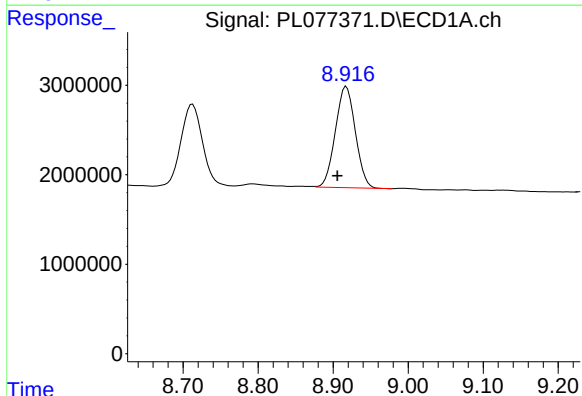

#28 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: 0.012 min
Response: 20991663
Conc: 17.91 ng/ml

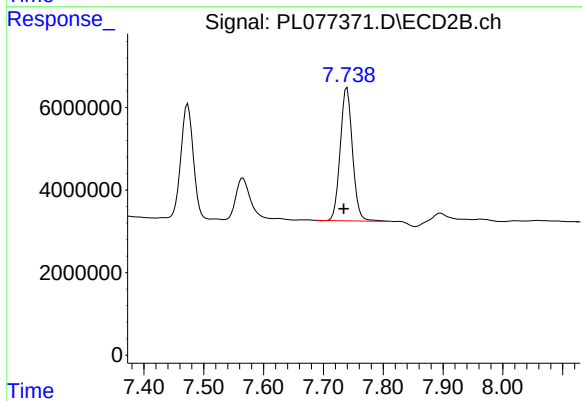

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.005 min
Response: 45955349
Conc: 16.47 ng/ml